

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081621\
 Data File : PS016403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2021 14:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 06:24:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	6.766	600.4E6	248.7E6	408.112	476.779
Target Compounds							
5) T	DICAMBA	7.377	6.930	6732827	3457427	1.202	1.587 #
10) T	Pentachlo...	8.609	8.268	10331991	5066061	<MDL	<MDL #
11) T	2,4,5-TP ...	9.165	8.631	7968936	3888040	1.102	1.333
12) T	2,4,5-T	9.467	9.017	27079036	6693578	3.552	2.311 #
14) T	DINOSEB	11.147	9.839	22106021	3769996	4.192	1.850 #
15) T	Picloram	10.995	10.828	279.3E6	125.2E6	27.987	31.097
16) T	DCPA	11.414	10.767	16974684	7032756	1.606	1.565



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081621\
Data File : PS016403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2021 14:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 06:24:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

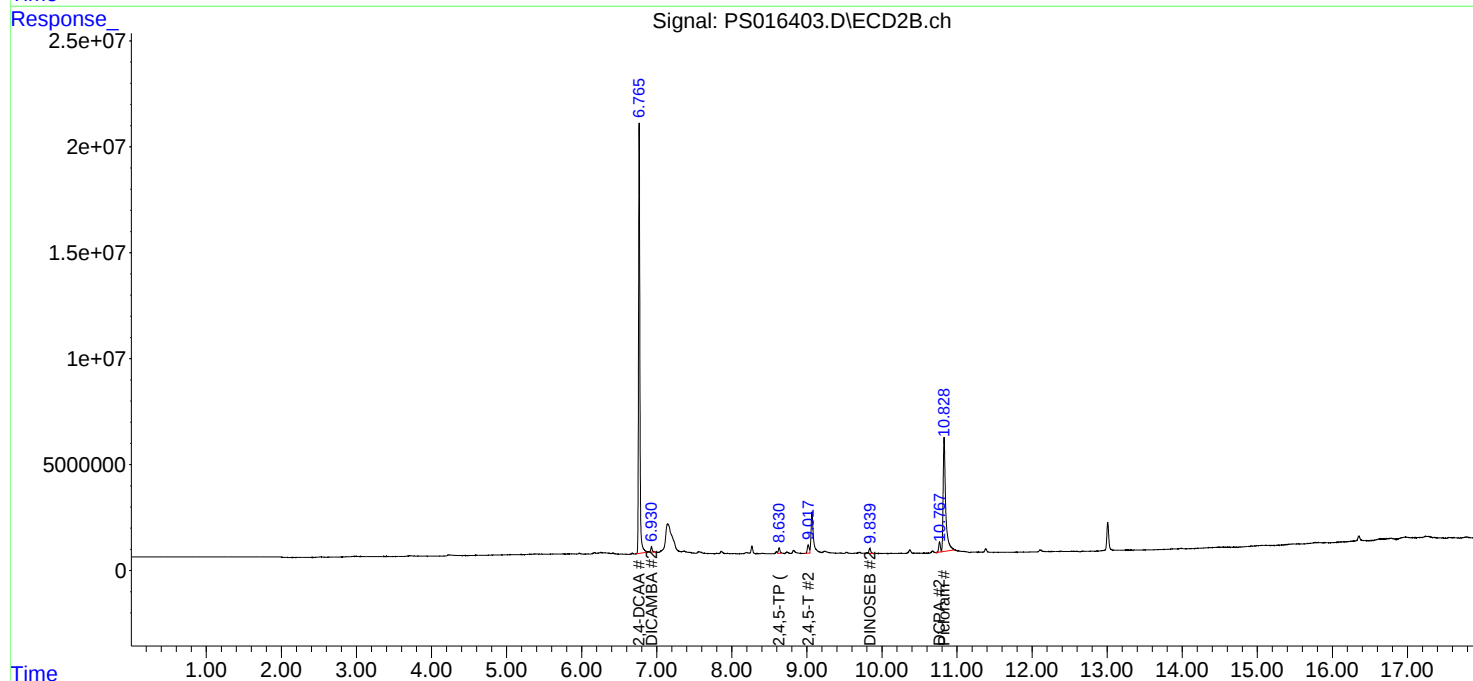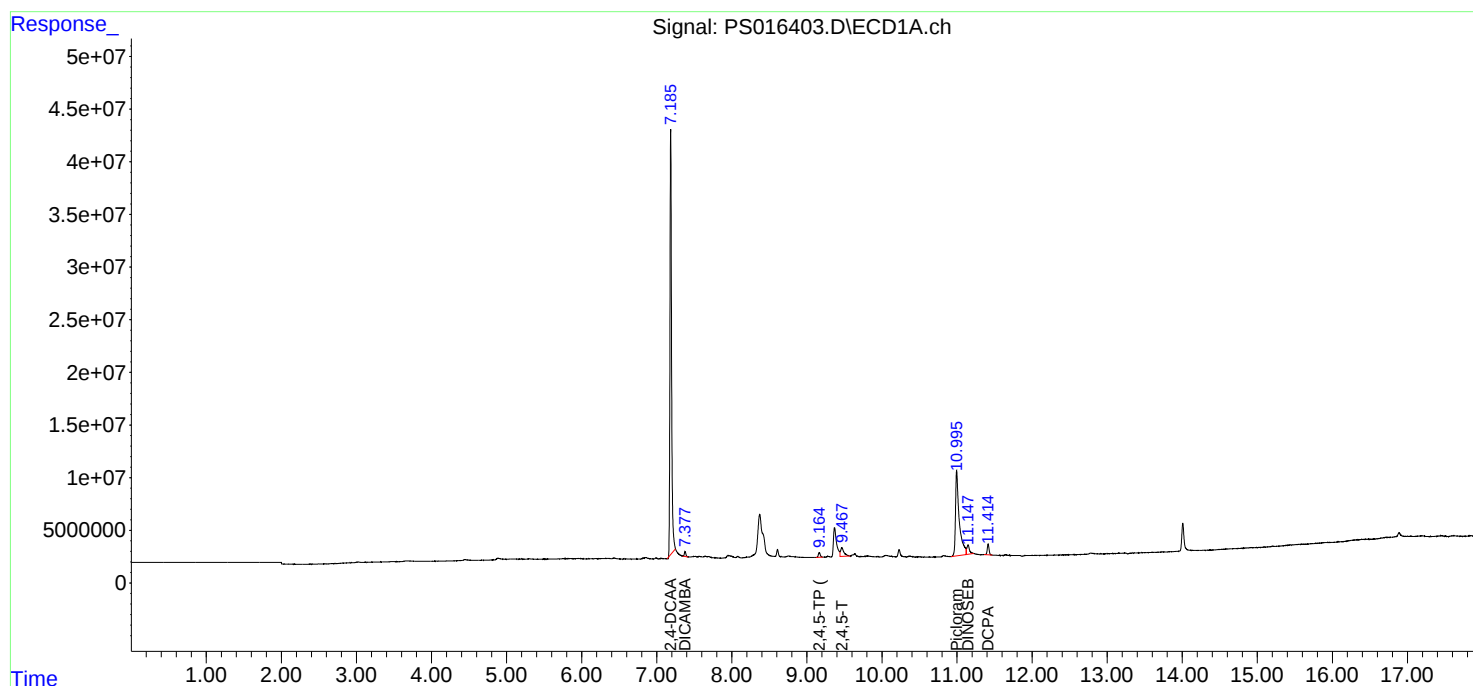


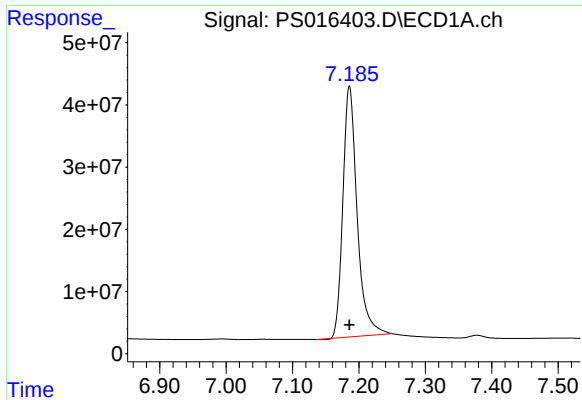

#4 2,4-DCAA


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 600375820
Conc: 408.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

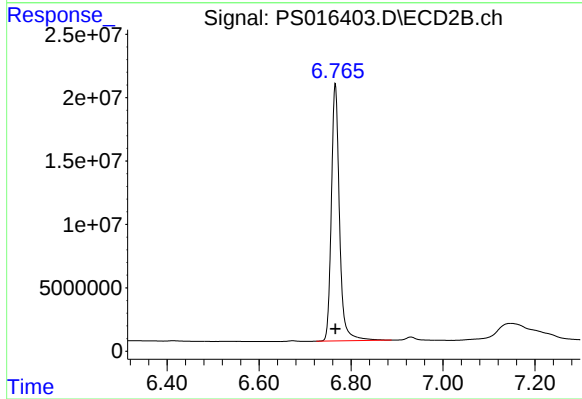


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: 0.000 min
Response: 248699818
Conc: 476.78 ng/ml

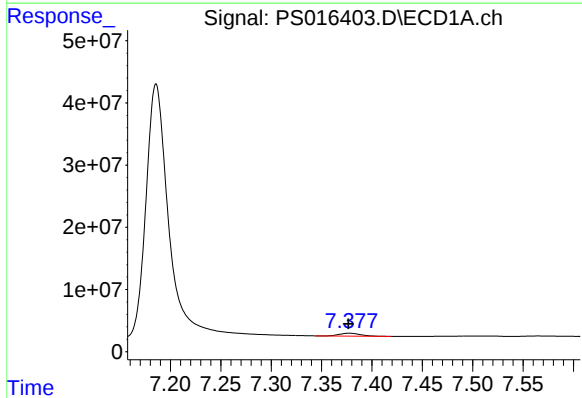


#5 DICAMBA

R.T.: 7.377 min
Delta R.T.: 0.000 min
Response: 6732827
Conc: 1.20 ng/ml

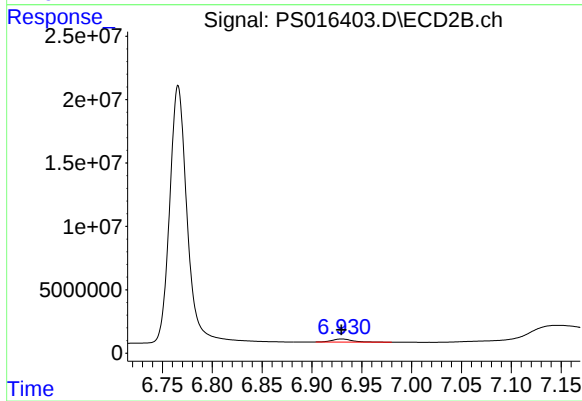

#5 DICAMBA


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 3457427
Conc: 1.59 ng/ml

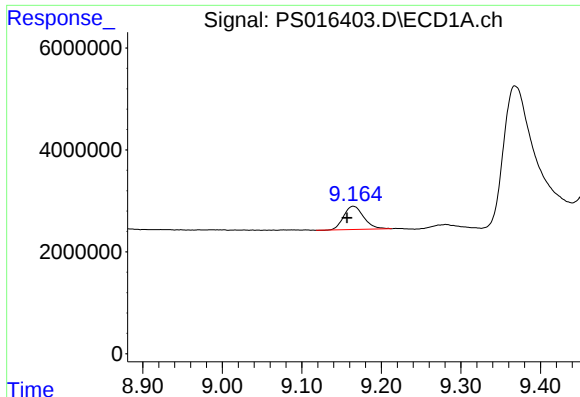

#11 2,4,5-TP (SILVEX)


R.T.: 9.165 min
Delta R.T.: 0.008 min
Response: 7968936
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

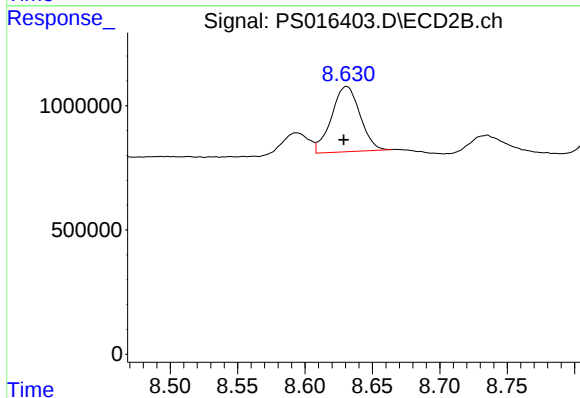


#11 2,4,5-TP (SILVEX)

R.T.: 8.631 min
Delta R.T.: 0.002 min
Response: 3888040
Conc: 1.33 ng/ml

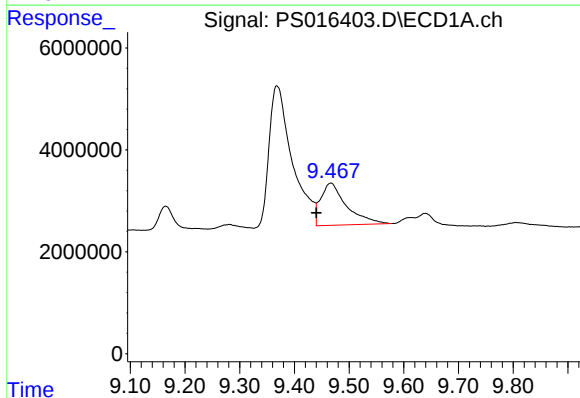


#12 2,4,5-T

R.T.: 9.467 min
Delta R.T.: 0.026 min
Response: 27079036
Conc: 3.55 ng/ml

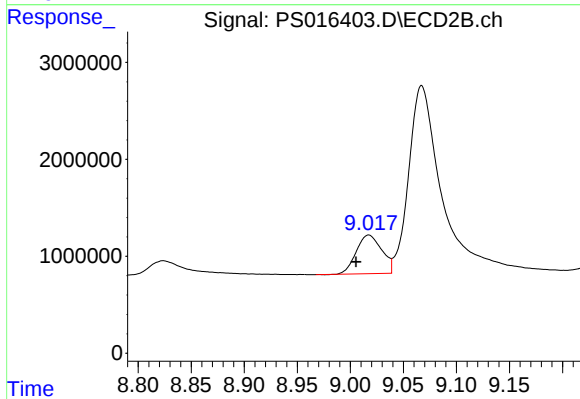

#12 2,4,5-T


R.T.: 9.017 min
Delta R.T.: 0.012 min
Response: 6693578
Conc: 2.31 ng/ml

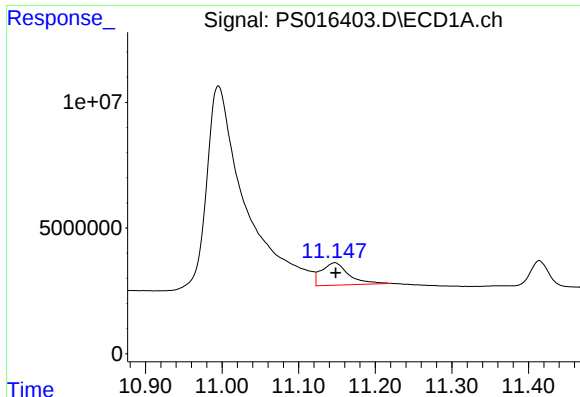

#14 DINOSEB


R.T.: 11.147 min
Delta R.T.: -0.001 min
Response: 22106021
Conc: 4.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

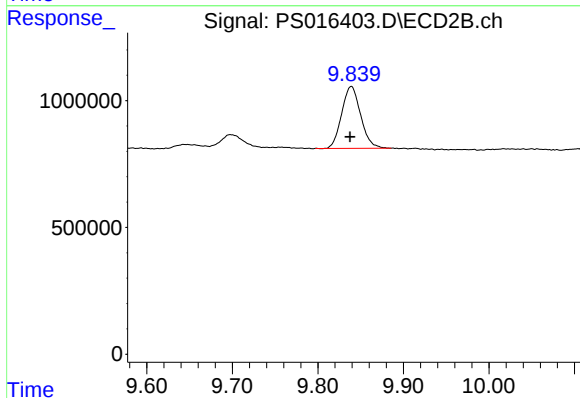


#14 DINOSEB

R.T.: 9.839 min
Delta R.T.: 0.001 min
Response: 3769996
Conc: 1.85 ng/ml

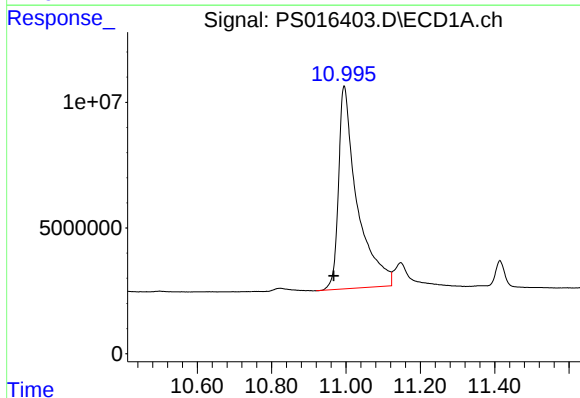


#15 Picloram

R.T.: 10.995 min
Delta R.T.: 0.028 min
Response: 279330159
Conc: 27.99 ng/ml

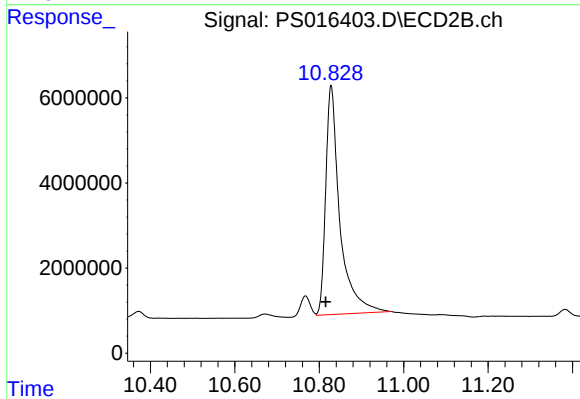

#15 Picloram


R.T.: 10.828 min
Delta R.T.: 0.013 min
Response: 125215479
Conc: 31.10 ng/ml

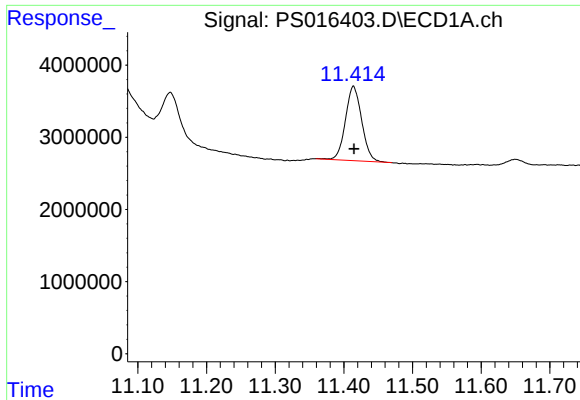

#16 DCPA

R.T.: 11.414 min
Delta R.T.: -0.001 min
Response: 16974684
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

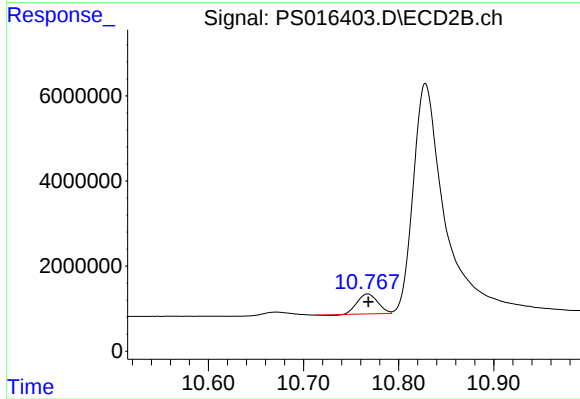

#16 DCPA

R.T.: 10.767 min
Delta R.T.: 0.000 min
Response: 7032756
Conc: 1.56 ng/ml