

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081622\
 Data File : PS020291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2022 09:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 11:37:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.758	1351.5E6	456.0E6	458.319	559.531
Target Compounds							
1) T	Dalapon	2.998	0.000	596023	0	<MDL	N.D. #
3) T	4-Nitroph...	6.988f	0.000	312251	0	<MDL	N.D. #
7) T	MCPA	7.702	0.000	1288236	0	<MDL	N.D. #
10) T	Pentachlo...	8.644f	0.000	196186	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.080f	0.000	1427509	0	<MDL	N.D. #
12) T	2,4,5-T	9.412	0.000	14519912	0	<MDL	N.D. #
13) T	2,4-DB	10.002	0.000	984827	0	<MDL	N.D. #
15) T	Picloram	10.955	10.847	8815294	8056563	<MDL	1.068 #
16) T	DCPA	11.415	0.000	3606594	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081622\
Data File : PS020291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2022 09:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 11:37:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

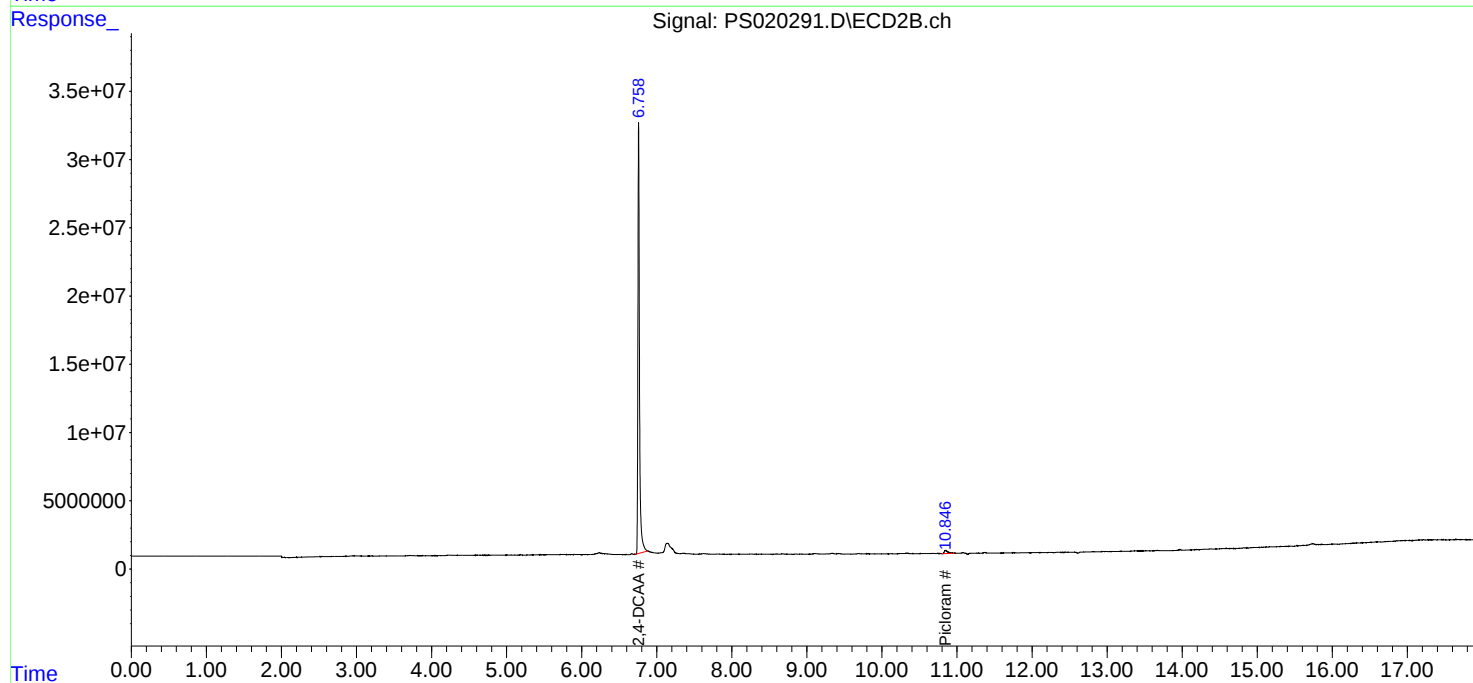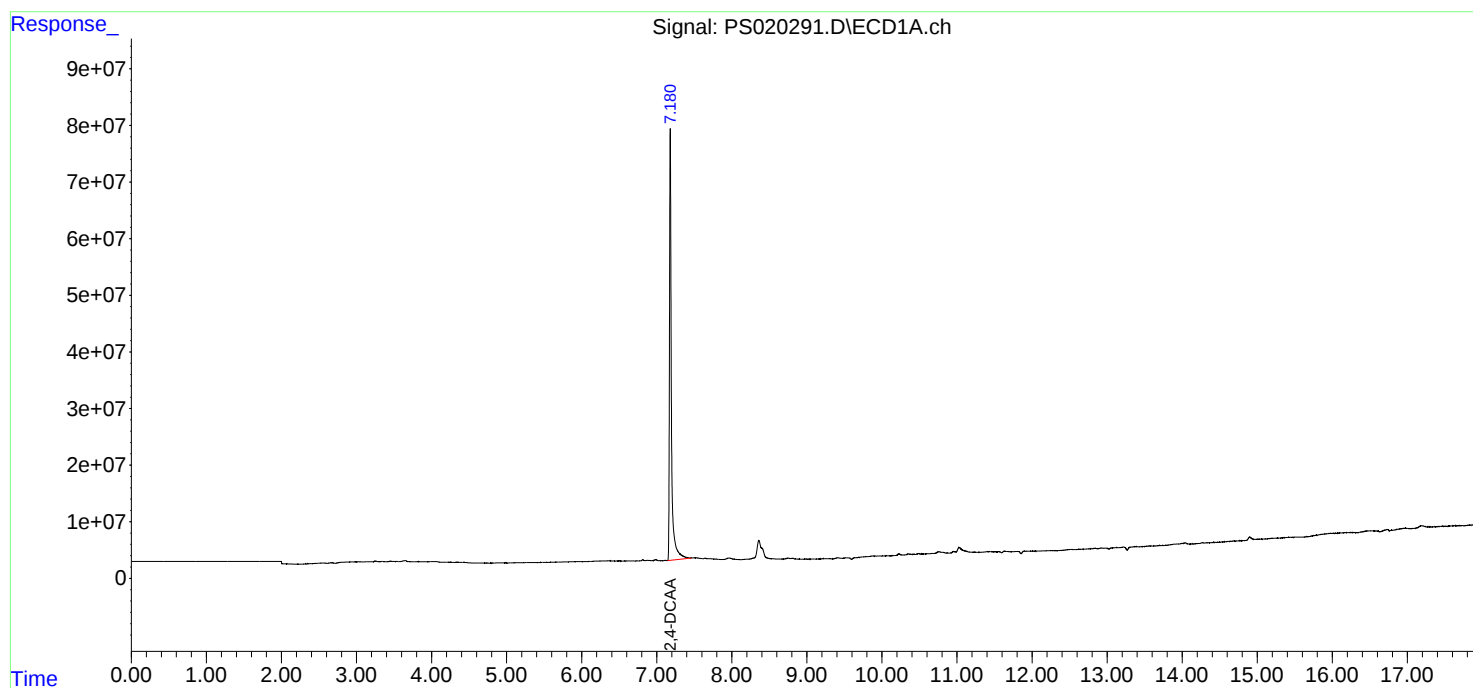


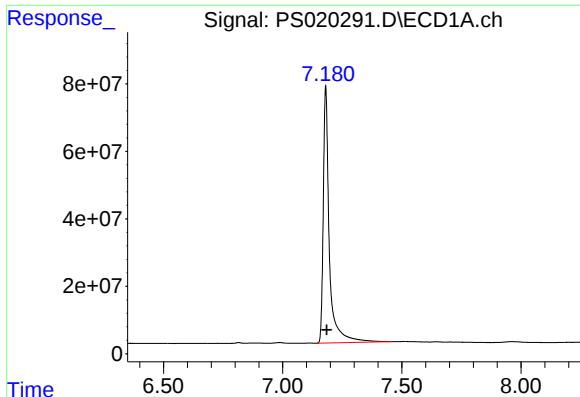

#4 2,4-DCAA


R.T.: 7.180 min
Delta R.T.: -0.005 min
Response: 1351457216
Conc: 458.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

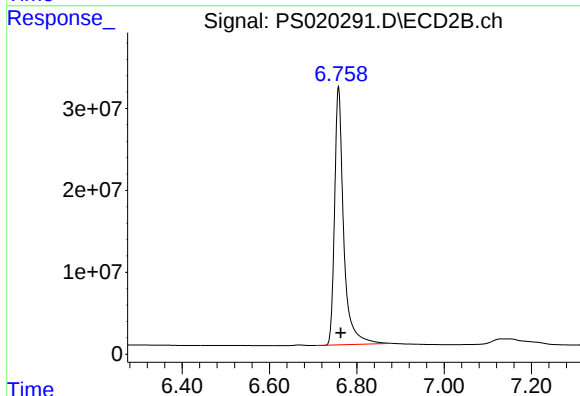


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: -0.005 min
Response: 455993267
Conc: 559.53 ng/ml

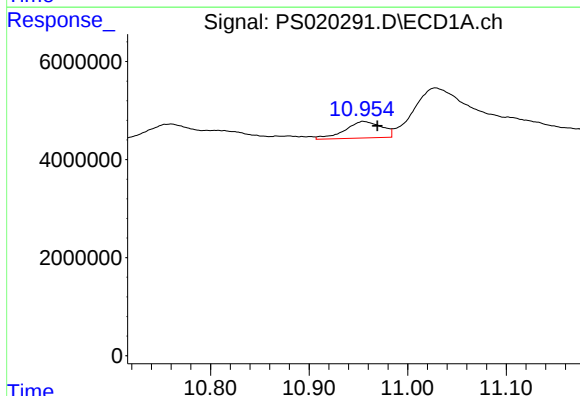

#15 Picloram

R.T.: 10.955 min
Delta R.T.: -0.014 min
Response: 8815294
Conc: N.D.

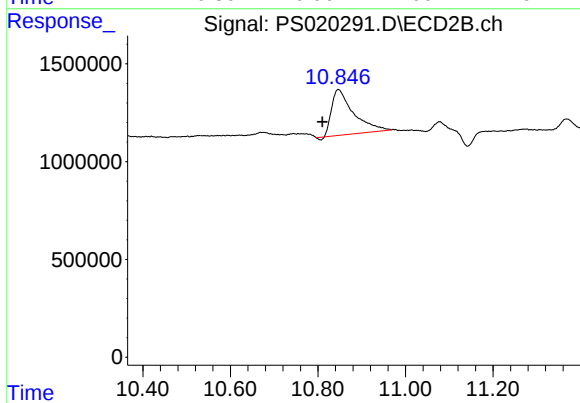

#15 Picloram

R.T.: 10.847 min
Delta R.T.: 0.036 min
Response: 8056563
Conc: 1.07 ng/ml