

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081622\
 Data File : PS020307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2022 19:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 23:56:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.757	1410.2E6	468.3E6	478.234	574.637
Target Compounds							
1) T	Dalapon	3.008	0.000	217355	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.421	0.000	12516	0	<MDL	N.D. #
7) T	MCPA	7.679	0.000	4816631	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.605f	0	2108040	N.D.	2.254
11) T	2,4,5-TP ...	9.156	8.583	2300398	1572425	<MDL	<MDL #
12) T	2,4,5-T	9.461	9.023	7994396	1197815	<MDL	<MDL #
13) T	2,4-DB	10.011	0.000	2940114	0	<MDL	N.D. #
14) T	DINOSEB	11.095	0.000	11566825	0	<MDL	N.D. #
15) T	Picloram	10.944	10.840	19080834	3299168	<MDL	<MDL #
16) T	DCPA	11.347f	0.000	763080	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081622\
Data File : PS020307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2022 19:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 23:56:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

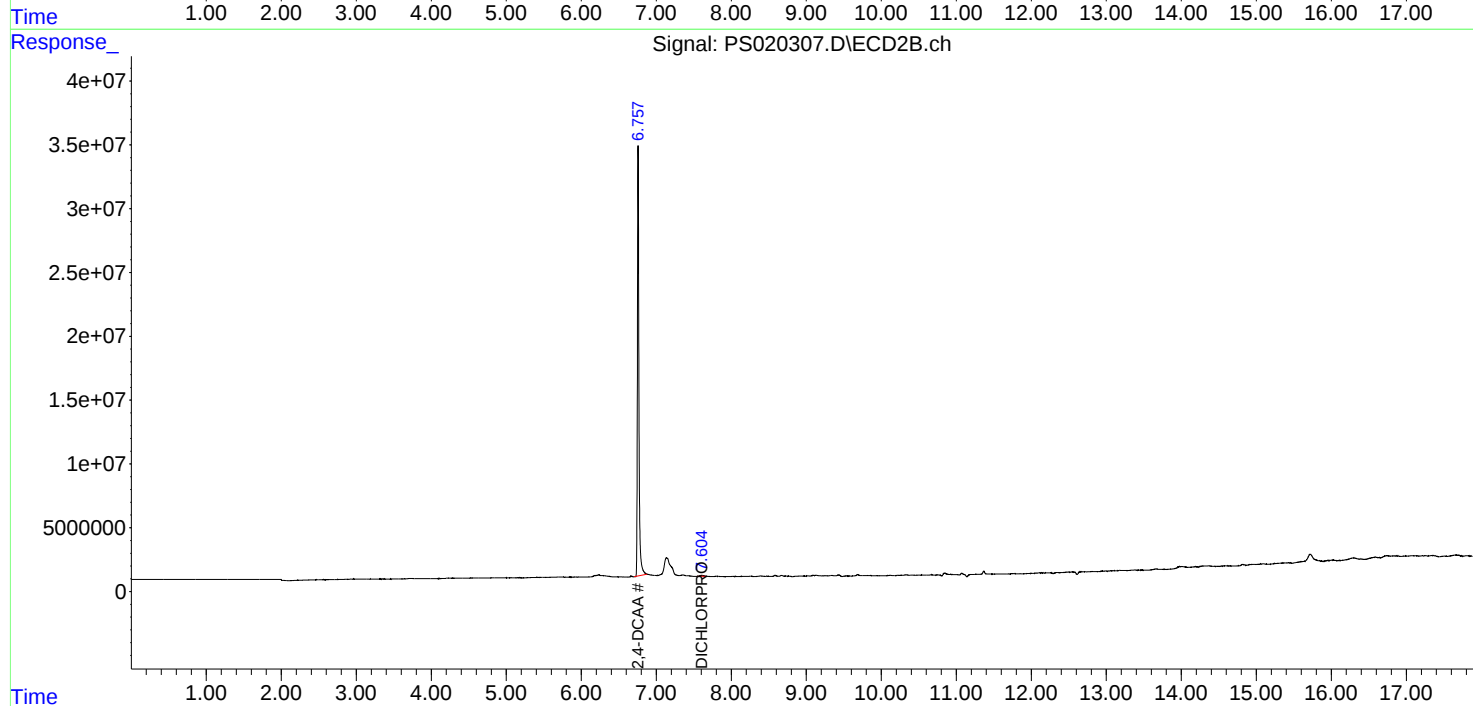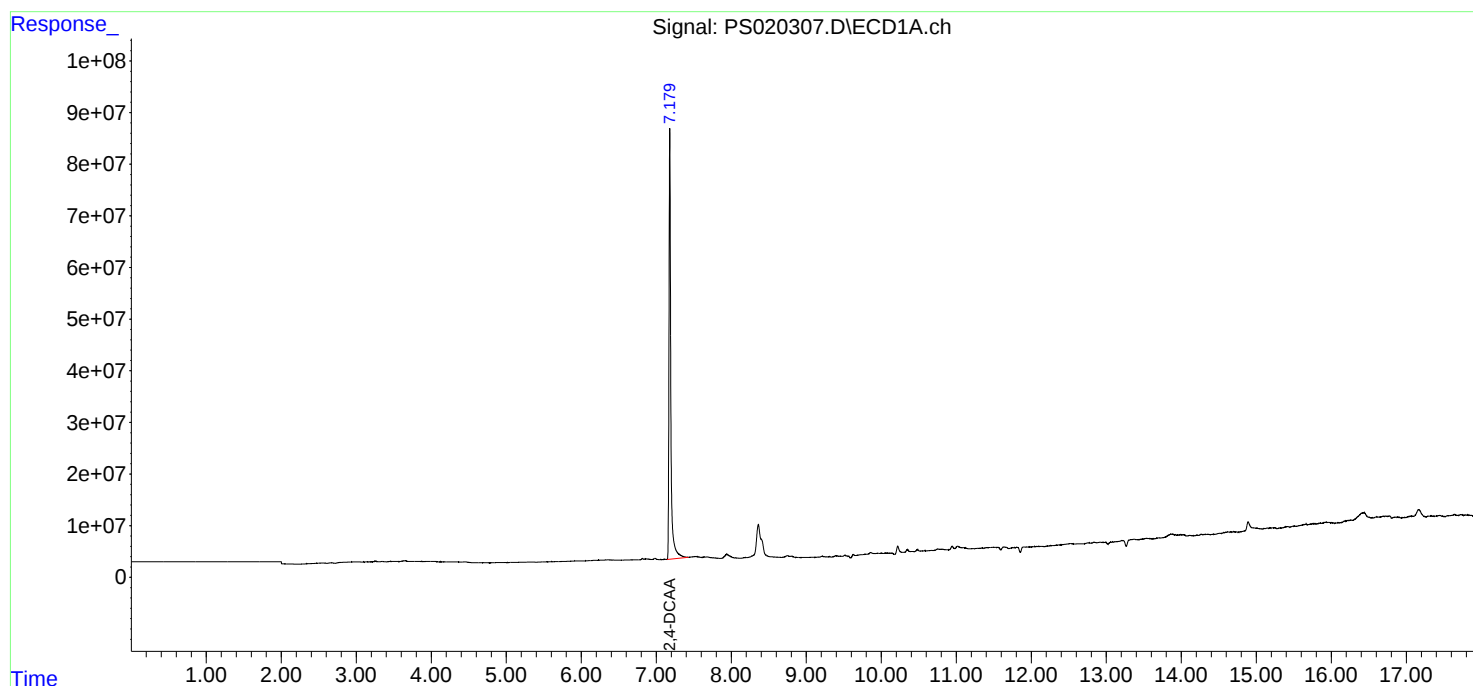


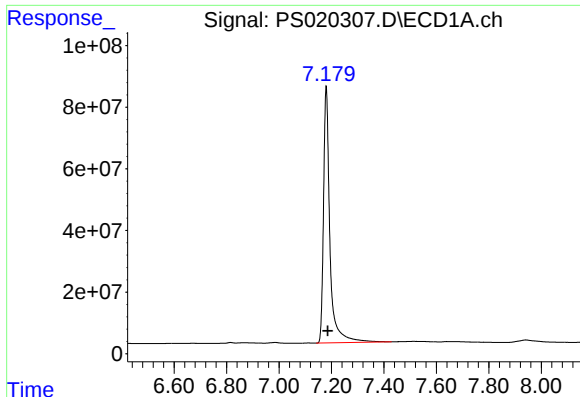

#4 2,4-DCAA


R.T.: 7.180 min
Delta R.T.: -0.006 min
Response: 1410180255
Conc: 478.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

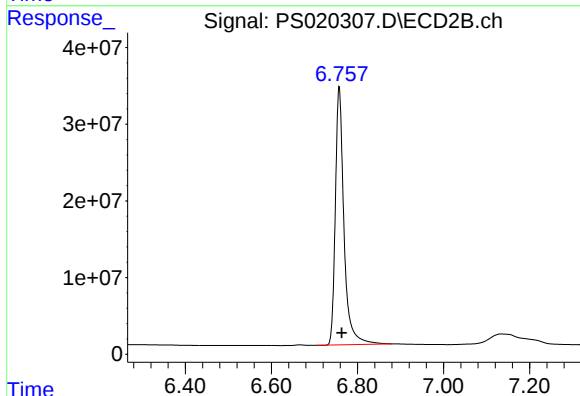


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 468303941
Conc: 574.64 ng/ml

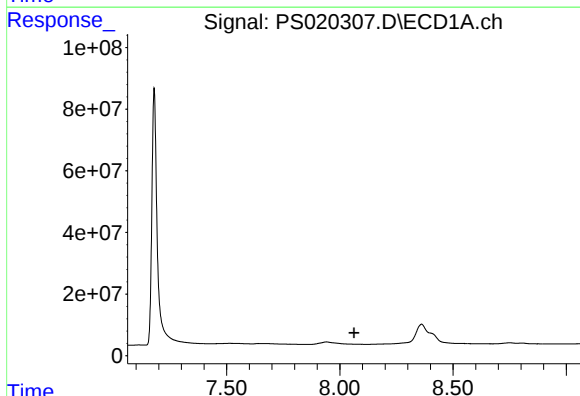

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

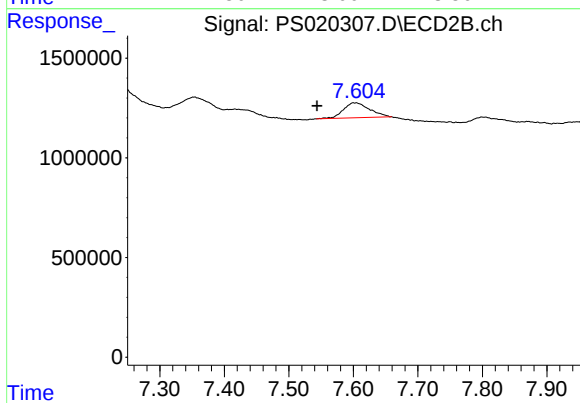

#8 DICHLORPROP

R.T.: 7.605 min
Delta R.T.: 0.061 min
Response: 2108040
Conc: 2.25 ng/ml