

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081623\
 Data File : PS024084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 10:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:14:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.368	6.797	869.5E6	289.0E6	439.031	429.683
Target Compounds							
1) T	Dalapon	2.526f	2.578	4411597	288492	2.011	<MDL #
3) T	4-Nitroph...	6.208	0.000	7457006	0	6.737	N.D. #
5) T	DICAMBA	6.499	6.955	1160410	509648	<MDL	<MDL #
6) T	MCP	6.688	7.001f	2254037	1612150	<MDL	<MDL #
7) T	MCPA	6.852f	7.206f	571971	18376753	<MDL	6.282 #
8) T	DICHLORPROP	7.149f	7.589	-52037	1338097	N.D.	1.830
9) T	2,4-D	7.265	7.806f	5140577	359611	2.074	<MDL #
11) T	2,4,5-TP ...	8.048	8.643	644541	535096	<MDL	<MDL #
12) T	2,4,5-T	8.306	9.060	1108235	1485500	<MDL	<MDL #
13) T	2,4-DB	8.800	9.513	-858668	769478	N.D.	1.688
14) T	DINOSEB	9.861	0.000	710955	0	<MDL	N.D. #
15) T	Picloram	9.693	10.806	28375453	19021082	2.195	3.817 #
16) T	DCPA	10.181f	10.806	-1073594	19021082	N.D.	3.700


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081623\
Data File : PS024084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 10:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:14:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

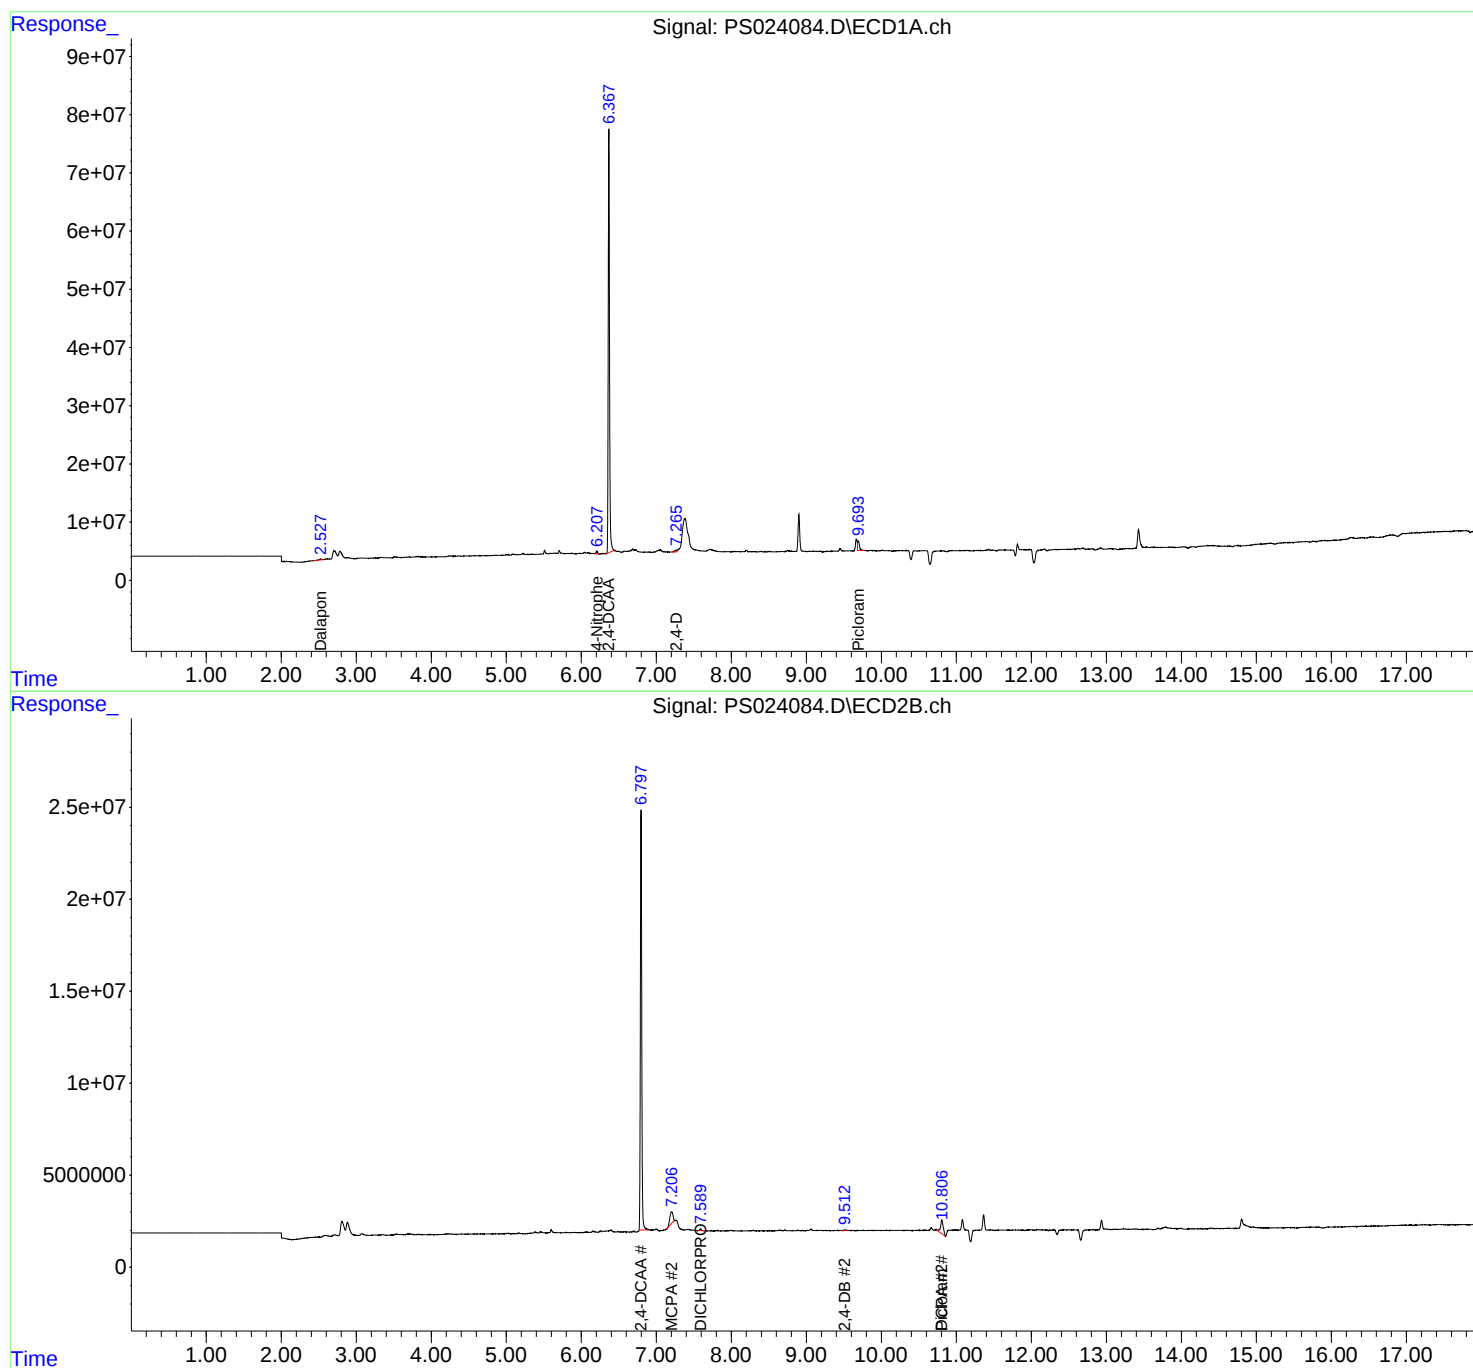


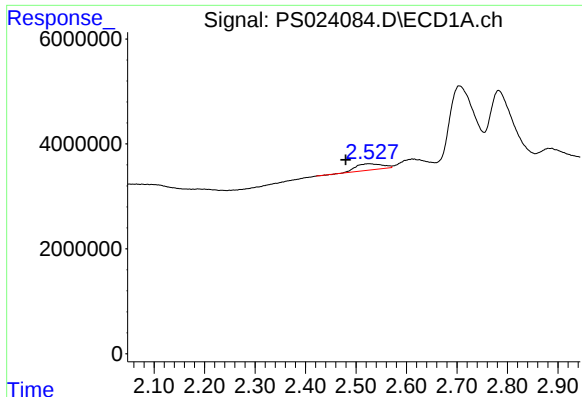

#1 Dalapon


R.T.: 2.526 min
Delta R.T.: 0.046 min
Response: 4411597
Conc: 2.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

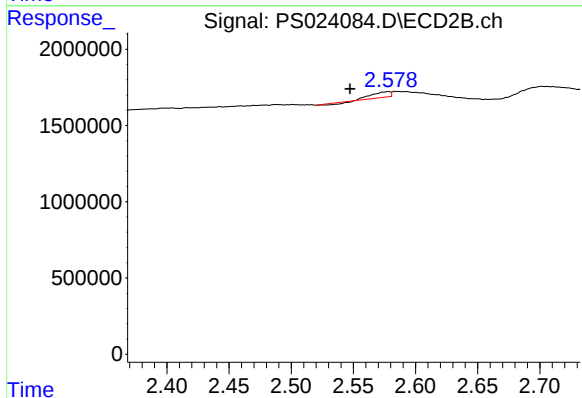


#1 Dalapon

R.T.: 2.578 min
Delta R.T.: 0.031 min
Response: 288492
Conc: N.D.

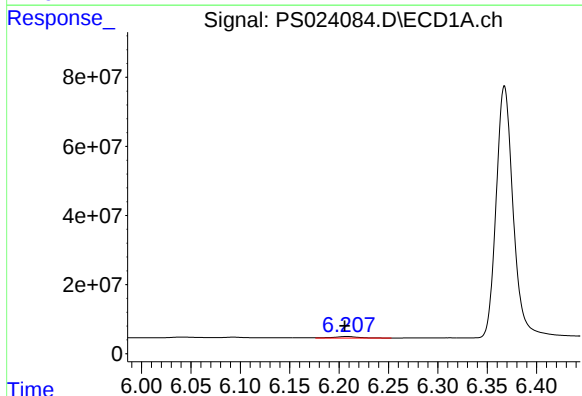


#3 4-Nitrophenol

R.T.: 6.208 min
Delta R.T.: 0.002 min
Response: 7457006
Conc: 6.74 ng/ml

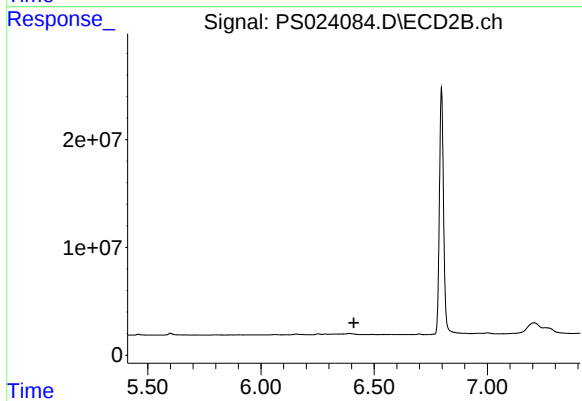

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

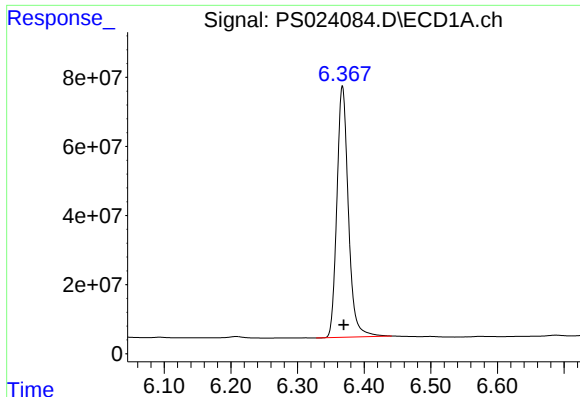

#4 2,4-DCAA


R.T.: 6.368 min
Delta R.T.: -0.002 min
Response: 869528367
Conc: 439.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

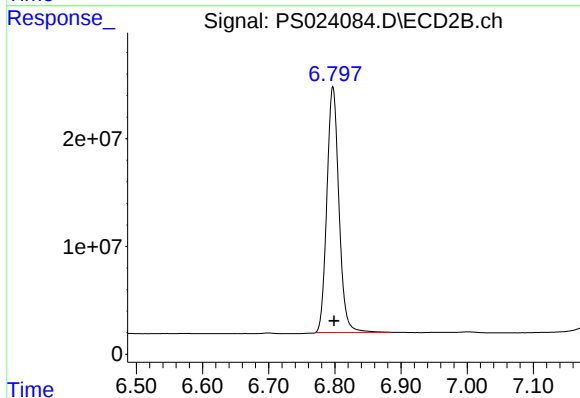


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.002 min
Response: 289016767
Conc: 429.68 ng/ml

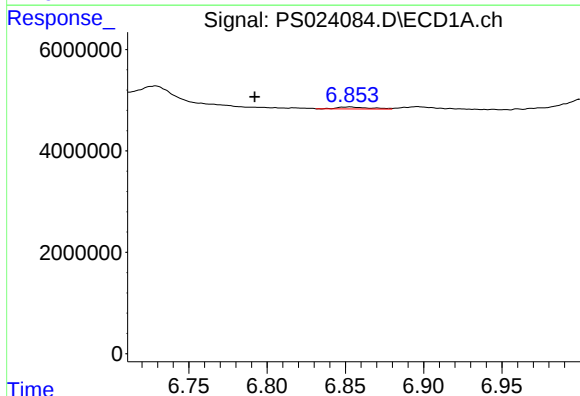


#7 MCPA

R.T.: 6.852 min
Delta R.T.: 0.060 min
Response: 571971
Conc: N.D.

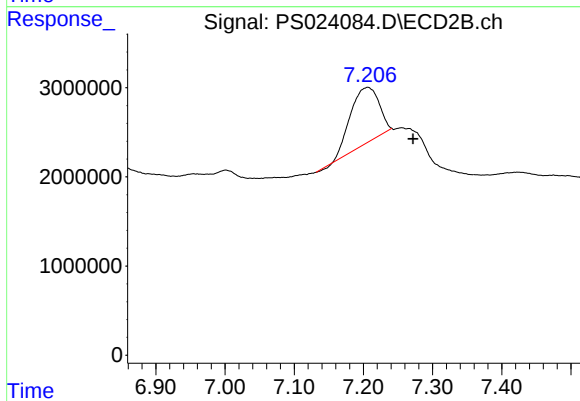

#7 MCPA


R.T.: 7.206 min
Delta R.T.: -0.066 min
Response: 18376753
Conc: 6.28 ug/ml

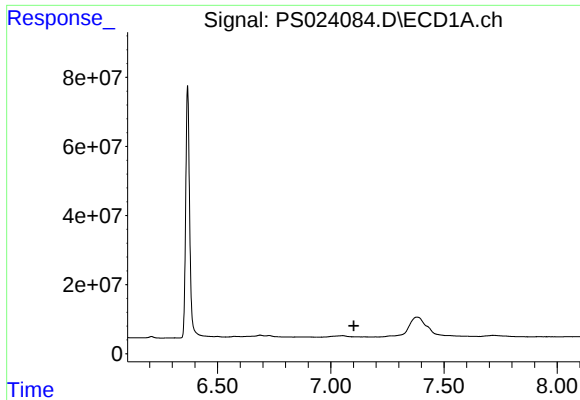

#8 DICHLORPROP


R.T.: 7.149 min
Delta R.T.: 0.047 min
Response: -52037
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

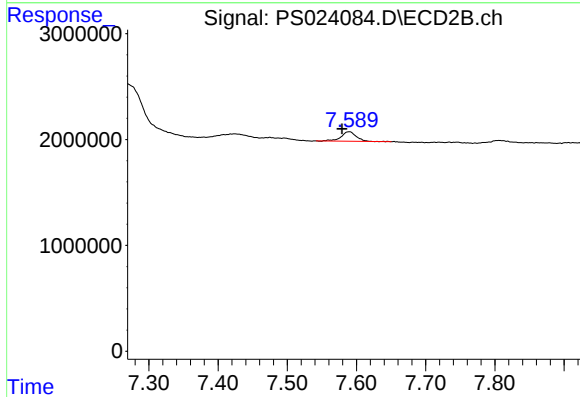


#8 DICHLORPROP

R.T.: 7.589 min
Delta R.T.: 0.010 min
Response: 1338097
Conc: 1.83 ng/ml

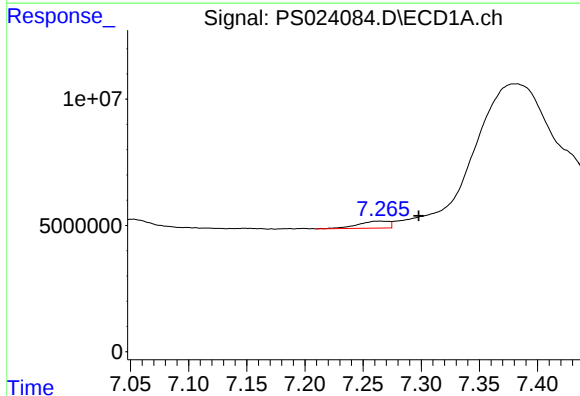


#9 2,4-D

R.T.: 7.265 min
Delta R.T.: -0.033 min
Response: 5140577
Conc: 2.07 ng/ml

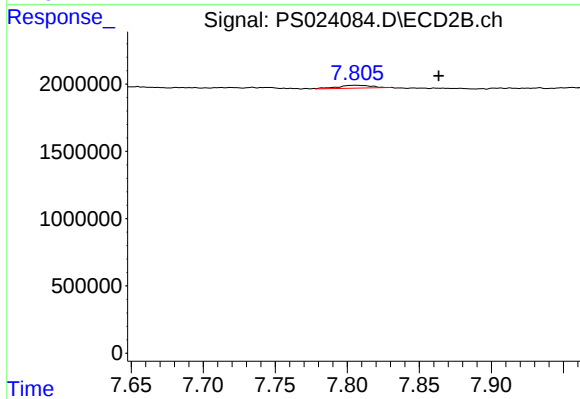

#9 2,4-D


R.T.: 7.806 min
Delta R.T.: -0.058 min
Response: 359611
Conc: N.D.

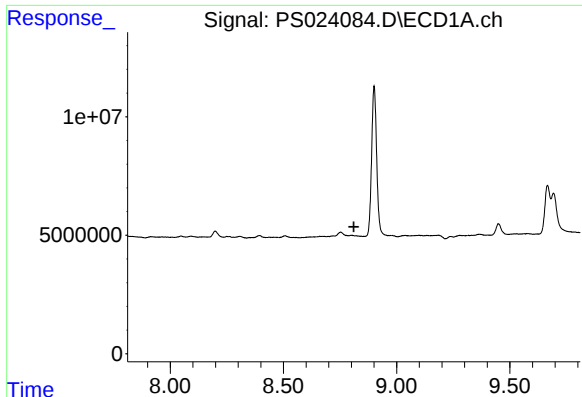

#13 2,4-DB


R.T.: 8.800 min
Delta R.T.: -0.011 min
Response: -858668
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

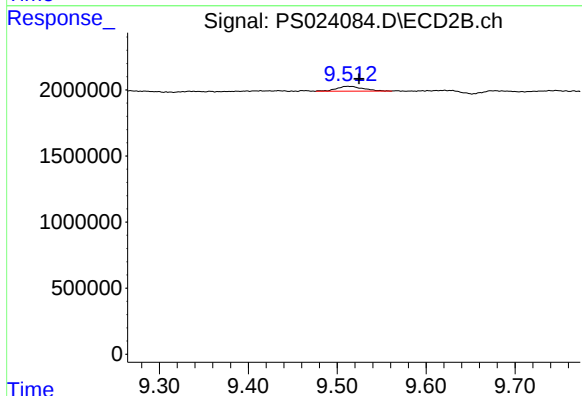


#13 2,4-DB

R.T.: 9.513 min
Delta R.T.: -0.012 min
Response: 769478
Conc: 1.69 ng/ml

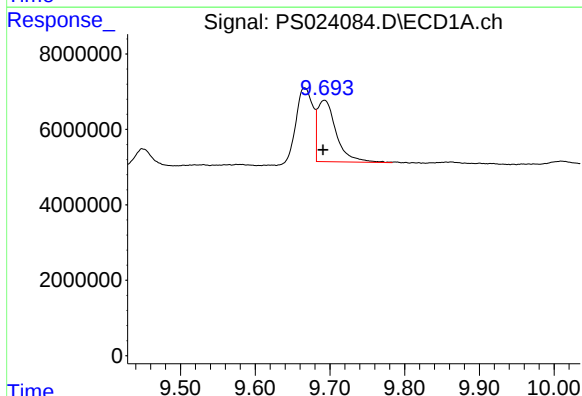


#15 Picloram

R.T.: 9.693 min
Delta R.T.: 0.002 min
Response: 28375453
Conc: 2.19 ng/ml

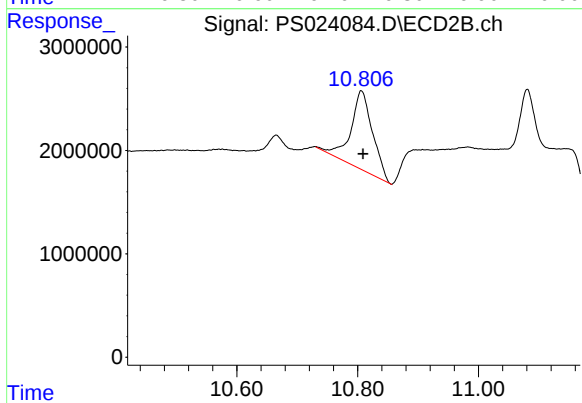

#15 Picloram


R.T.: 10.806 min
Delta R.T.: -0.003 min
Response: 19021082
Conc: 3.82 ng/ml

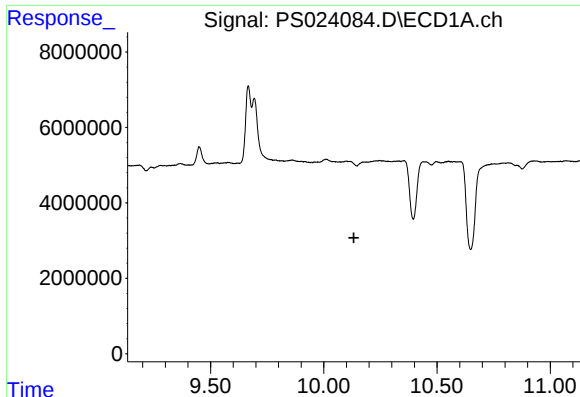

#16 DCPA

R.T.: 10.181 min
Delta R.T.: 0.048 min
Response: -1073594
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

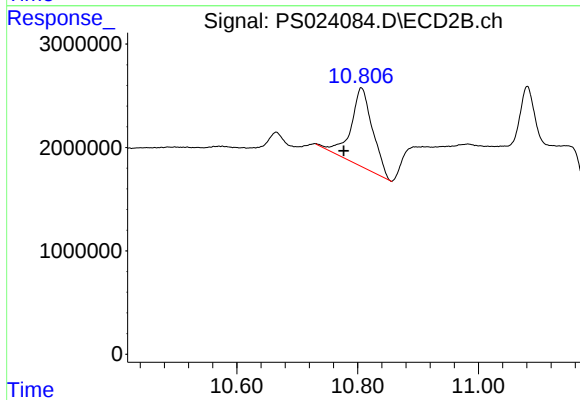

#16 DCPA

R.T.: 10.806 min
Delta R.T.: 0.030 min
Response: 19021082
Conc: 3.70 ng/ml