

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 12:51
 Operator : UA
 Sample : PB112138TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:38:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.614	11.034	77550395	66732217	417.949	366.913
Target Compounds							
1) T	Dalapon	2.963	2.403	7418179	5586692	31.284	24.517
2) T	3,5-DICHL...	0.000	9.121	0	562982	N.D.	2.210 #
5) T	DICAMBA	0.000	11.277	0	5979618	N.D.	8.724 #
6) T	MCP	12.306	0.000	9087259	0	18.080	N.D. #
15) T	Picloram	17.152	16.969	2702100	5108142	1.709	3.706 #
16) T	DCPA	0.000	16.969	0	5108142	N.D.	3.537 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 12:51
Operator : UA
Sample : PB112138TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:38:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

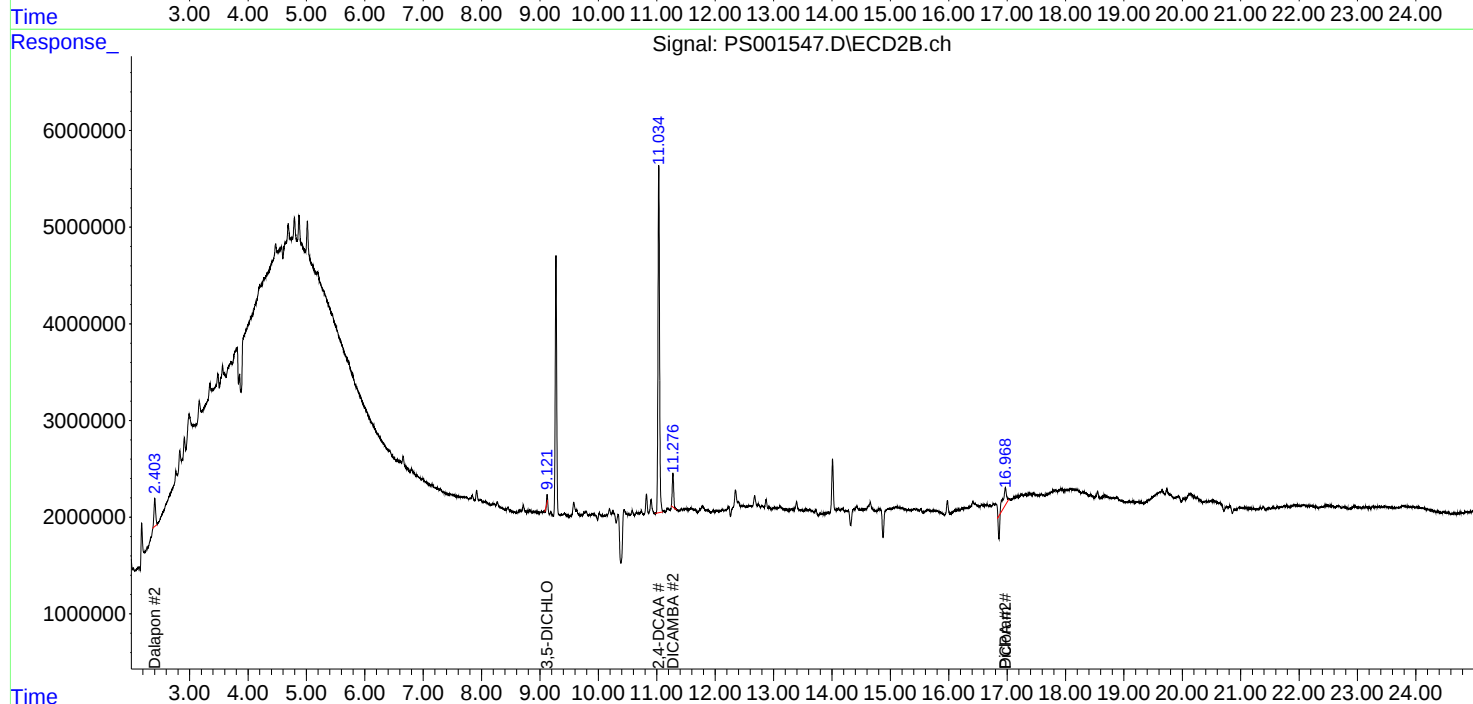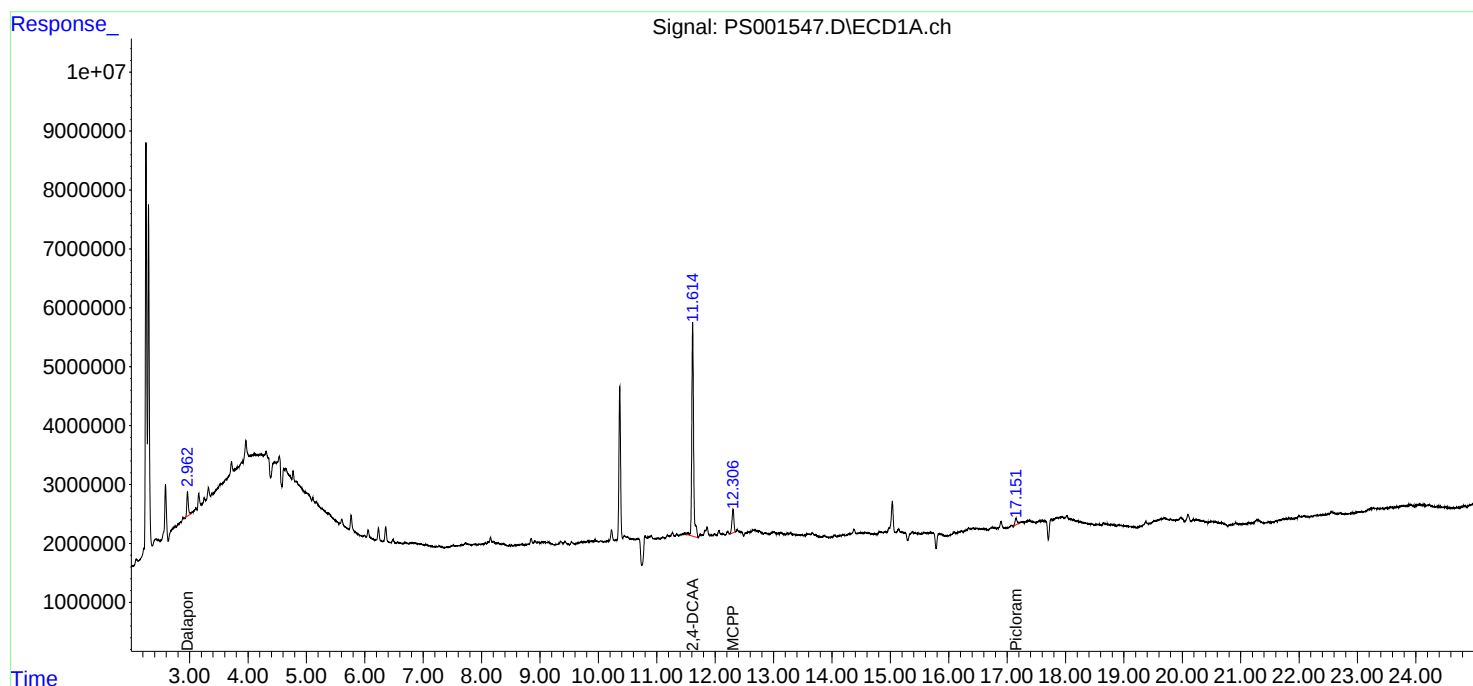


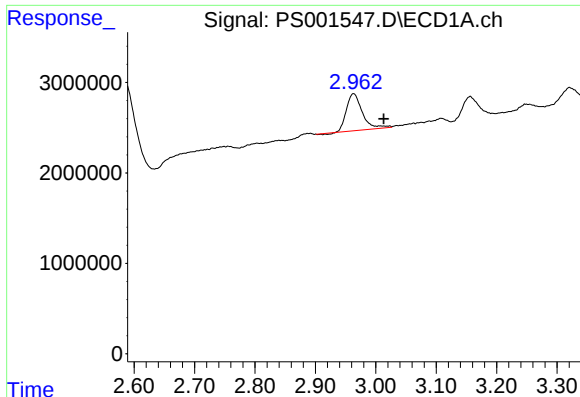

#1 Dalapon


R.T.: 2.963 min
Delta R.T.: -0.050 min
Response: 7418179
Conc: 31.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

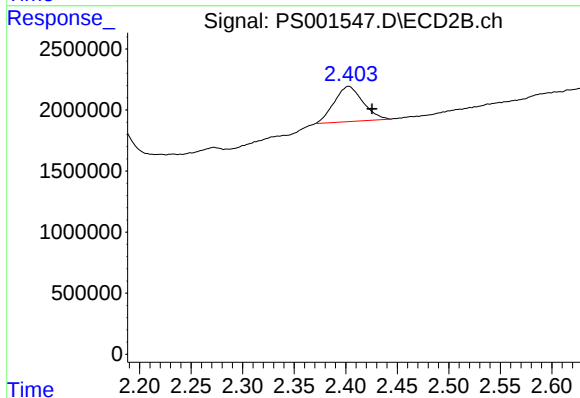


#1 Dalapon

R.T.: 2.403 min
Delta R.T.: -0.023 min
Response: 5586692
Conc: 24.52 ng/ml

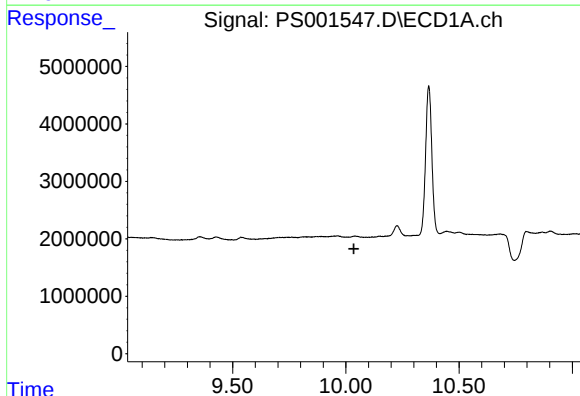


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

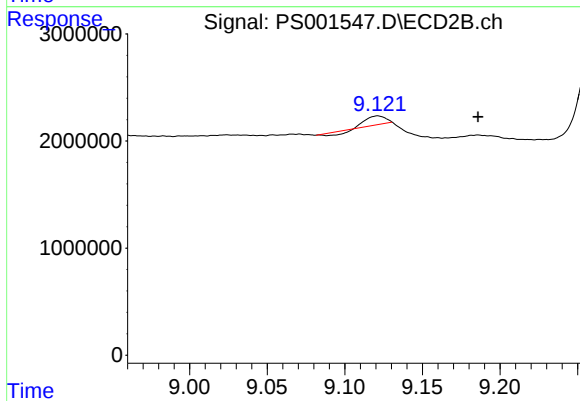

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.121 min
Delta R.T.: -0.065 min
Response: 562982
Conc: 2.21 ng/ml

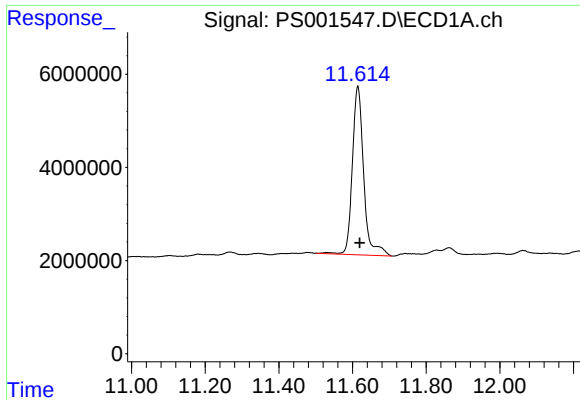

#4 2,4-DCAA


R.T.: 11.614 min
Delta R.T.: -0.005 min
Response: 77550395
Conc: 417.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

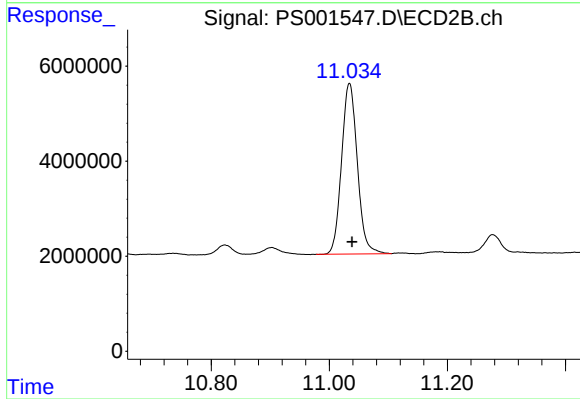


#4 2,4-DCAA

R.T.: 11.034 min
Delta R.T.: -0.005 min
Response: 66732217
Conc: 366.91 ng/ml

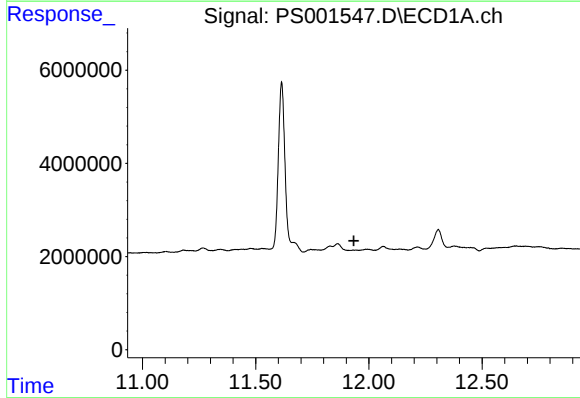


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

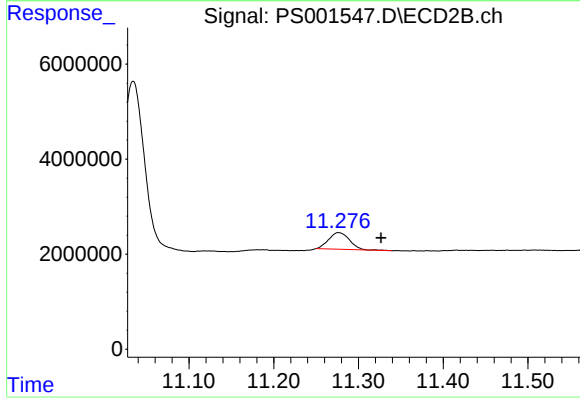

#5 DICAMBA


R.T.: 11.277 min
Delta R.T.: -0.050 min
Response: 5979618
Conc: 8.72 ng/ml

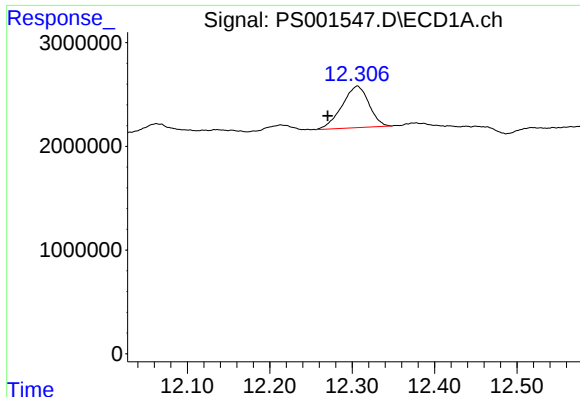

#6 MCPP


R.T.: 12.306 min
Delta R.T.: 0.036 min
Response: 9087259
Conc: 18.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

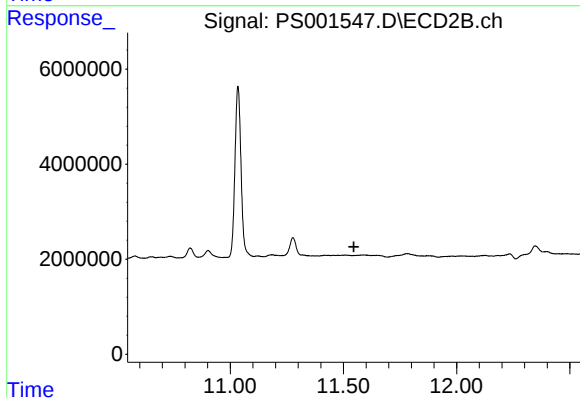


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

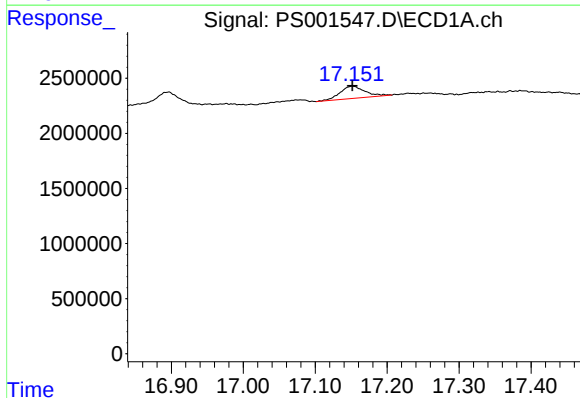


#15 Picloram

R.T.: 17.152 min
Delta R.T.: 0.000 min
Response: 2702100
Conc: 1.71 ng/ml

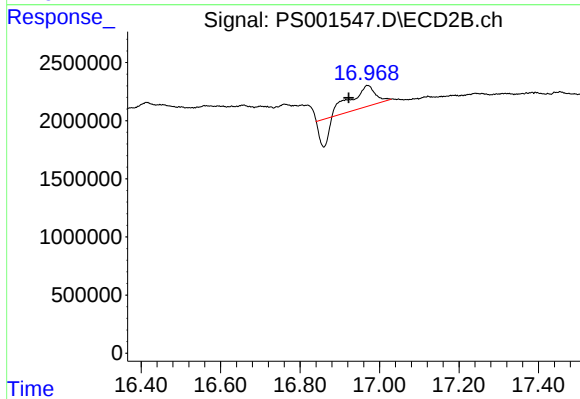

#15 Picloram


R.T.: 16.969 min
Delta R.T.: 0.047 min
Response: 5108142
Conc: 3.71 ng/ml

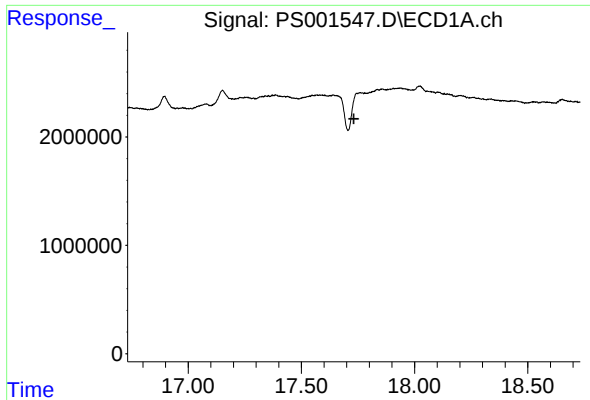

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

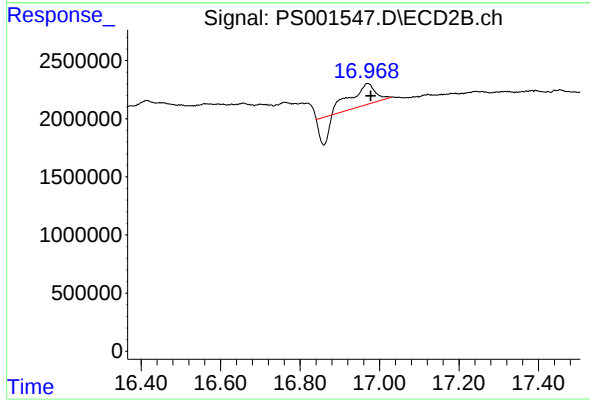

#16 DCPA

R.T.: 16.969 min
Delta R.T.: -0.009 min
Response: 5108142
Conc: 3.54 ng/ml