

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 13:22
 Operator : UA
 Sample : J4269-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:39:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.610	11.032	98133846	83254225	528.881	457.756
Target Compounds							
1) T	Dalapon	2.960	2.399	7705824	5828658	32.497	25.579
5) T	DICAMBA	11.987	11.275	2627859	5371519	3.655	7.837 #
6) T	MCPD	12.303	0.000	9770676	0	19.440	N.D. #
9) T	2,4-D	0.000	12.869	0	2183114	N.D.	9.200 #
15) T	Picloram	0.000	16.971	0	17020027	N.D.	12.347 #
16) T	DCPA	0.000	16.971	0	17020027	N.D.	11.784 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 13:22
Operator : UA
Sample : J4269-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:39:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

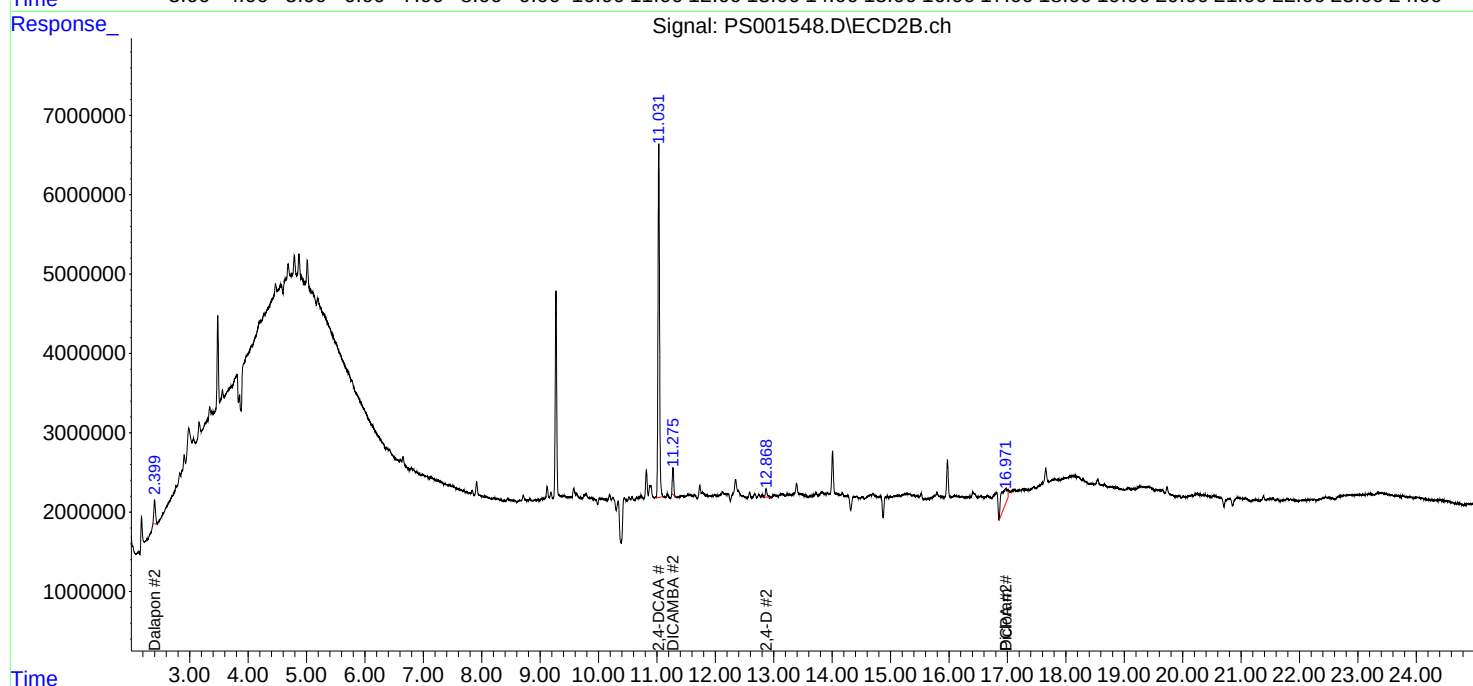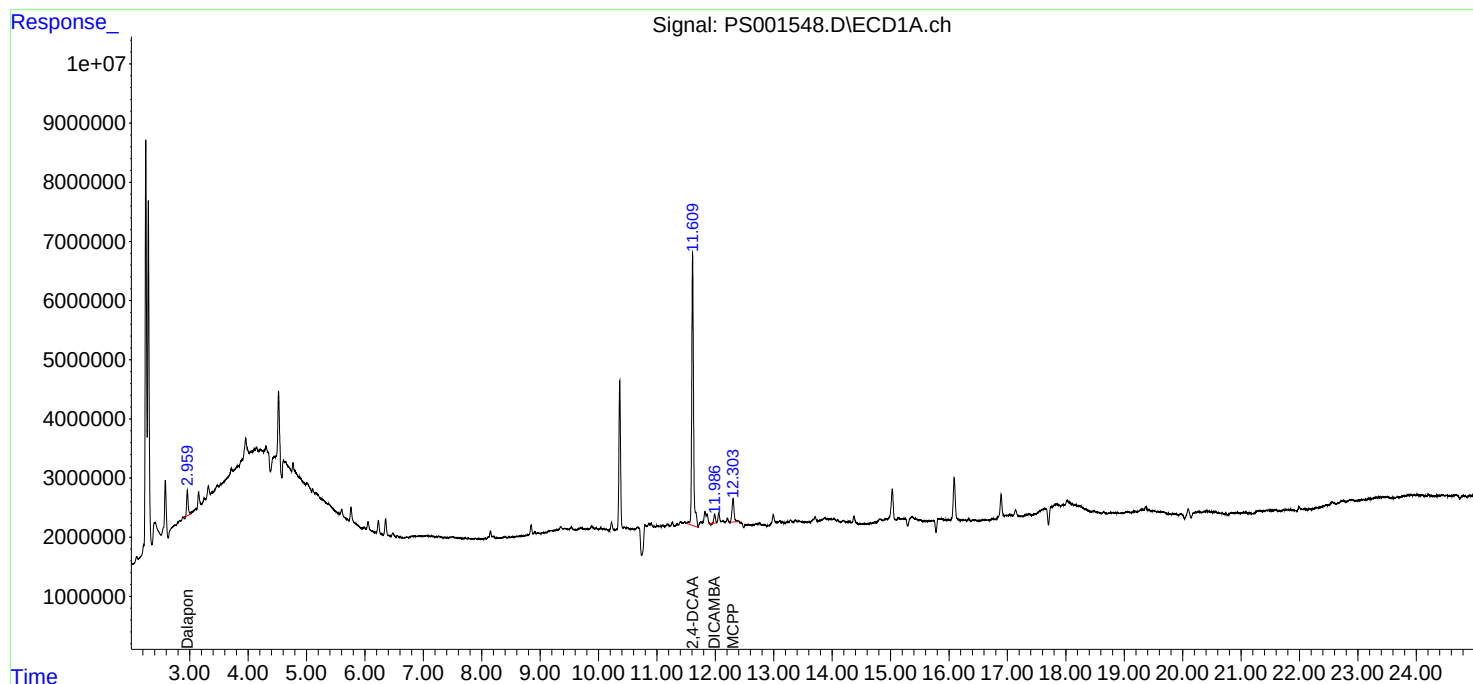


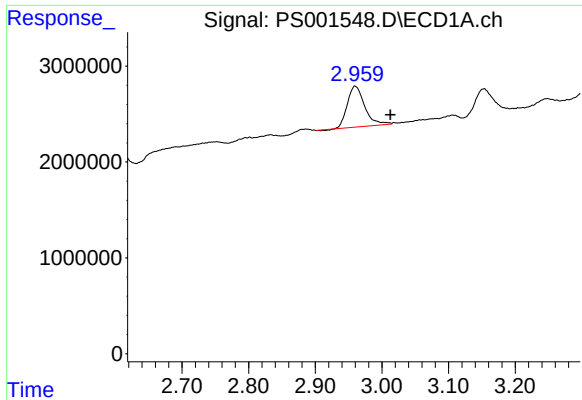

#1 Dalapon


R.T.: 2.960 min
Delta R.T.: -0.053 min
Response: 7705824
Conc: 32.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

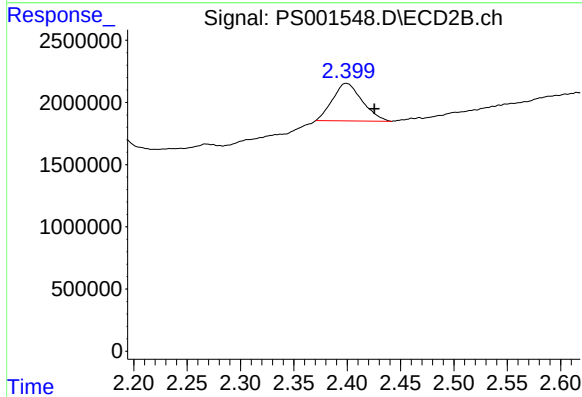


#1 Dalapon

R.T.: 2.399 min
Delta R.T.: -0.026 min
Response: 5828658
Conc: 25.58 ng/ml

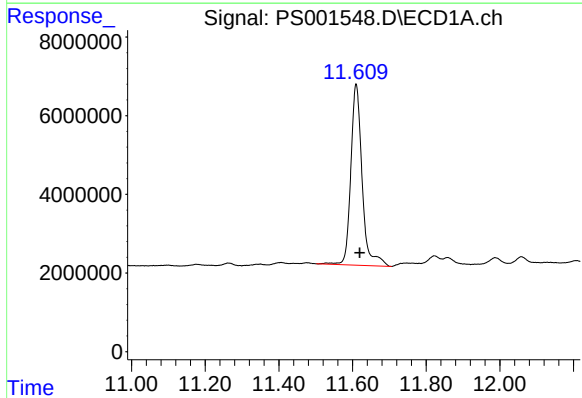


#4 2,4-DCAA

R.T.: 11.610 min
Delta R.T.: -0.010 min
Response: 98133846
Conc: 528.88 ng/ml

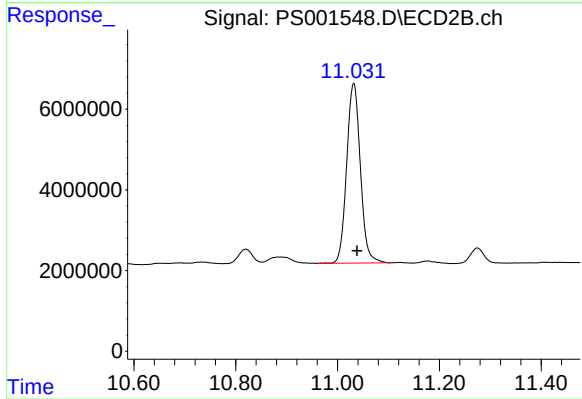

#4 2,4-DCAA


R.T.: 11.032 min
Delta R.T.: -0.007 min
Response: 83254225
Conc: 457.76 ng/ml

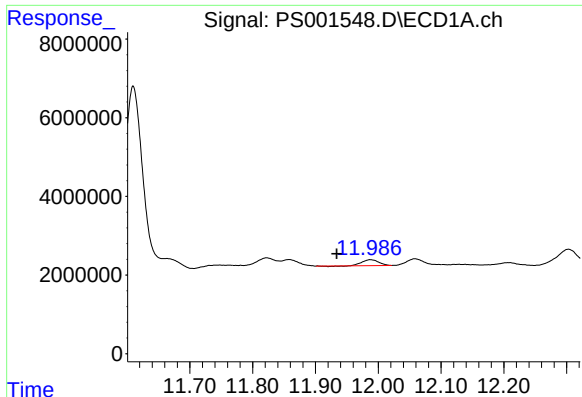

#5 DICAMBA


R.T.: 11.987 min
Delta R.T.: 0.054 min
Response: 2627859
Conc: 3.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

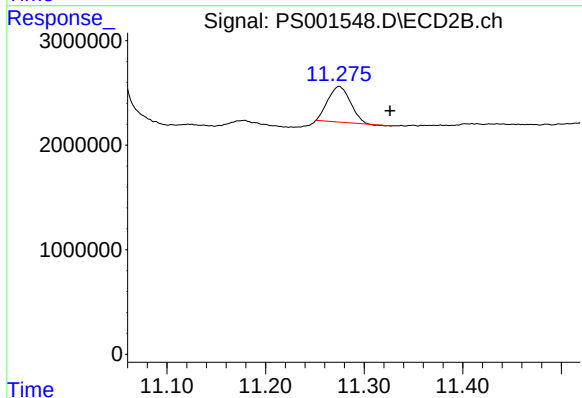


#5 DICAMBA

R.T.: 11.275 min
Delta R.T.: -0.052 min
Response: 5371519
Conc: 7.84 ng/ml

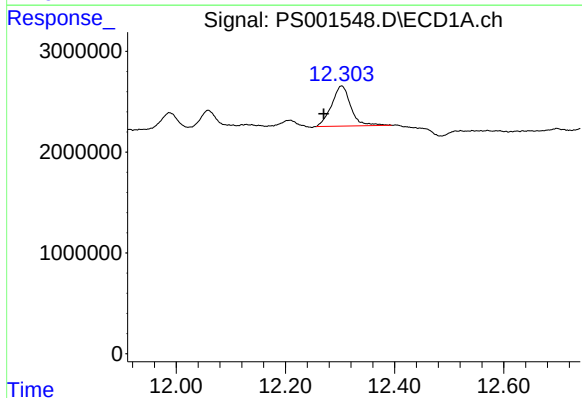


#6 MCP

R.T.: 12.303 min
Delta R.T.: 0.033 min
Response: 9770676
Conc: 19.44 ug/ml

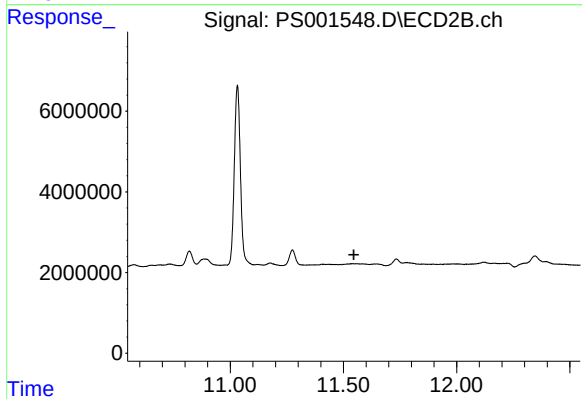

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

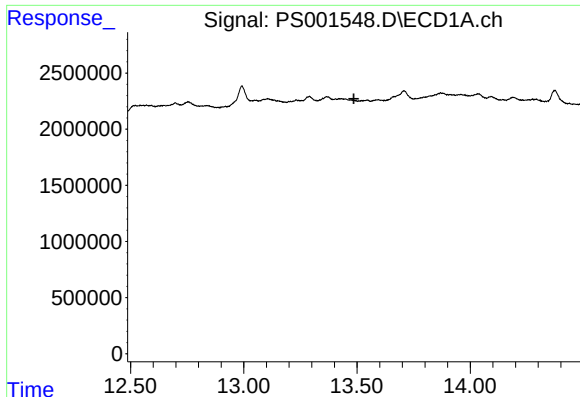

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

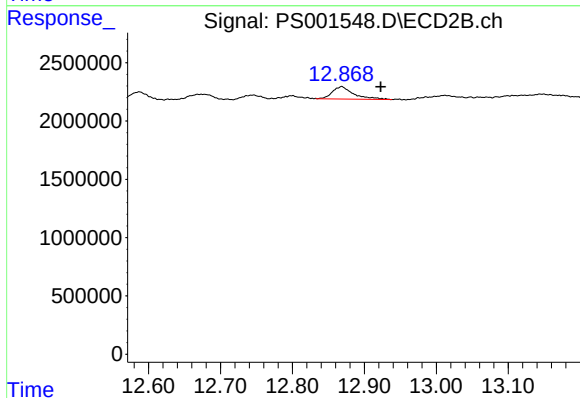


#9 2,4-D

R.T.: 12.869 min
Delta R.T.: -0.054 min
Response: 2183114
Conc: 9.20 ng/ml

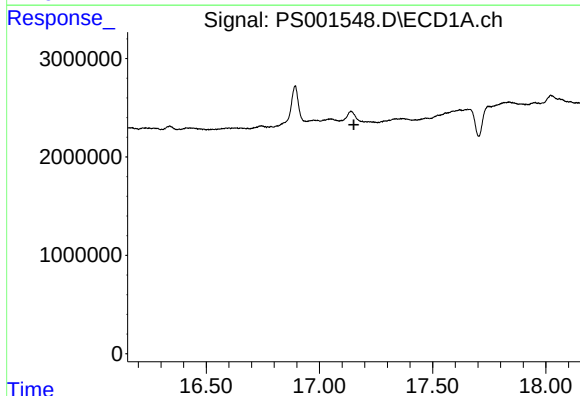


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

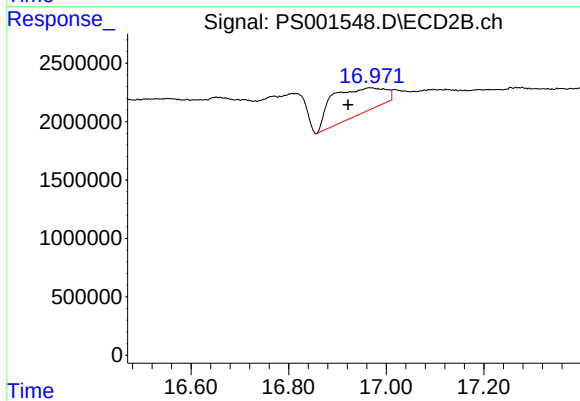

#15 Picloram


R.T.: 16.971 min
Delta R.T.: 0.049 min
Response: 17020027
Conc: 12.35 ng/ml

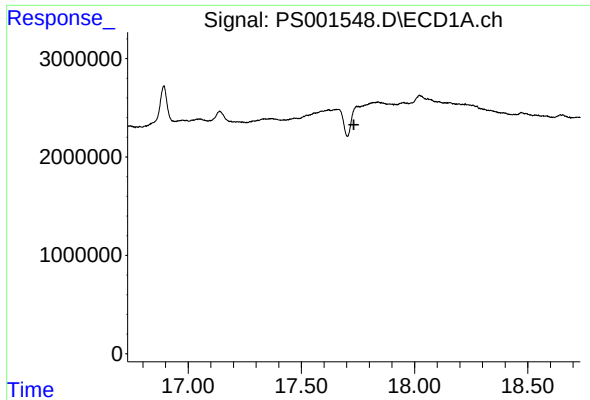

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

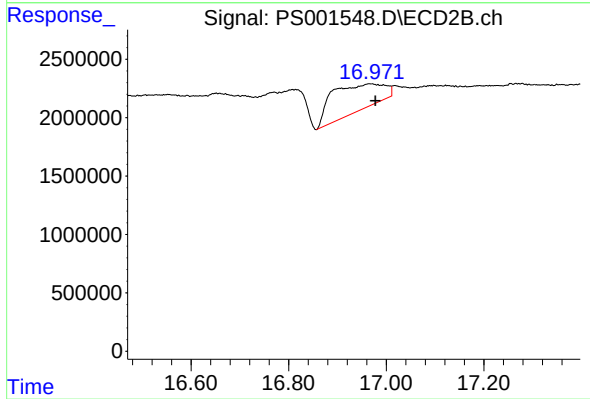

#16 DCPA

R.T.: 16.971 min
Delta R.T.: -0.007 min
Response: 17020027
Conc: 11.78 ng/ml