

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 13:53
 Operator : UA
 Sample : J4269-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:39:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.643	11.065	82517793	70035164	444.720	385.073
Target Compounds							
1) T	Dalapon	2.992	2.433	7439102	8767127	31.372	38.474
2) T	3,5-DICHL...	0.000	9.153	0	1901988	N.D.	7.466 #
5) T	DICAMBA	0.000	11.308	0	6429150	N.D.	9.380 #
6) T	MCP	12.335	0.000	7150213	0	14.226	N.D. #
10) T	Pentachlo...	0.000	13.423	0	583741	N.D.	0.212 #
11) T	2,4,5-TP ...	0.000	14.040	0	298986	N.D.	0.273 #
15) T	Picloram	0.000	16.992	0	10793958	N.D.	7.830 #
16) T	DCPA	0.000	16.992	0	10793958	N.D.	7.474 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 13:53
Operator : UA
Sample : J4269-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:39:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

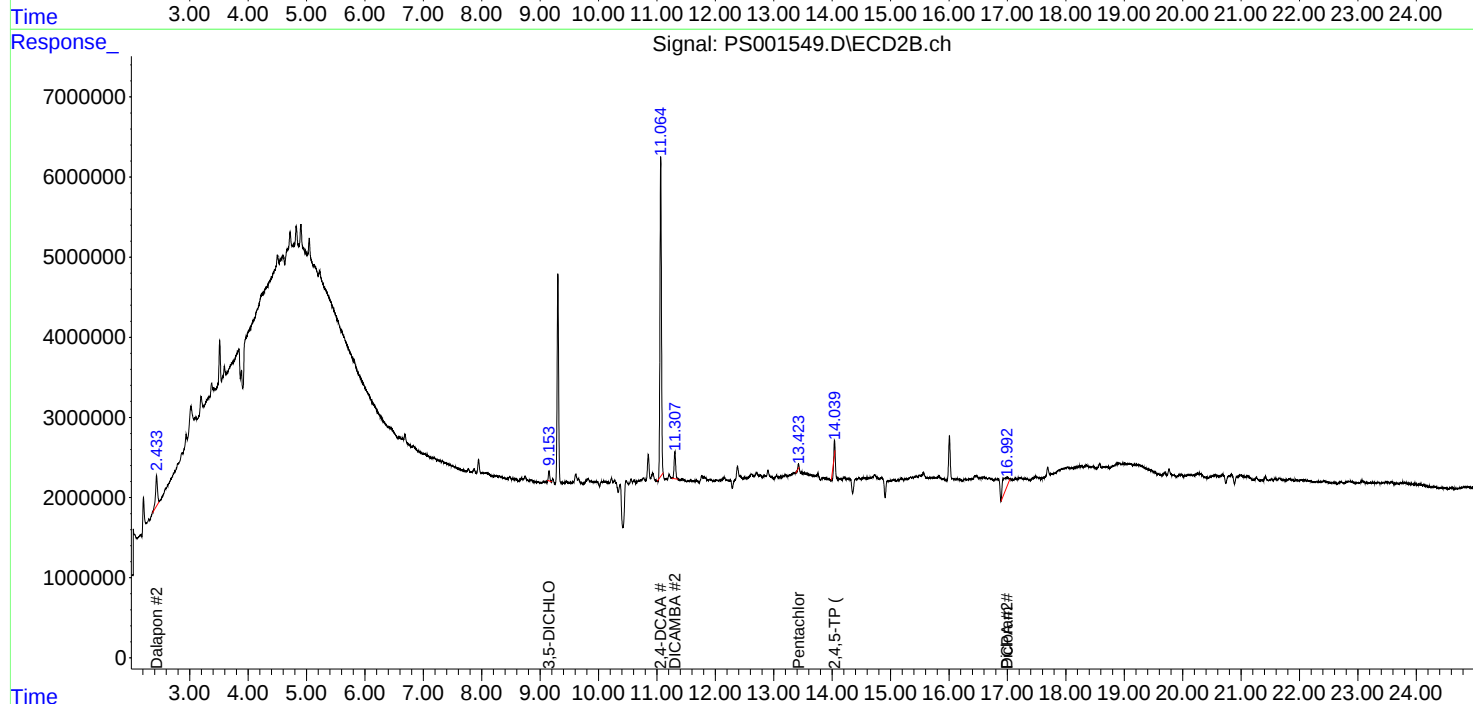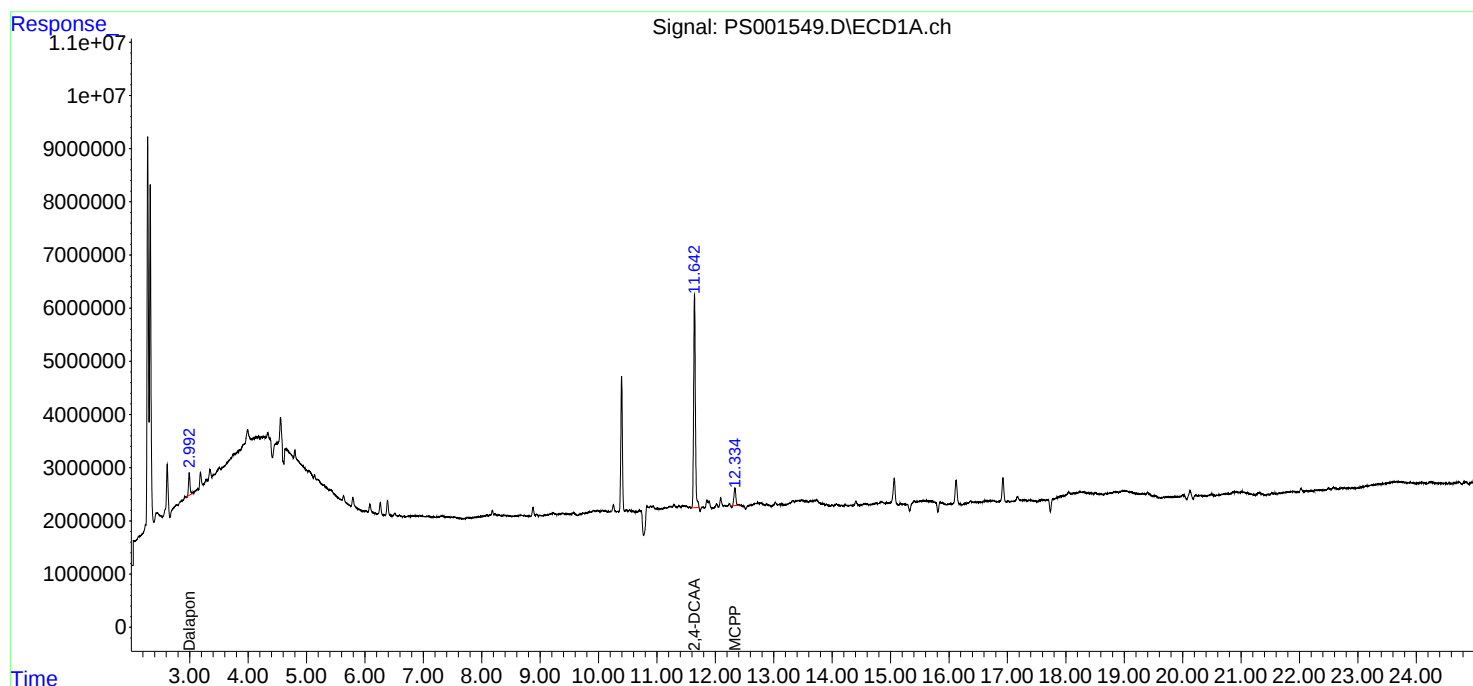


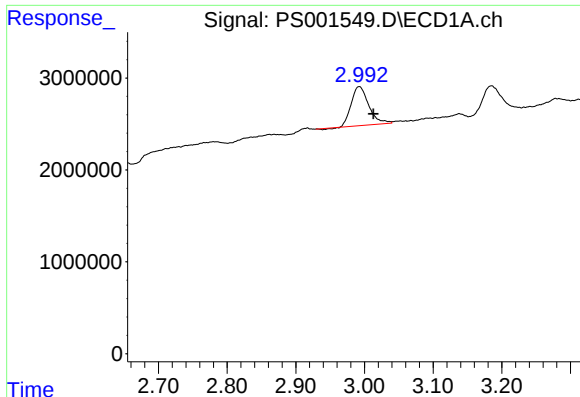

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.021 min
Response: 7439102
Conc: 31.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

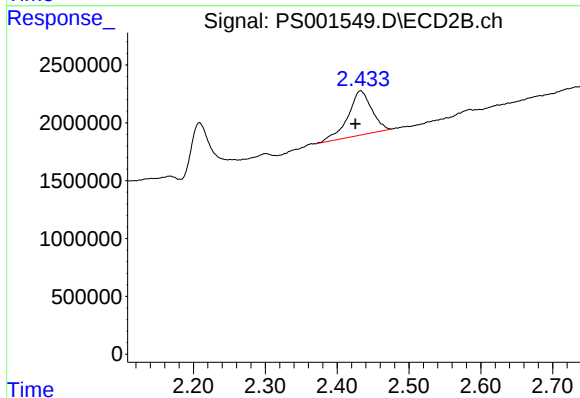


#1 Dalapon

R.T.: 2.433 min
Delta R.T.: 0.007 min
Response: 8767127
Conc: 38.47 ng/ml

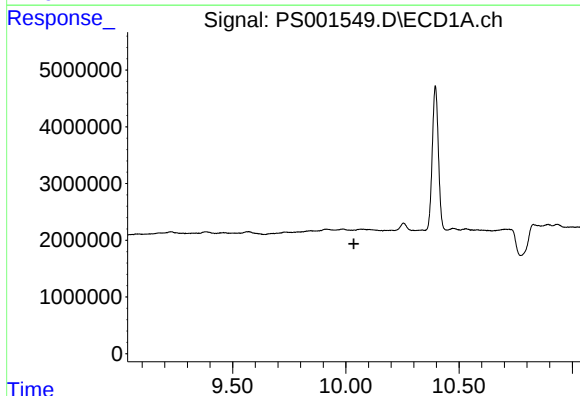


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

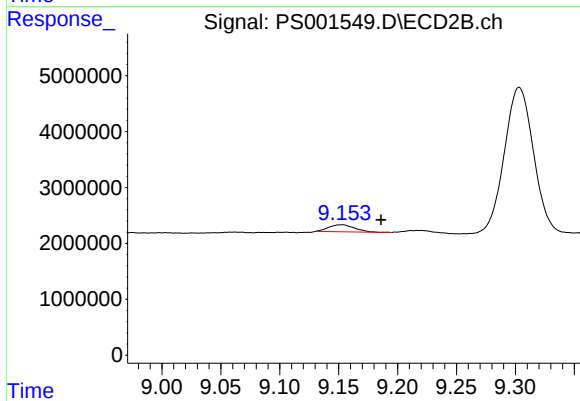

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.153 min
Delta R.T.: -0.033 min
Response: 1901988
Conc: 7.47 ng/ml

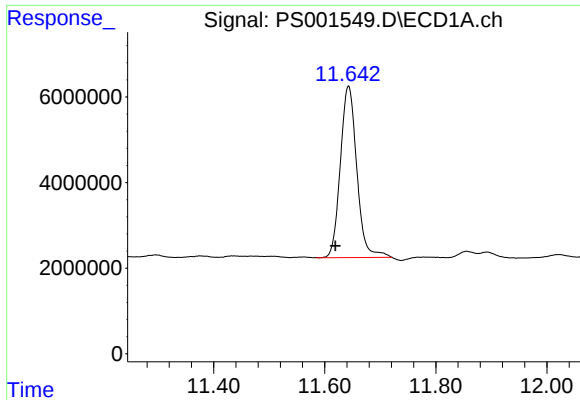

#4 2,4-DCAA


R.T.: 11.643 min
Delta R.T.: 0.023 min
Response: 82517793
Conc: 444.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

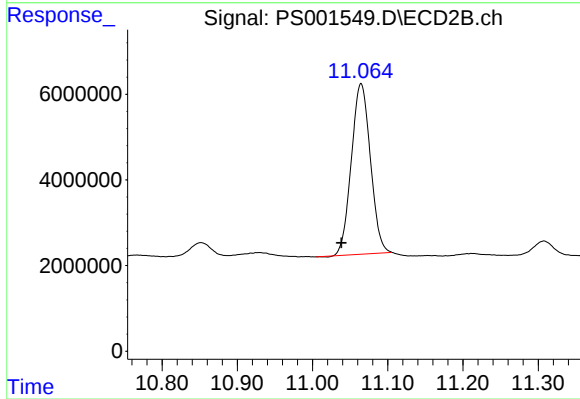


#4 2,4-DCAA

R.T.: 11.065 min
Delta R.T.: 0.026 min
Response: 70035164
Conc: 385.07 ng/ml

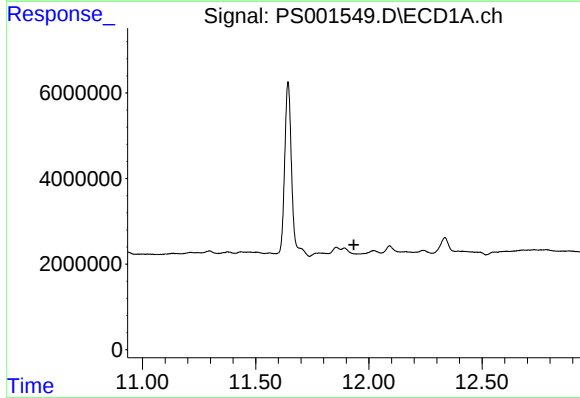


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

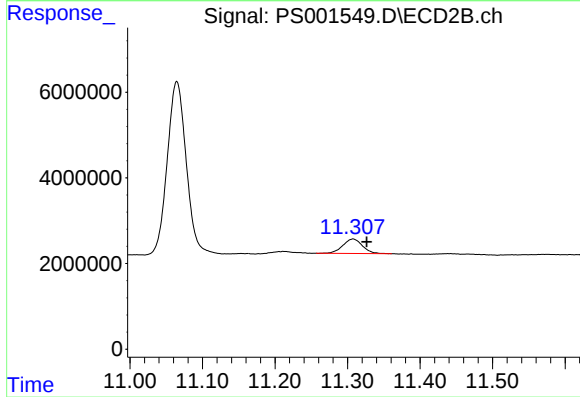

#5 DICAMBA


R.T.: 11.308 min
Delta R.T.: -0.019 min
Response: 6429150
Conc: 9.38 ng/ml

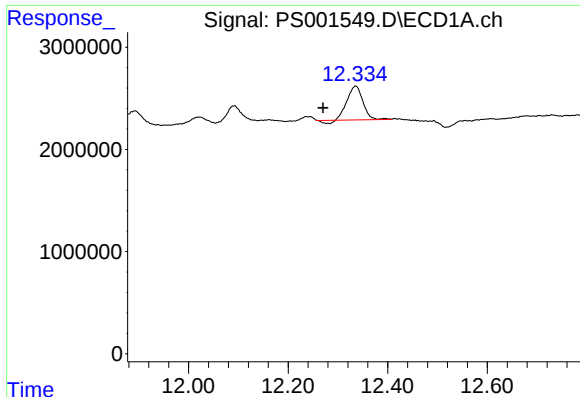

#6 MCP


R.T.: 12.335 min
Delta R.T.: 0.065 min
Response: 7150213
Conc: 14.23 ug/ml

Instrument :
ECD_S
ClientSampleId :

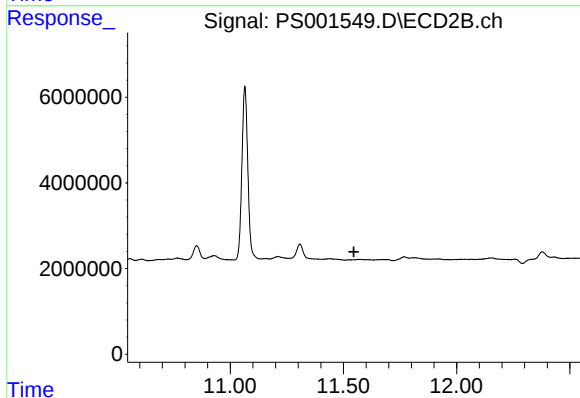


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

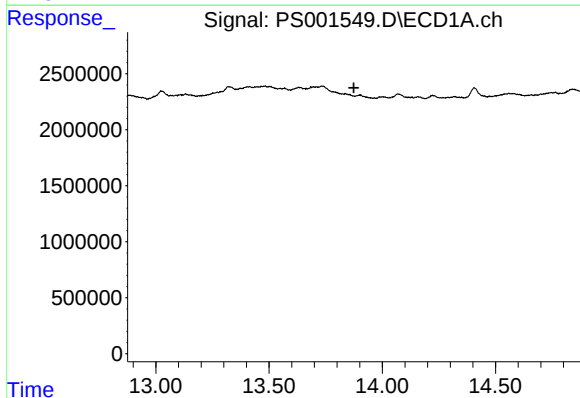


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.874 min
Response: 0
Conc: N.D.

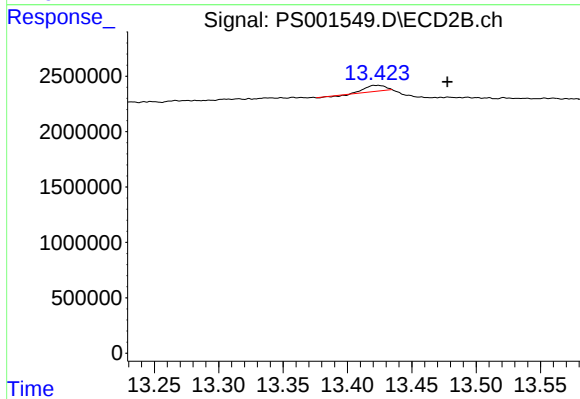

#10 Pentachlorophenol


R.T.: 13.423 min
Delta R.T.: -0.055 min
Response: 583741
Conc: 0.21 ng/ml

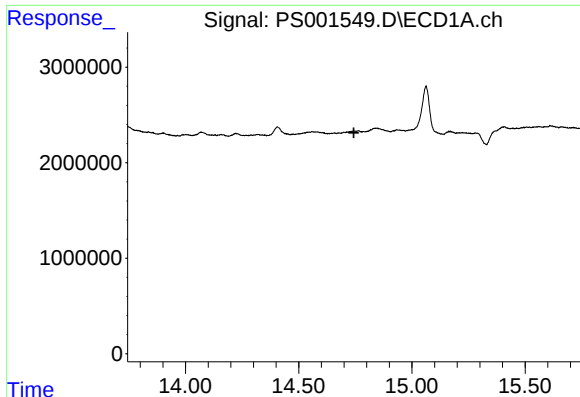

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

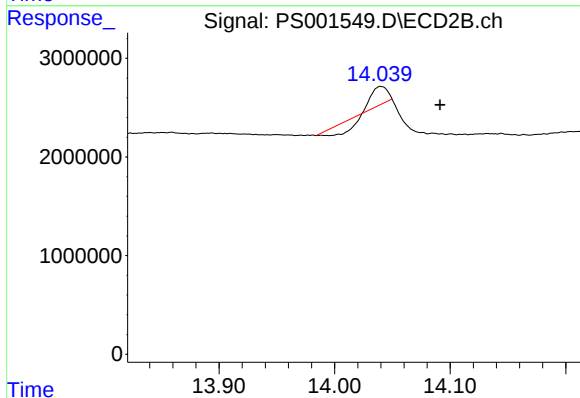


#11 2,4,5-TP (SILVEX)

R.T.: 14.040 min
Delta R.T.: -0.051 min
Response: 298986
Conc: 0.27 ng/ml

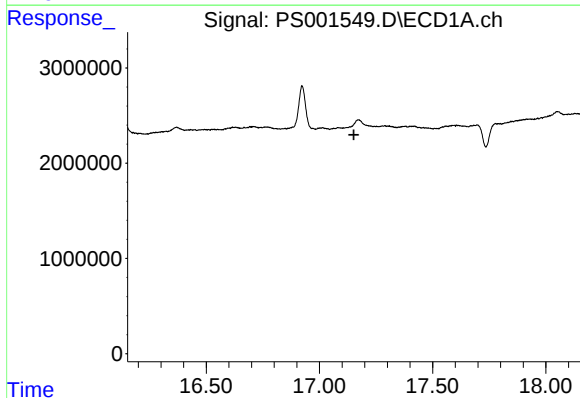


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

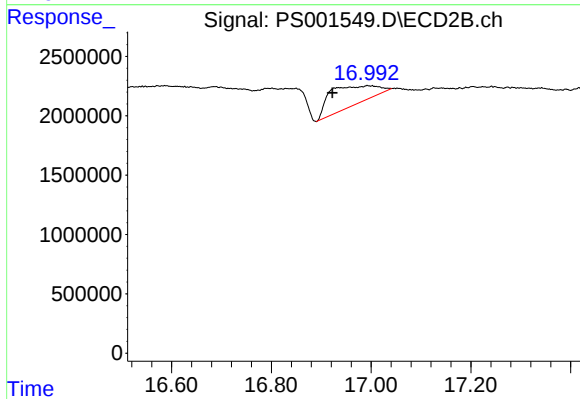

#15 Picloram


R.T.: 16.992 min
Delta R.T.: 0.070 min
Response: 10793958
Conc: 7.83 ng/ml

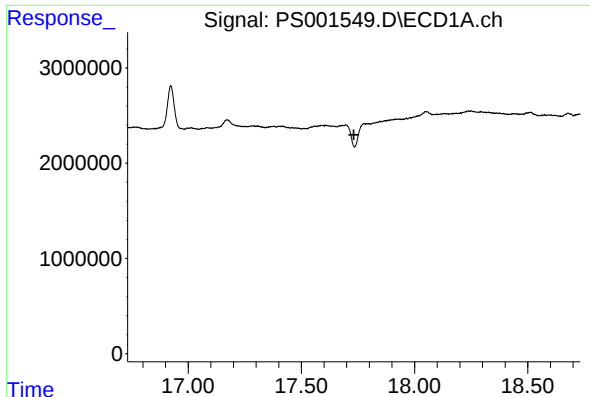

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

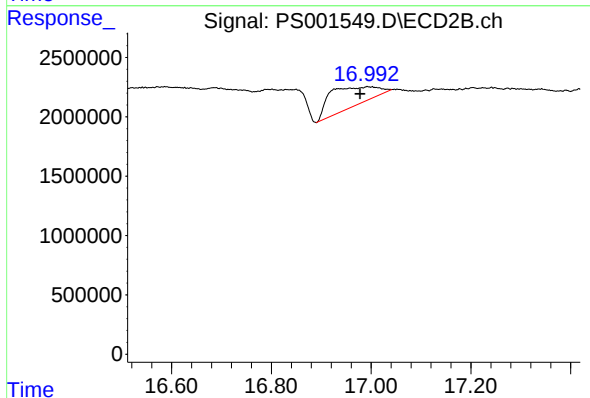

#16 DCPA

R.T.: 16.992 min
Delta R.T.: 0.014 min
Response: 10793958
Conc: 7.47 ng/ml