

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 14:24
 Operator : UA
 Sample : J4282-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:39:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.627	11.047	85615883	73665033	461.417	405.031
Target Compounds							
1) T	Dalapon	2.975	2.416	7267277	9680935	30.647	42.484 #
5) T	DICAMBA	0.000	11.290	0	6760741	N.D.	9.864 #
6) T	MCPD	12.319	0.000	9939712	0	19.776	N.D. #
8) T	DICHLORPROP	0.000	12.417	0	916935	N.D.	5.176 #
11) T	2,4,5-TP ...	0.000	14.023	0	7987695	N.D.	7.305 #
15) T	Picloram	0.000	16.988	0	15409240	N.D.	11.178 #
16) T	DCPA	17.764	16.988	-4116258	15409240	N.D.	10.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 14:24
Operator : UA
Sample : J4282-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:39:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

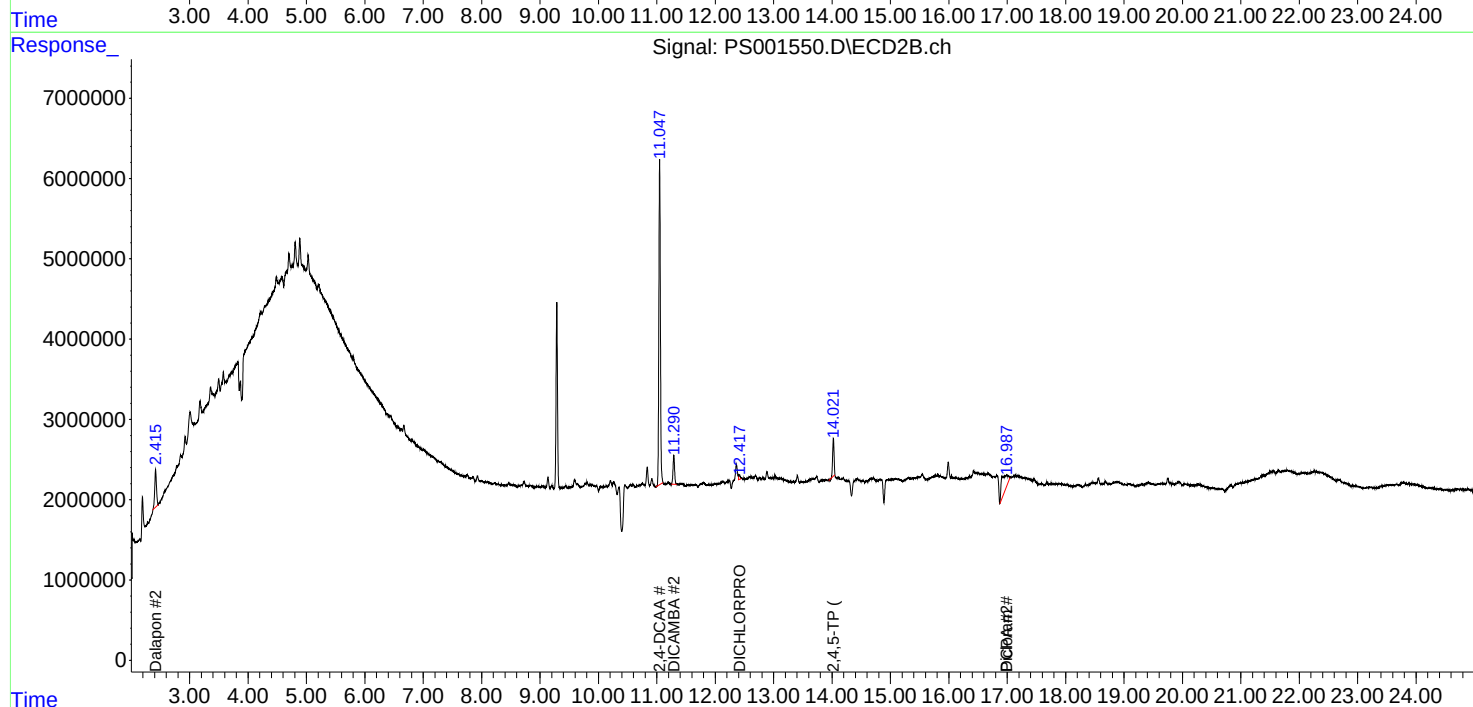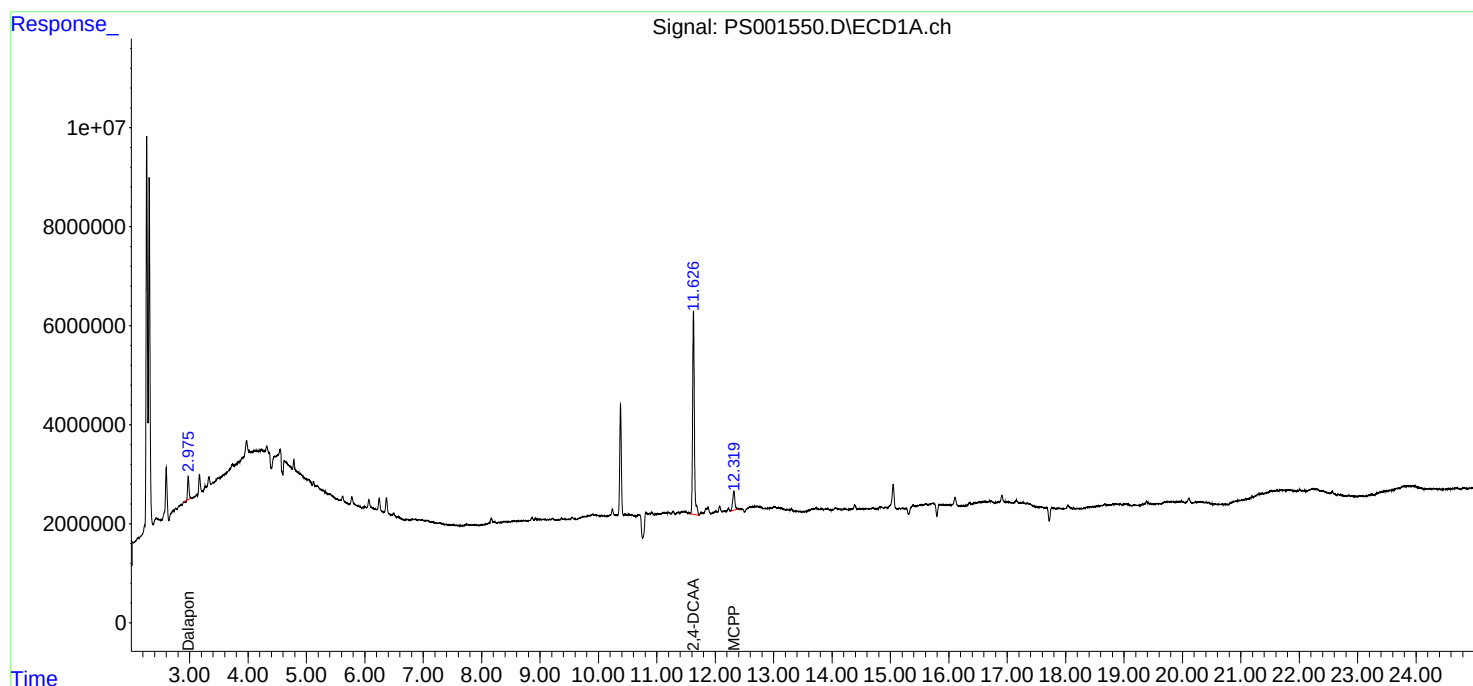


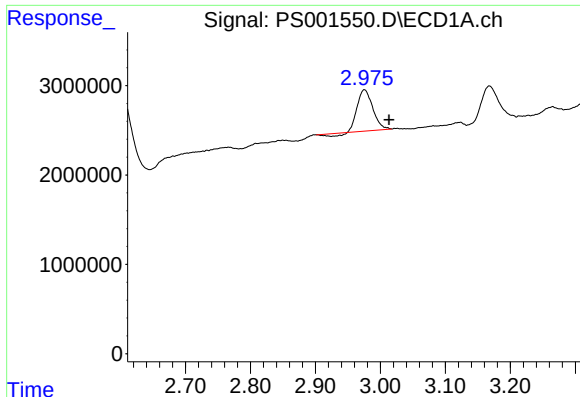

#1 Dalapon


R.T.: 2.975 min
Delta R.T.: -0.038 min
Response: 7267277
Conc: 30.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

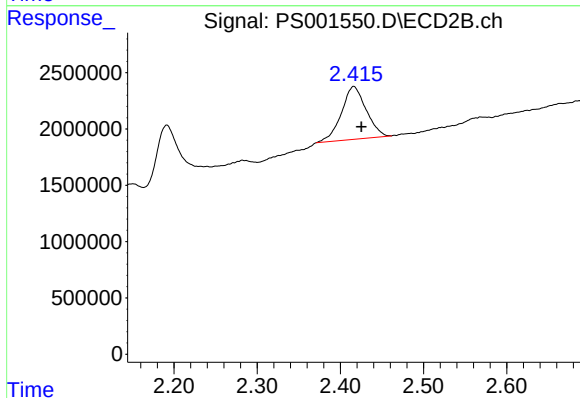


#1 Dalapon

R.T.: 2.416 min
Delta R.T.: -0.009 min
Response: 9680935
Conc: 42.48 ng/ml

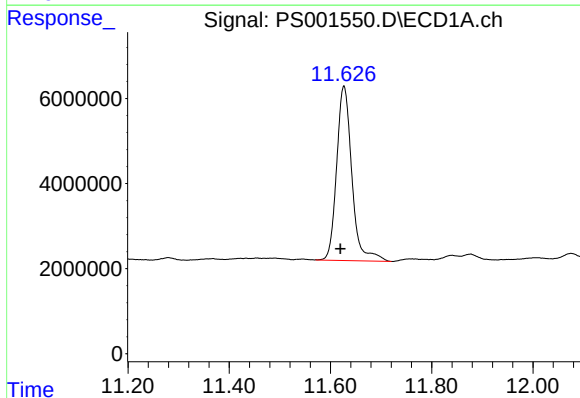


#4 2,4-DCAA

R.T.: 11.627 min
Delta R.T.: 0.007 min
Response: 85615883
Conc: 461.42 ng/ml

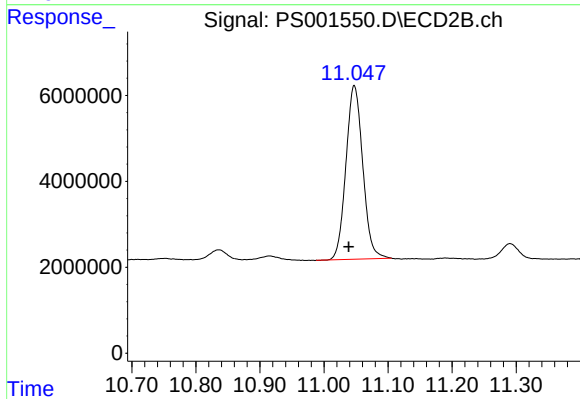

#4 2,4-DCAA


R.T.: 11.047 min
Delta R.T.: 0.009 min
Response: 73665033
Conc: 405.03 ng/ml

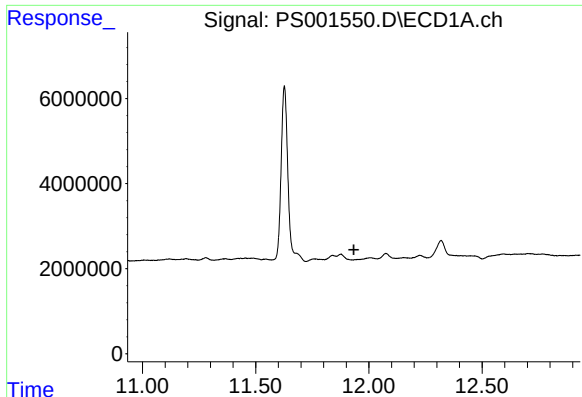

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

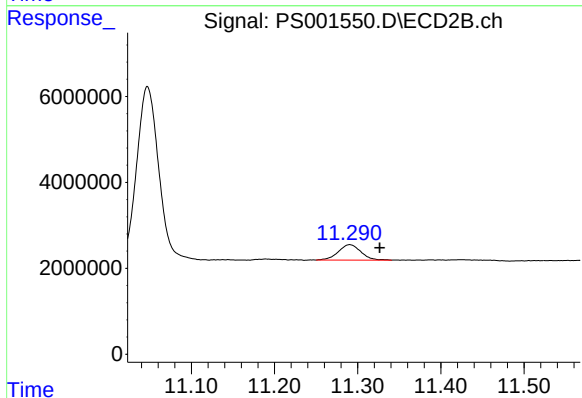


#5 DICAMBA

R.T.: 11.290 min
Delta R.T.: -0.036 min
Response: 6760741
Conc: 9.86 ng/ml

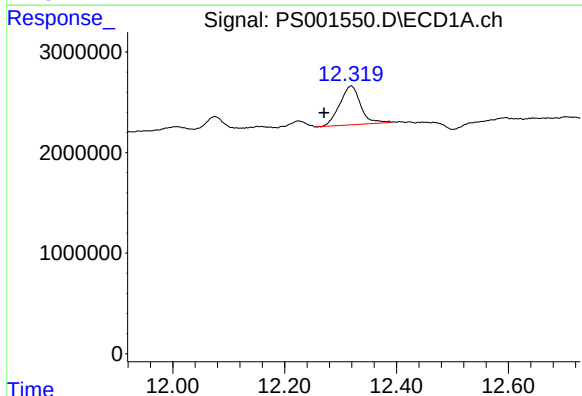


#6 MCP

R.T.: 12.319 min
Delta R.T.: 0.048 min
Response: 9939712
Conc: 19.78 ug/ml

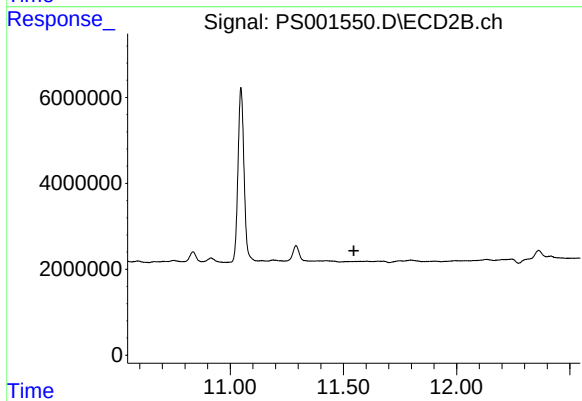

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

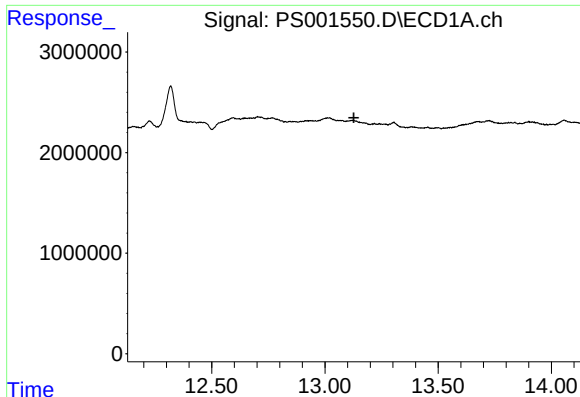

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

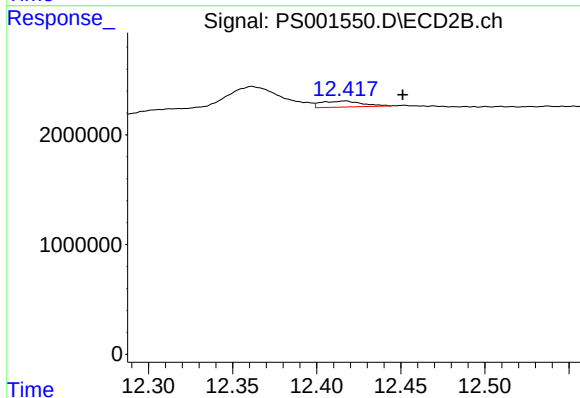


#8 DICHLORPROP

R.T.: 12.417 min
Delta R.T.: -0.034 min
Response: 916935
Conc: 5.18 ng/ml

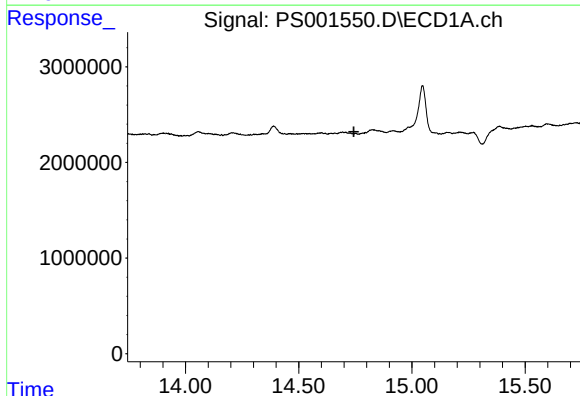


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

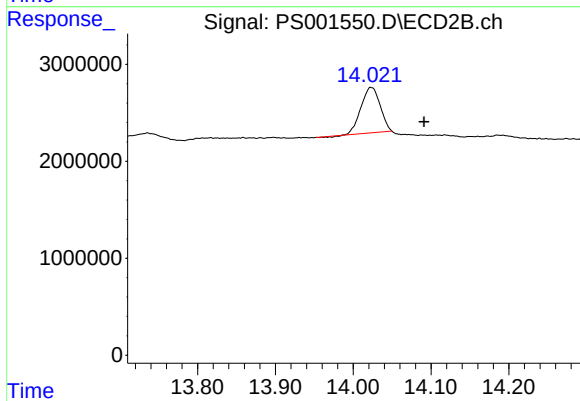

#11 2,4,5-TP (SILVEX)


R.T.: 14.023 min
Delta R.T.: -0.068 min
Response: 7987695
Conc: 7.31 ng/ml

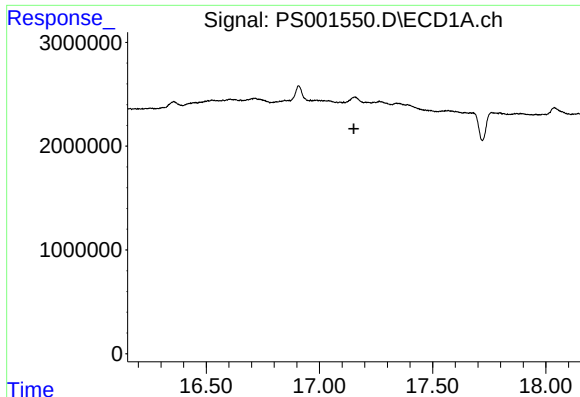

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

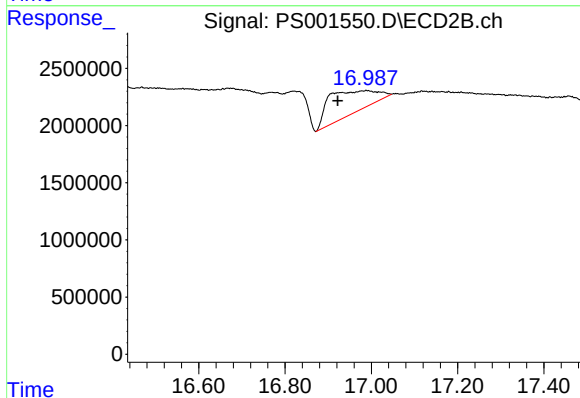


#15 Picloram

R.T.: 16.988 min
Delta R.T.: 0.066 min
Response: 15409240
Conc: 11.18 ng/ml

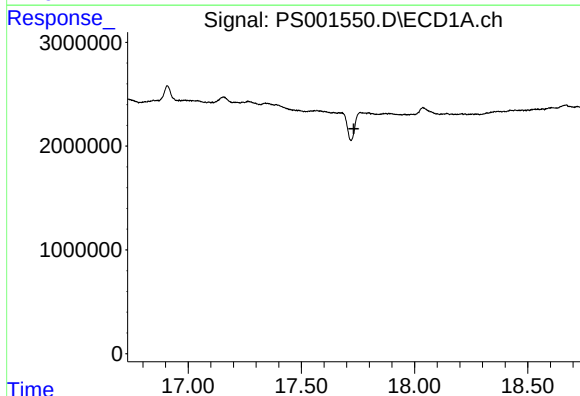

#16 DCPA

R.T.: 17.764 min
Delta R.T.: 0.032 min
Response: -4116258
Conc: N.D.

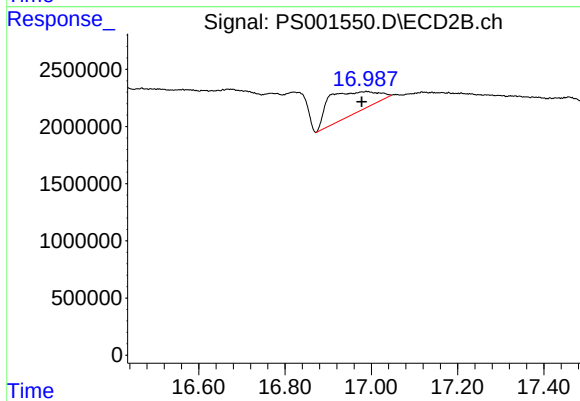

#16 DCPA

R.T.: 16.988 min
Delta R.T.: 0.010 min
Response: 15409240
Conc: 10.67 ng/ml