

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 15:27
 Operator : UA
 Sample : J4486-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:40:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.623	11.044	90362158	78607299	486.997	432.205
Target Compounds							
1) T	Dalapon	2.972	2.413	7256788	7543901	30.603	33.106
5) T	DICAMBA	0.000	11.287	0	6783153	N.D.	9.897 #
6) T	MCP	12.315	0.000	10365778	0	20.624	N.D. #
8) T	DICHLORPROP	0.000	12.410	0	1300393	N.D.	7.341 #
13) T	2,4-DB	15.832	0.000	5309873	0	36.883	N.D. #
15) T	Picloram	0.000	16.975	0	2827491	N.D.	2.051 #
16) T	DCPA	17.761	16.975	6205962	2827491	4.597	1.958 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 15:27
Operator : UA
Sample : J4486-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:40:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

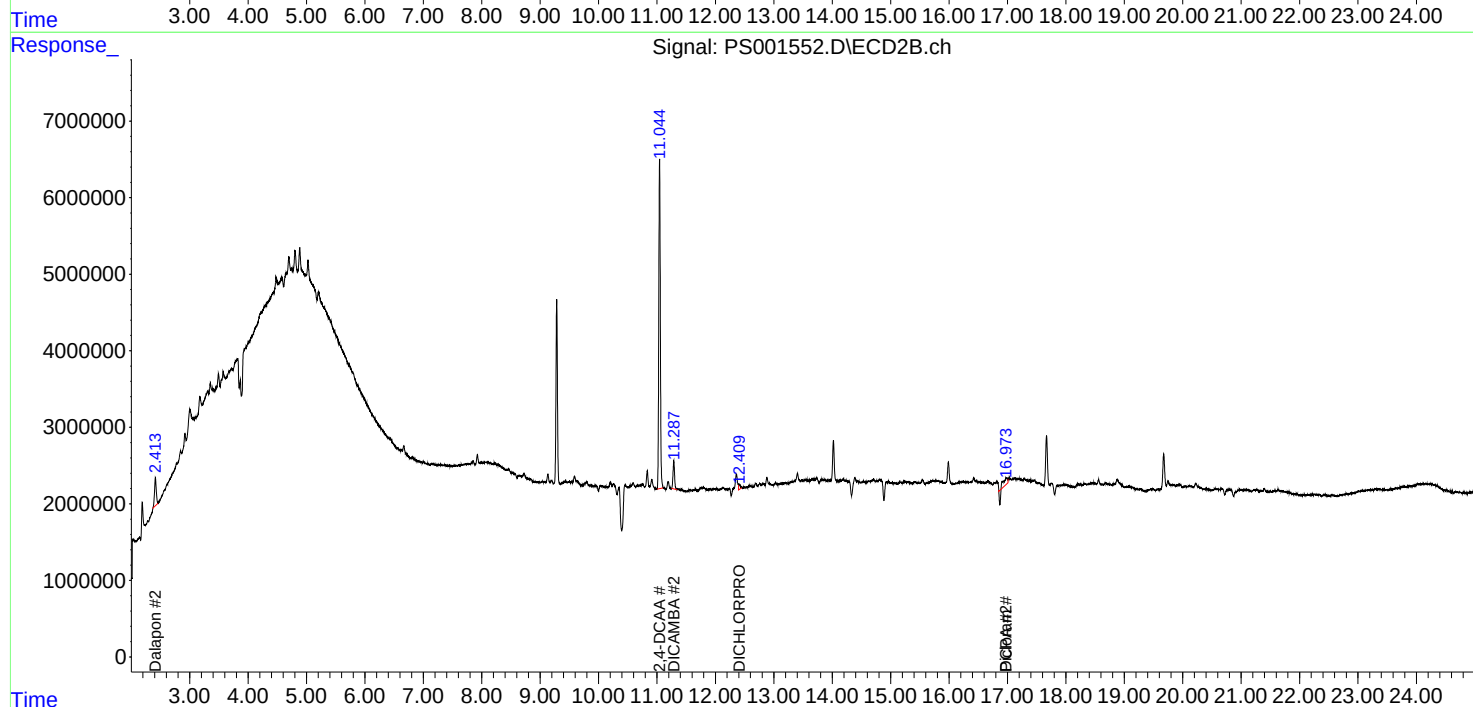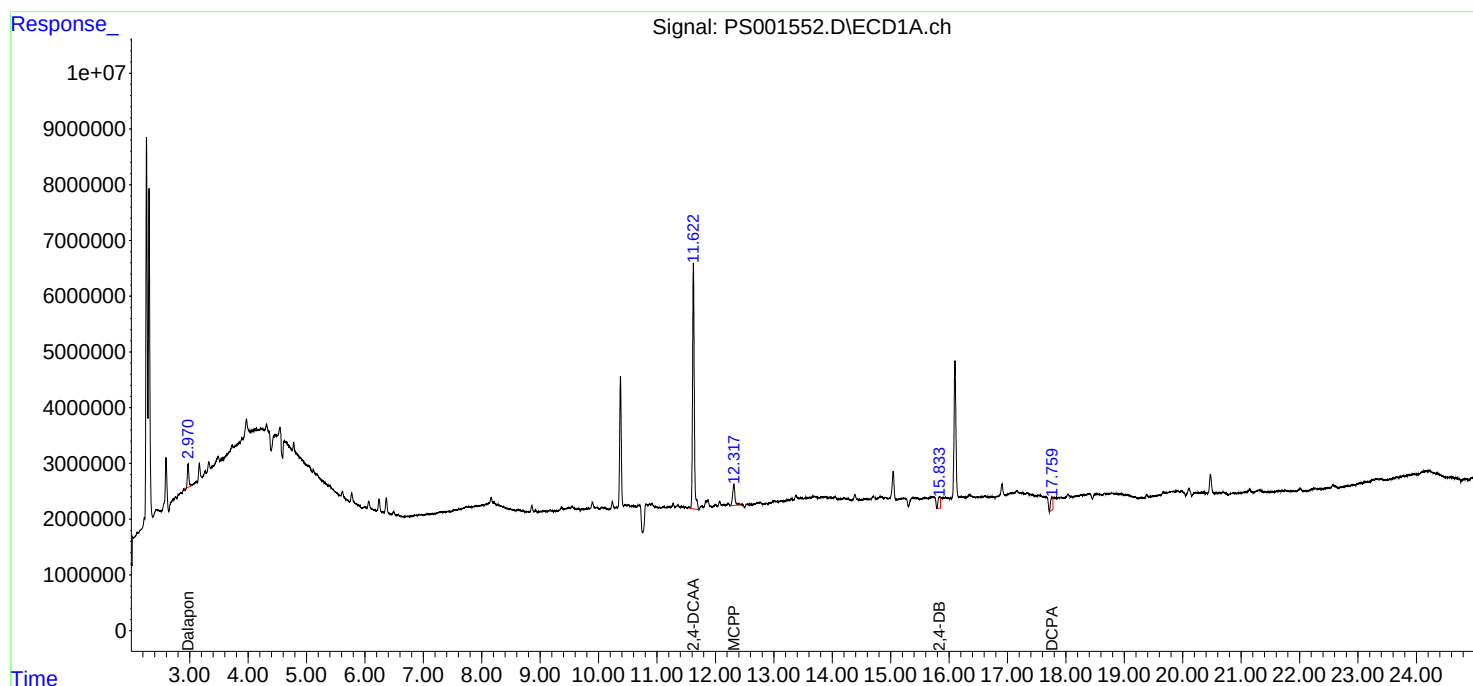


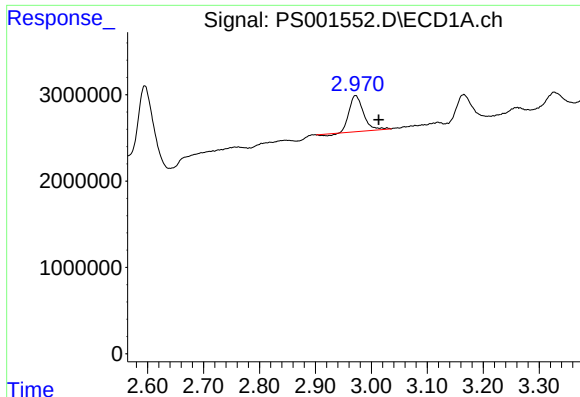

#1 Dalapon


R.T.: 2.972 min
Delta R.T.: -0.041 min
Response: 7256788
Conc: 30.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

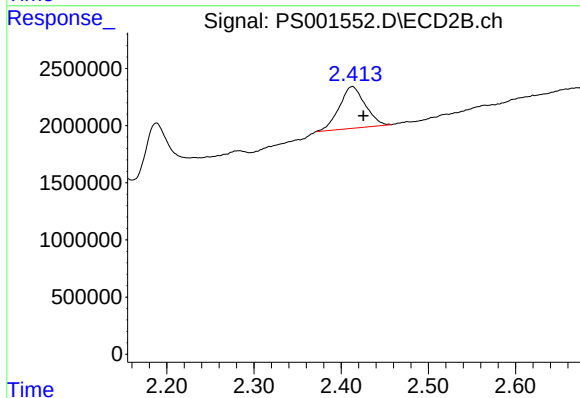


#1 Dalapon

R.T.: 2.413 min
Delta R.T.: -0.012 min
Response: 7543901
Conc: 33.11 ng/ml

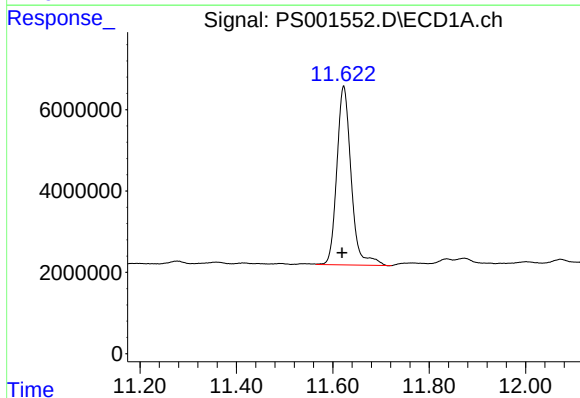


#4 2,4-DCAA

R.T.: 11.623 min
Delta R.T.: 0.003 min
Response: 90362158
Conc: 487.00 ng/ml

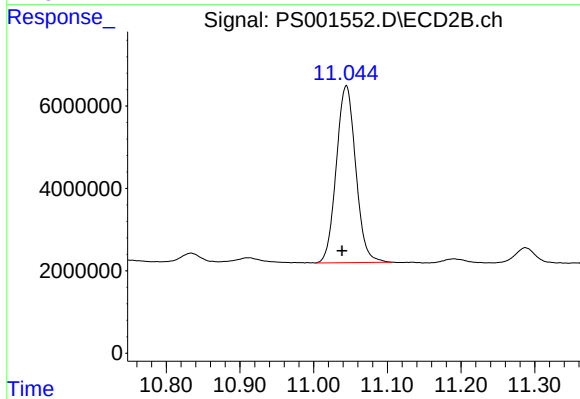

#4 2,4-DCAA


R.T.: 11.044 min
Delta R.T.: 0.006 min
Response: 78607299
Conc: 432.21 ng/ml

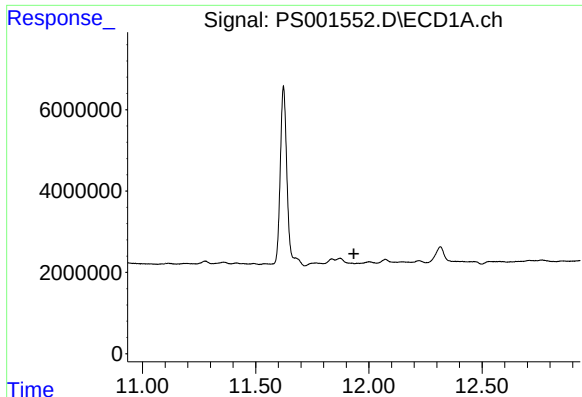

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

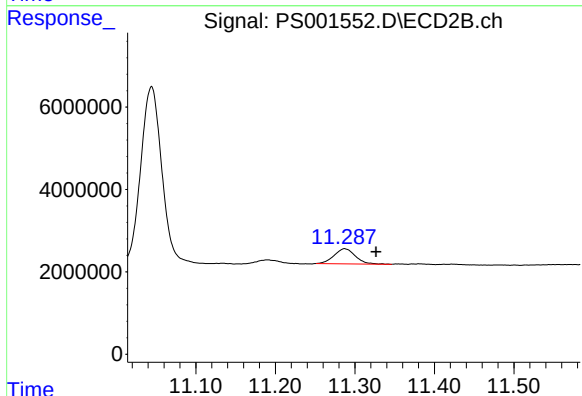


#5 DICAMBA

R.T.: 11.287 min
Delta R.T.: -0.039 min
Response: 6783153
Conc: 9.90 ng/ml

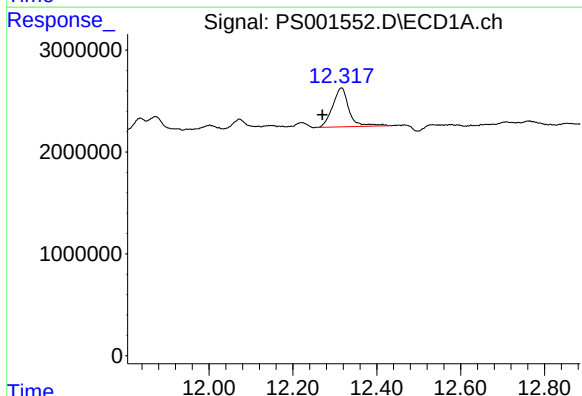


#6 MCP

R.T.: 12.315 min
Delta R.T.: 0.045 min
Response: 10365778
Conc: 20.62 ug/ml

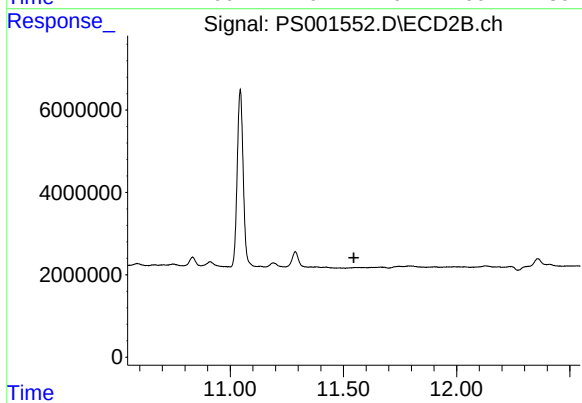

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

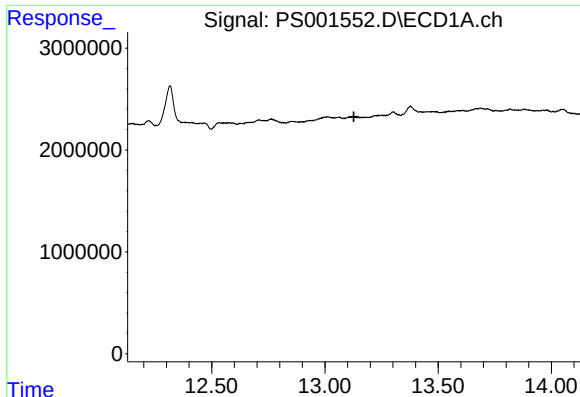

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

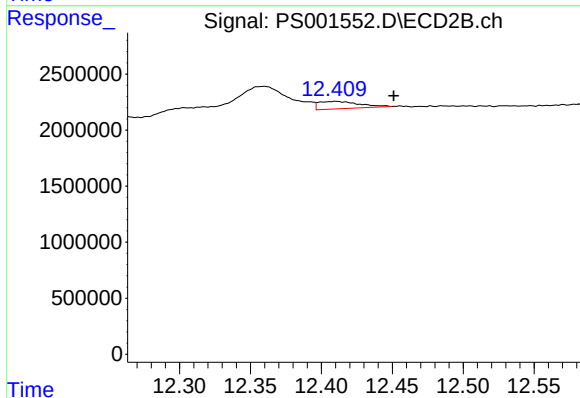


#8 DICHLORPROP

R.T.: 12.410 min
Delta R.T.: -0.041 min
Response: 1300393
Conc: 7.34 ng/ml

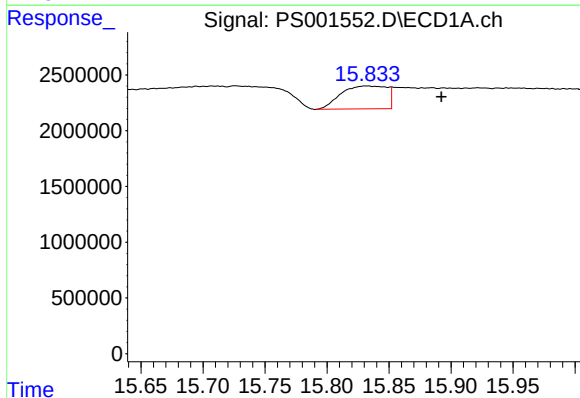


#13 2,4-DB

R.T.: 15.832 min
Delta R.T.: -0.060 min
Response: 5309873
Conc: 36.88 ng/ml

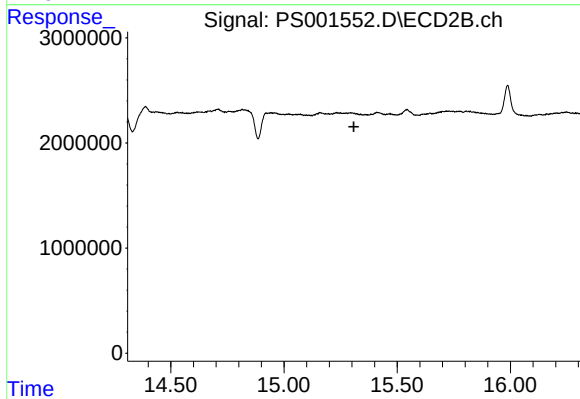

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.308 min
Response: 0
Conc: N.D.

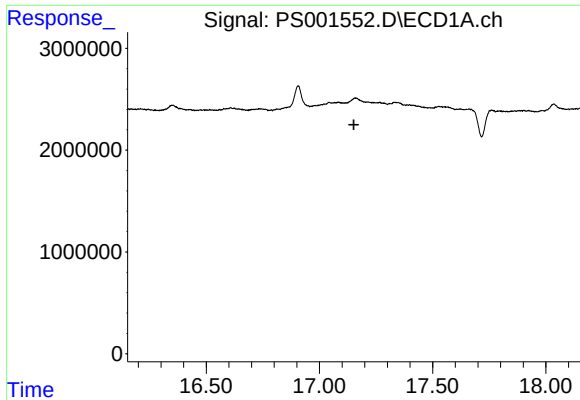

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

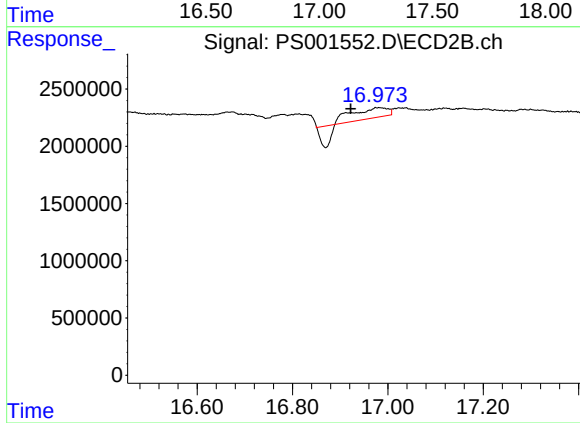


#15 Picloram

R.T.: 16.975 min
Delta R.T.: 0.052 min
Response: 2827491
Conc: 2.05 ng/ml

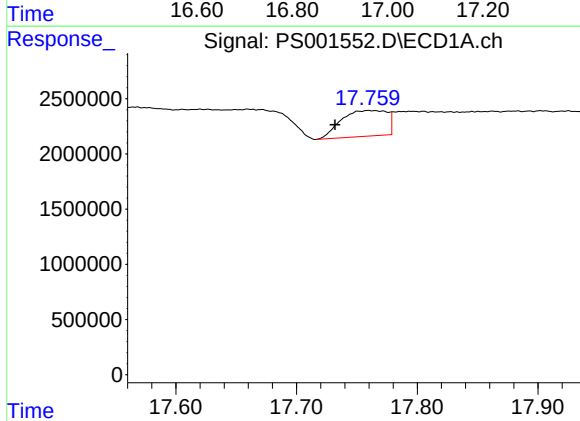

#16 DCPA

R.T.: 17.761 min
Delta R.T.: 0.029 min
Response: 6205962
Conc: 4.60 ng/ml

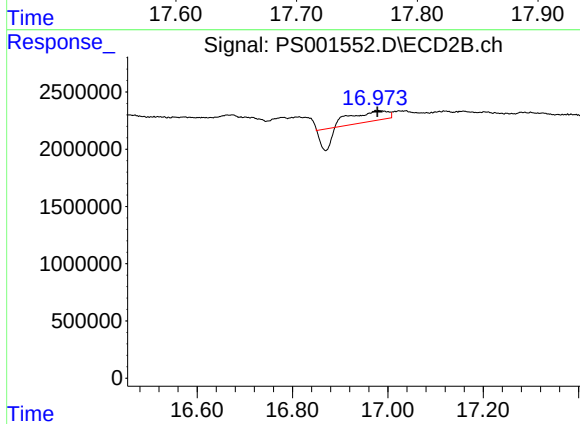

#16 DCPA

R.T.: 16.975 min
Delta R.T.: -0.003 min
Response: 2827491
Conc: 1.96 ng/ml