

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 17:00
 Operator : UA
 Sample : J4500-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:41:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.608	11.029	89671412	78832362	483.274	433.443
Target Compounds							
1) T	Dalapon	2.957	2.397	8676704	5593804	36.591	24.548 #
2) T	3,5-DICHL...	0.000	9.116	0	734286	N.D.	2.882 #
3) T	4-Nitroph...	0.000	10.186	0	13976010	N.D.	137.102 #
5) T	DICAMBA	0.000	11.271	0	3705173	N.D.	5.406 #
6) T	MCP	12.300	0.000	8213592	0	16.342	N.D. #
10) T	Pentachlo...	13.863	13.466	3700456	3027695	1.314	1.100
15) T	Picloram	17.145	16.907	3425285	8248552	2.167	5.984 #
16) T	DCPA	0.000	16.966	0	11241990	N.D.	7.784 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 17:00
Operator : UA
Sample : J4500-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:41:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

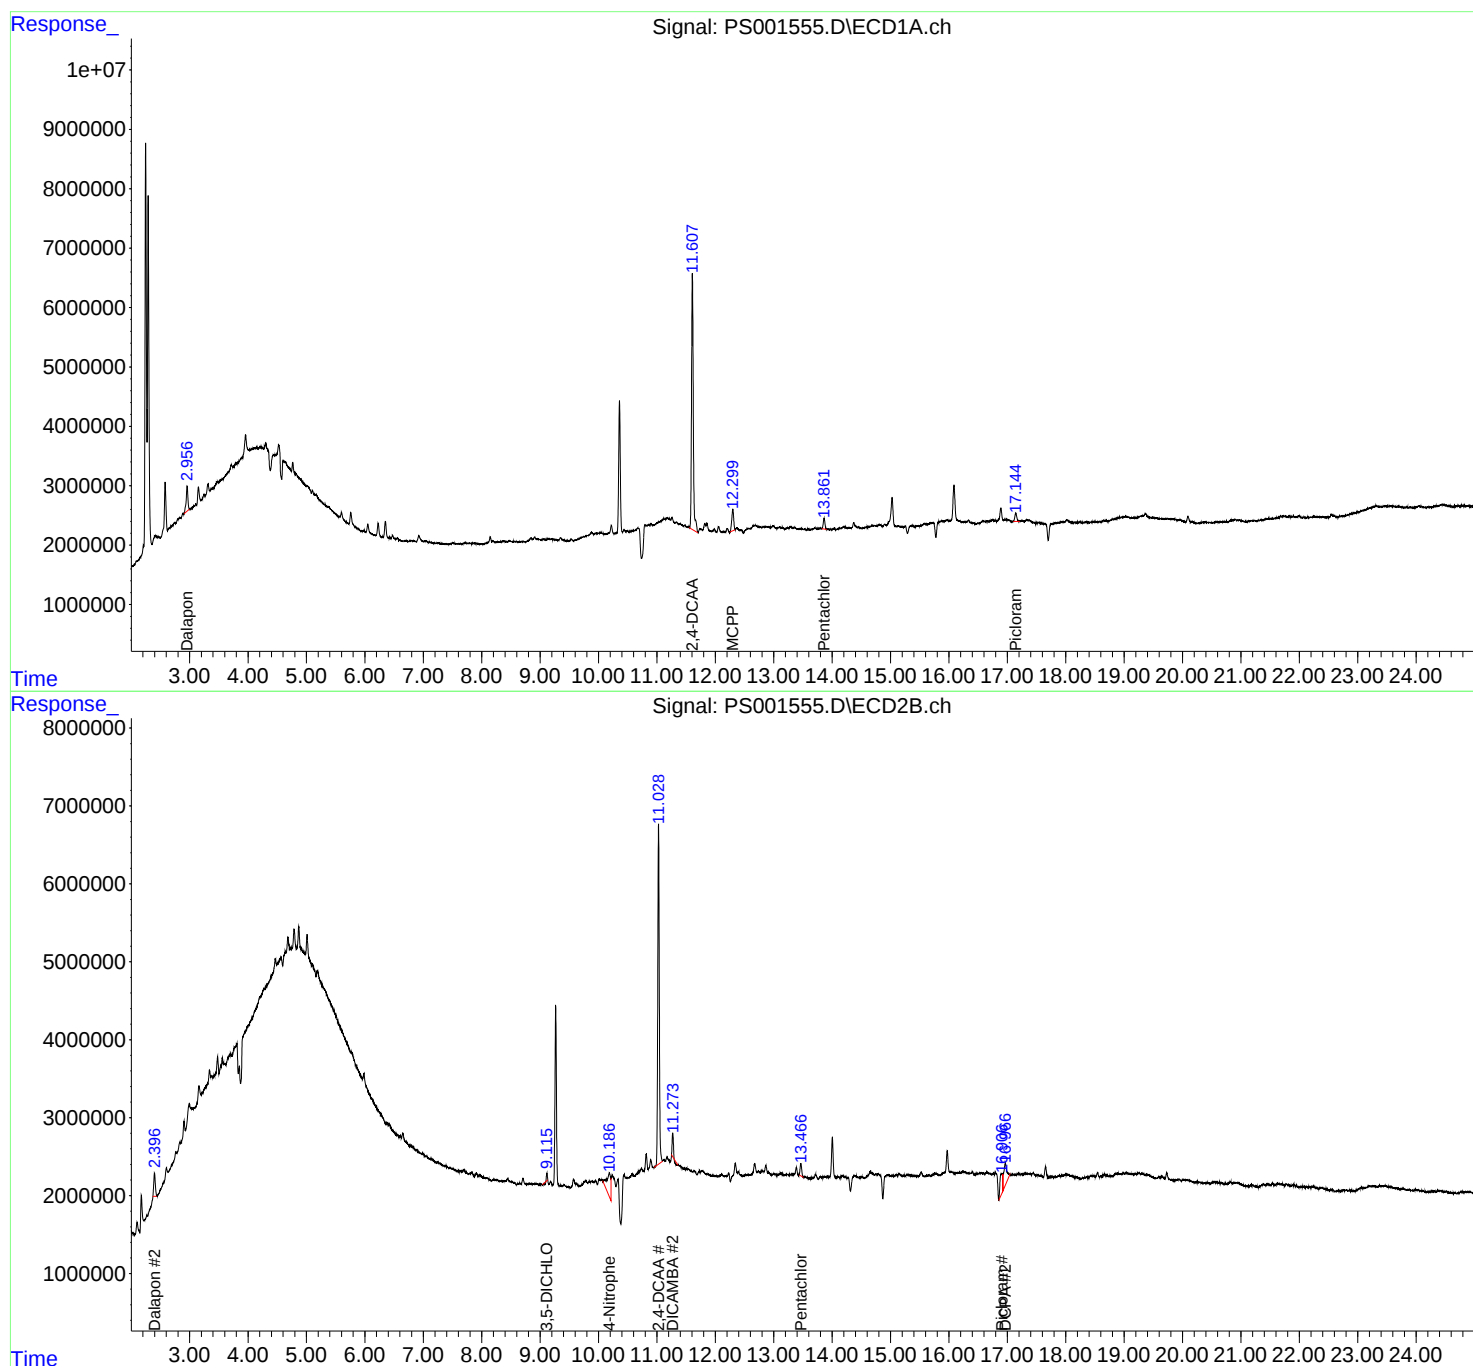


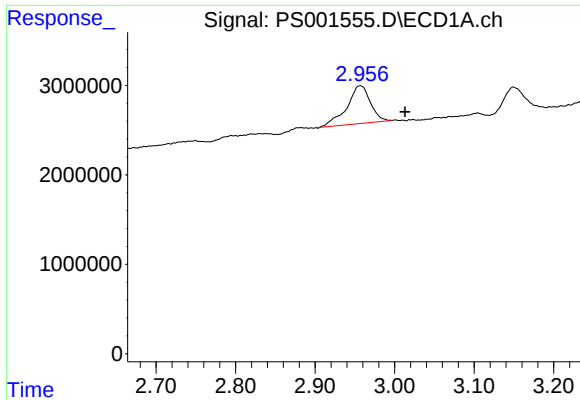

#1 Dalapon


R.T.: 2.957 min
Delta R.T.: -0.056 min
Response: 8676704
Conc: 36.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

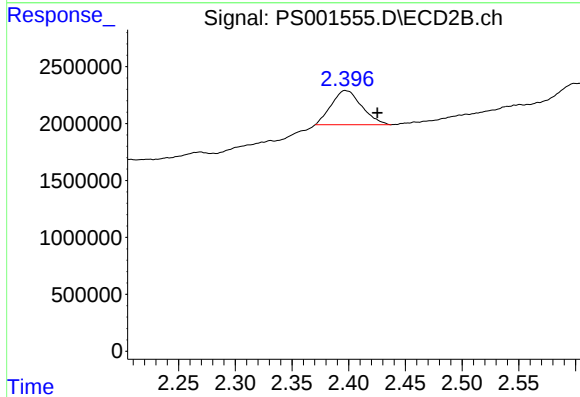


#1 Dalapon

R.T.: 2.397 min
Delta R.T.: -0.029 min
Response: 5593804
Conc: 24.55 ng/ml

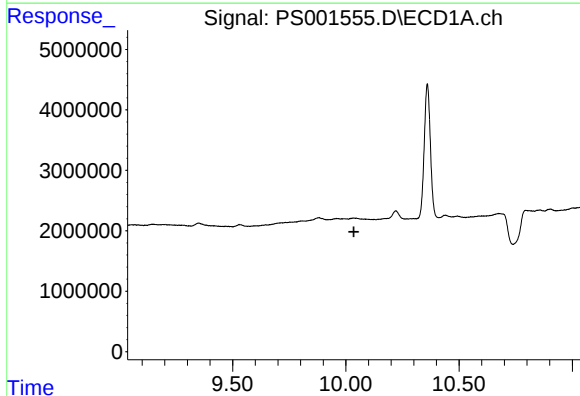


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

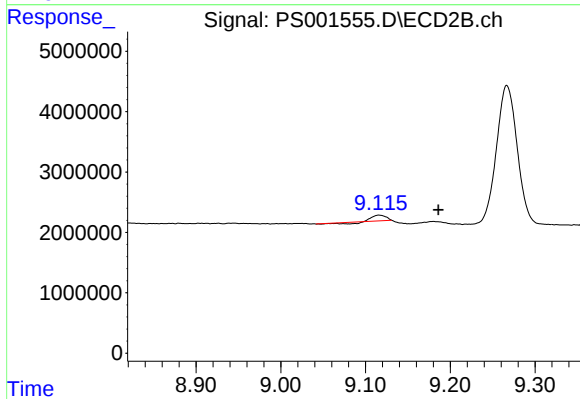

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.116 min
Delta R.T.: -0.070 min
Response: 734286
Conc: 2.88 ng/ml

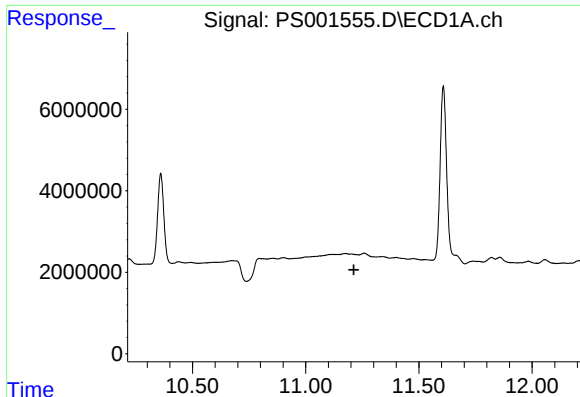

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

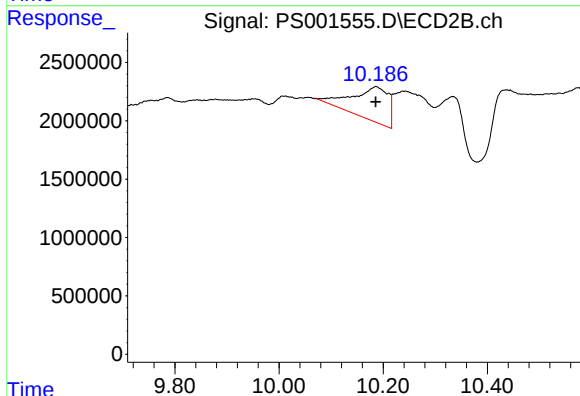


#3 4-Nitrophenol

R.T.: 10.186 min
Delta R.T.: 0.000 min
Response: 13976010
Conc: 137.10 ng/ml

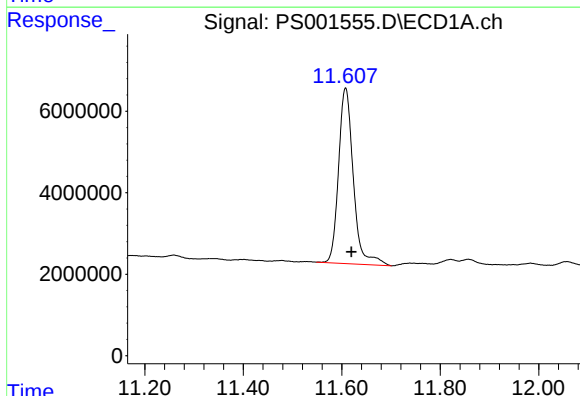


#4 2,4-DCAA

R.T.: 11.608 min
Delta R.T.: -0.012 min
Response: 89671412
Conc: 483.27 ng/ml

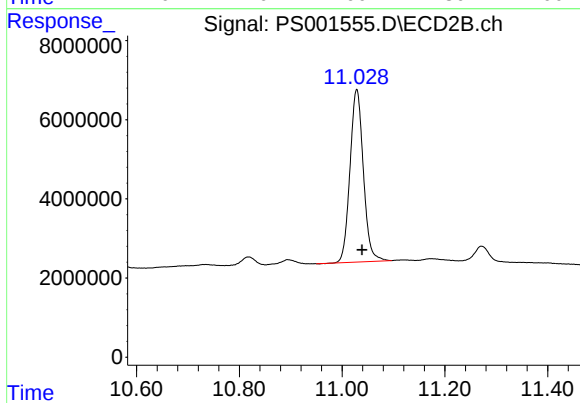

#4 2,4-DCAA


R.T.: 11.029 min
Delta R.T.: -0.010 min
Response: 78832362
Conc: 433.44 ng/ml

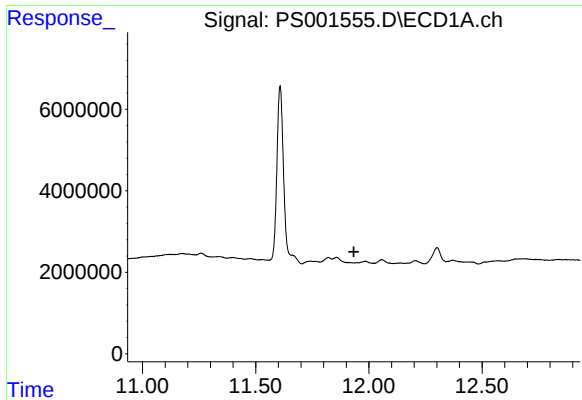

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

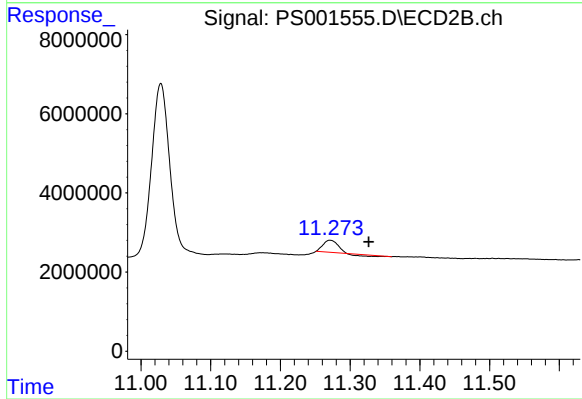


#5 DICAMBA

R.T.: 11.271 min
Delta R.T.: -0.055 min
Response: 3705173
Conc: 5.41 ng/ml

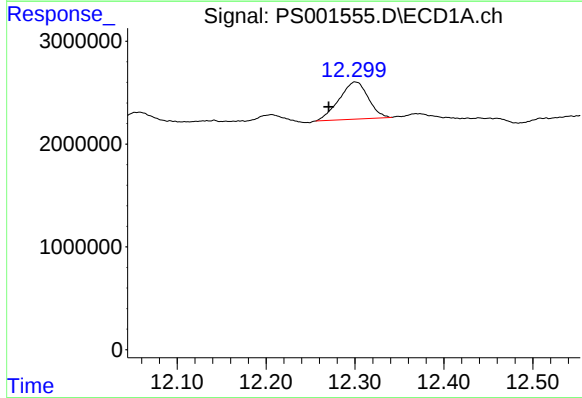


#6 MCP

R.T.: 12.300 min
Delta R.T.: 0.030 min
Response: 8213592
Conc: 16.34 ug/ml

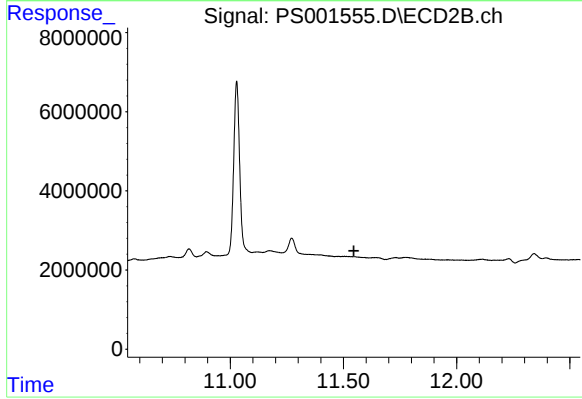

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

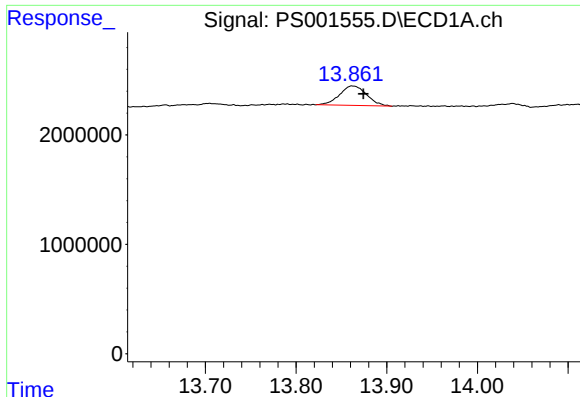

#10 Pentachlorophenol


R.T.: 13.863 min
Delta R.T.: -0.012 min
Response: 3700456
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

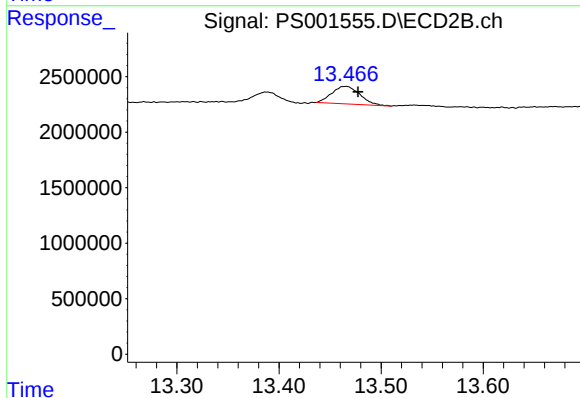


#10 Pentachlorophenol

R.T.: 13.466 min
Delta R.T.: -0.012 min
Response: 3027695
Conc: 1.10 ng/ml

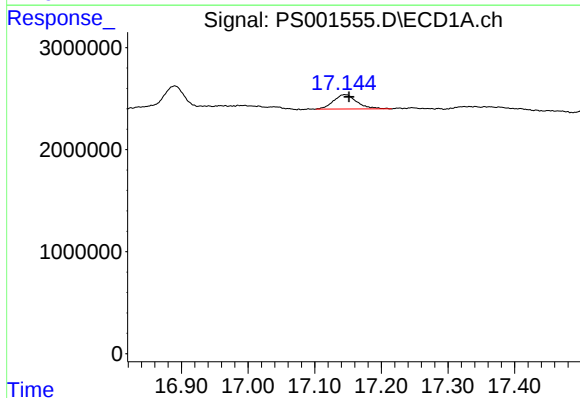


#15 Picloram

R.T.: 17.145 min
Delta R.T.: -0.006 min
Response: 3425285
Conc: 2.17 ng/ml

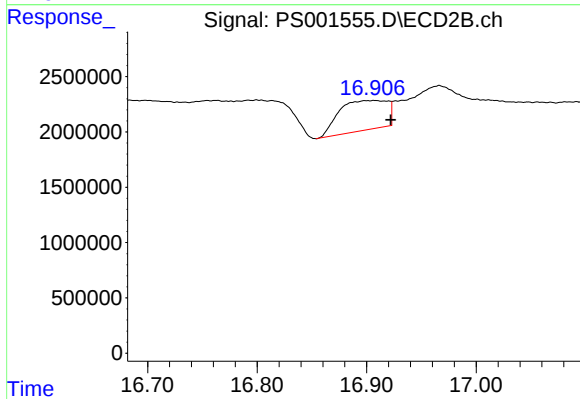

#15 Picloram


R.T.: 16.907 min
Delta R.T.: -0.015 min
Response: 8248552
Conc: 5.98 ng/ml

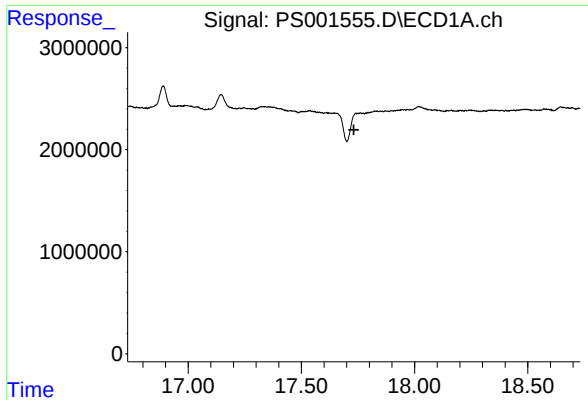

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

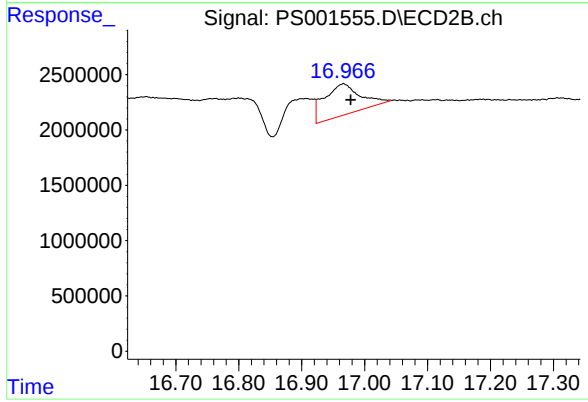

#16 DCPA

R.T.: 16.966 min
Delta R.T.: -0.012 min
Response: 11241990
Conc: 7.78 ng/ml