

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
 Data File : PS001558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 18:33
 Operator : UA
 Sample : J4500-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:42:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.642	11.062	80537462	72119971	434.047	396.536
Target Compounds							
1) T	Dalapon	2.991	2.431	9085151	7952494	38.314	34.899
2) T	3,5-DICHL...	0.000	9.149	0	2147633	N.D.	8.430 #
5) T	DICAMBA	0.000	11.305	0	7695306	N.D.	11.228 #
6) T	MCP	12.333	0.000	7757345	0	15.434	N.D. #
8) T	DICHLORPROP	0.000	12.425	0	964471	N.D.	5.444 #
9) T	2,4-D	0.000	12.899	0	2921342	N.D.	12.311 #
10) T	Pentachlo...	0.000	13.422	0	325813	N.D.	0.118 #
11) T	2,4,5-TP ...	0.000	14.038	0	2943270	N.D.	2.692 #
15) T	Picloram	17.175	0.000	3072180	0	1.944	N.D. #
16) T	DCPA	0.000	16.998	0	17025627	N.D.	11.788 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081718\
Data File : PS001558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 18:33
Operator : UA
Sample : J4500-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:42:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

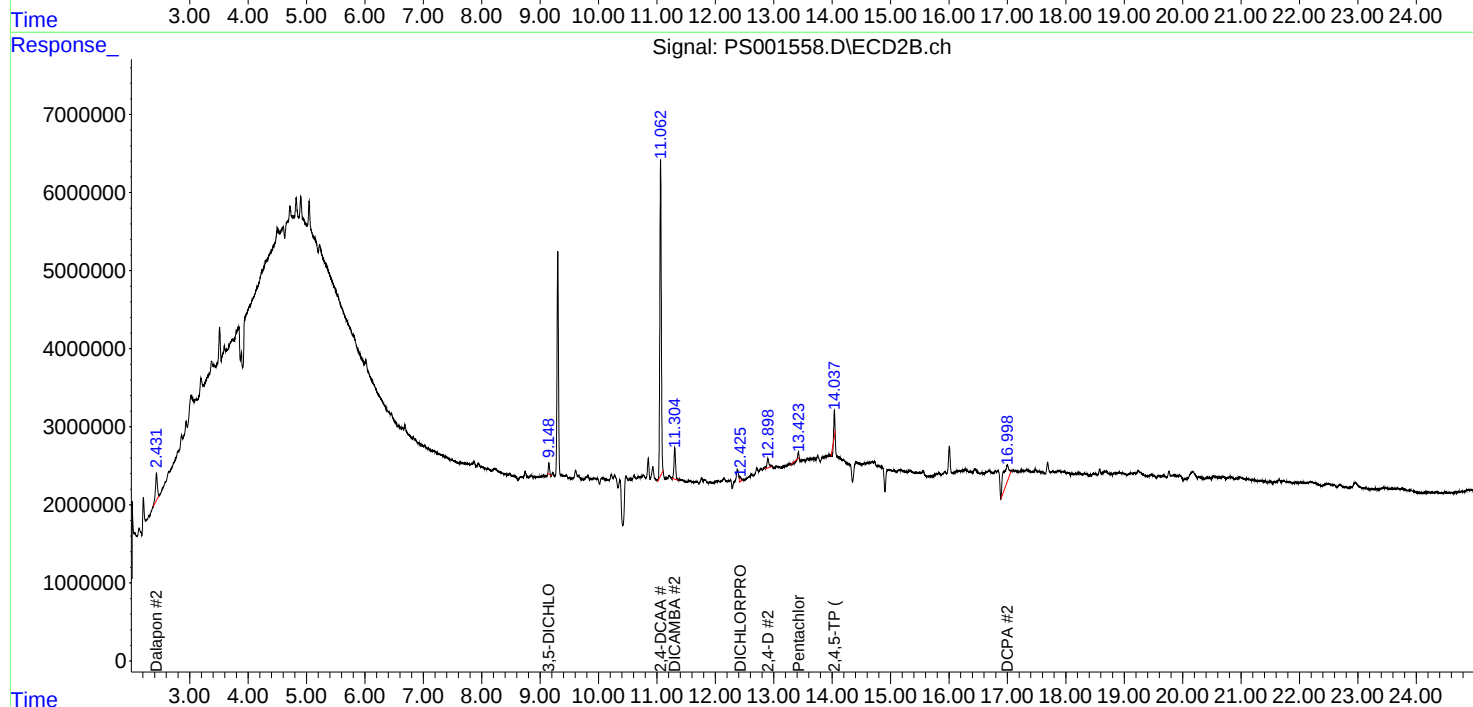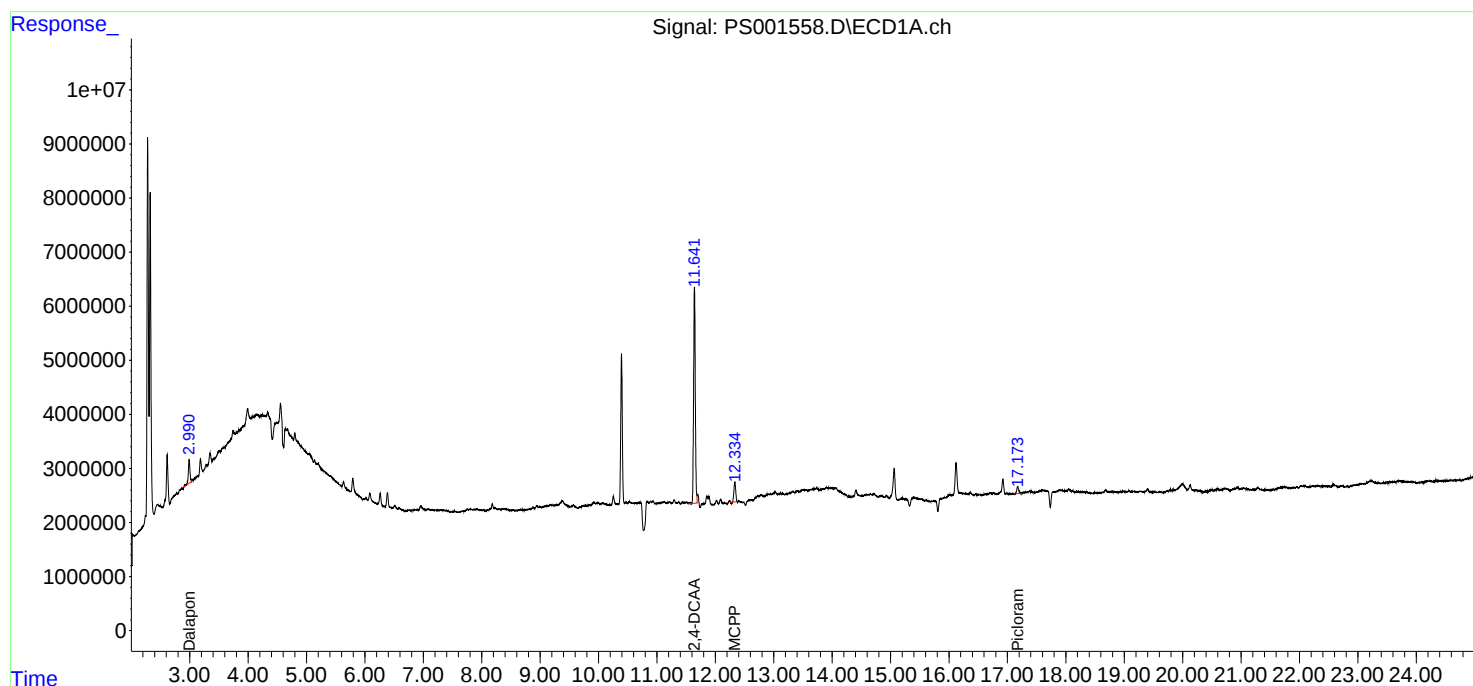


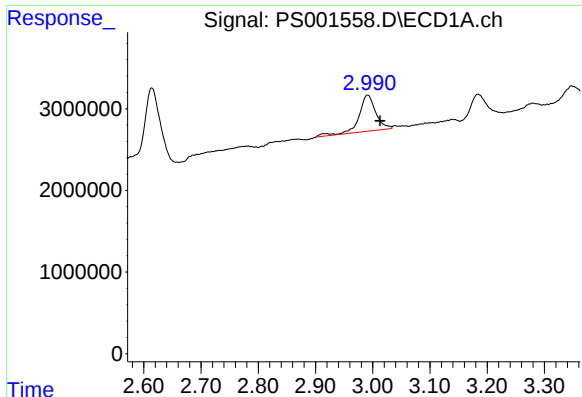

#1 Dalapon


R.T.: 2.991 min
Delta R.T.: -0.022 min
Response: 9085151
Conc: 38.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

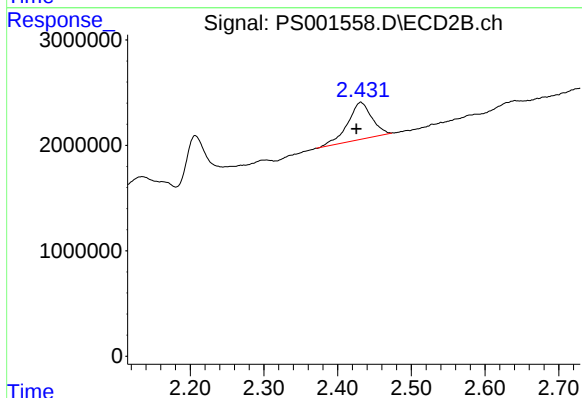


#1 Dalapon

R.T.: 2.431 min
Delta R.T.: 0.006 min
Response: 7952494
Conc: 34.90 ng/ml

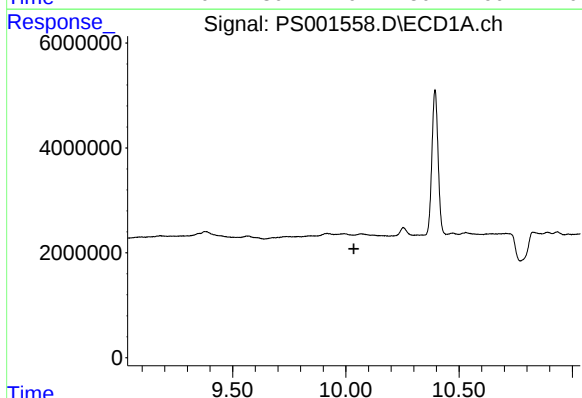


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

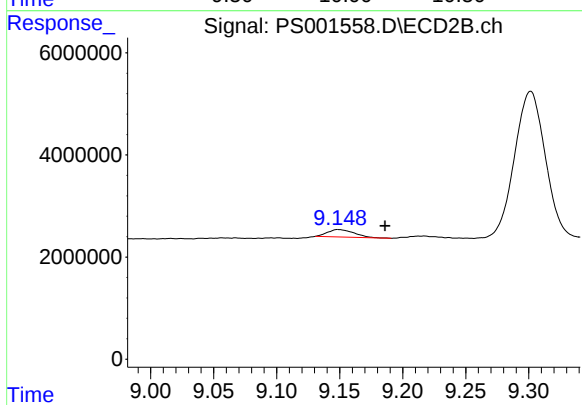

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.149 min
Delta R.T.: -0.037 min
Response: 2147633
Conc: 8.43 ng/ml

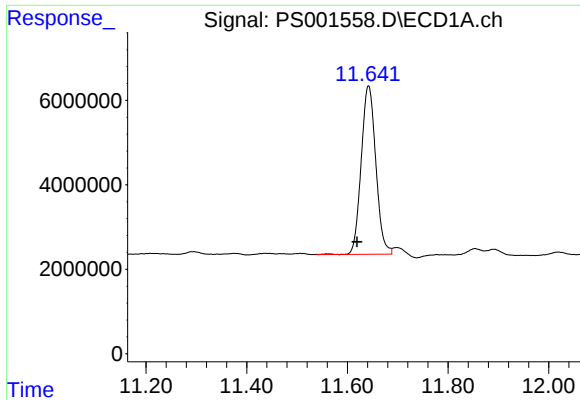

#4 2,4-DCAA


R.T.: 11.642 min
Delta R.T.: 0.023 min
Response: 80537462
Conc: 434.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

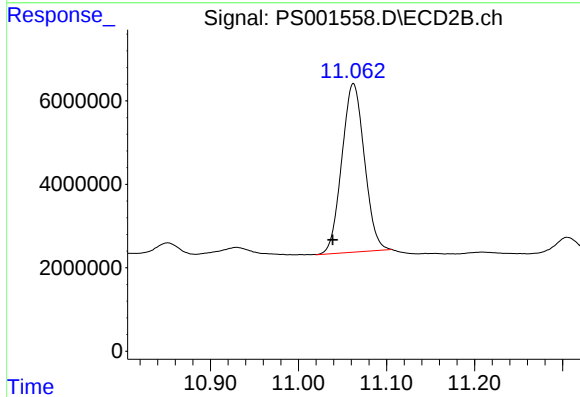


#4 2,4-DCAA

R.T.: 11.062 min
Delta R.T.: 0.024 min
Response: 72119971
Conc: 396.54 ng/ml

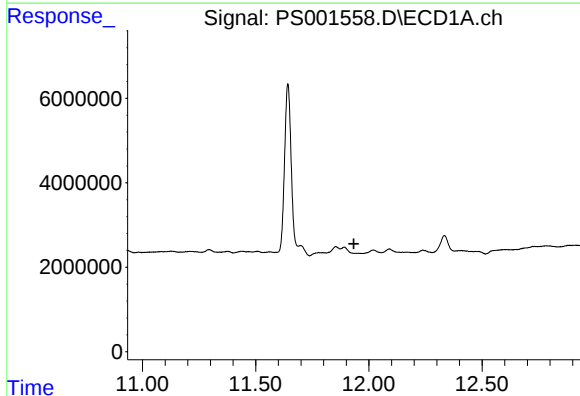


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

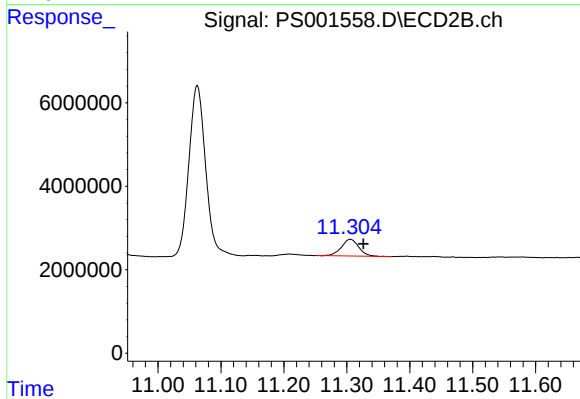

#5 DICAMBA


R.T.: 11.305 min
Delta R.T.: -0.021 min
Response: 7695306
Conc: 11.23 ng/ml

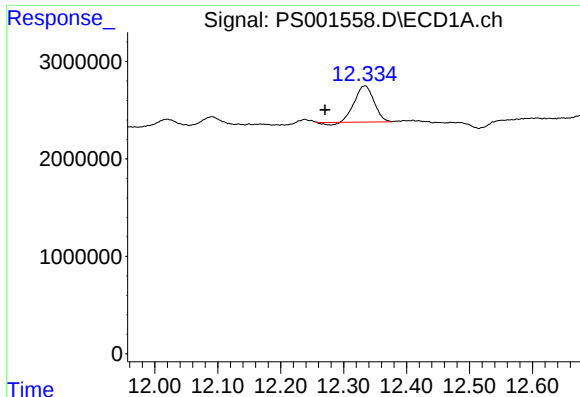

#6 MCP


R.T.: 12.333 min
Delta R.T.: 0.063 min
Response: 7757345
Conc: 15.43 ug/ml

Instrument :
ECD_S
ClientSampleId :

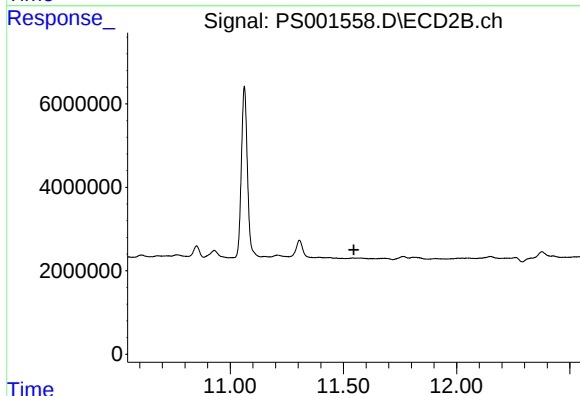


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

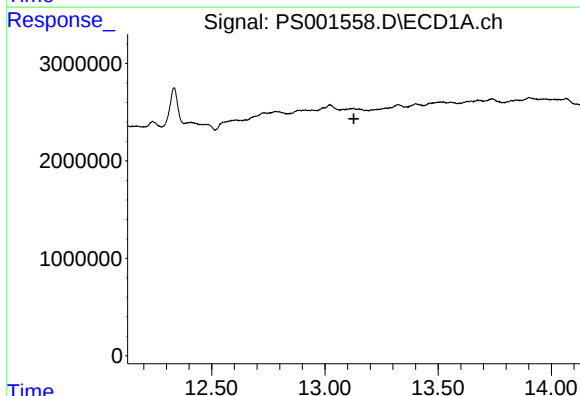


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.128 min
Response: 0
Conc: N.D.

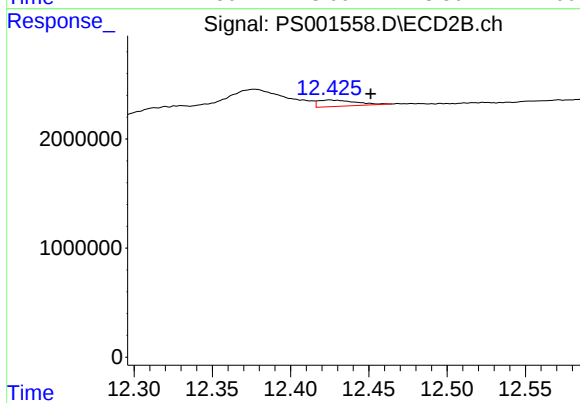

#8 DICHLORPROP


R.T.: 12.425 min
Delta R.T.: -0.026 min
Response: 964471
Conc: 5.44 ng/ml

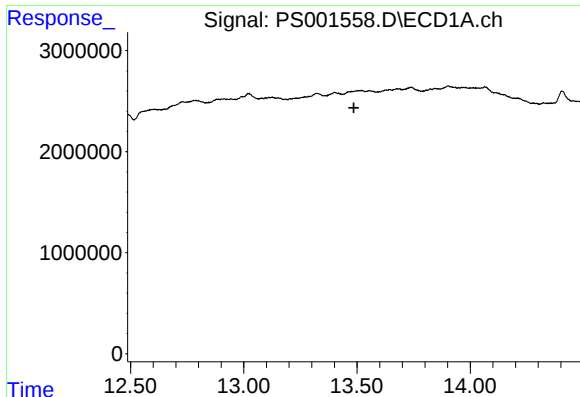

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

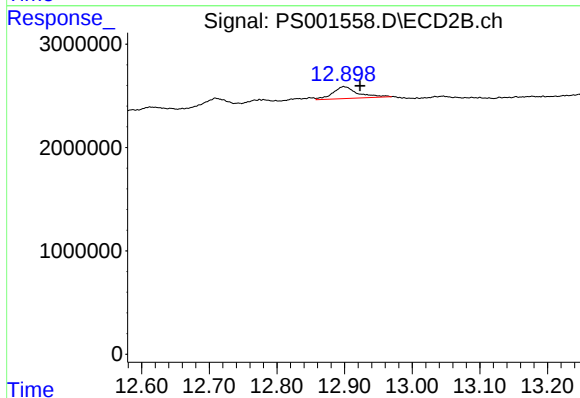


#9 2,4-D

R.T.: 12.899 min
Delta R.T.: -0.024 min
Response: 2921342
Conc: 12.31 ng/ml

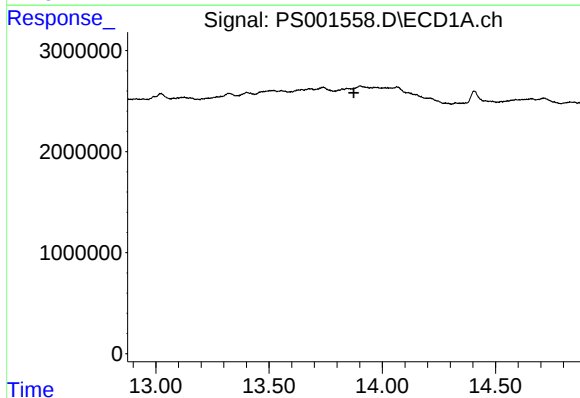


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.874 min
Response: 0
Conc: N.D.

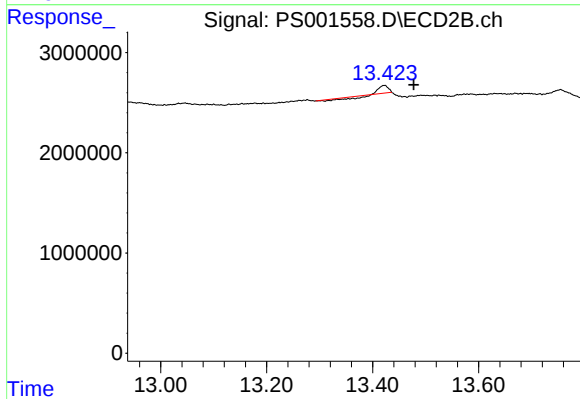

#10 Pentachlorophenol


R.T.: 13.422 min
Delta R.T.: -0.055 min
Response: 325813
Conc: 0.12 ng/ml

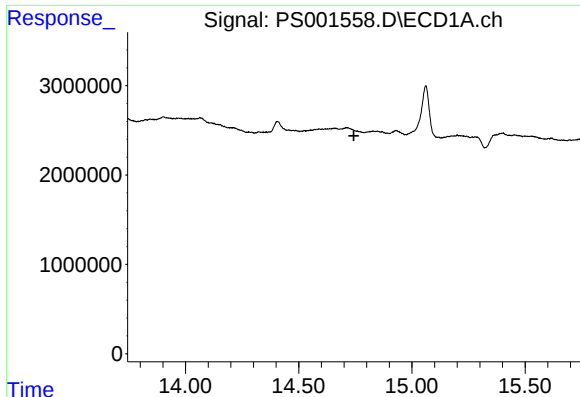

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

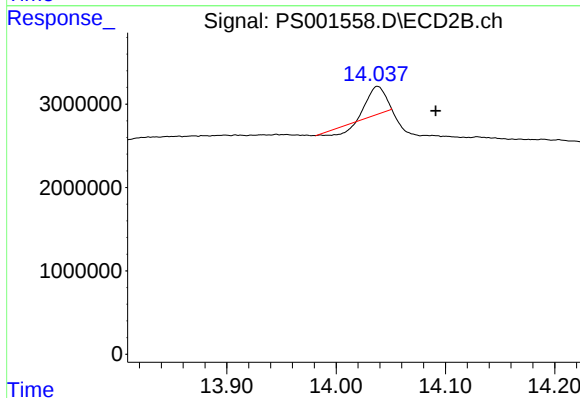


#11 2,4,5-TP (SILVEX)

R.T.: 14.038 min
Delta R.T.: -0.053 min
Response: 2943270
Conc: 2.69 ng/ml

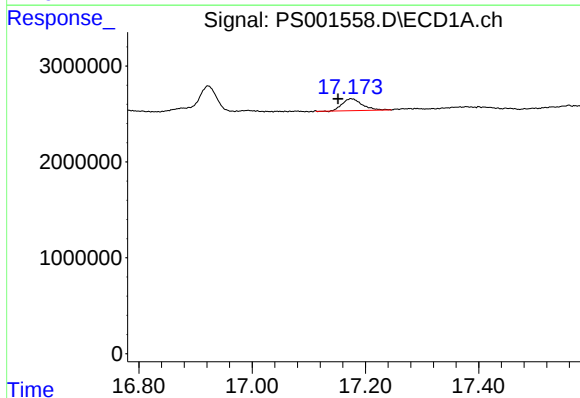


#15 Picloram

R.T.: 17.175 min
Delta R.T.: 0.023 min
Response: 3072180
Conc: 1.94 ng/ml

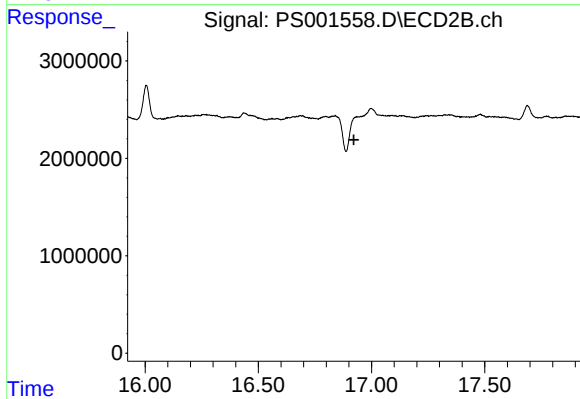

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.922 min
Response: 0
Conc: N.D.

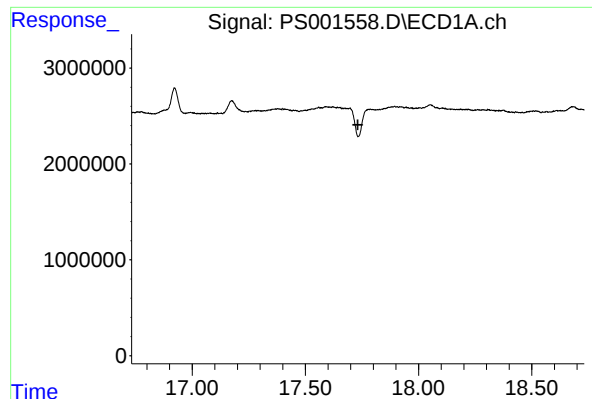

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

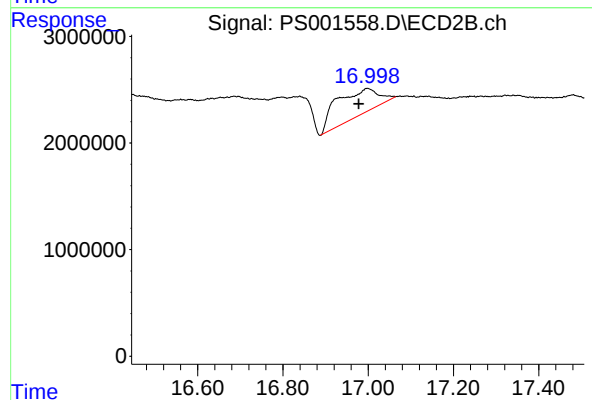

#16 DCPA

R.T.: 16.998 min
Delta R.T.: 0.020 min
Response: 17025627
Conc: 11.79 ng/ml