

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
 Data File : FF008949.D
 Signal(s) : FID2B.ch
 Acq On : 17 Aug 2021 16:14
 Operator : DD\AJ
 Sample : M3425-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 18 05:05:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2137063	17.837 ug/ml
Target Compounds			
7) N-EICOSANE	12.602	65577	0.468 ug/ml
10) N-TETRACOSANE	14.936	531141	3.837 ug/ml
12) N-OCTACOSANE	16.942	102051	0.763 ug/ml
13) N-TRIACONTANE	17.798	86659	0.663 ug/ml
14) N-DOTRIACONTANE	18.627	128248	1.037 ug/ml
15) N-TETRATRIACONTANE	19.407	86080	0.739 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
Data File : FF08949.D
Signal(s) : FID2B.ch
Acq On : 17 Aug 2021 16:14
Operator : DD\AJ
Sample : M3425-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 05:05:10 2021
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

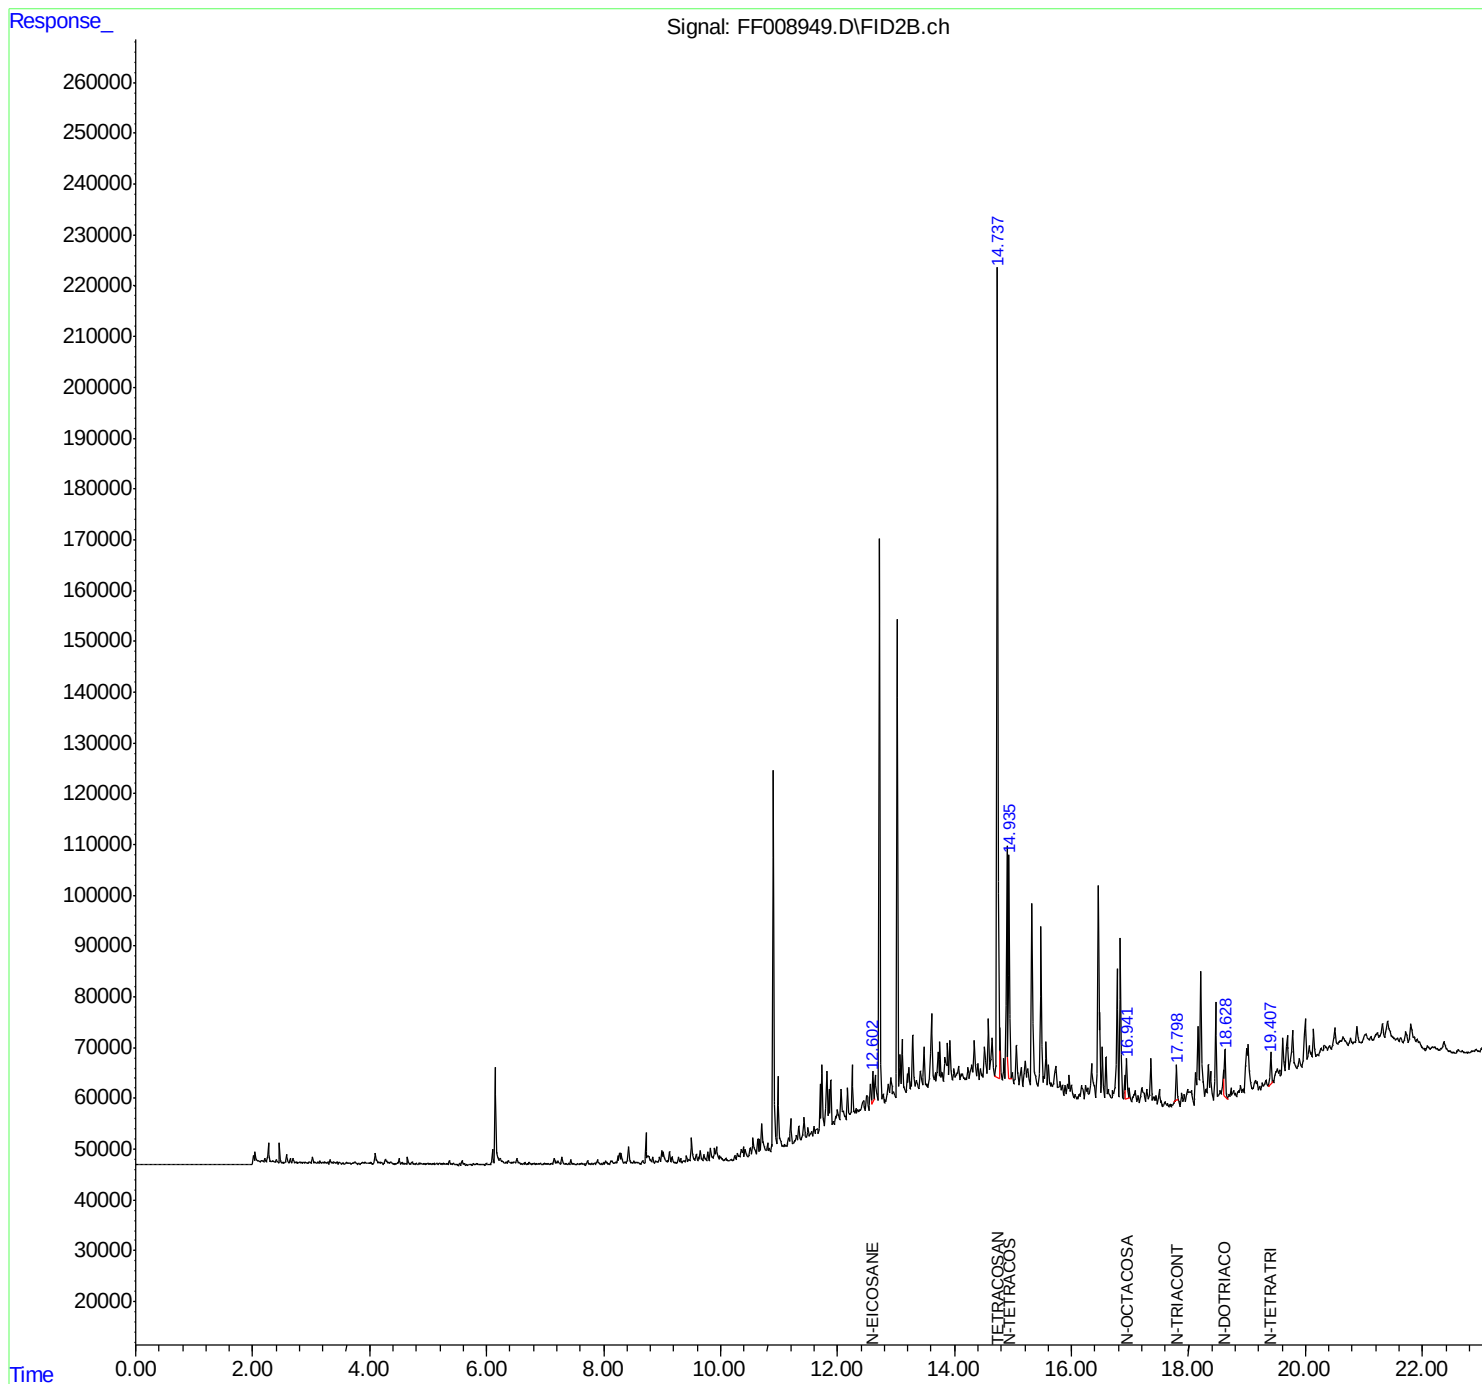


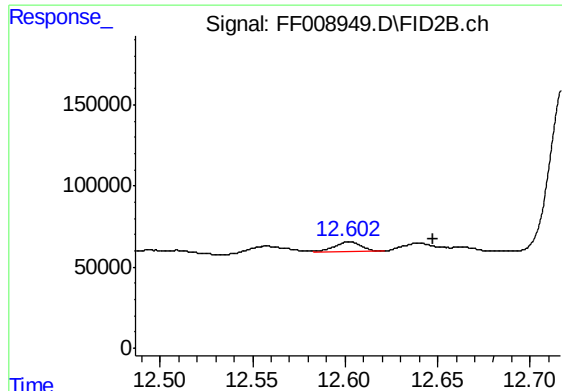

#7 N-EICOSANE


R.T.: 12.602 min
Delta R.T.: -0.045 min
Response: 65577
Conc: 0.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

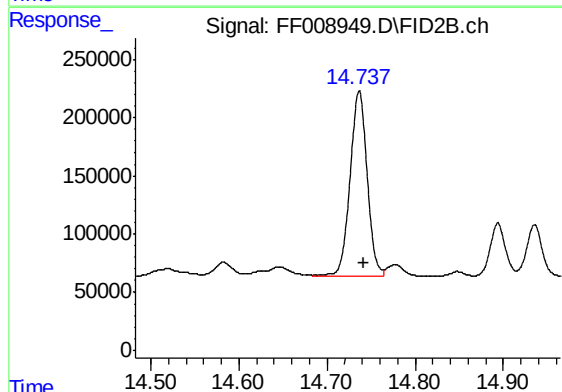


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.005 min
Response: 2137063
Conc: 17.84 ug/ml

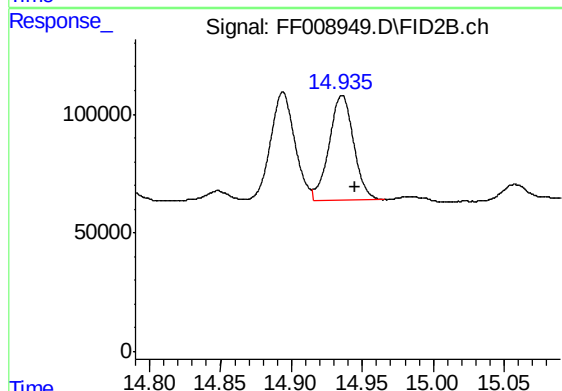


#10 N-TETRACOSANE

R.T.: 14.936 min
Delta R.T.: -0.009 min
Response: 531141
Conc: 3.84 ug/ml

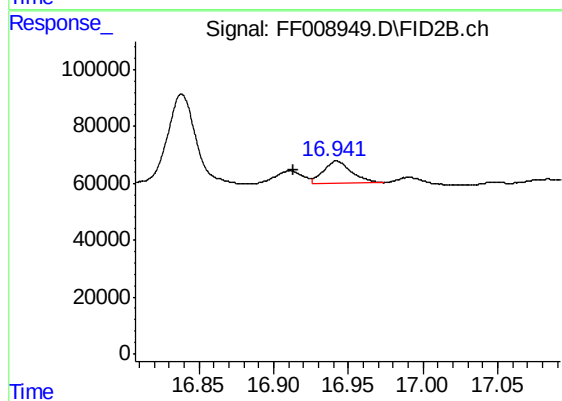

#12 N-OCTACOSANE


R.T.: 16.942 min
Delta R.T.: 0.029 min
Response: 102051
Conc: 0.76 ug/ml

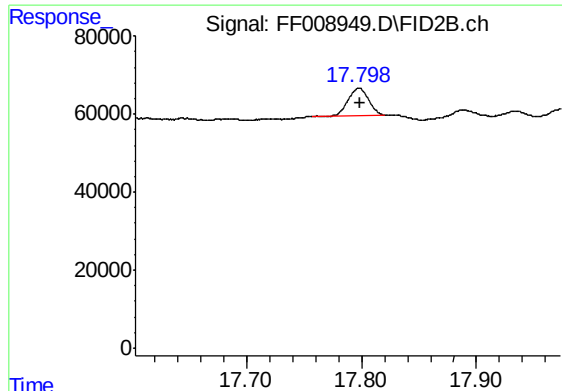

#13 N-TRIACONTANE


R.T.: 17.798 min
Delta R.T.: -0.001 min
Response: 86659
Conc: 0.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

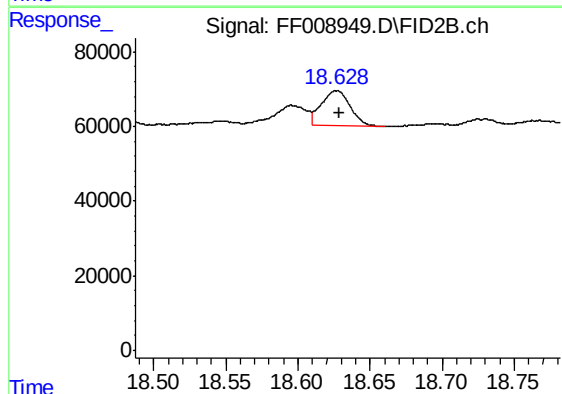

#14 N-DOTRIACONTANE

R.T.: 18.627 min
Delta R.T.: -0.002 min
Response: 128248
Conc: 1.04 ug/ml

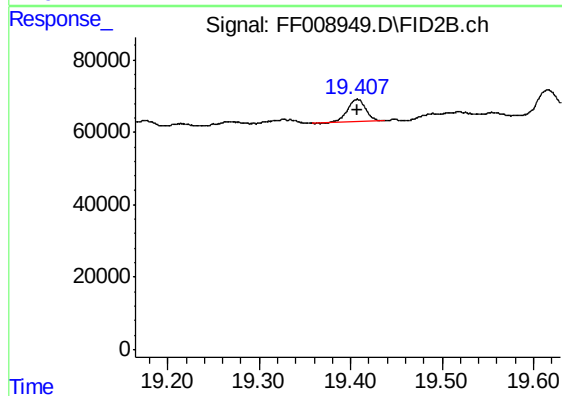

#15 N-TETRATRIACONTANE

R.T.: 19.407 min
Delta R.T.: 0.000 min
Response: 86080
Conc: 0.74 ug/ml