

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
 Data File : FF008951.D
 Signal(s) : FID2B.ch
 Acq On : 17 Aug 2021 17:16
 Operator : DD\AJ
 Sample : M3425-17
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 18 05:05:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	1981227	16.537 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.935	169199	1.222 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
Data File : FF08951.D
Signal(s) : FID2B.ch
Acq On : 17 Aug 2021 17:16
Operator : DD\AJ
Sample : M3425-17
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 05:05:30 2021
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

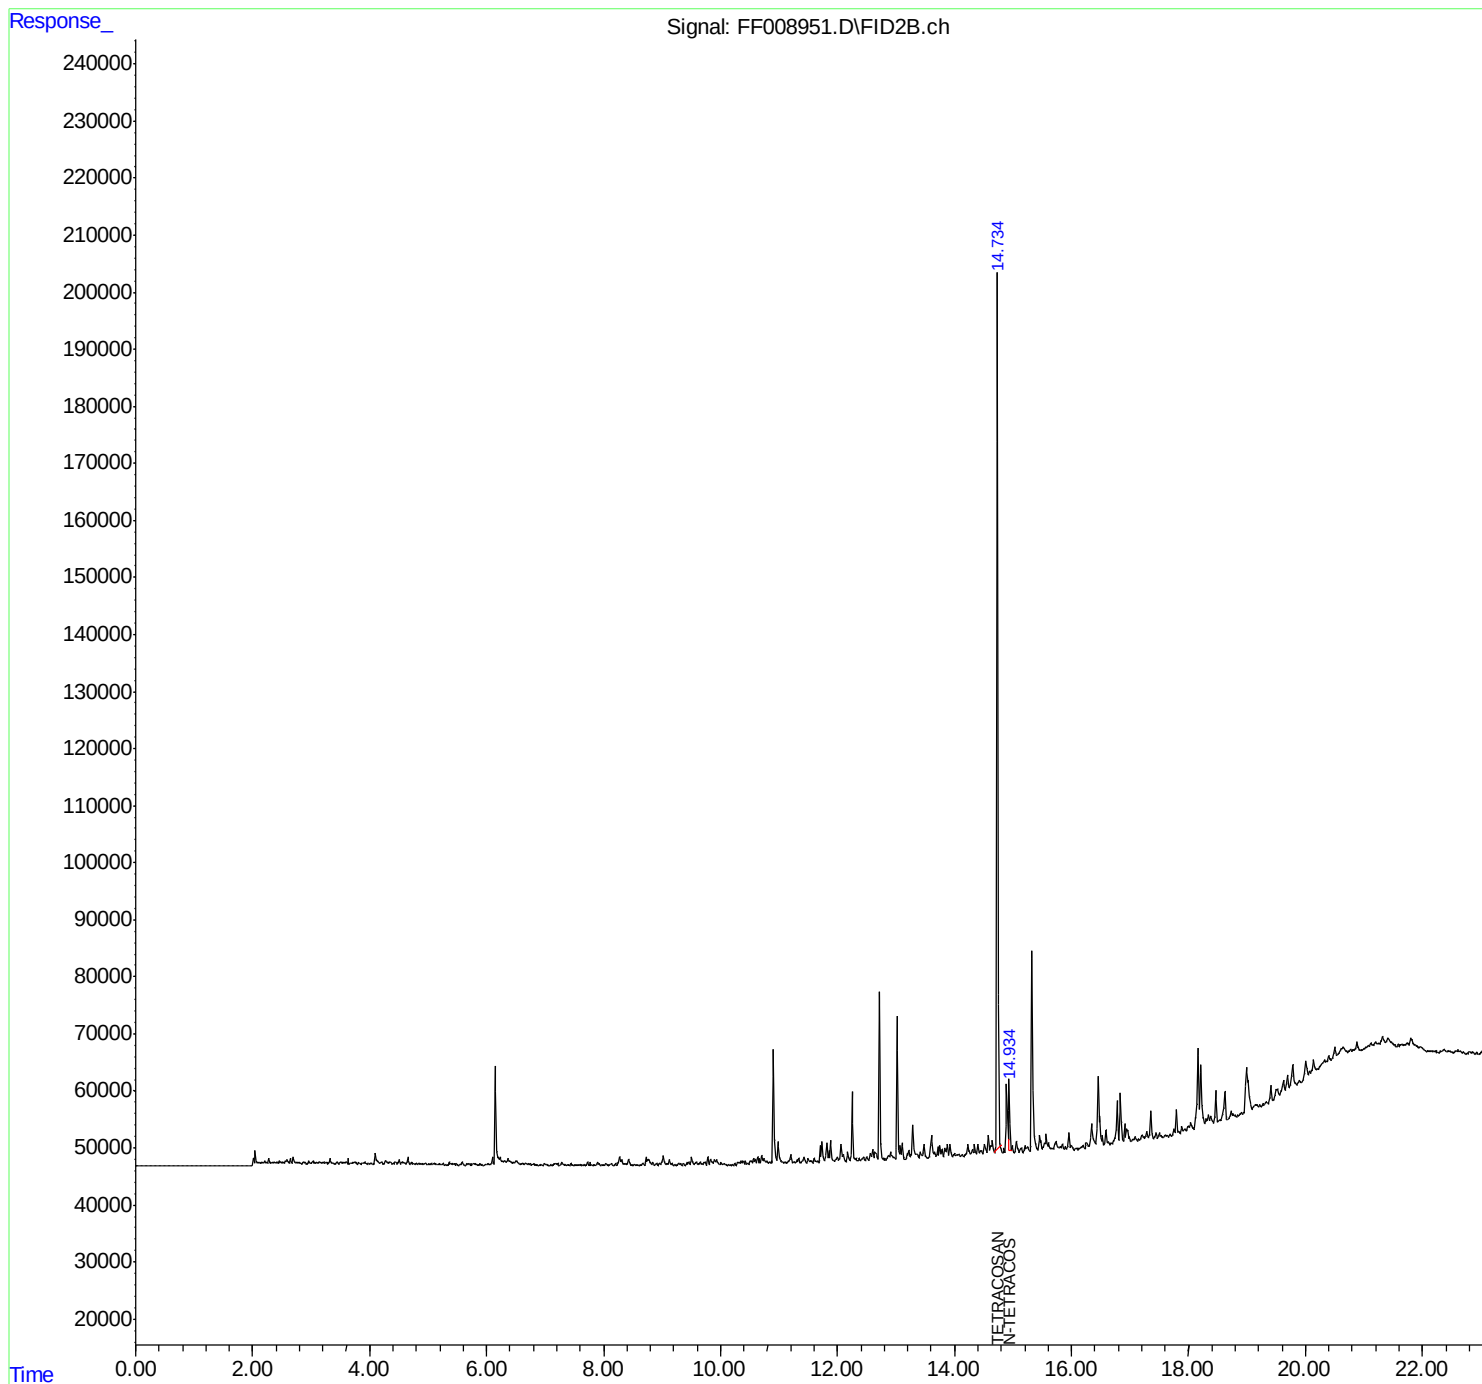


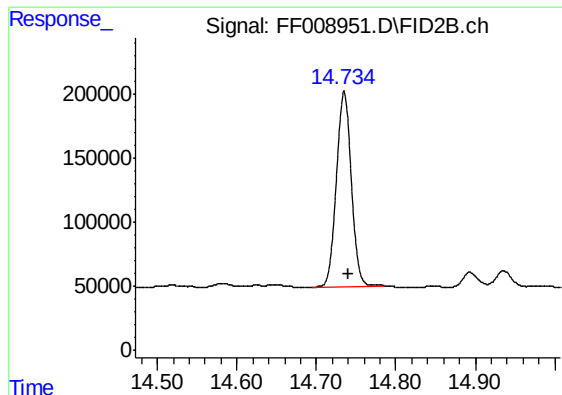

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.006 min
Response: 1981227
Conc: 16.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

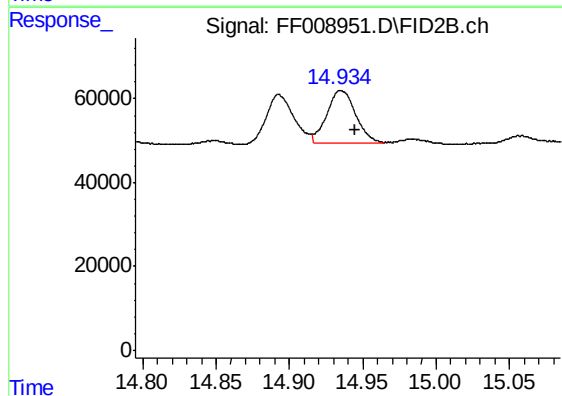

#10 N-TETRACOSANE

R.T.: 14.935 min
Delta R.T.: -0.010 min
Response: 169199
Conc: 1.22 ug/ml