

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
Data File : FF008953.D
Signal(s) : FID2B.ch
Acq On : 17 Aug 2021 18:19
Operator : DD\AJ
Sample : M3424-11 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 05:05:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	187707	1.567 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.936	96719	0.699 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081721\
Data File : FF08953.D
Signal(s) : FID2B.ch
Acq On : 17 Aug 2021 18:19
Operator : DD\AJ
Sample : M3424-11 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 05:05:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

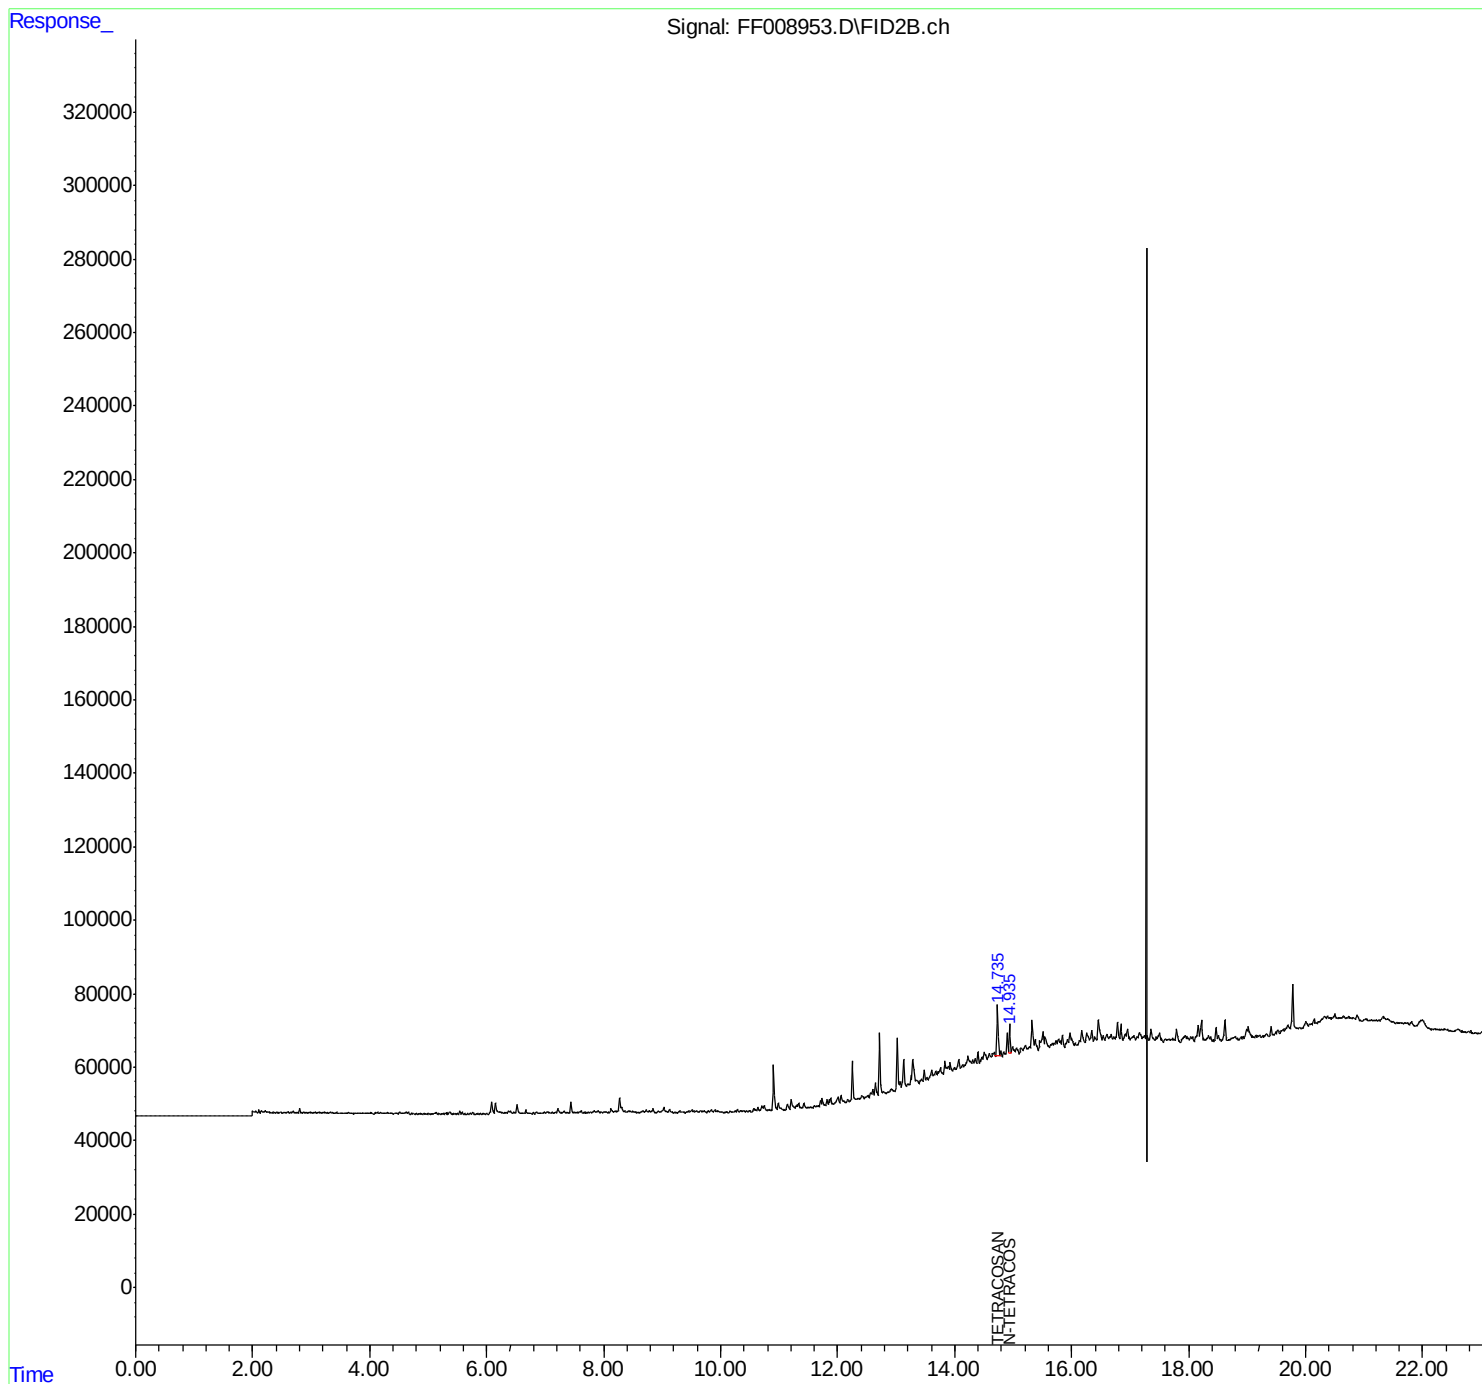


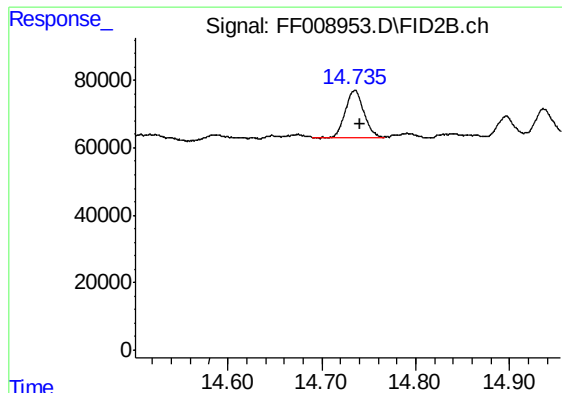

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.006 min
Response: 187707
Conc: 1.57 ug/ml

Instrument :
ECD_S
ClientSampleId :

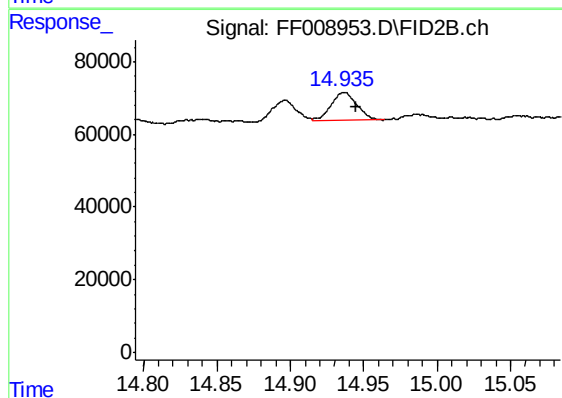

#10 N-TETRACOSANE

R.T.: 14.936 min
Delta R.T.: -0.009 min
Response: 96719
Conc: 0.70 ug/ml