

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 16:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:24:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	8289650	23698495	20.041	23.341
28)	SA Decachlor...	10.409	11.496	11287013	19862376	19.640	20.472
Target Compounds							
3)	MA gamma-BHC...	0.000	6.543	0	278161	N.D.	0.214 #
4)	MA Heptachlor	6.158f	7.212	737155	989812	1.255	0.737 #
6)	B beta-BHC	6.158	6.819f	737155	11818049	2.615	18.242 #
14)	MA Endrin	8.088f	0.000	433032	0	0.899	N.D. #
15)	B Endosulfa...	0.000	9.216	0	1320413	N.D.	1.440 #
21)	B Endrin ke...	0.000	10.089f	0	1163693	N.D.	1.143 #
22)	Mirex	0.000	10.555f	0	725242	N.D.	0.917 #
23)	Chlordane-1	0.000	6.962	0	1004440	N.D.	23.819 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 16:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:24:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

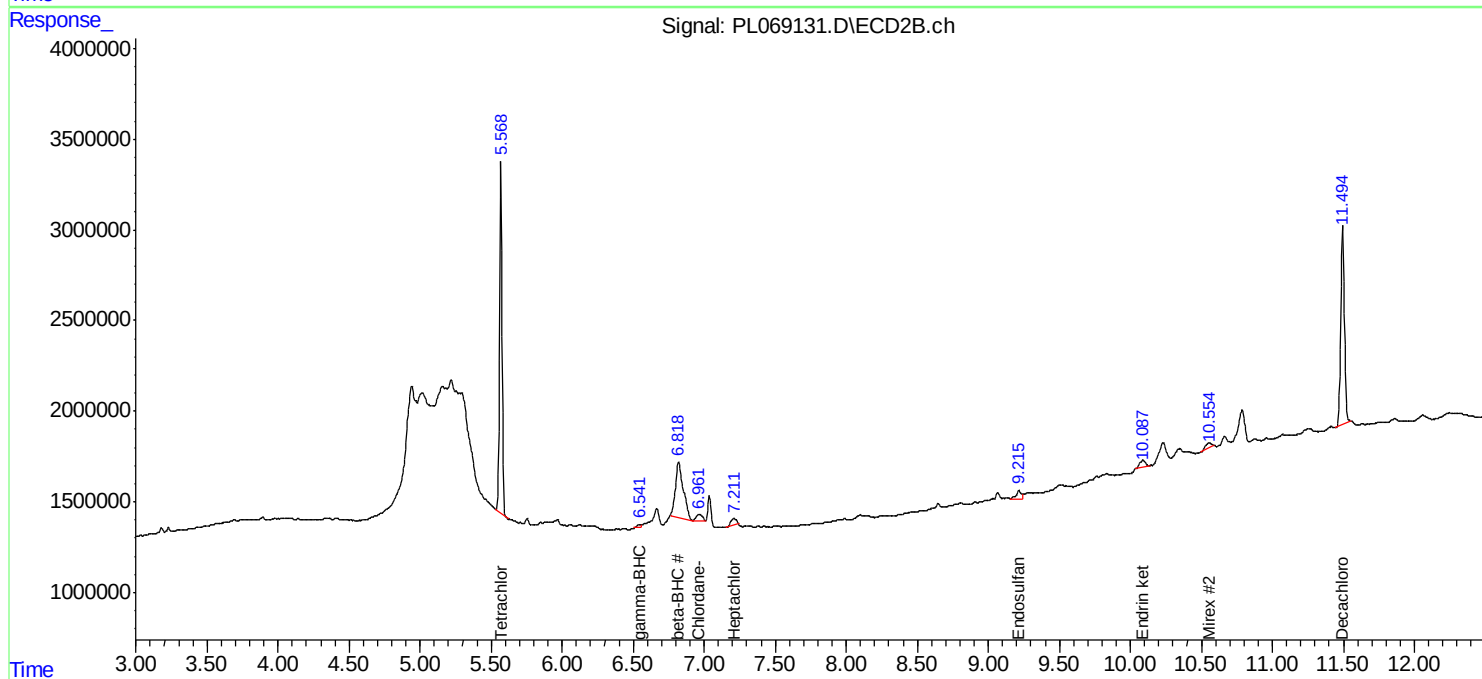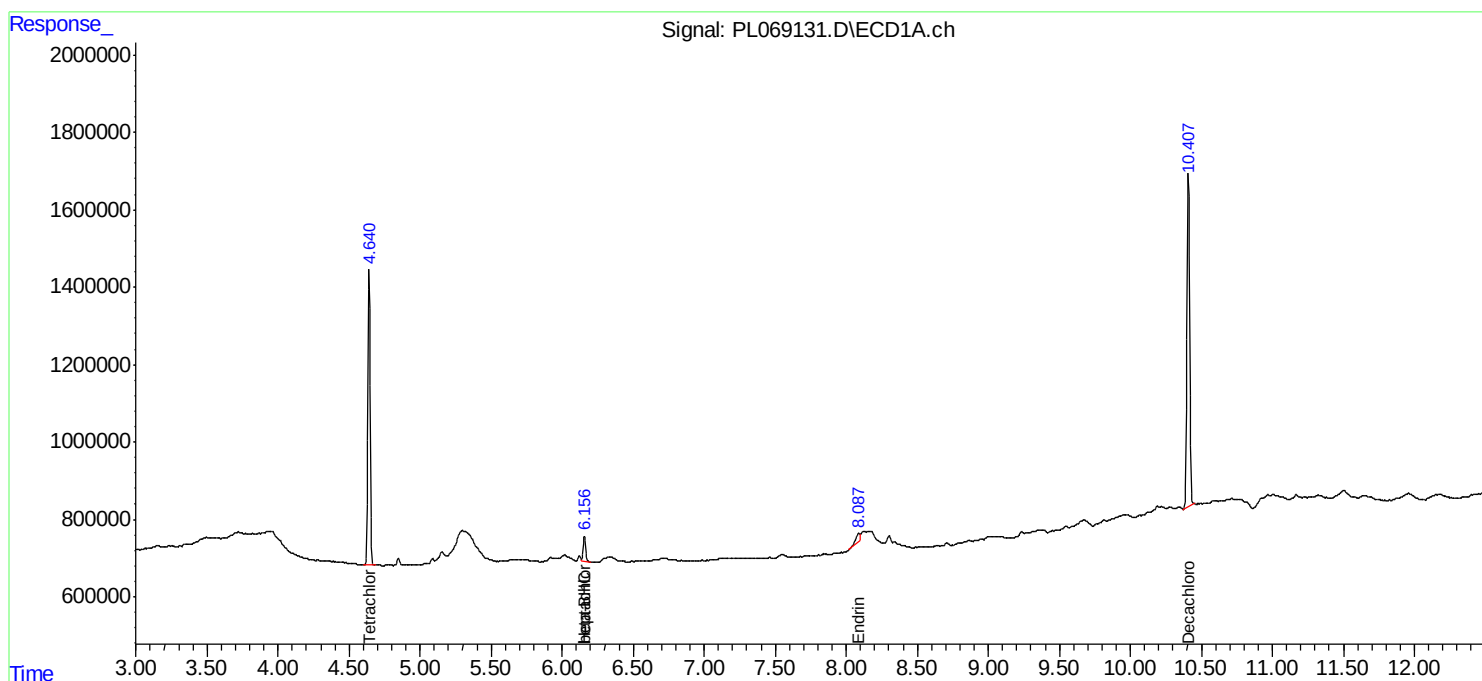


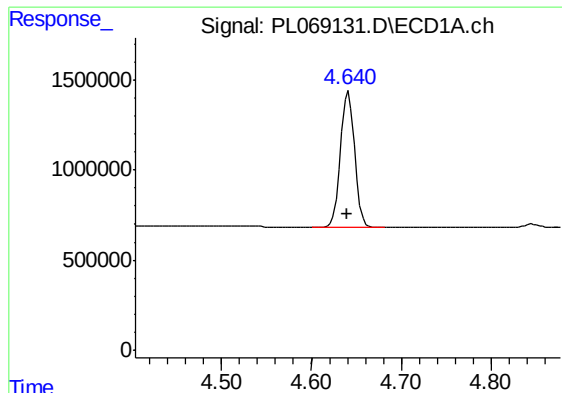

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.002 min
Response: 8289650
Conc: 20.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

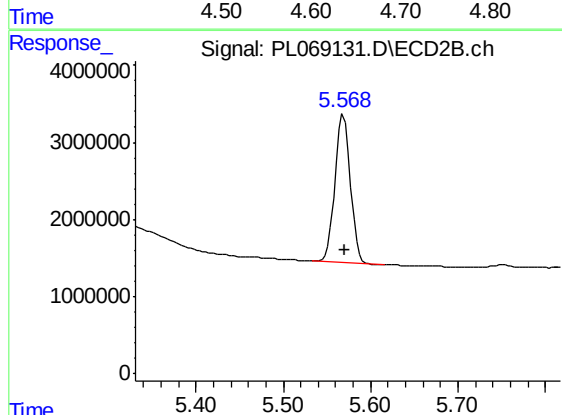


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 23698495
Conc: 23.34 ng/ml

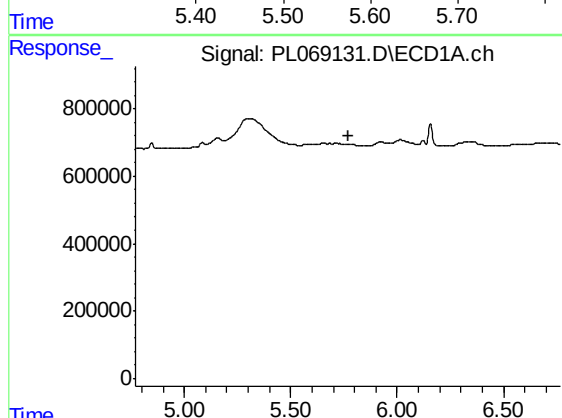


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.770 min
Response: 0
Conc: N.D.

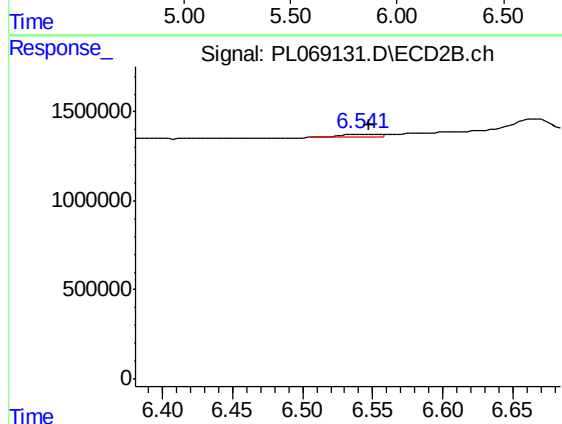

#3 gamma-BHC (Lindane)


R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 278161
Conc: 0.21 ng/ml

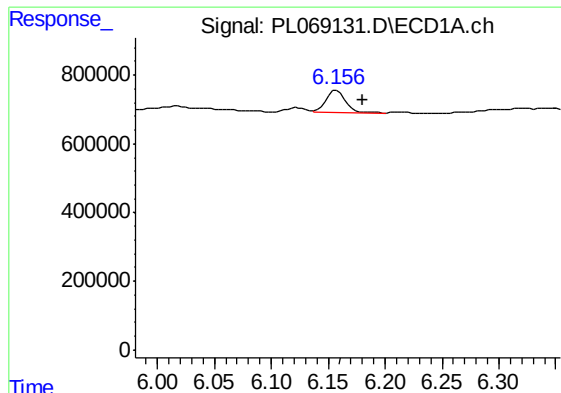

#4 Heptachlor


R.T.: 6.158 min
Delta R.T.: -0.023 min
Response: 737155
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

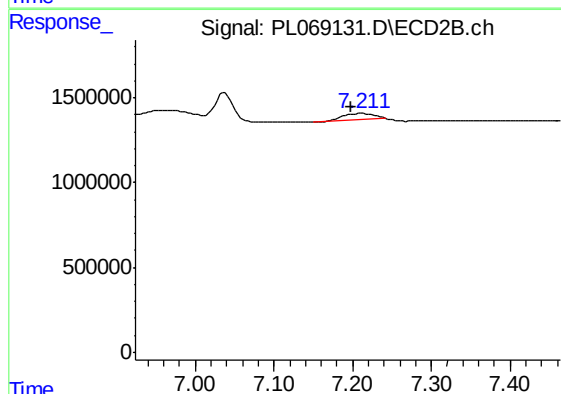


#4 Heptachlor

R.T.: 7.212 min
Delta R.T.: 0.015 min
Response: 989812
Conc: 0.74 ng/ml

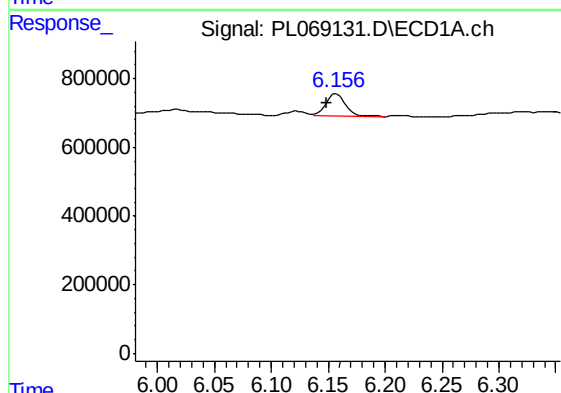


#6 beta-BHC

R.T.: 6.158 min
Delta R.T.: 0.009 min
Response: 737155
Conc: 2.61 ng/ml

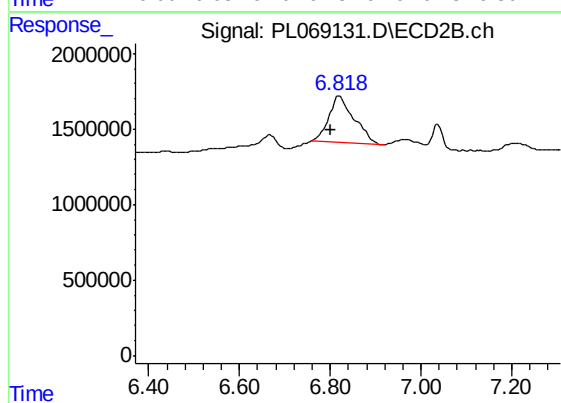

#6 beta-BHC


R.T.: 6.819 min
Delta R.T.: 0.019 min
Response: 11818049
Conc: 18.24 ng/ml

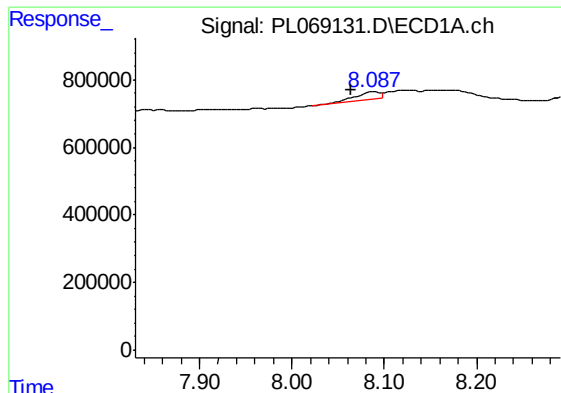

#14 Endrin


R.T.: 8.088 min
Delta R.T.: 0.023 min
Response: 433032
Conc: 0.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

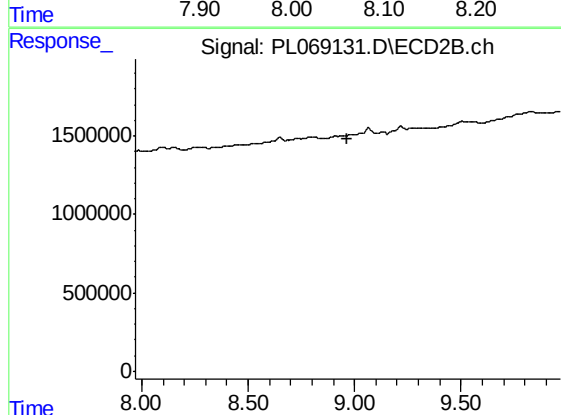


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

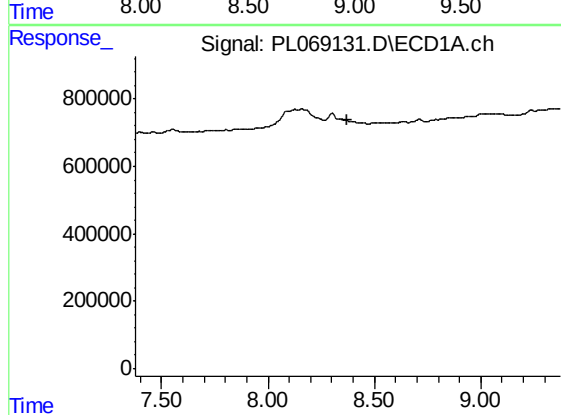


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

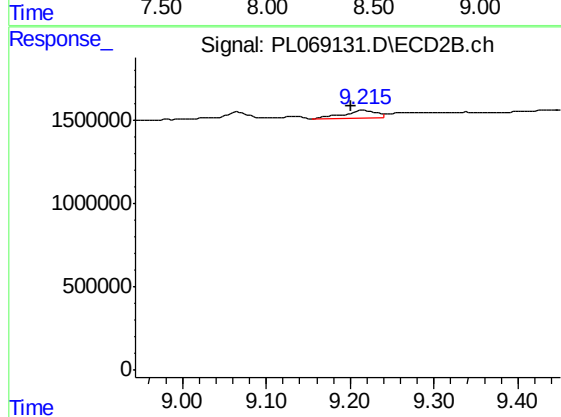

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.015 min
Response: 1320413
Conc: 1.44 ng/ml

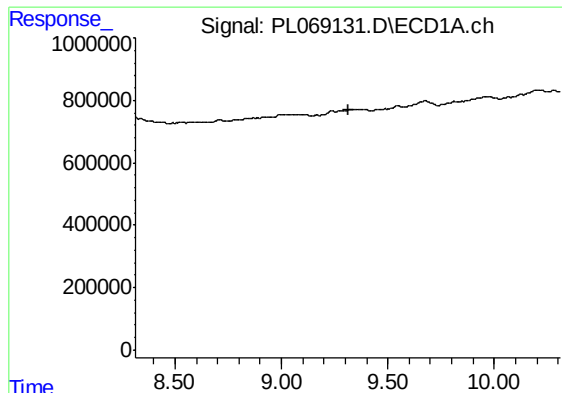

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

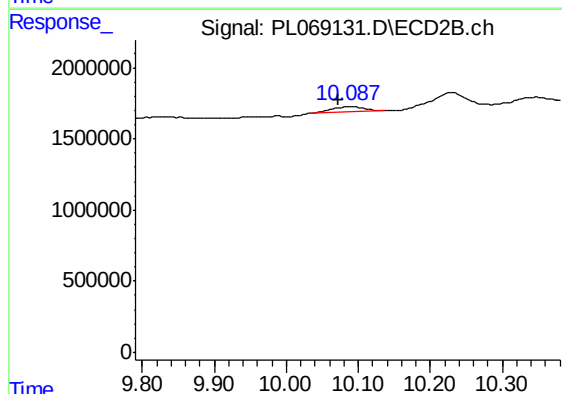


#21 Endrin ketone

R.T.: 10.089 min
Delta R.T.: 0.016 min
Response: 1163693
Conc: 1.14 ng/ml

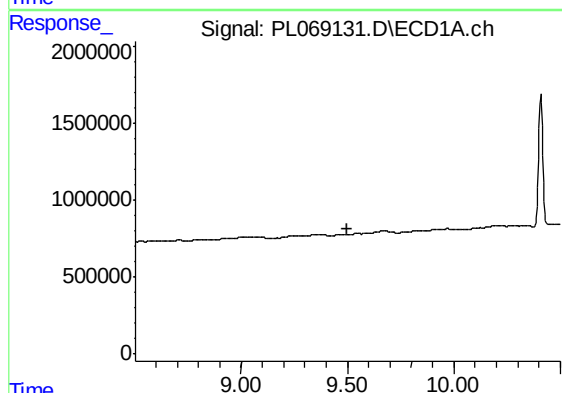


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

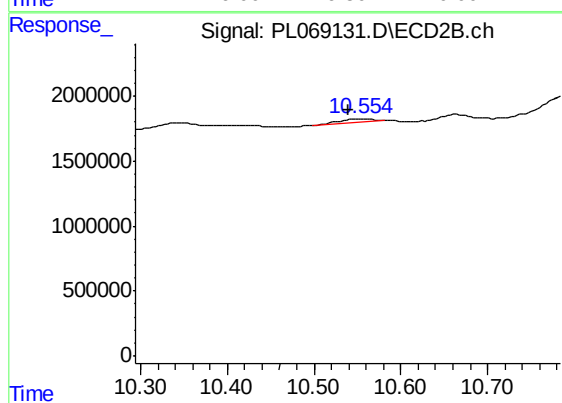

#22 Mirex


R.T.: 10.555 min
Delta R.T.: 0.015 min
Response: 725242
Conc: 0.92 ng/ml

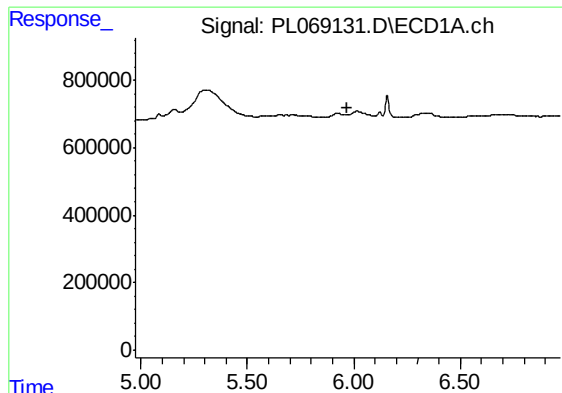

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

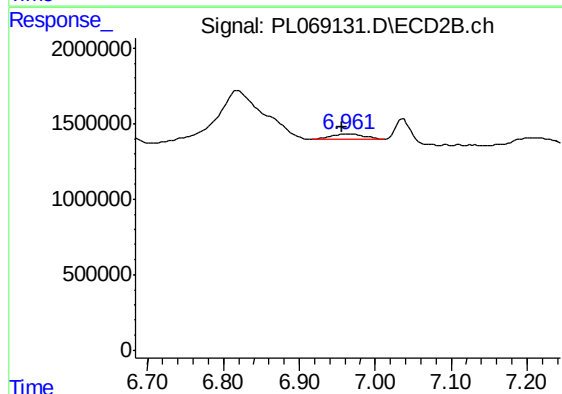


#23 Chlordane-1

R.T.: 6.962 min
Delta R.T.: 0.007 min
Response: 1004440
Conc: 23.82 ng/ml

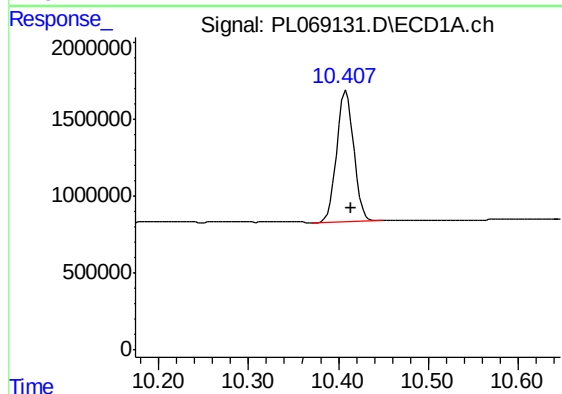

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.005 min
Response: 11287013
Conc: 19.64 ng/ml

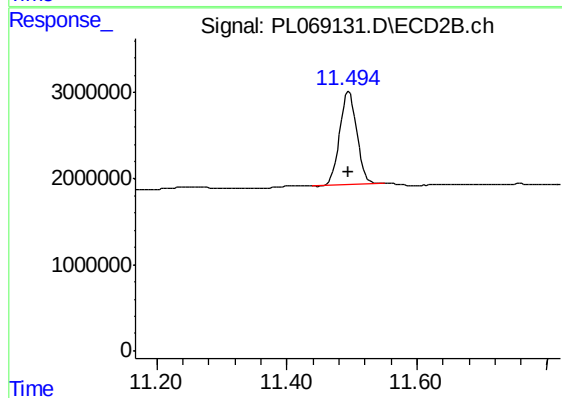

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.000 min
Response: 19862376
Conc: 20.47 ng/ml