

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 00:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:33:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.567	8646377	25349494	20.903	24.967
28)	SA Decachlor...	10.398f	11.485	11805078	22252276	20.541	22.935
Target Compounds							
2)	A alpha-BHC	5.369f	0.000	961438	0	1.738	N.D. #
3)	MA gamma-BHC...	5.762	0.000	640469	0	1.180	N.D. #
6)	B beta-BHC	6.148	0.000	609982	0	2.164	N.D. #
15)	B Endosulfa...	0.000	9.212	0	1047332	N.D.	1.142 #
23)	Chlordane-1	0.000	6.967	0	548253	N.D.	13.001 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 00:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:33:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

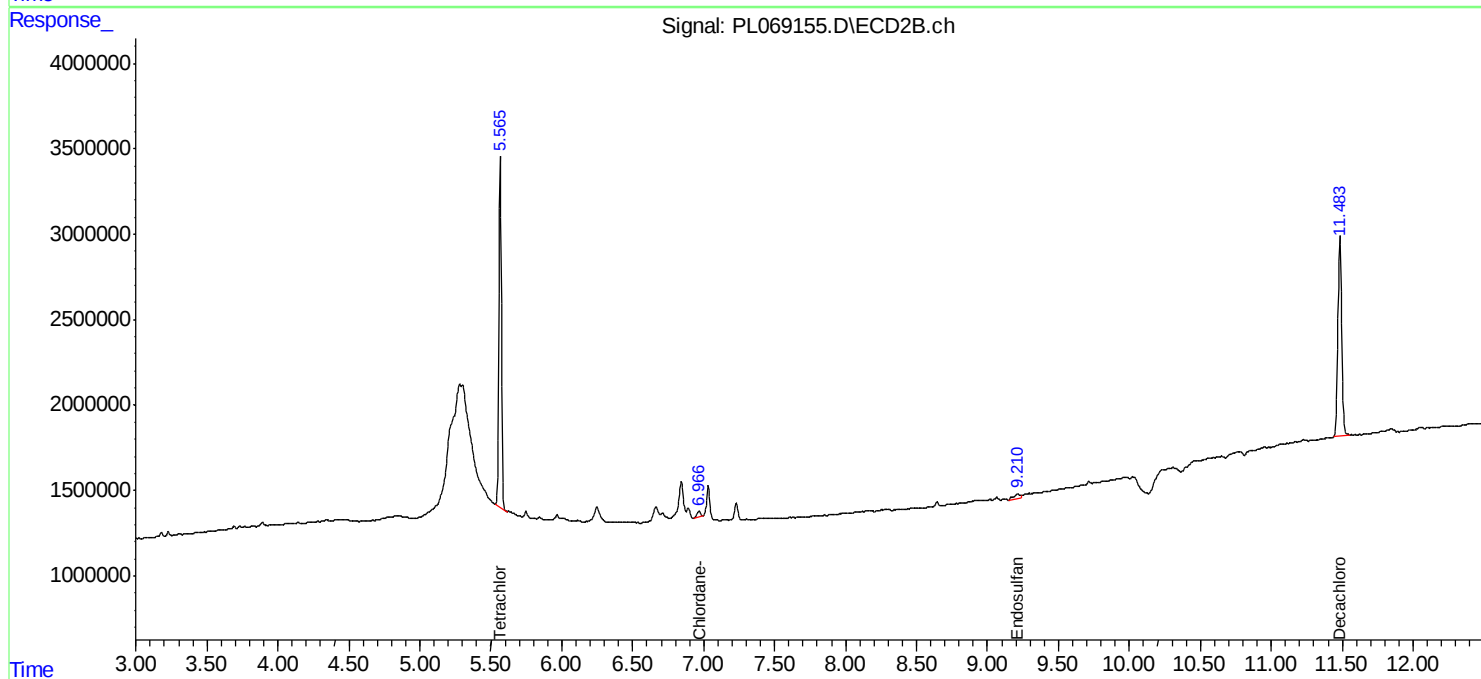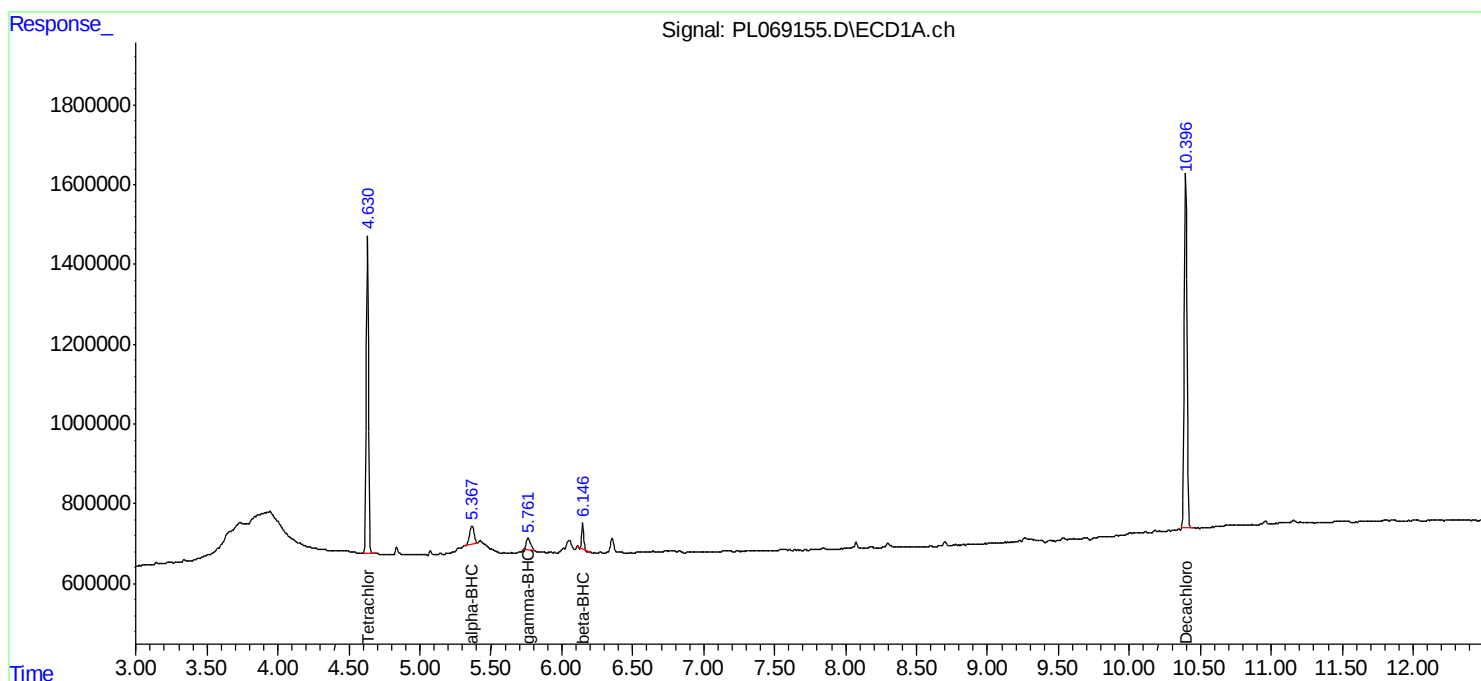


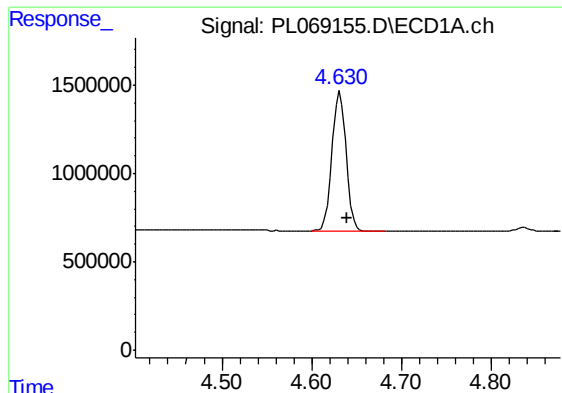

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.008 min
Response: 8646377
Conc: 20.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

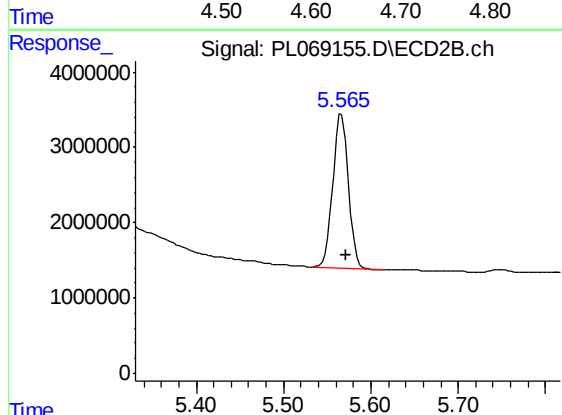


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 25349494
Conc: 24.97 ng/ml

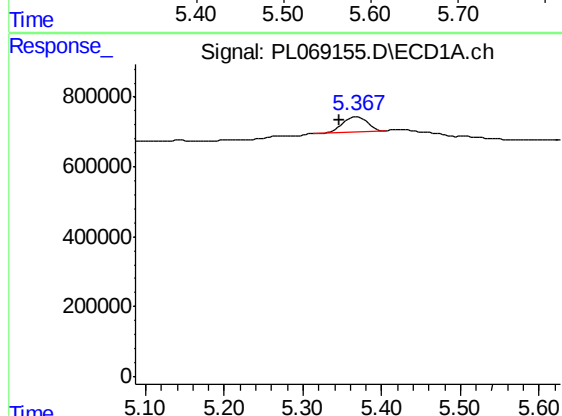


#2 alpha-BHC

R.T.: 5.369 min
Delta R.T.: 0.022 min
Response: 961438
Conc: 1.74 ng/ml

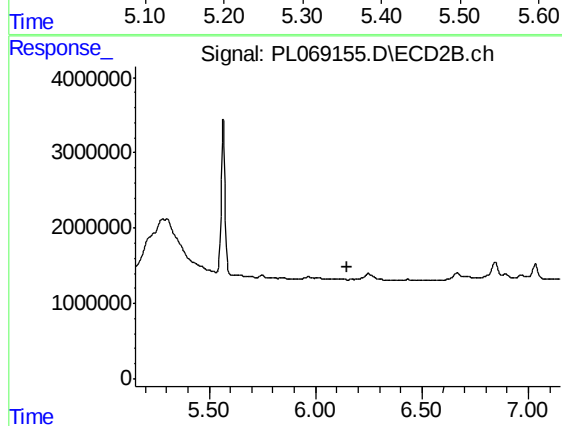

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

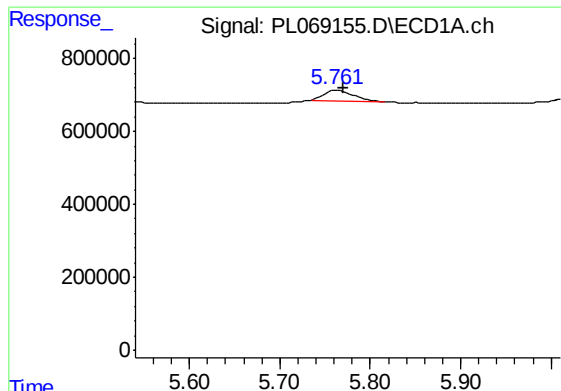

#3 gamma-BHC (Lindane)


R.T.: 5.762 min
Delta R.T.: -0.008 min
Response: 640469
Conc: 1.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

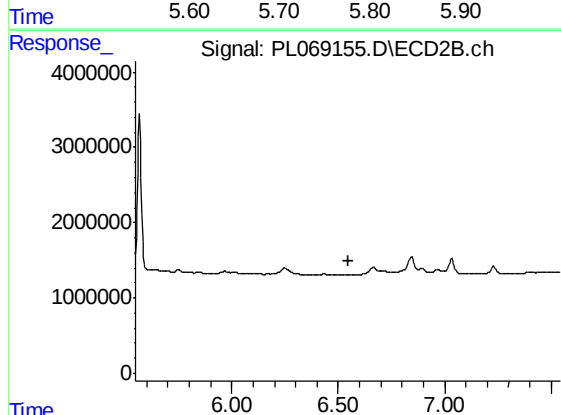


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.547 min
Response: 0
Conc: N.D.

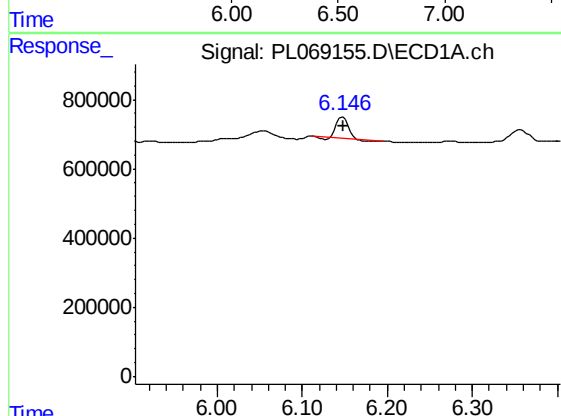


#6 beta-BHC

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 609982
Conc: 2.16 ng/ml

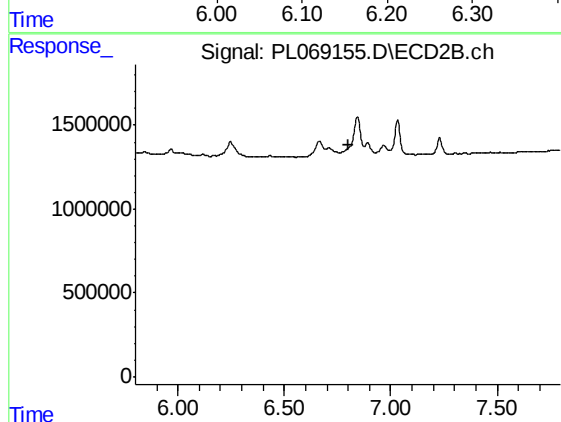

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

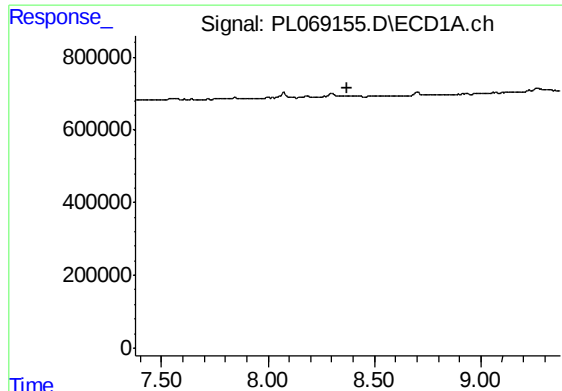

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

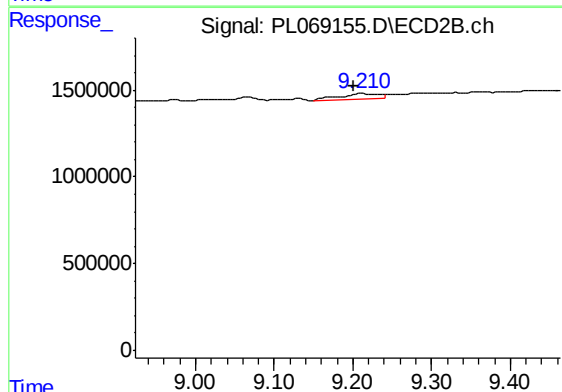


#15 Endosulfan II

R.T.: 9.212 min
Delta R.T.: 0.010 min
Response: 1047332
Conc: 1.14 ng/ml

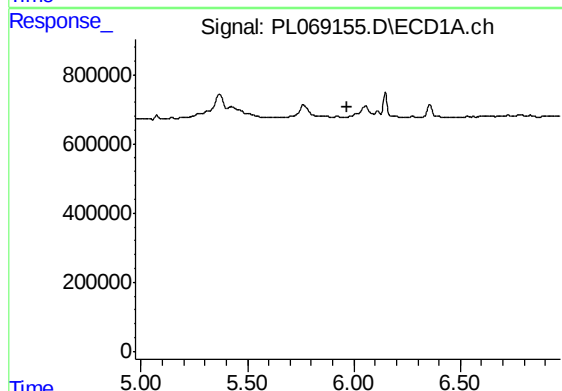


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

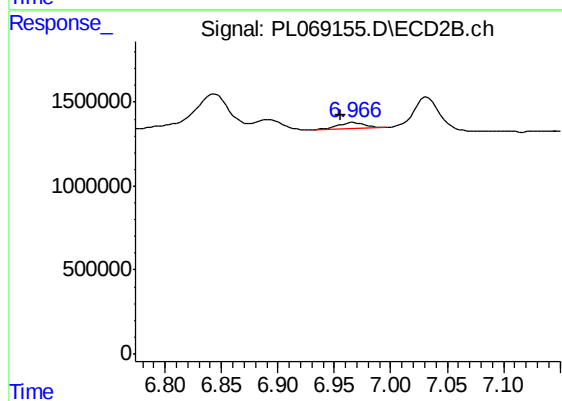

#23 Chlordane-1


R.T.: 6.967 min
Delta R.T.: 0.012 min
Response: 548253
Conc: 13.00 ng/ml

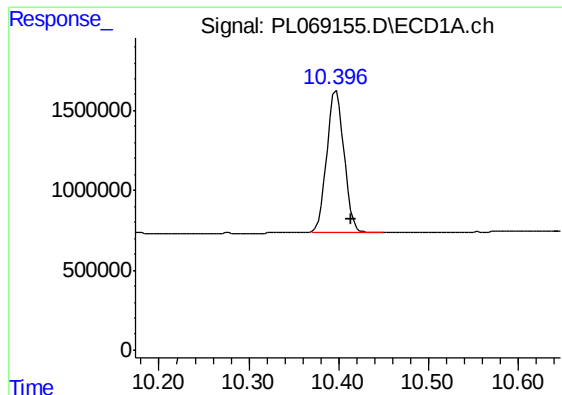

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.016 min
Response: 11805078
Conc: 20.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

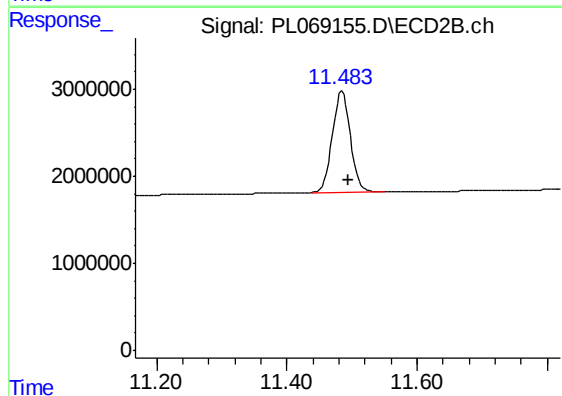

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.010 min
Response: 22252276
Conc: 22.93 ng/ml