

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081721\
 Data File : PS016453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 11:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:53:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.185	6.765	602.2E6	251.1E6	409.377	481.311
Target Compounds							
8) T	DICHLORPROP	0.000	7.578	0	4785192	N.D.	8.833
12) T	2,4,5-T	0.000	9.013	0	2749420	N.D.	<MDL
15) T	Picloram	10.989	10.825	124.5E6	62547084	12.473	15.533
16) T	DCPA	0.000	10.765	0	2589605	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081721\
Data File : PS016453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 11:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:53:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

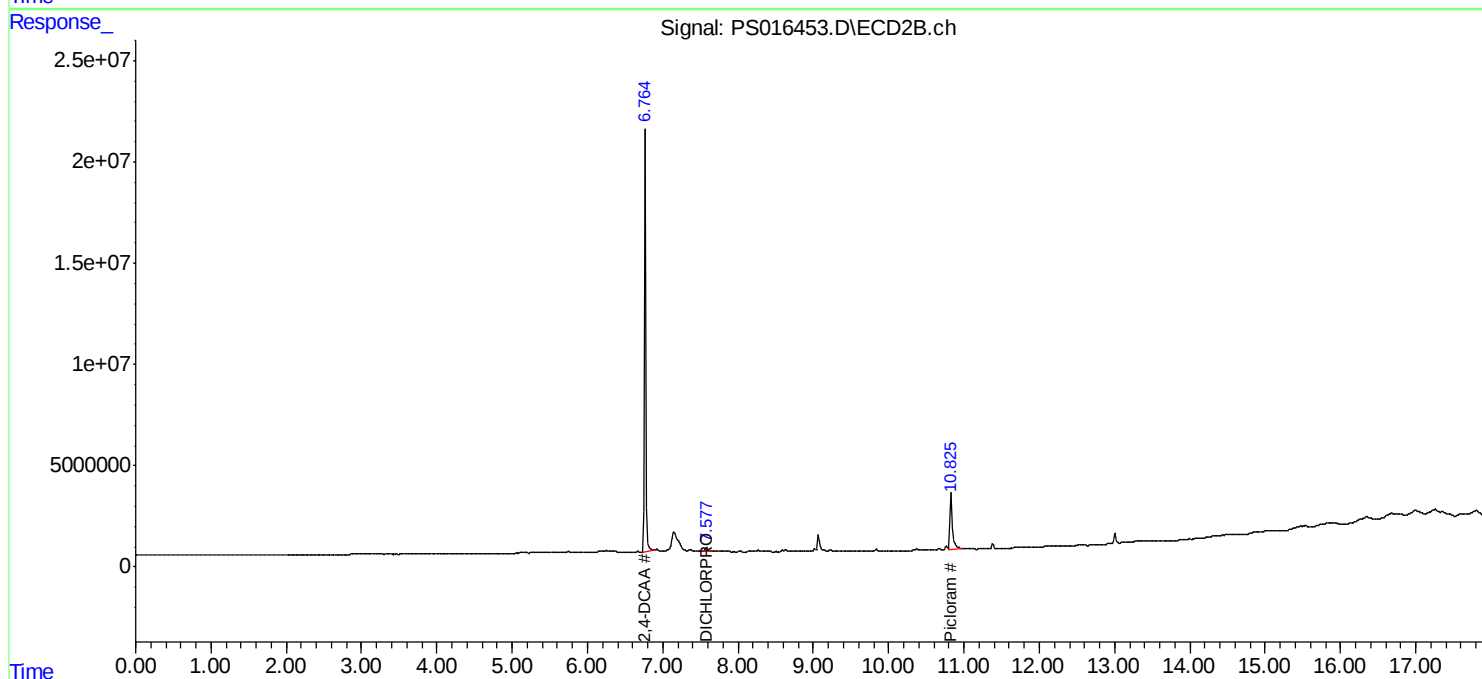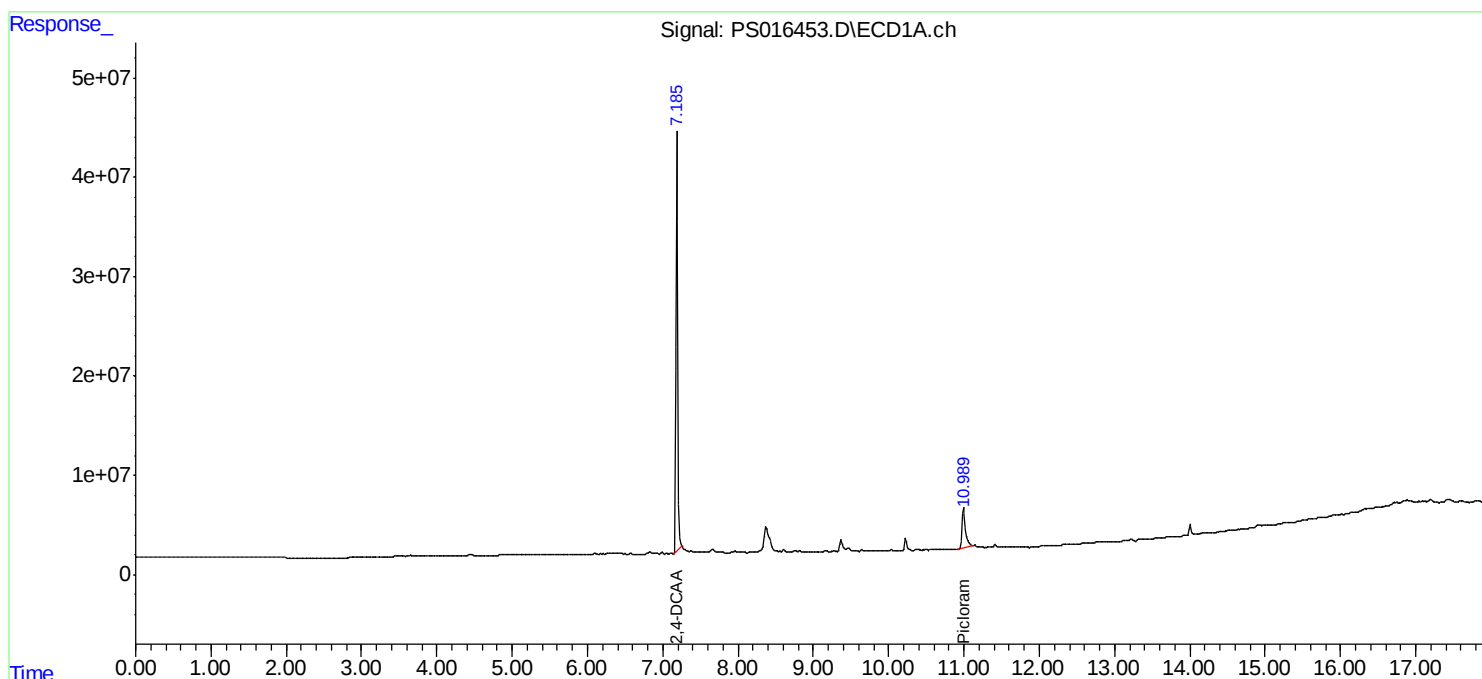


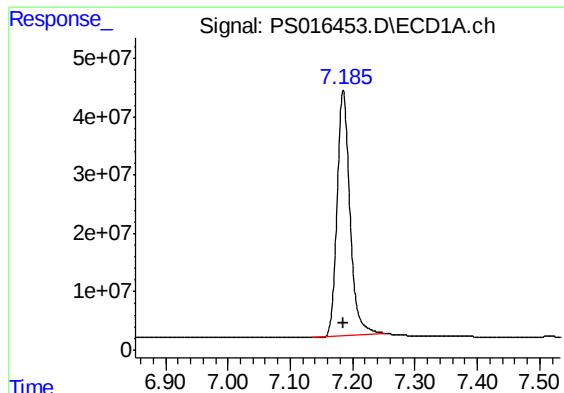

#4 2,4-DCAA


R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 602237779
Conc: 409.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

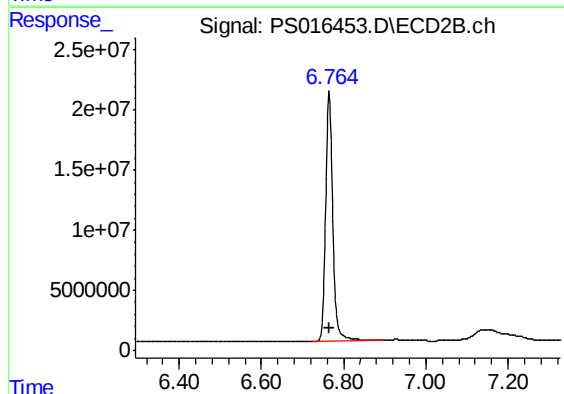


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.001 min
Response: 251063515
Conc: 481.31 ng/ml

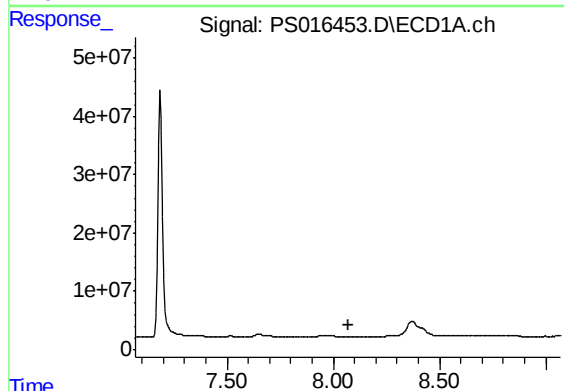


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.069 min
Response: 0
Conc: N.D.

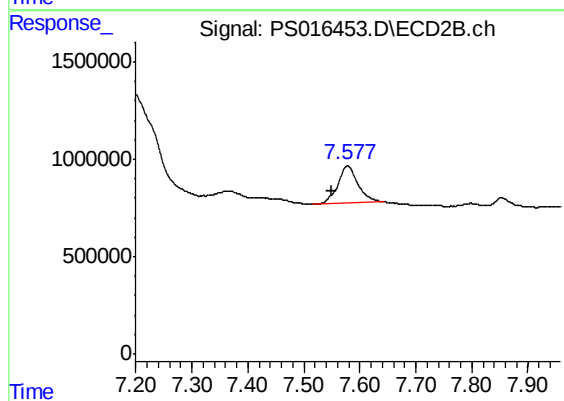

#8 DICHLORPROP


R.T.: 7.578 min
Delta R.T.: 0.028 min
Response: 4785192
Conc: 8.83 ng/ml

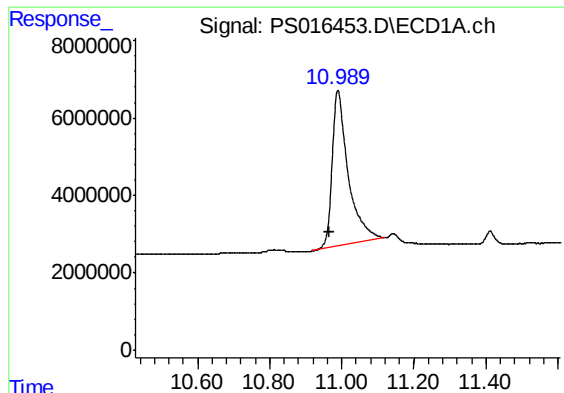

#15 Picloram

R.T.: 10.989 min
Delta R.T.: 0.022 min
Response: 124491691
Conc: 12.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

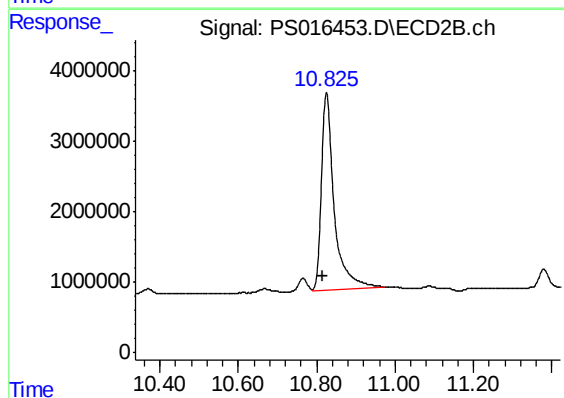

#15 Picloram

R.T.: 10.825 min
Delta R.T.: 0.009 min
Response: 62547084
Conc: 15.53 ng/ml