

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081723\
 Data File : PS024099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 08:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 21:35:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.385	6.850f	4172917	1011945	2.107	1.504 #
Target Compounds							
2) T	3,5-DICHL...	5.727	5.961	486540	373068	<MDL	<MDL #
3) T	4-Nitroph...	6.189	0.000	5603549	0	5.063	N.D. #
5) T	DICAMBA	6.507	0.000	298985	0	<MDL	N.D. #
6) T	MCP	6.720f	0.000	919014	0	<MDL	N.D. #
7) T	MCPA	6.785	0.000	3580145	0	<MDL	N.D. #
8) T	DICHLORPROP	7.109	0.000	3202072	0	1.423	N.D. #
9) T	2,4-D	7.283	0.000	10181424	0	4.109	N.D. #
10) T	Pentachlo...	7.510	0.000	350990	0	<MDL	N.D. #
12) T	2,4,5-T	8.309	9.013	259027	678623	<MDL	<MDL #
13) T	2,4-DB	8.814	0.000	250412	0	<MDL	N.D. #
14) T	DINOSEB	9.868	0.000	275677	0	<MDL	N.D. #
15) T	Picloram	9.671	0.000	133163	0	<MDL	N.D. #
16) T	DCPA	10.124	0.000	506524	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081723\
Data File : PS024099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 08:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 21:35:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

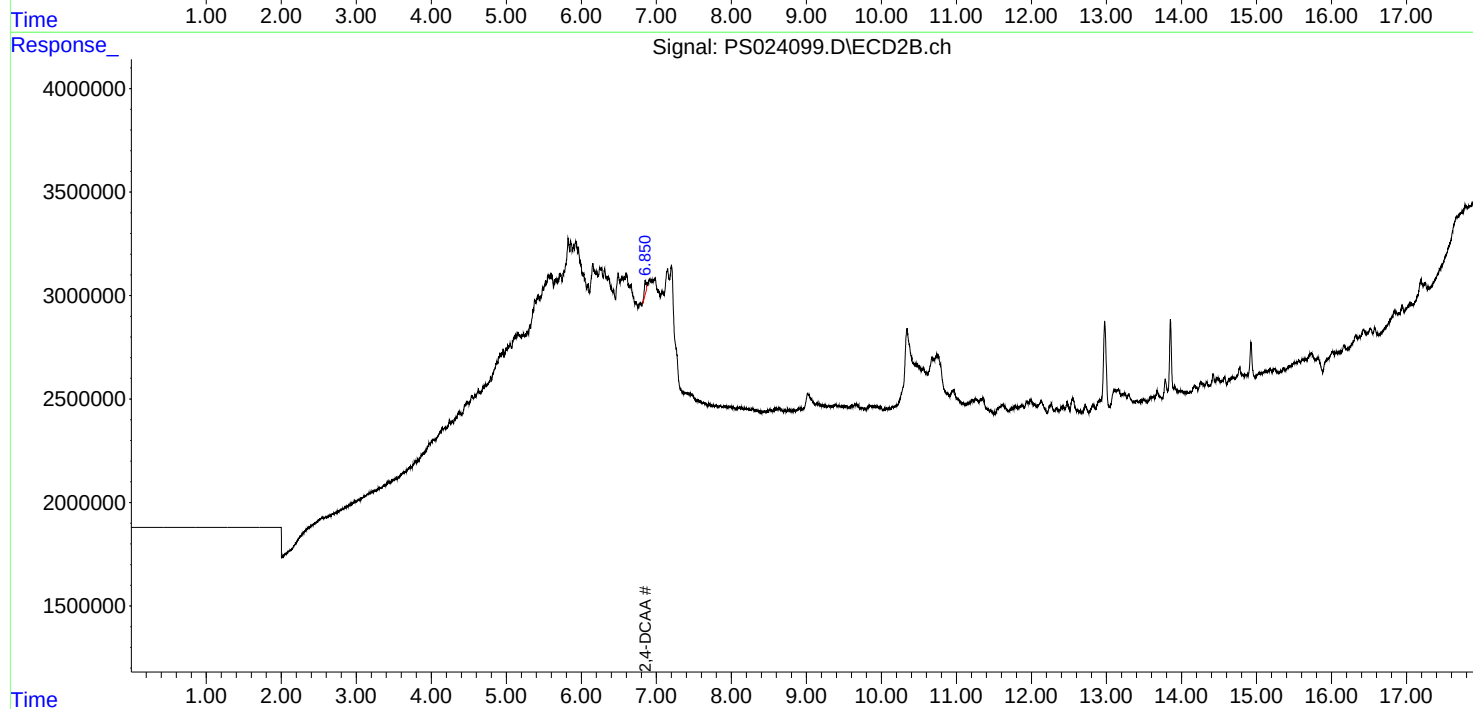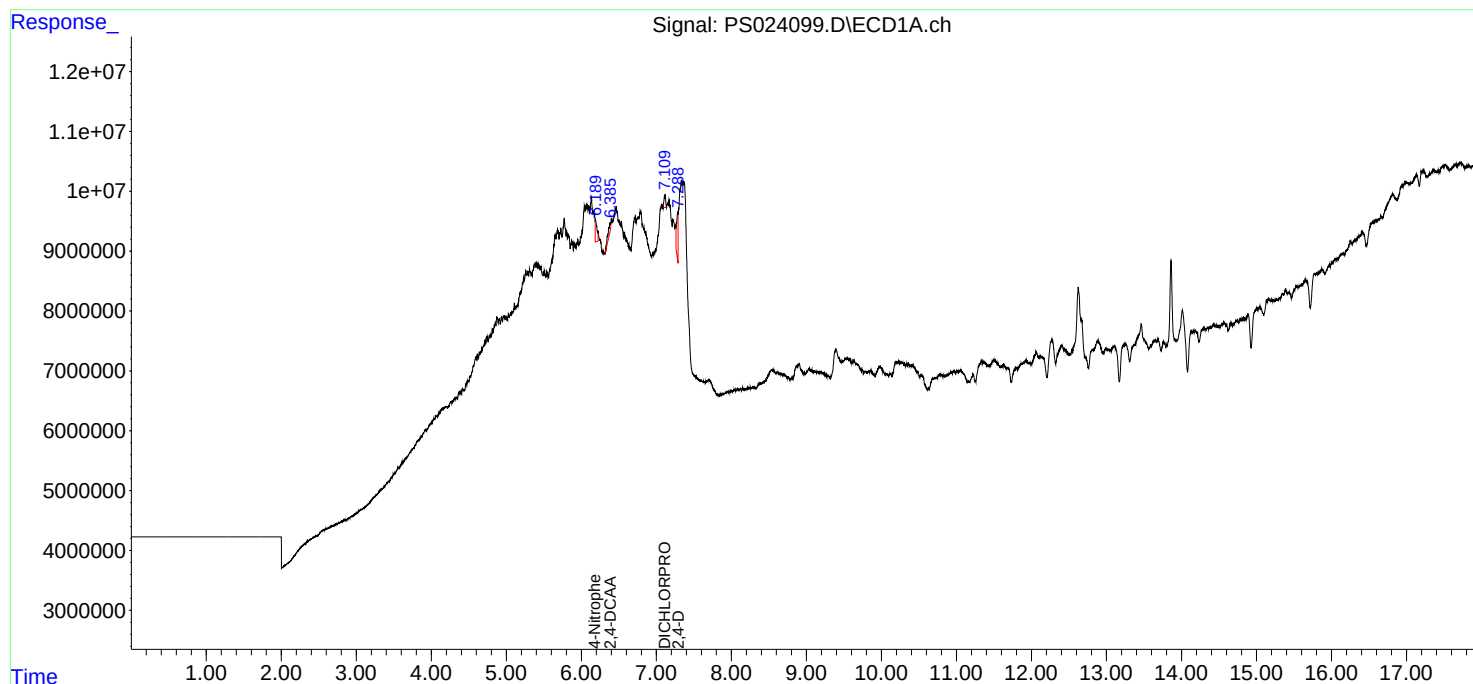


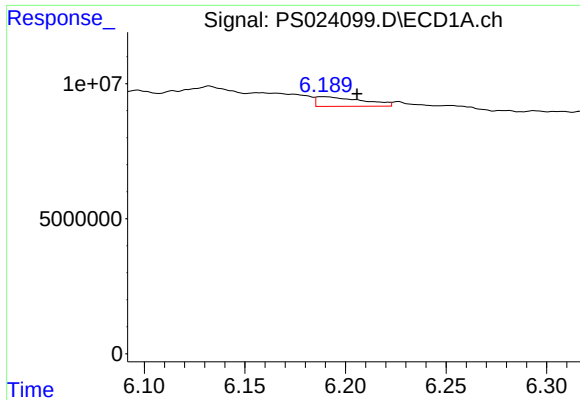

#3 4-Nitrophenol


R.T.: 6.189 min
Delta R.T.: -0.017 min
Response: 5603549
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

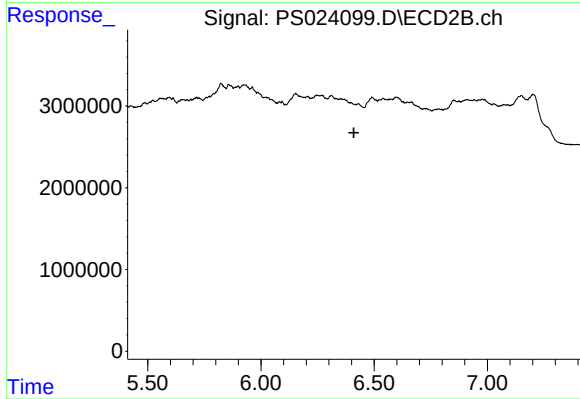


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

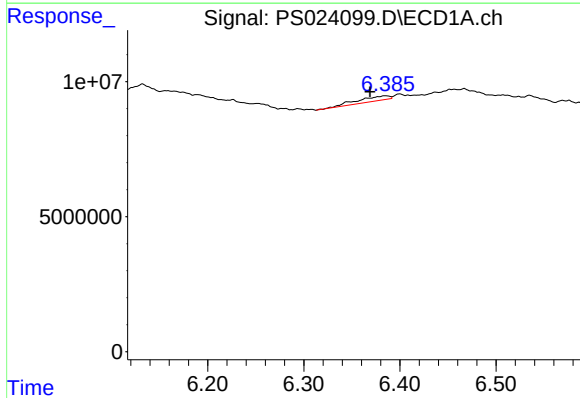


#4 2,4-DCAA

R.T.: 6.385 min
Delta R.T.: 0.016 min
Response: 4172917
Conc: 2.11 ng/ml

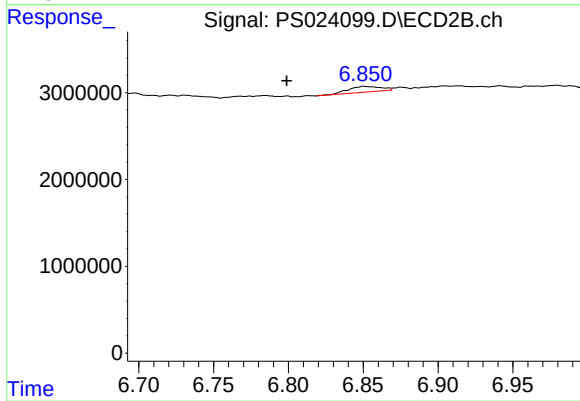

#4 2,4-DCAA


R.T.: 6.850 min
Delta R.T.: 0.051 min
Response: 1011945
Conc: 1.50 ng/ml

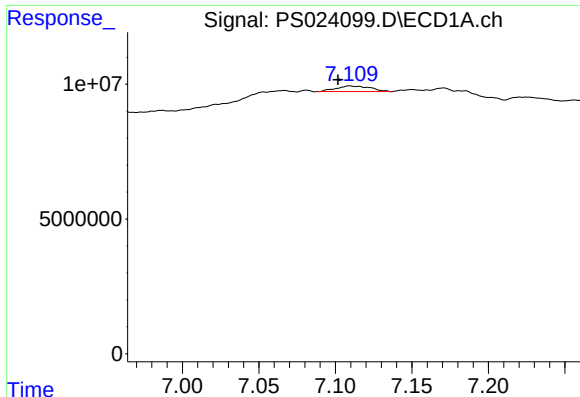

#8 DICHLORPROP


R.T.: 7.109 min
Delta R.T.: 0.008 min
Response: 3202072
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

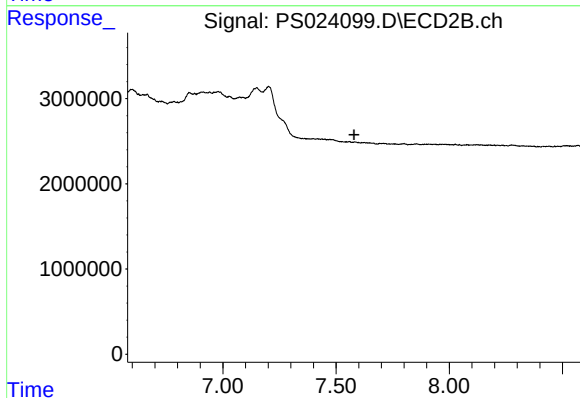


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.579 min
Response: 0
Conc: N.D.

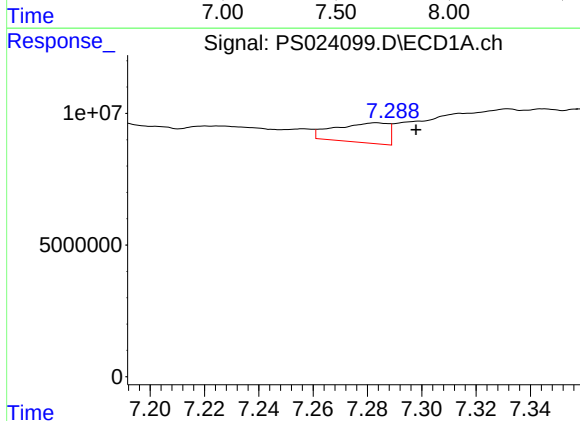

#9 2,4-D

R.T.: 7.283 min
Delta R.T.: -0.015 min
Response: 10181424
Conc: 4.11 ng/ml

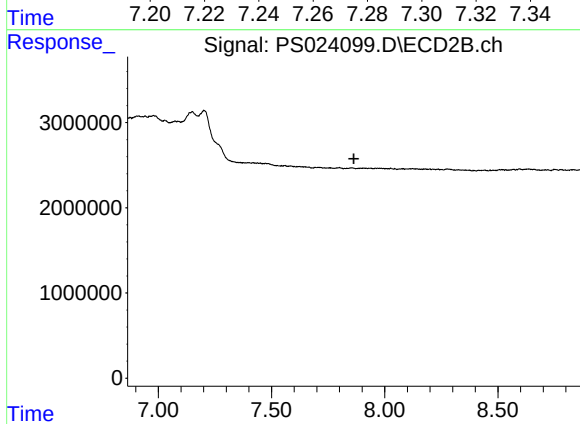

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.