

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081723\
 Data File : PS024100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 09:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 21:35:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.367	6.796	1087.7E6	367.5E6	549.208	546.371
Target Compounds							
1) T	Dalapon	2.515	2.575	6778285	4669836	3.089	4.271 #
3) T	4-Nitroph...	6.204	6.391	18267012	917238	16.504	2.317 #
5) T	DICAMBA	6.498	7.003f	1423023	2543582	<MDL	<MDL #
6) T	MCP	6.686	7.111f	8056462	294486	1.292	<MDL #
8) T	DICHLORPROP	7.116	7.587	-201890	6680860	N.D.	9.138
9) T	2,4-D	7.260	7.917f	8296863	-43730	3.348	N.D. #
10) T	Pentachlo...	7.537	8.279	6711380	870199	<MDL	<MDL #
11) T	2,4,5-TP ...	8.052	8.640	1148503	1136883	<MDL	<MDL #
12) T	2,4,5-T	8.306	9.057	1953352	2579979	<MDL	<MDL #
13) T	2,4-DB	8.795	9.514	-709334	1481732	N.D.	3.251
14) T	DINOSEB	9.864	0.000	1345959	0	<MDL	N.D. #
15) T	Picloram	9.664	10.803	351.5E6	34527596	27.187	6.929 #
16) T	DCPA	10.178f	10.803	-4967766	34527596	N.D.	6.716



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081723\
Data File : PS024100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 09:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 21:35:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

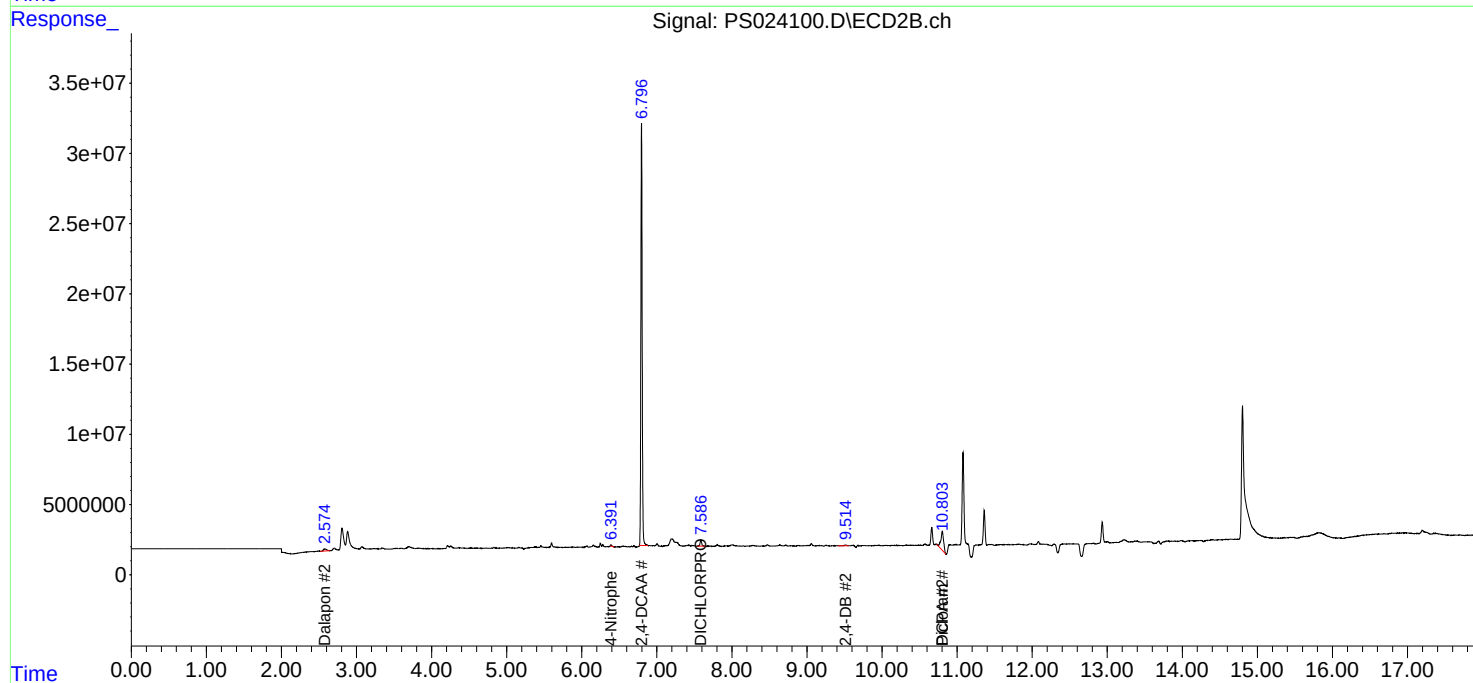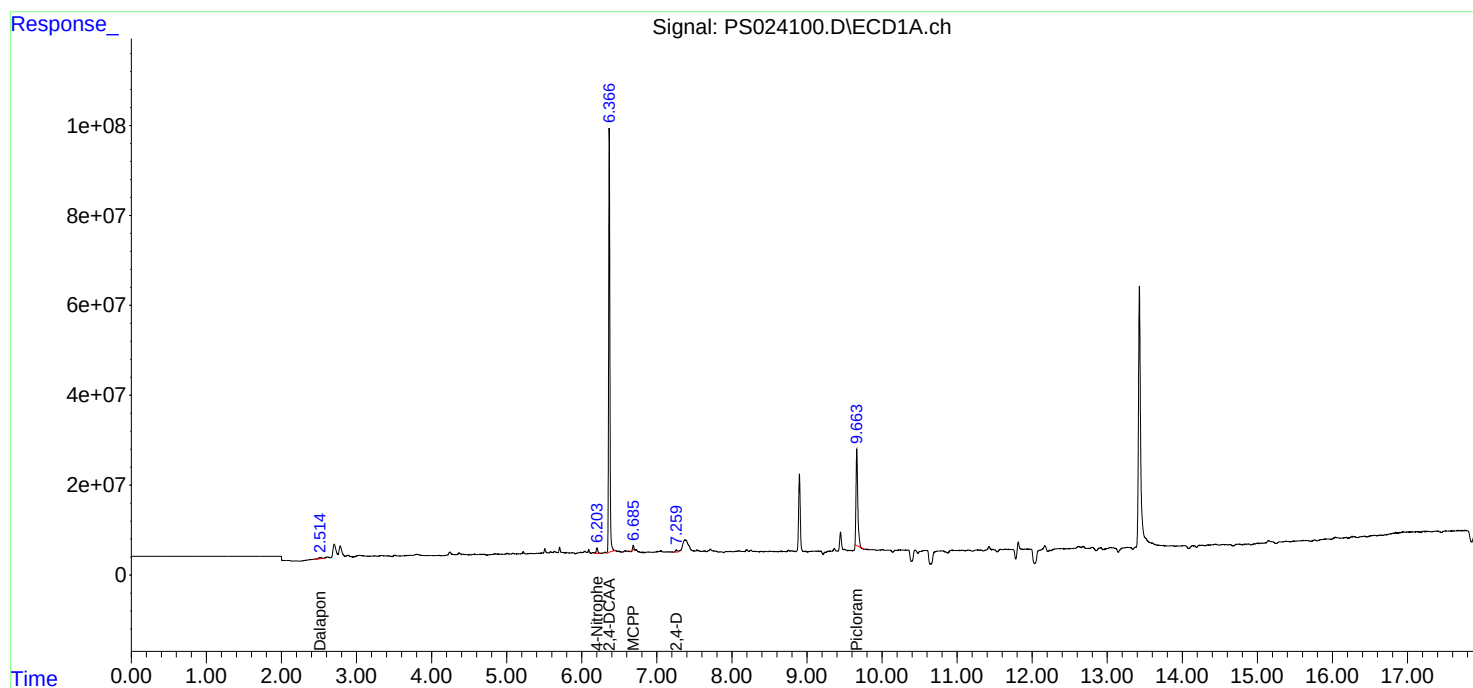


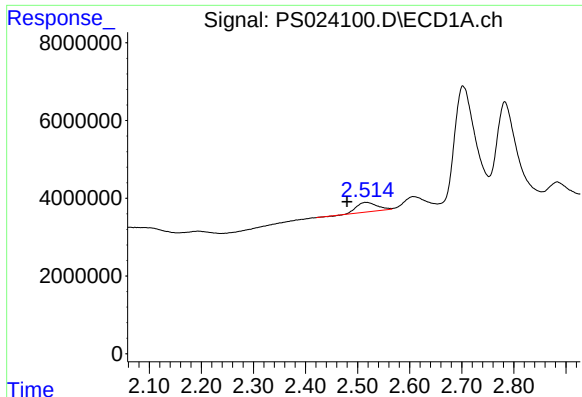

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.035 min
Response: 6778285
Conc: 3.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

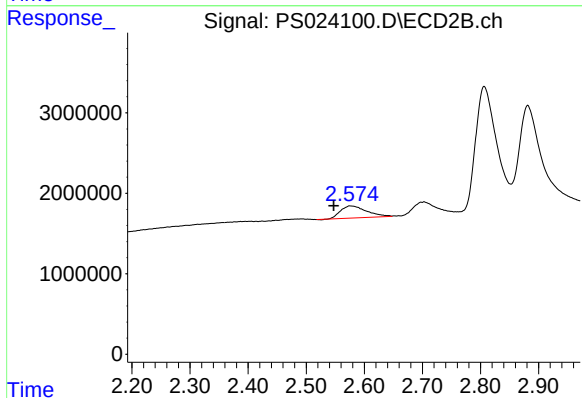


#1 Dalapon

R.T.: 2.575 min
Delta R.T.: 0.027 min
Response: 4669836
Conc: 4.27 ng/ml

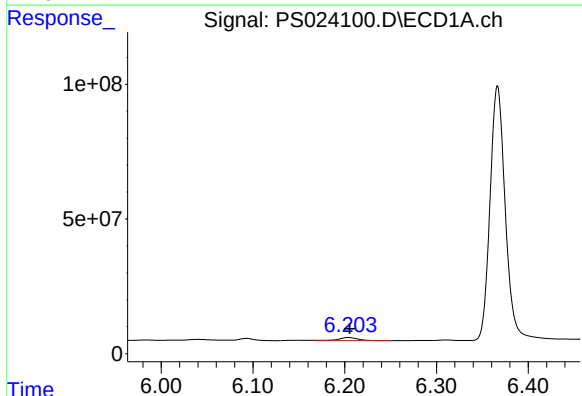


#3 4-Nitrophenol

R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 18267012
Conc: 16.50 ng/ml

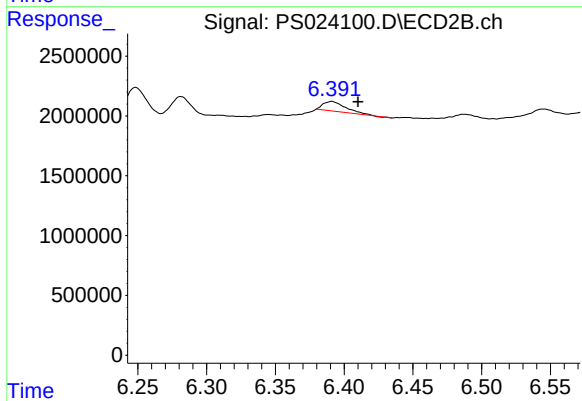

#3 4-Nitrophenol


R.T.: 6.391 min
Delta R.T.: -0.019 min
Response: 917238
Conc: 2.32 ng/ml

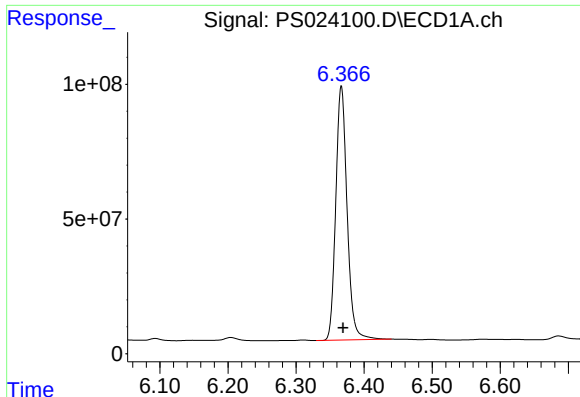

#4 2,4-DCAA


R.T.: 6.367 min
Delta R.T.: -0.002 min
Response: 1087741818
Conc: 549.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

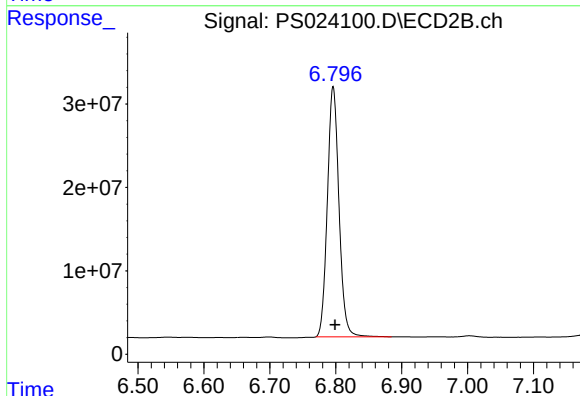


#4 2,4-DCAA

R.T.: 6.796 min
Delta R.T.: -0.003 min
Response: 367503736
Conc: 546.37 ng/ml

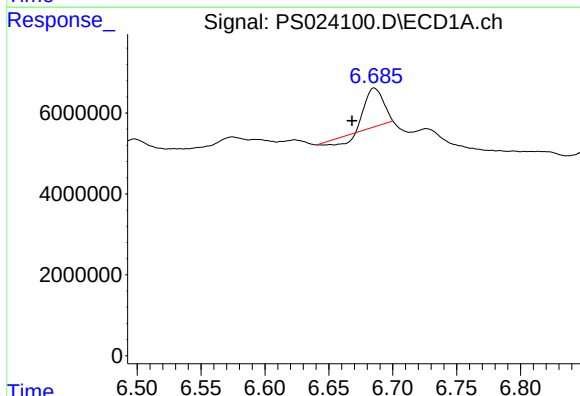


#6 MCP

R.T.: 6.686 min
Delta R.T.: 0.018 min
Response: 8056462
Conc: 1.29 ug/ml

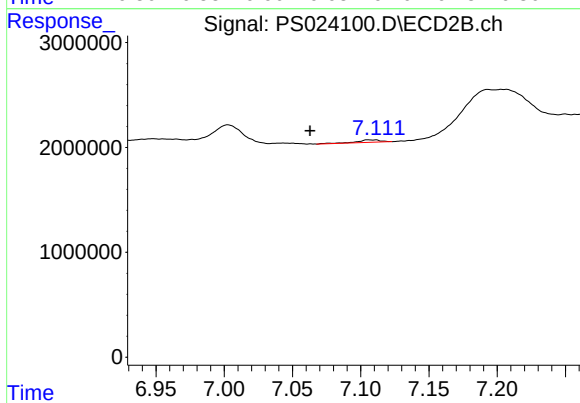

#6 MCP


R.T.: 7.111 min
Delta R.T.: 0.048 min
Response: 294486
Conc: N.D.

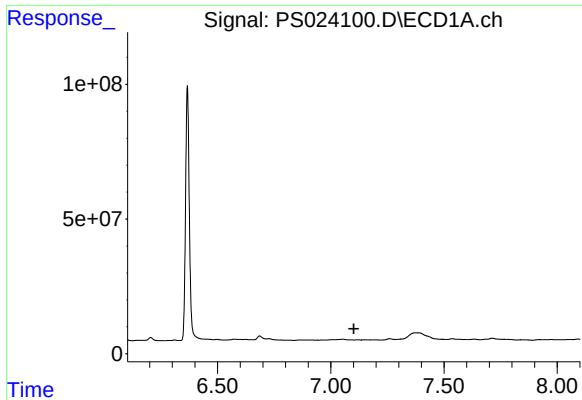

#8 DICHLORPROP


R.T.: 7.116 min
Delta R.T.: 0.014 min
Response: -201890
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

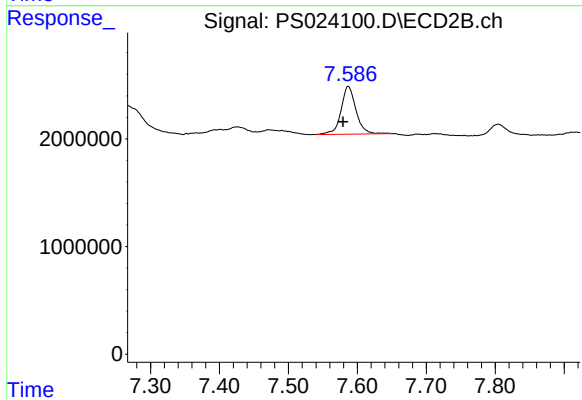


#8 DICHLORPROP

R.T.: 7.587 min
Delta R.T.: 0.008 min
Response: 6680860
Conc: 9.14 ng/ml

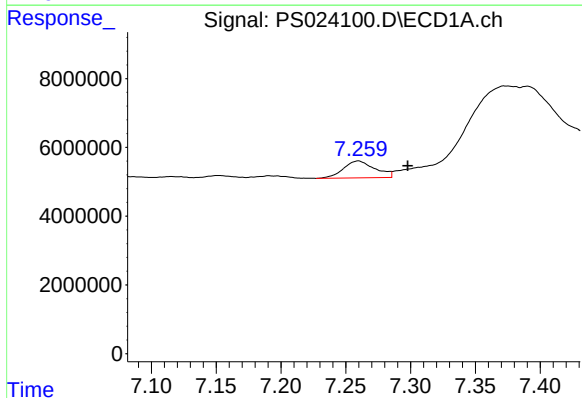


#9 2,4-D

R.T.: 7.260 min
Delta R.T.: -0.038 min
Response: 8296863
Conc: 3.35 ng/ml

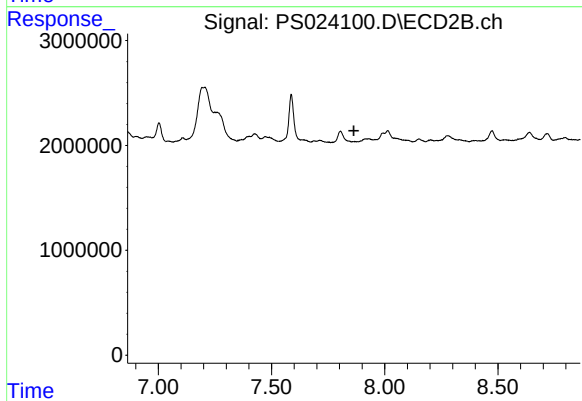

#9 2,4-D


R.T.: 7.917 min
Delta R.T.: 0.054 min
Response: -43730
Conc: N.D.

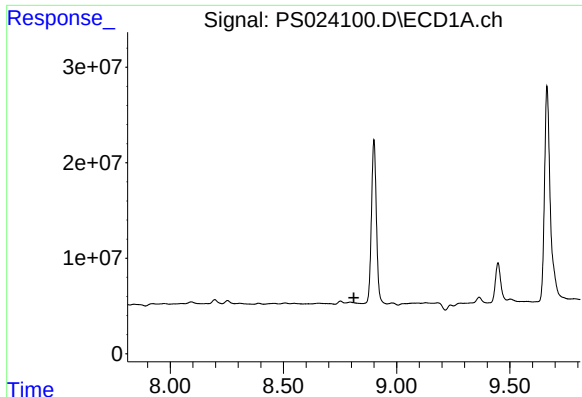

#13 2,4-DB


R.T.: 8.795 min
Delta R.T.: -0.016 min
Response: -709334
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

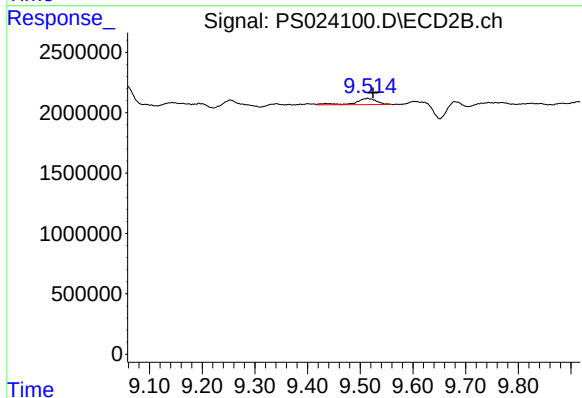


#13 2,4-DB

R.T.: 9.514 min
Delta R.T.: -0.010 min
Response: 1481732
Conc: 3.25 ng/ml

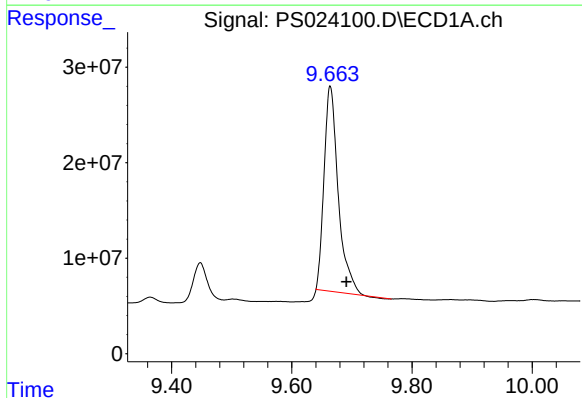


#15 Picloram

R.T.: 9.664 min
Delta R.T.: -0.027 min
Response: 351513707
Conc: 27.19 ng/ml

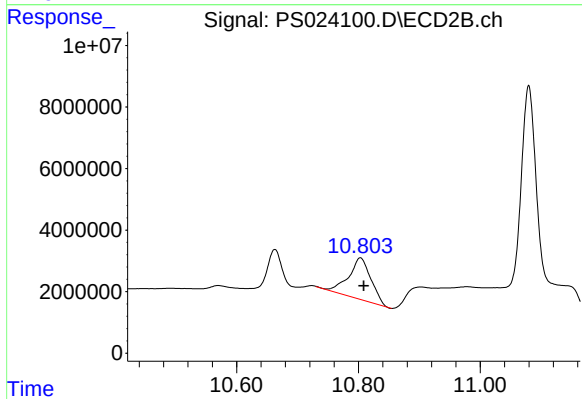

#15 Picloram


R.T.: 10.803 min
Delta R.T.: -0.006 min
Response: 34527596
Conc: 6.93 ng/ml

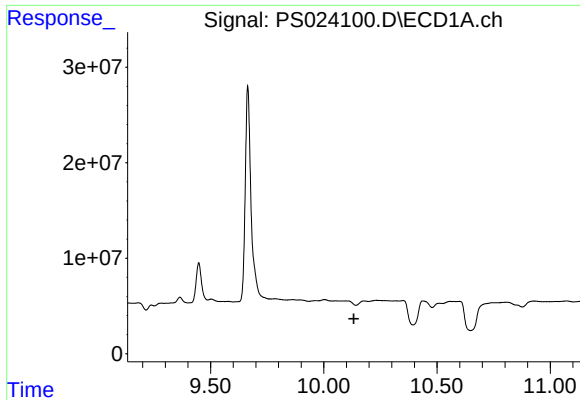

#16 DCPA

R.T.: 10.178 min
Delta R.T.: 0.045 min
Response: -4967766
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

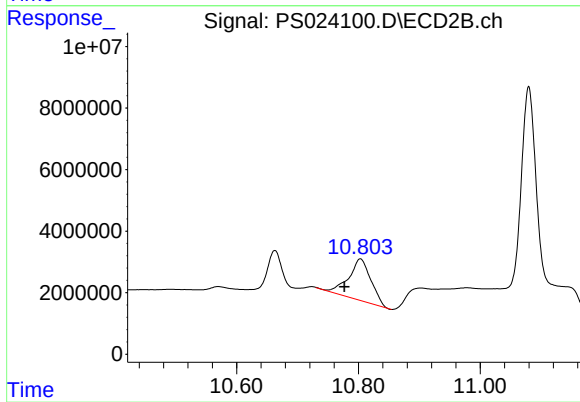

#16 DCPA

R.T.: 10.803 min
Delta R.T.: 0.026 min
Response: 34527596
Conc: 6.72 ng/ml