

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 17:03
 Operator : DD\AJ
 Sample : PB131061BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 18:55:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.222	6.912	506.0E6	293.0E6	463.937	547.863
Target Compounds							
2) T	3,5-DICHL...	0.000	6.093	0	61042443	N.D.	74.205
3) T	4-Nitroph...	6.995	0.000	826559	0	1.403	N.D. #
5) T	DICAMBA	7.402	7.046	11732932	10606038	2.864	4.909 #
6) T	MCP	7.578	0.000	5657058	0	1.771	N.D. #
7) T	MCPA	7.770	7.374	31624226	18783825	6.953	6.855
11) T	2,4,5-TP ...	0.000	8.762	0	28442703	N.D.	9.728
12) T	2,4,5-T	9.500	0.000	11234087	0	1.896	N.D. #
15) T	Picloram	11.018	11.016	26757971	45742177	3.424	10.092 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 17:03
Operator : DD\AJ
Sample : PB131061BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 18:55:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

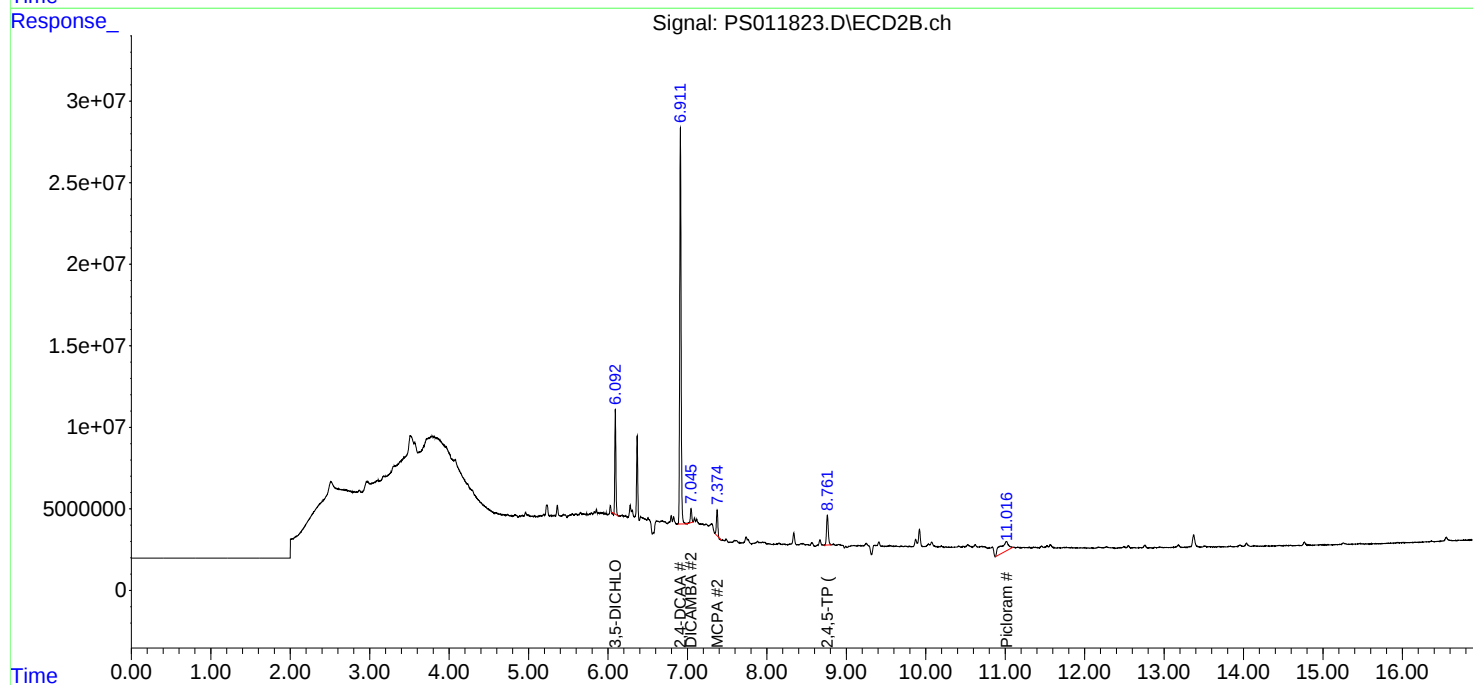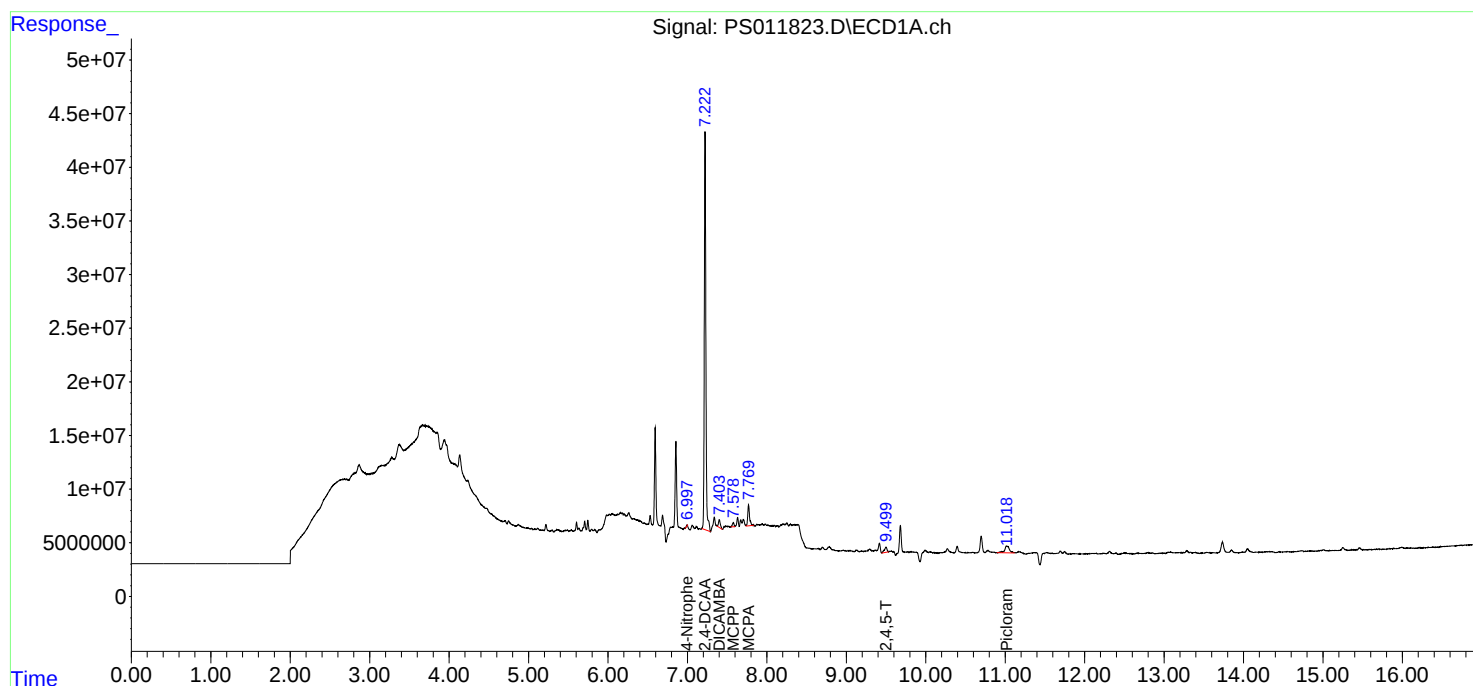


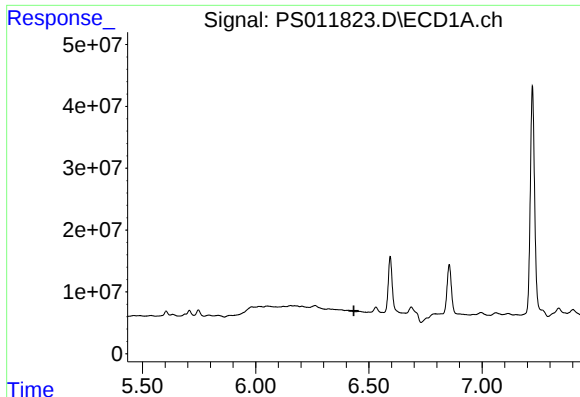

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

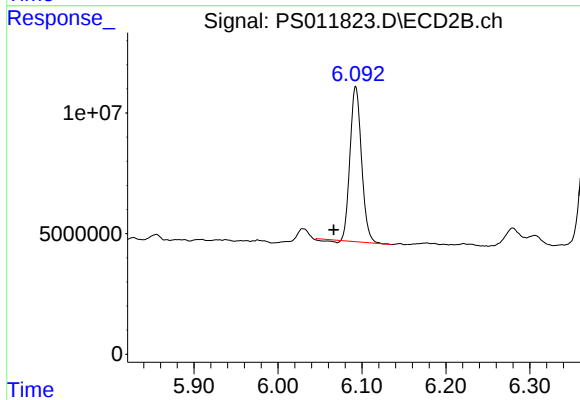


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.093 min
Delta R.T.: 0.026 min
Response: 61042443
Conc: 74.20 ng/ml

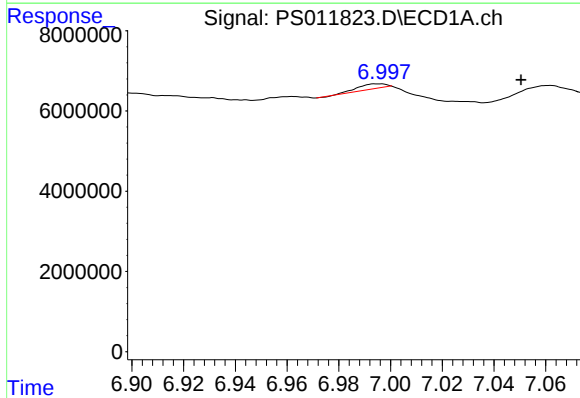


#3 4-Nitrophenol

R.T.: 6.995 min
Delta R.T.: -0.055 min
Response: 826559
Conc: 1.40 ng/ml

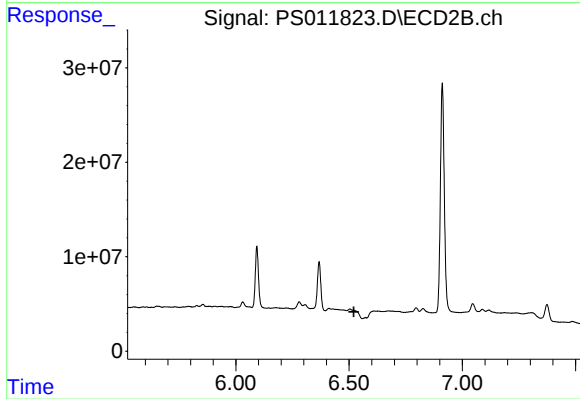

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

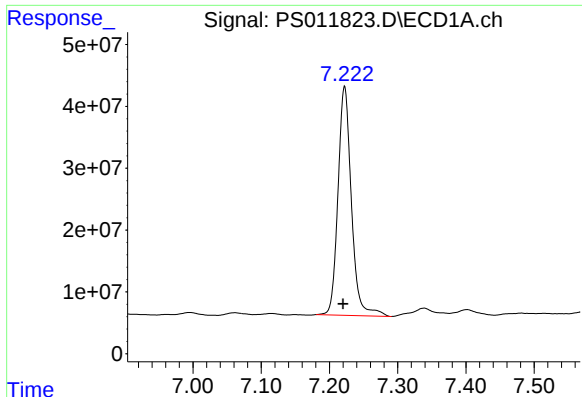

#4 2,4-DCAA


R.T.: 7.222 min
Delta R.T.: 0.002 min
Response: 506047966
Conc: 463.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

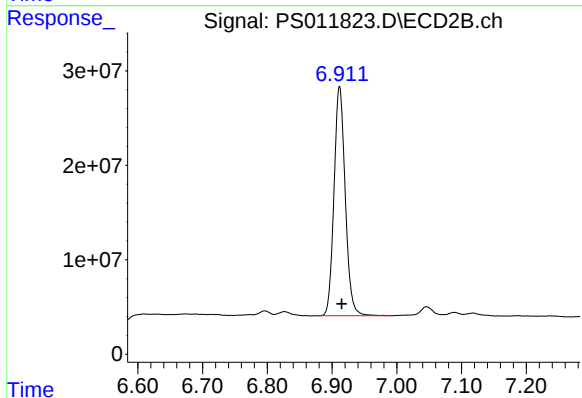


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 292989820
Conc: 547.86 ng/ml

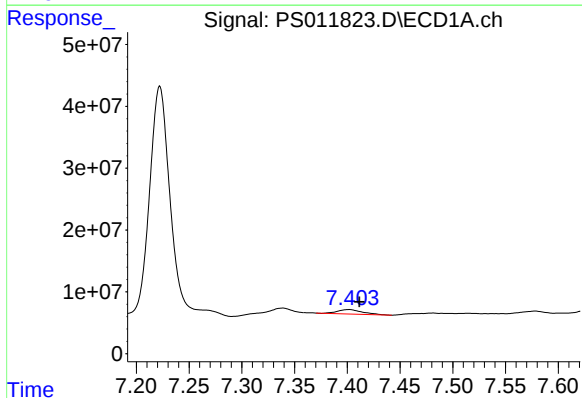


#5 DICAMBA

R.T.: 7.402 min
Delta R.T.: -0.010 min
Response: 11732932
Conc: 2.86 ng/ml

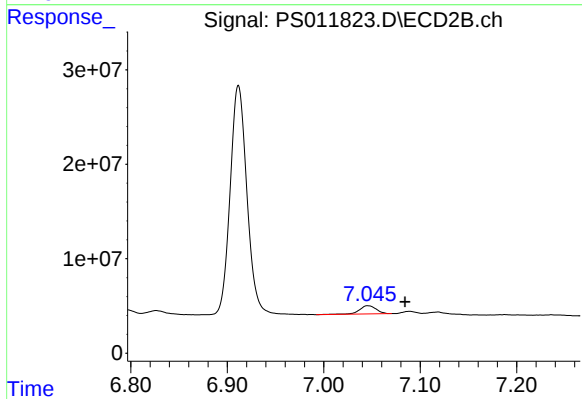

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.038 min
Response: 10606038
Conc: 4.91 ng/ml

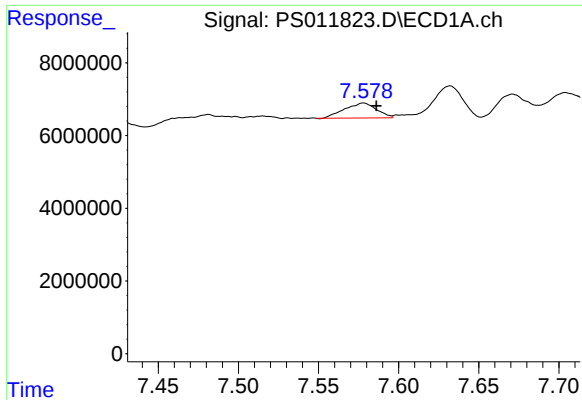

#6 MCPP


R.T.: 7.578 min
Delta R.T.: -0.008 min
Response: 5657058
Conc: 1.77 ug/ml

Instrument :
ECD_S
ClientSampleId :

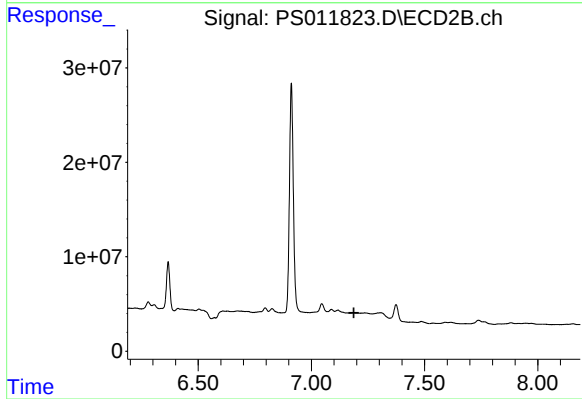


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

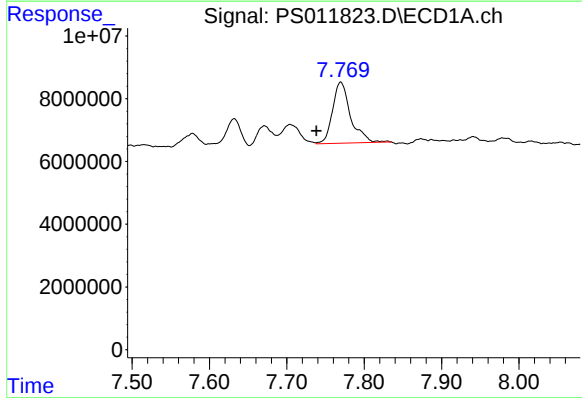


#7 MCPA

R.T.: 7.770 min
Delta R.T.: 0.031 min
Response: 31624226
Conc: 6.95 ug/ml

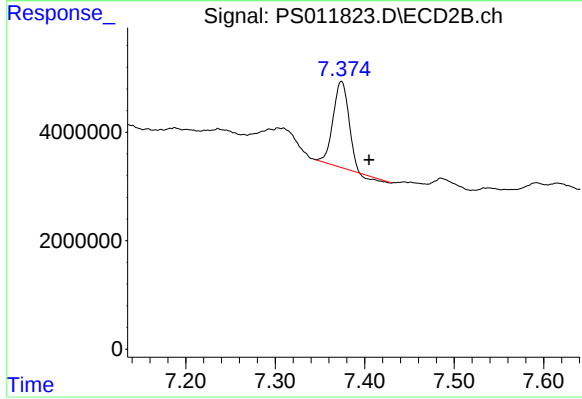

#7 MCPA


R.T.: 7.374 min
Delta R.T.: -0.031 min
Response: 18783825
Conc: 6.86 ug/ml

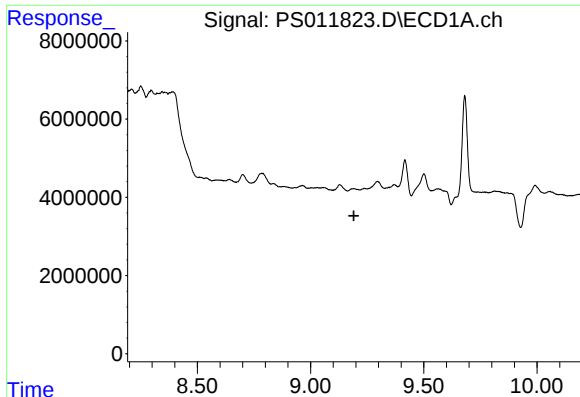

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

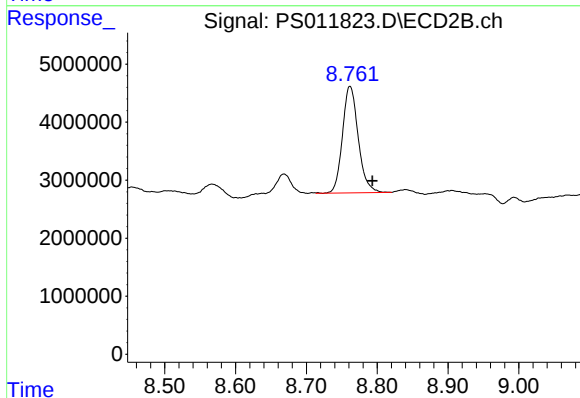


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.032 min
Response: 28442703
Conc: 9.73 ng/ml

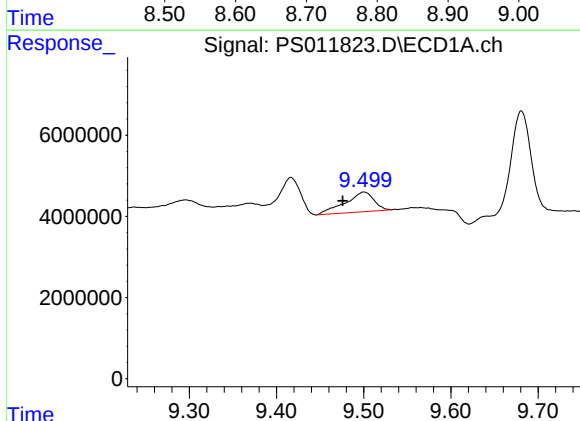


#12 2,4,5-T

R.T.: 9.500 min
Delta R.T.: 0.024 min
Response: 11234087
Conc: 1.90 ng/ml

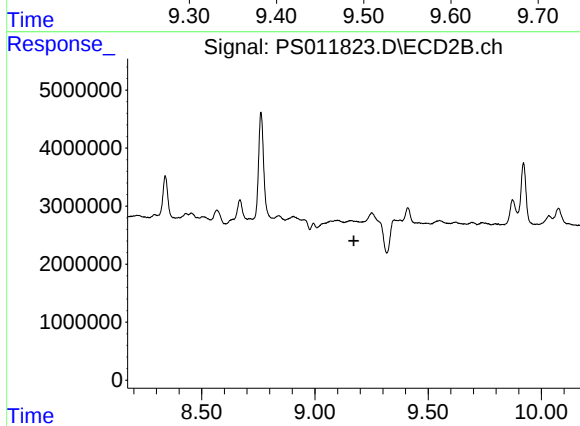

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

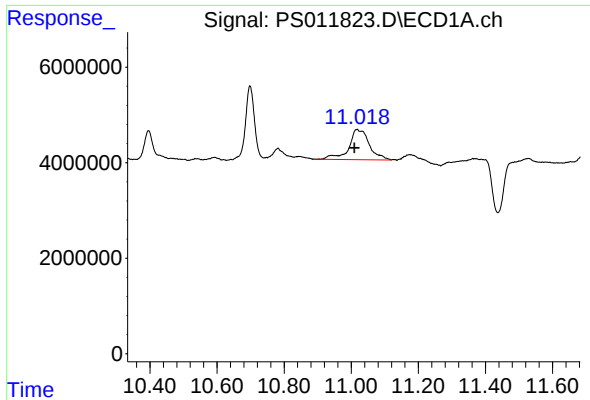

#15 Picloram

R.T.: 11.018 min
Delta R.T.: 0.008 min
Response: 26757971
Conc: 3.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

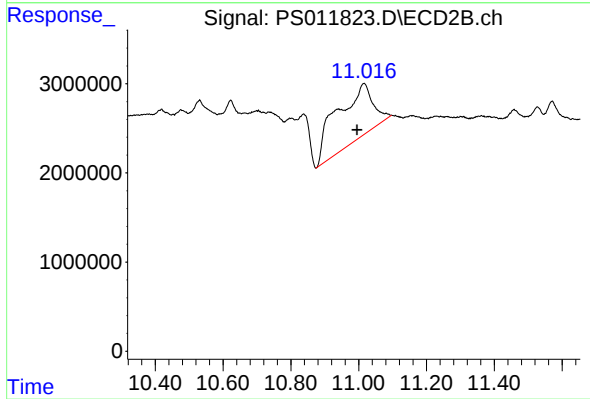

#15 Picloram

R.T.: 11.016 min
Delta R.T.: 0.020 min
Response: 45742177
Conc: 10.09 ng/ml