

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 17:49
 Operator : DD\AJ
 Sample : PB131061TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 18:56:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.916	224.4E6	144.5E6	205.694	270.202 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	58999728	N.D.	71.722
3) T	4-Nitroph...	7.117	6.545	13504966	8407332	22.927	23.058
5) T	DICAMBA	7.397	7.049	6571205	13592823	1.604	6.291 #
6) T	MCP	7.574	0.000	7850588	0	2.457	N.D. #
7) T	MCPA	7.700	0.000	43364040	0	9.534	N.D. #
8) T	DICHLORPROP	8.049	7.740	5026706	19606769	5.003	34.725 #
9) T	2,4-D	8.401	0.000	104.9E6	0	92.913	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	30535328	N.D.	10.444
12) T	2,4,5-T	9.412	0.000	23214592	0	3.918	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 17:49
Operator : DD\AJ
Sample : PB131061TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 18:56:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

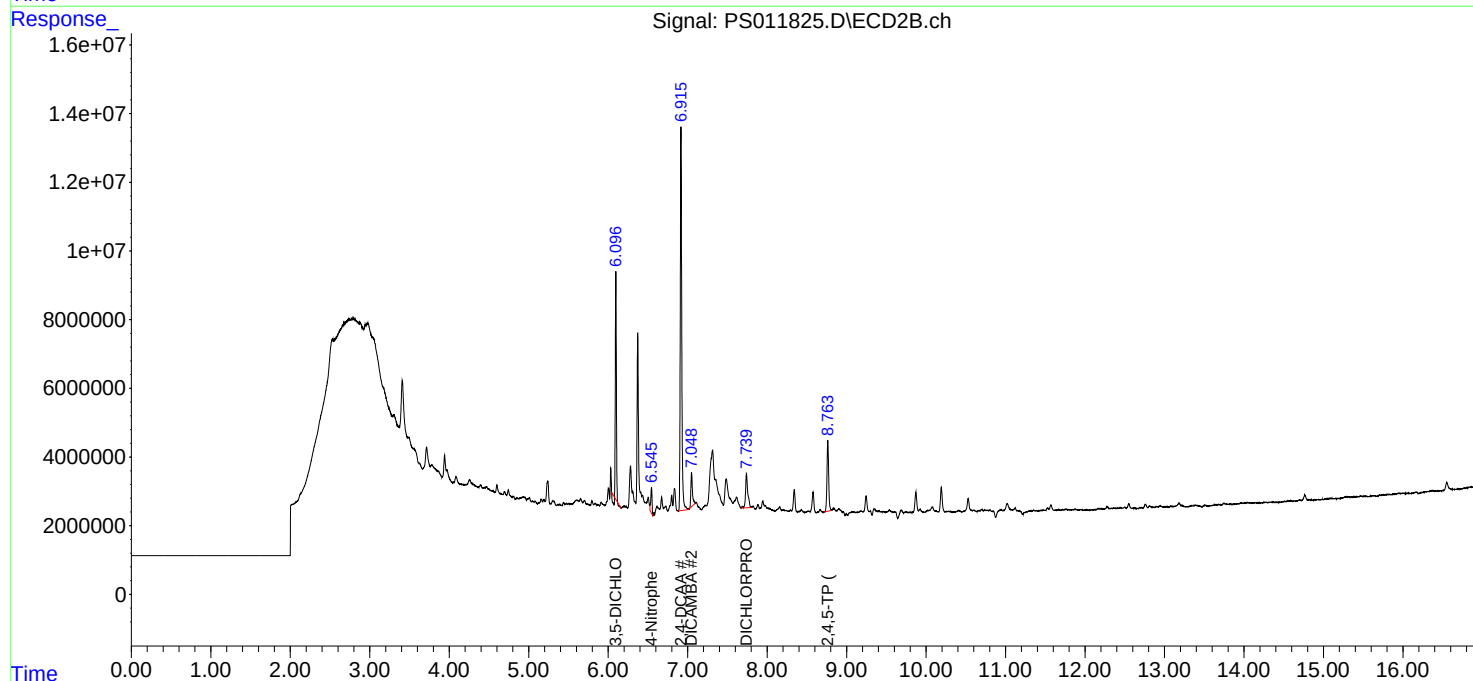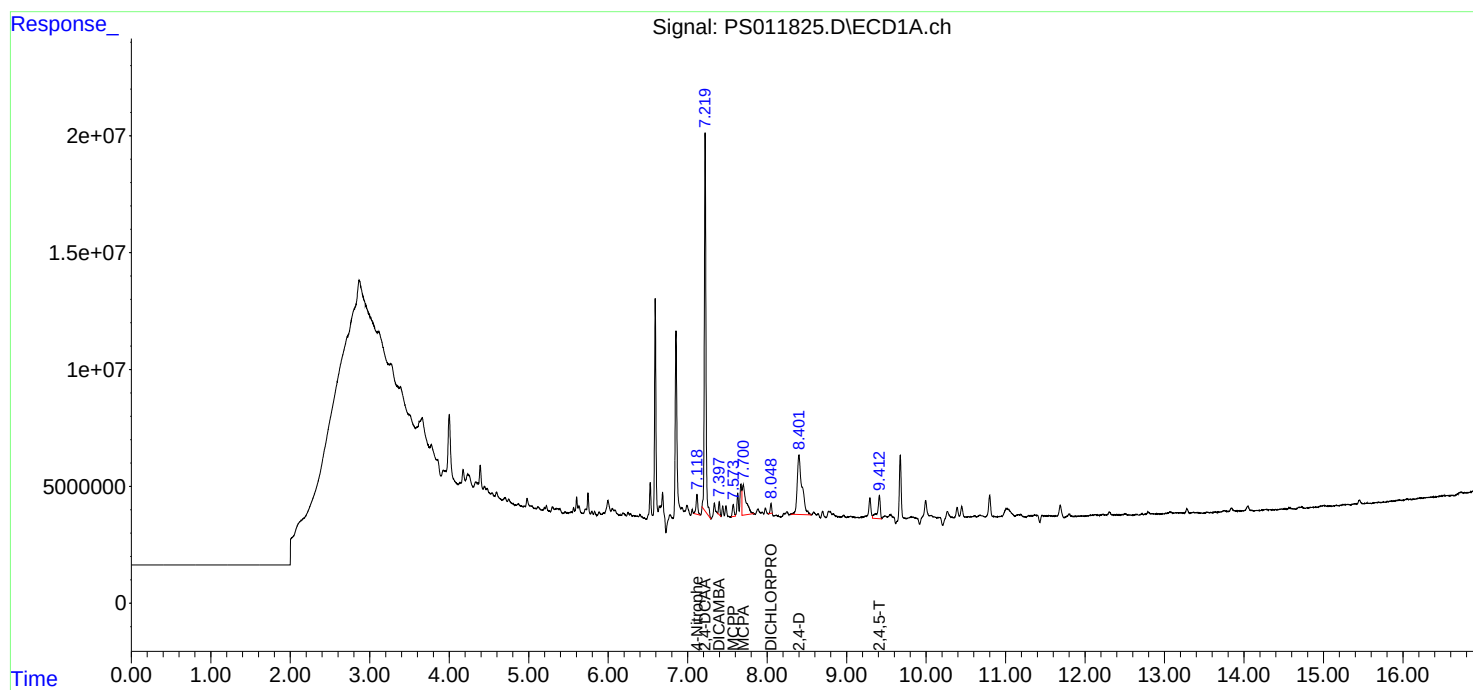


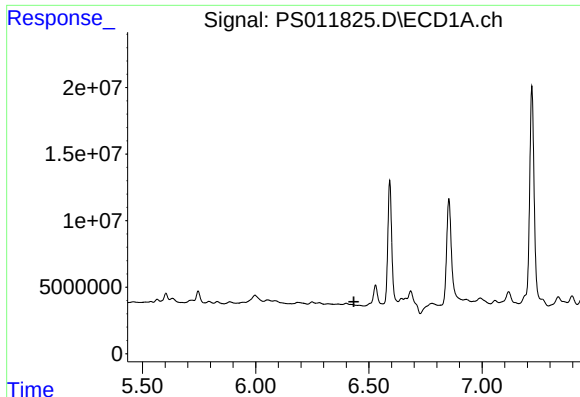

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

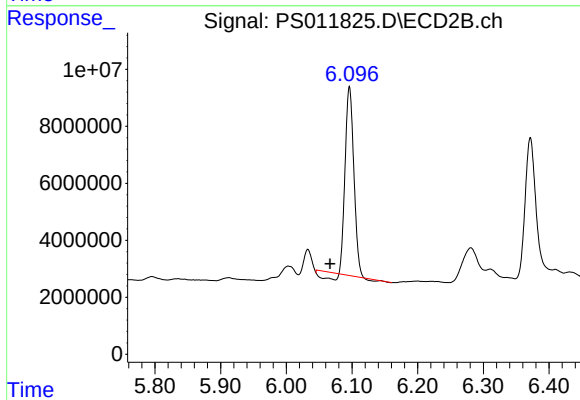


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 58999728
Conc: 71.72 ng/ml

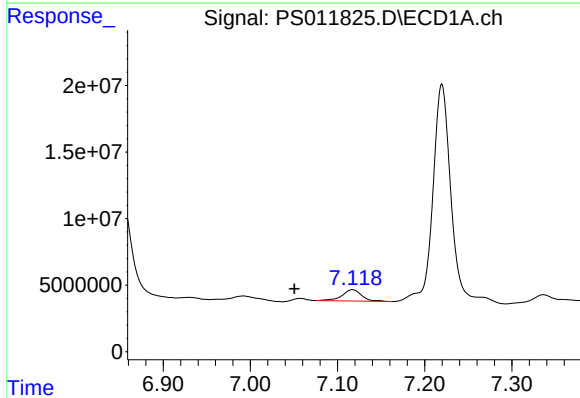


#3 4-Nitrophenol

R.T.: 7.117 min
Delta R.T.: 0.067 min
Response: 13504966
Conc: 22.93 ng/ml

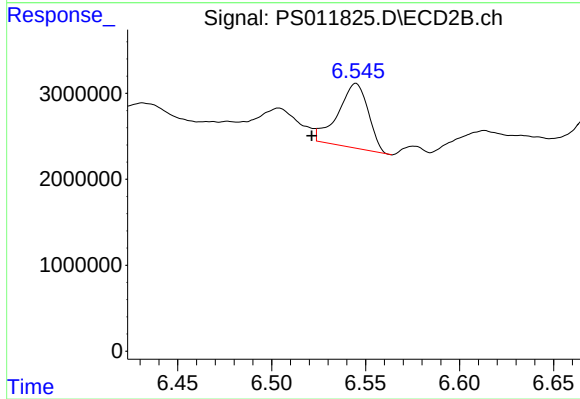

#3 4-Nitrophenol


R.T.: 6.545 min
Delta R.T.: 0.023 min
Response: 8407332
Conc: 23.06 ng/ml

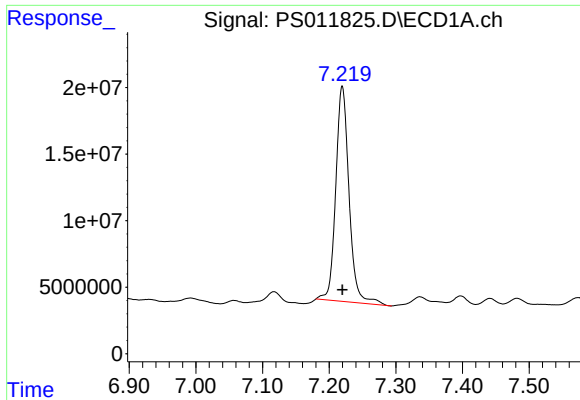

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 224364337
Conc: 205.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

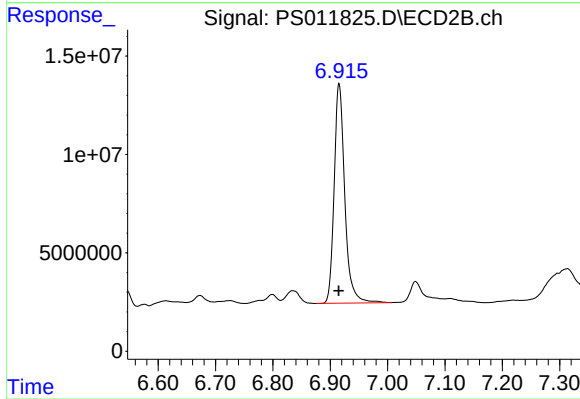


#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 144500659
Conc: 270.20 ng/ml

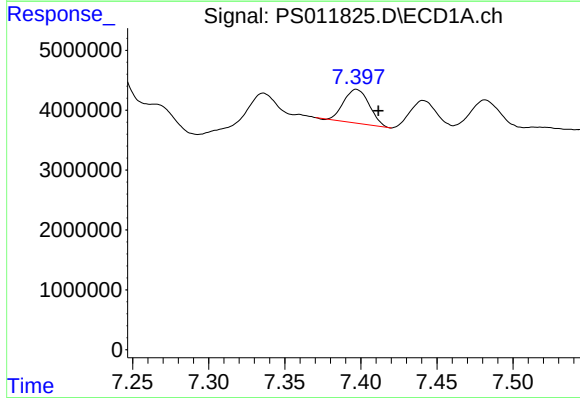


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.014 min
Response: 6571205
Conc: 1.60 ng/ml

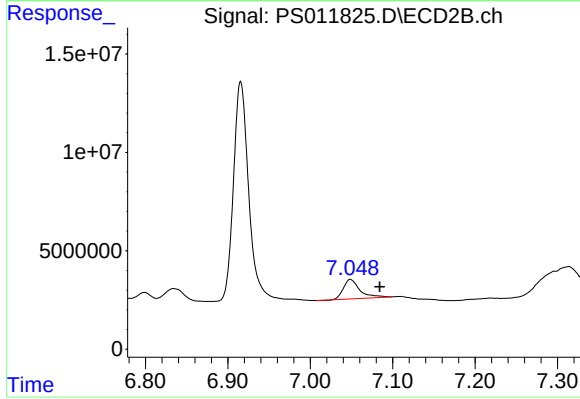

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 13592823
Conc: 6.29 ng/ml

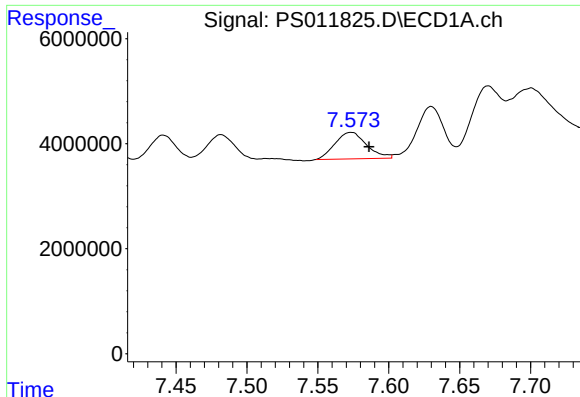

#6 MCPP


R.T.: 7.574 min
Delta R.T.: -0.012 min
Response: 7850588
Conc: 2.46 ug/ml

Instrument :
ECD_S
ClientSampleId :

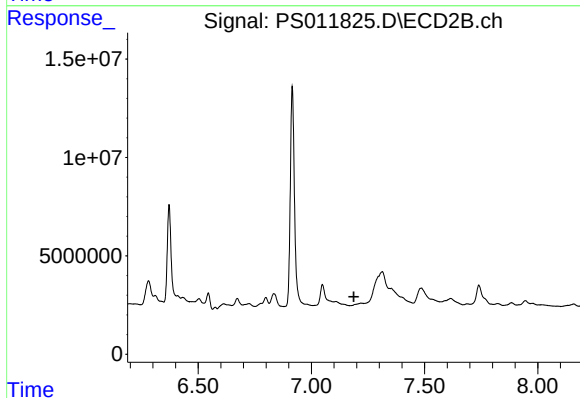


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

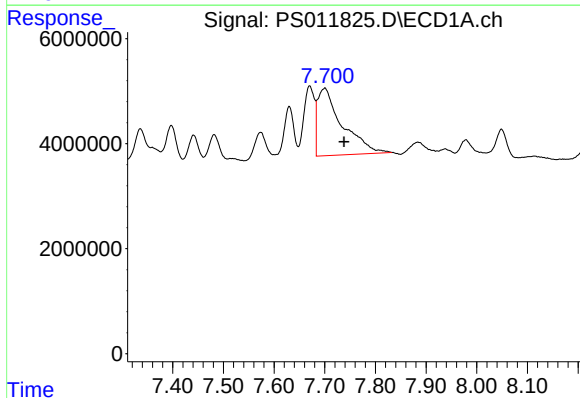


#7 MCPA

R.T.: 7.700 min
Delta R.T.: -0.038 min
Response: 43364040
Conc: 9.53 ug/ml

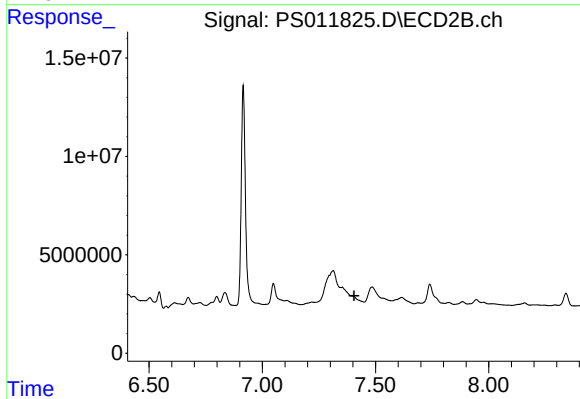

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

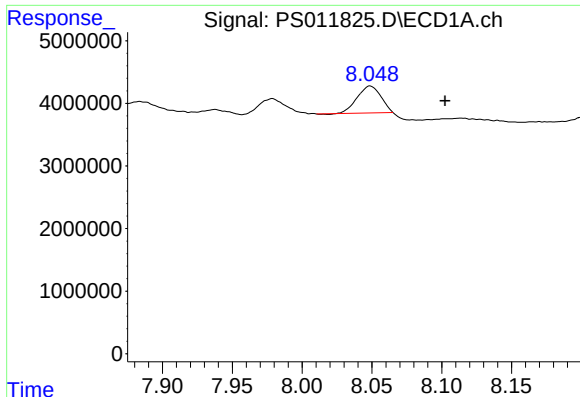

#8 DICHLORPROP


R.T.: 8.049 min
Delta R.T.: -0.054 min
Response: 5026706
Conc: 5.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

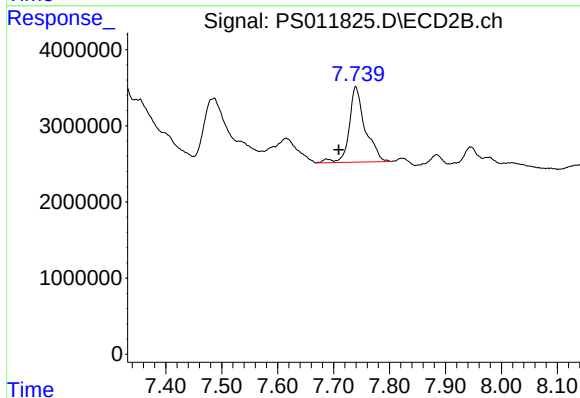


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.030 min
Response: 19606769
Conc: 34.72 ng/ml

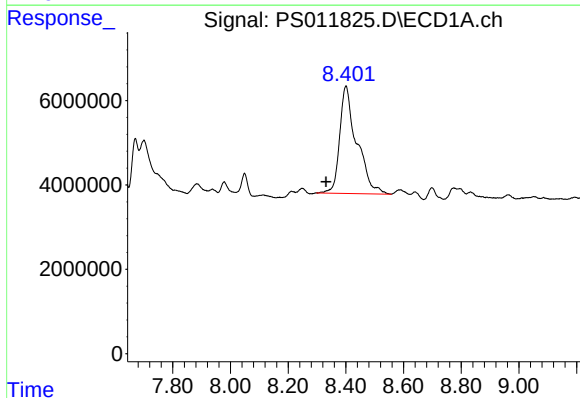


#9 2,4-D

R.T.: 8.401 min
Delta R.T.: 0.069 min
Response: 104907485
Conc: 92.91 ng/ml

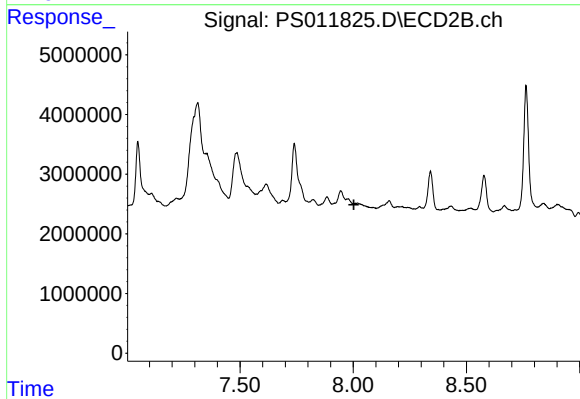

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

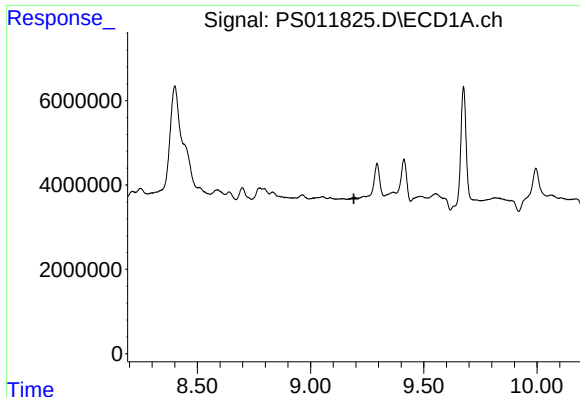

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

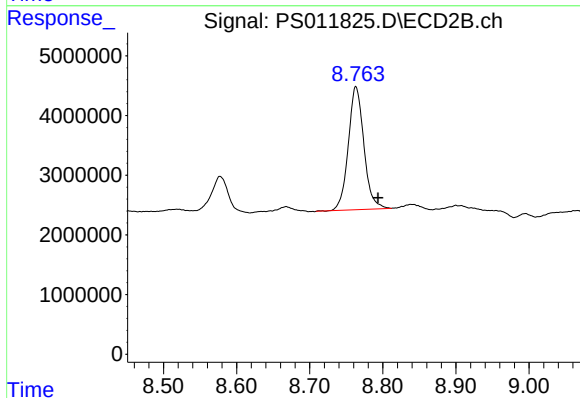


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 30535328
Conc: 10.44 ng/ml

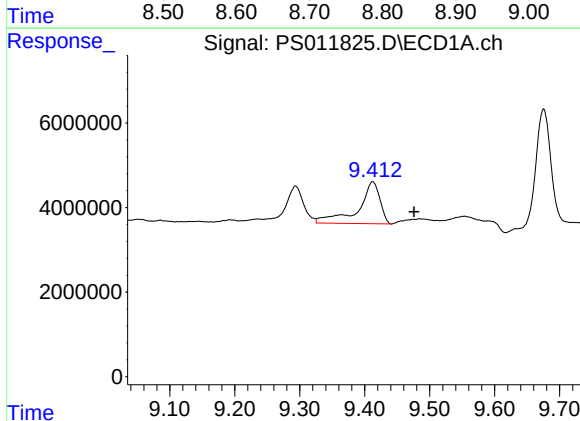

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 23214592
Conc: 3.92 ng/ml

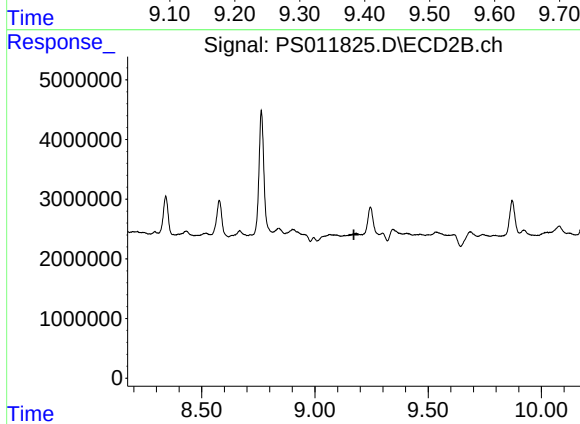

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.