

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 18:12
 Operator : DD\AJ
 Sample : L3496-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 18:56:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.915	250.3E6	159.7E6	229.435	298.670 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	67473700	N.D.	82.023
3) T	4-Nitroph...	6.989	0.000	1928485	0	3.274	N.D. #
5) T	DICAMBA	7.397	7.049	6600004	9662109	1.611	4.472 #
6) T	MCP	7.629	0.000	7309372	0	2.288	N.D. #
7) T	MCPA	7.692	7.468	156.0E6	88444886	34.294	32.277
8) T	DICHLORPROP	0.000	7.738	0	21715510	N.D.	38.459
9) T	2,4-D	8.400	0.000	105.8E6	0	93.691	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	31904452	N.D.	10.913
12) T	2,4,5-T	9.412	0.000	18236718	0	3.077	N.D. #
14) T	DINOSEB	0.000	10.060	0	16294044	N.D.	7.664
15) T	Picloram	10.998	0.000	17036877	0	2.180	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 18:12
Operator : DD\AJ
Sample : L3496-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 18:56:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

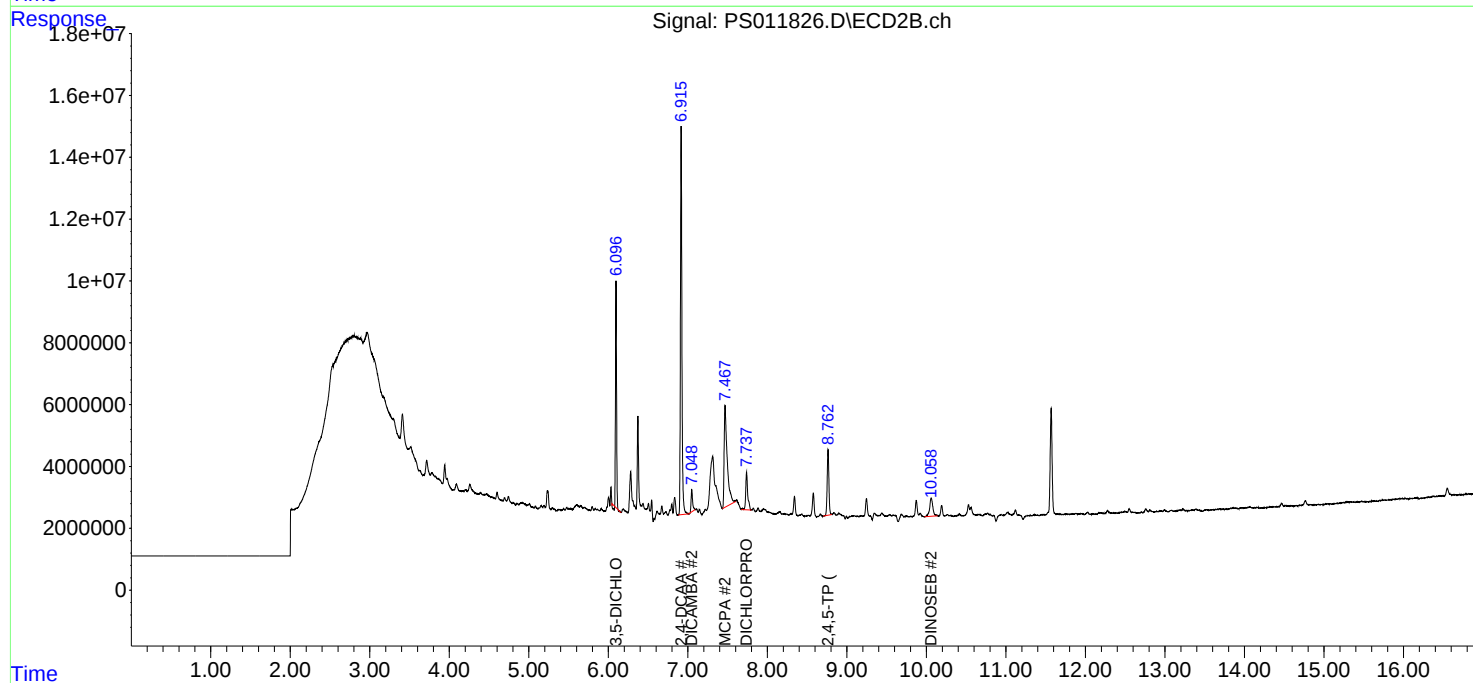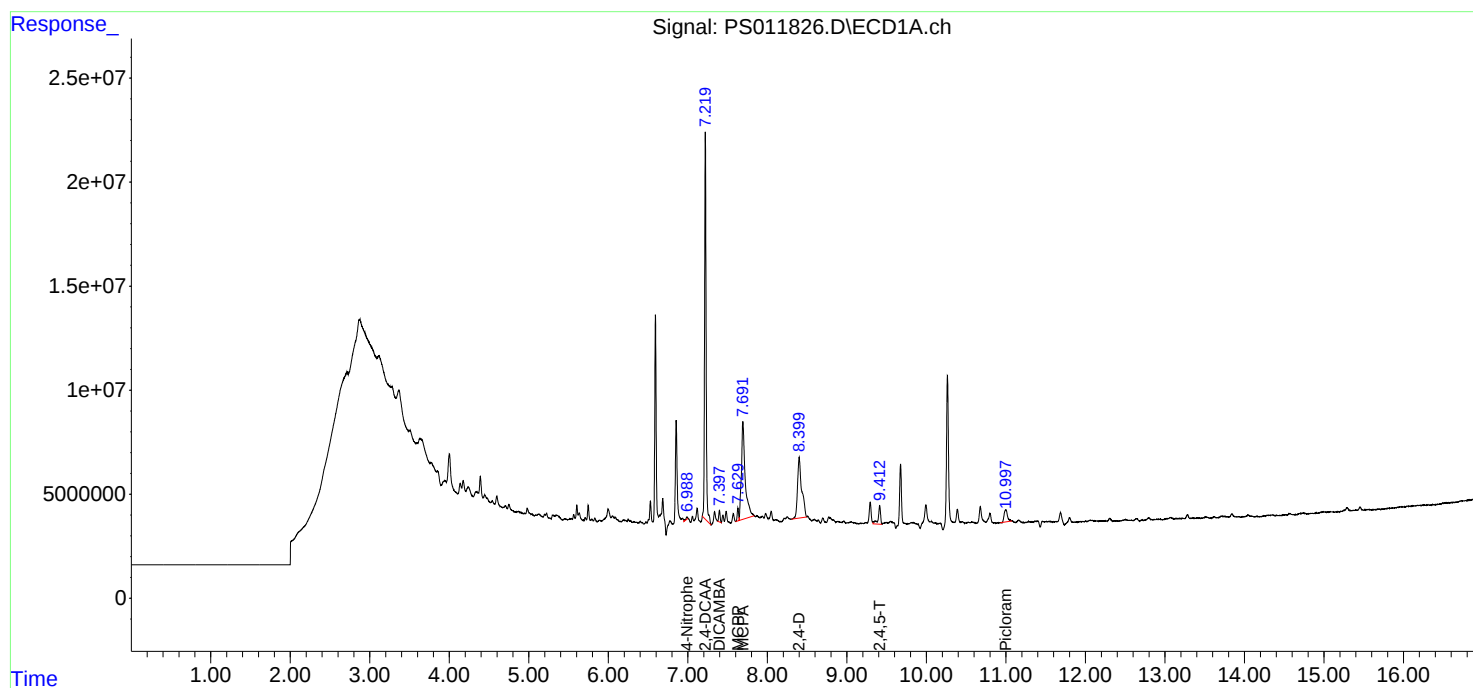


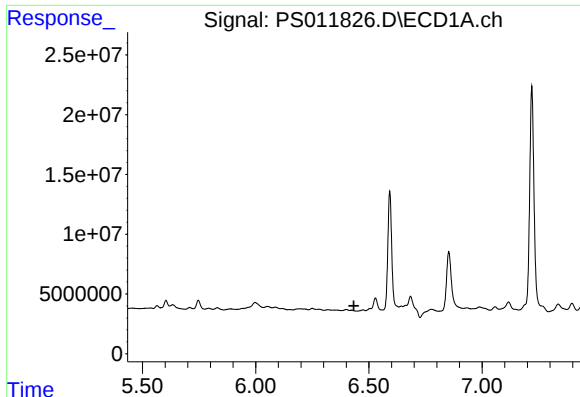

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

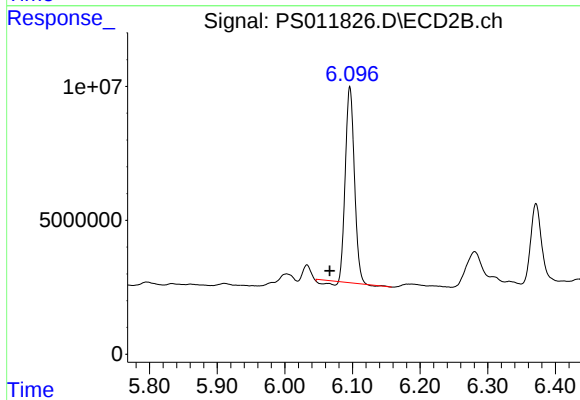


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 67473700
Conc: 82.02 ng/ml

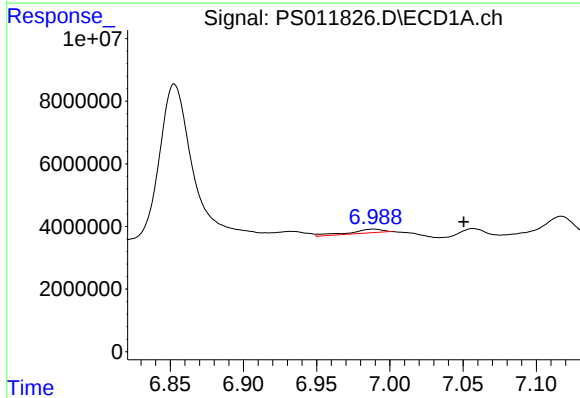


#3 4-Nitrophenol

R.T.: 6.989 min
Delta R.T.: -0.062 min
Response: 1928485
Conc: 3.27 ng/ml

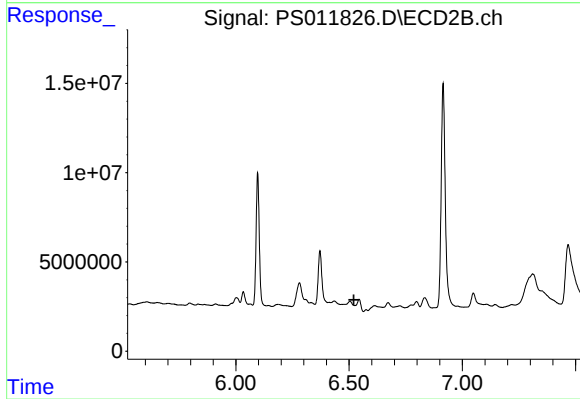

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

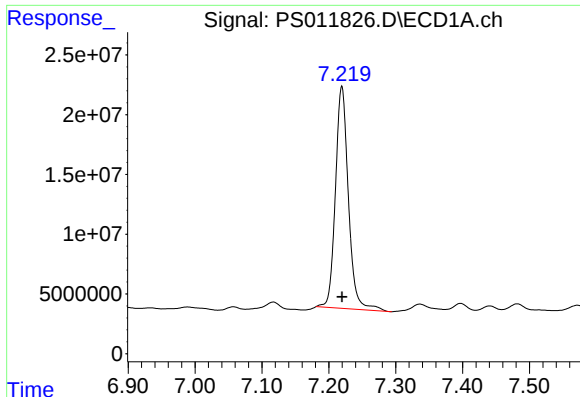

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 250260623
Conc: 229.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

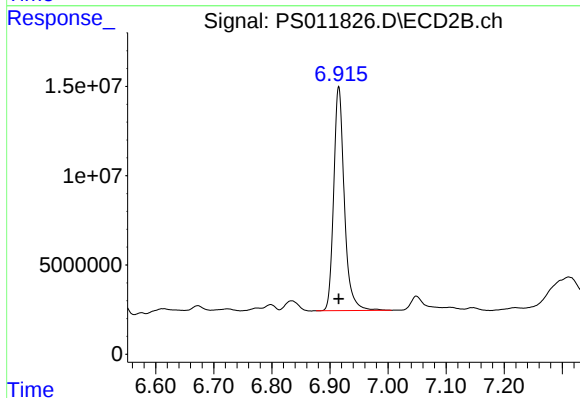


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 159724808
Conc: 298.67 ng/ml

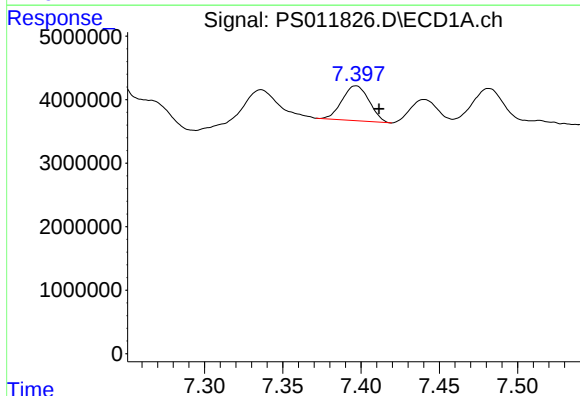


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 6600004
Conc: 1.61 ng/ml

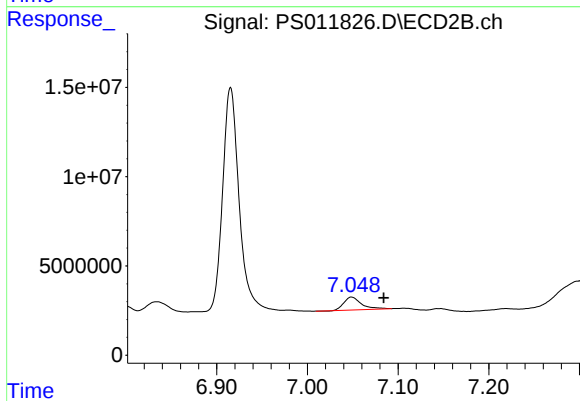

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 9662109
Conc: 4.47 ng/ml

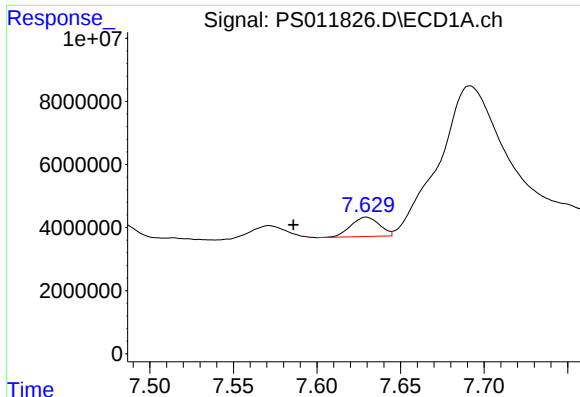

#6 MCP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 7309372
Conc: 2.29 ug/ml

Instrument :
ECD_S
ClientSampleId :

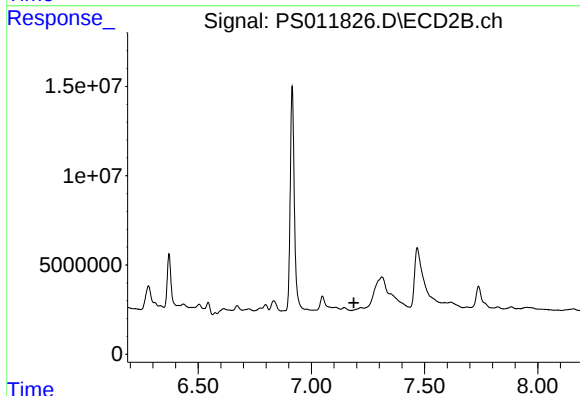


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

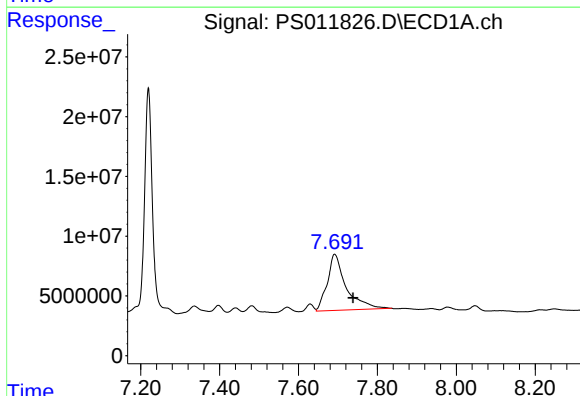


#7 MCP

R.T.: 7.692 min
Delta R.T.: -0.047 min
Response: 155987303
Conc: 34.29 ug/ml

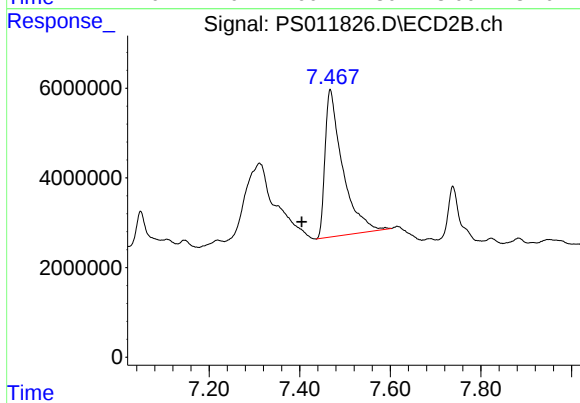

#7 MCP


R.T.: 7.468 min
Delta R.T.: 0.063 min
Response: 88444886
Conc: 32.28 ug/ml

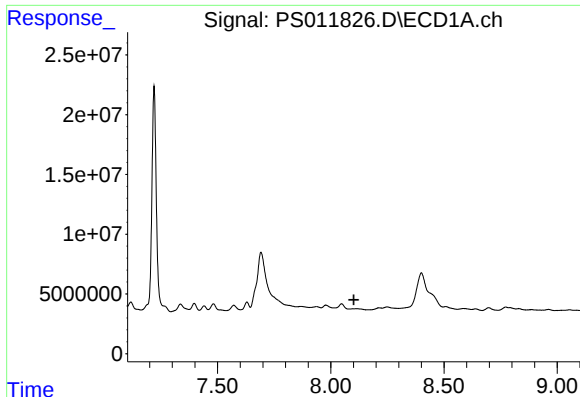

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

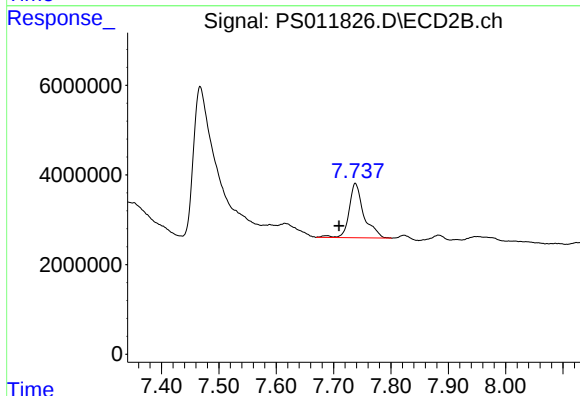


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 21715510
Conc: 38.46 ng/ml

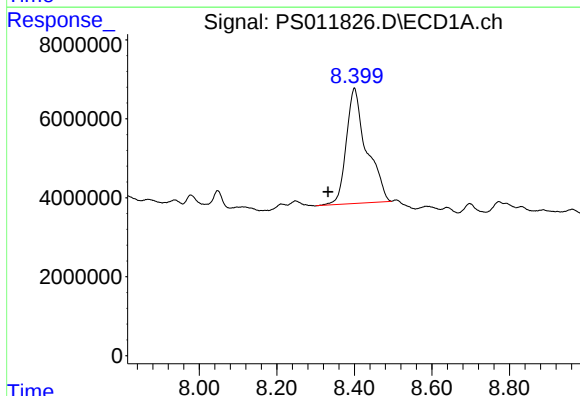


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 105786214
Conc: 93.69 ng/ml

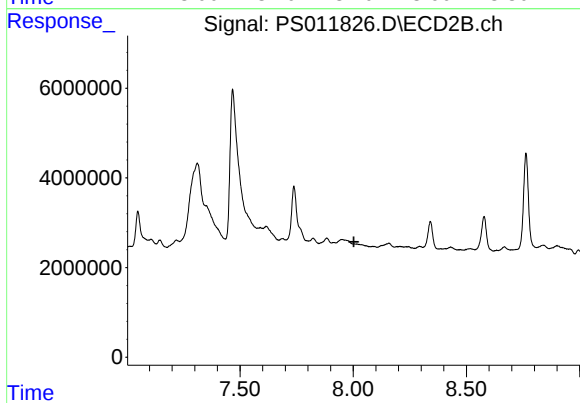

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

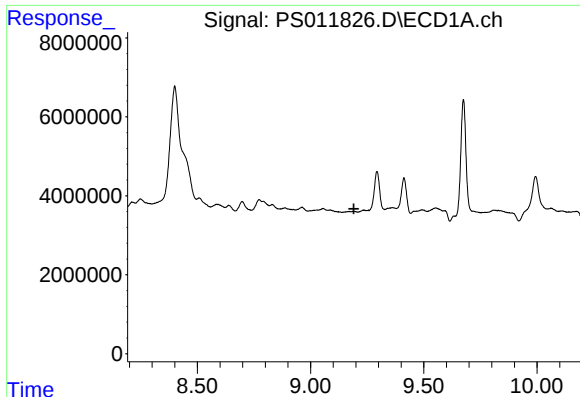

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

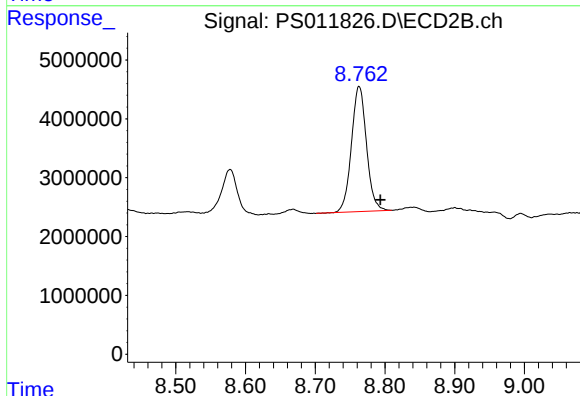


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 31904452
Conc: 10.91 ng/ml

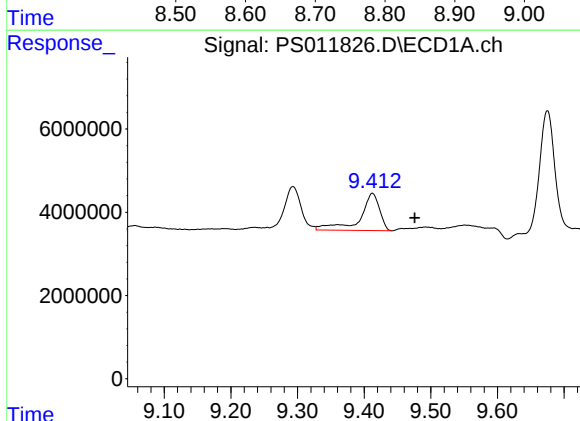


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 18236718
Conc: 3.08 ng/ml

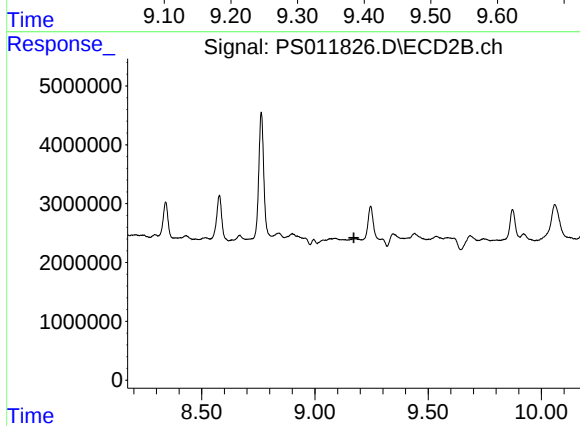

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

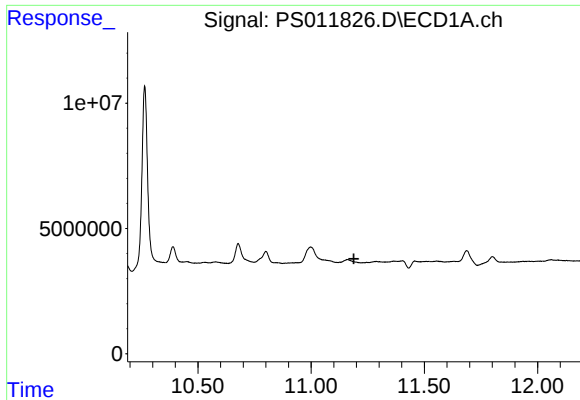

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

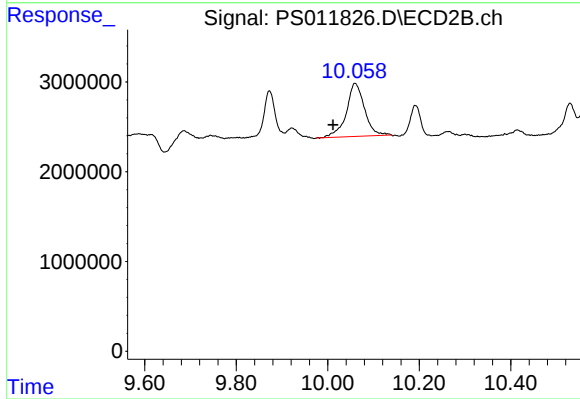


#14 DINOSEB

R.T.: 10.060 min
Delta R.T.: 0.048 min
Response: 16294044
Conc: 7.66 ng/ml

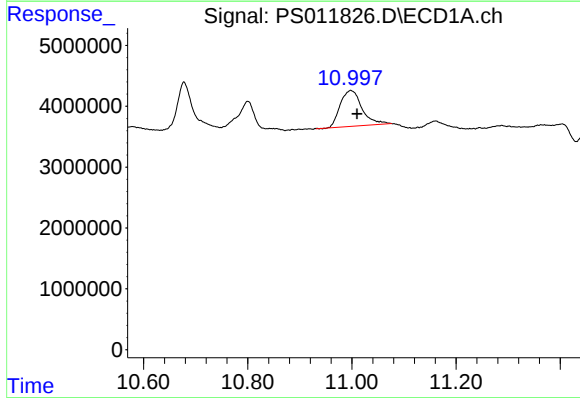

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.012 min
Response: 17036877
Conc: 2.18 ng/ml

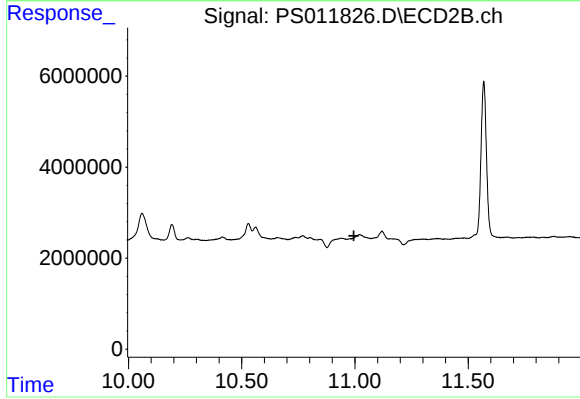

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.