

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 18:35
 Operator : DD\AJ
 Sample : L3500-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 18:56:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.916	213.8E6	135.8E6	196.026	253.859 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	51943200	N.D.	63.144
5) T	DICAMBA	7.397	7.049	6072749	11528704	1.483	5.336 #
6) T	MCP	7.630	0.000	9817598	0	3.073	N.D. #
7) T	MCPA	7.694	7.469	152.4E6	91896920	33.511	33.537
8) T	DICHLORPROP	0.000	7.740	0	15324011	N.D.	27.140
9) T	2,4-D	8.401	0.000	123.3E6	0	109.212	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	27510869	N.D.	9.410
12) T	2,4,5-T	9.413	0.000	12105701	0	2.043	N.D. #
15) T	Picloram	11.006	0.000	10672448	0	1.366	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 18:35
Operator : DD\AJ
Sample : L3500-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 18:56:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

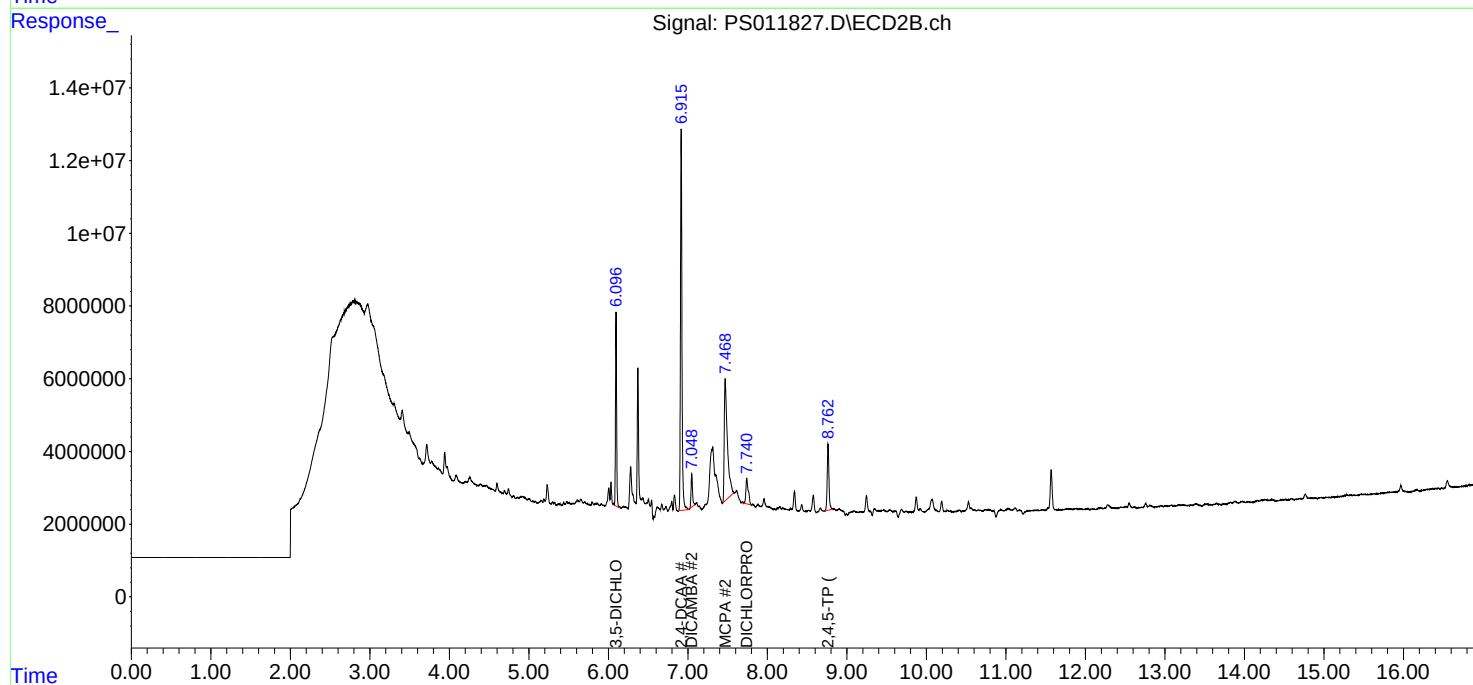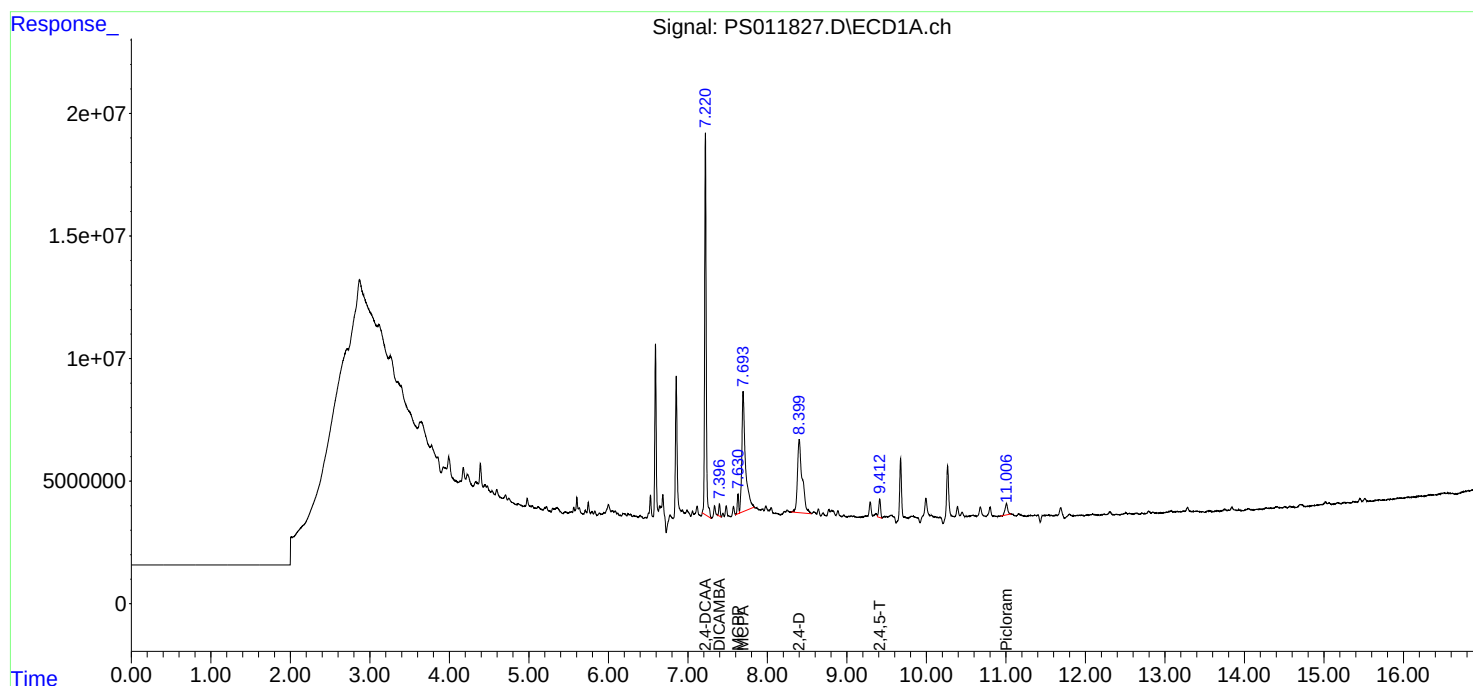


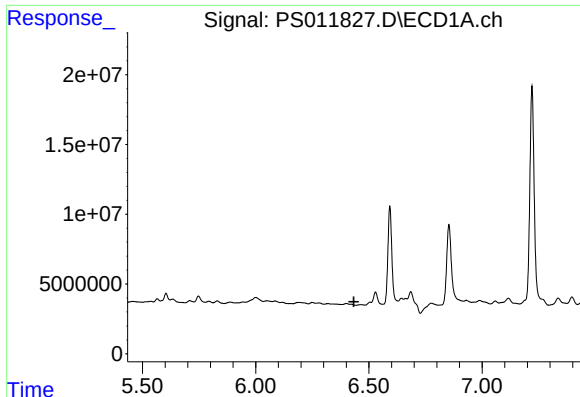

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

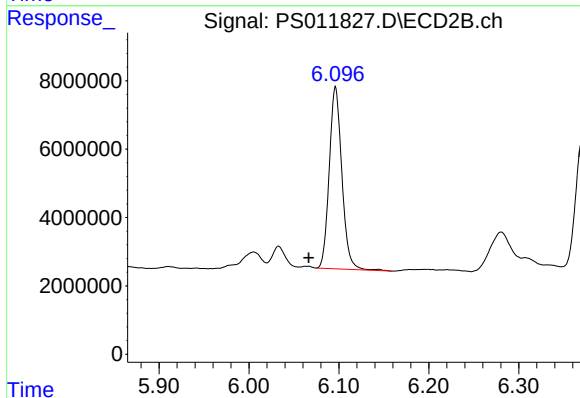


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 51943200
Conc: 63.14 ng/ml

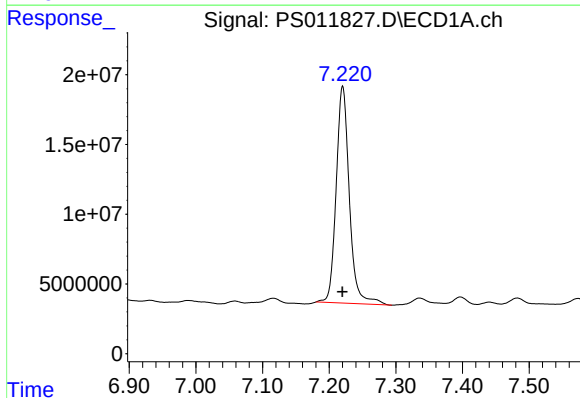


#4 2,4-DCAA

R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 213819449
Conc: 196.03 ng/ml

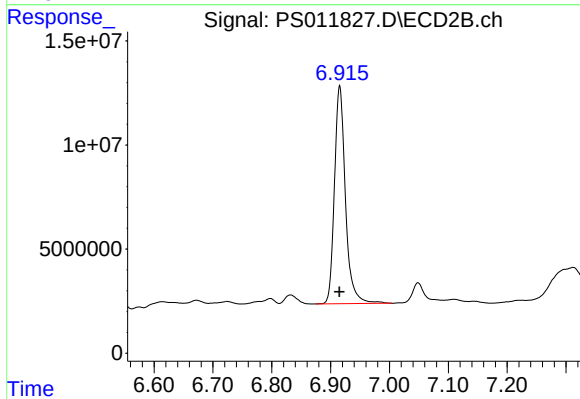

#4 2,4-DCAA


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 135760686
Conc: 253.86 ng/ml

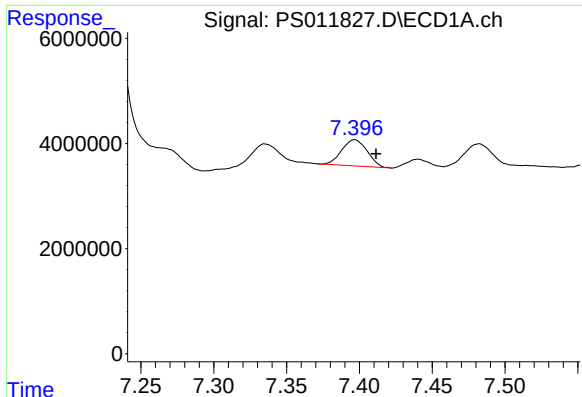

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 6072749
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

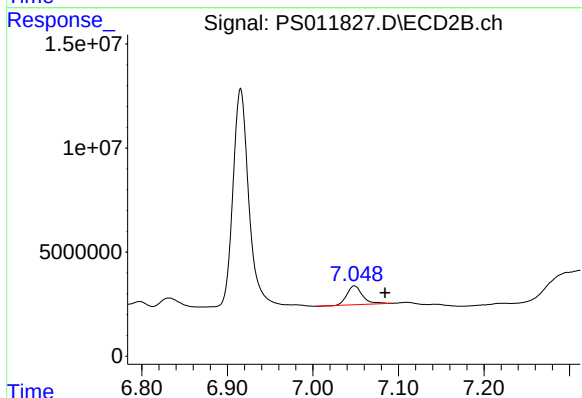


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 11528704
Conc: 5.34 ng/ml

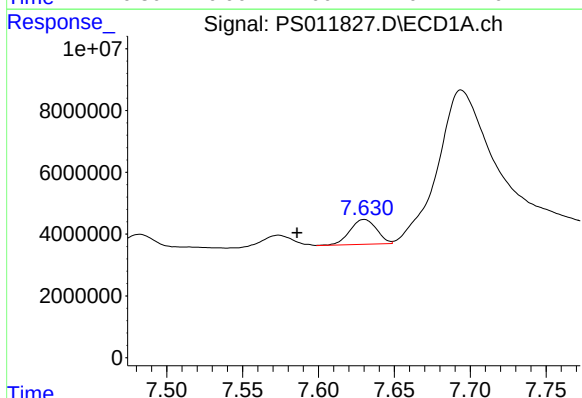


#6 MCPP

R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 9817598
Conc: 3.07 ug/ml

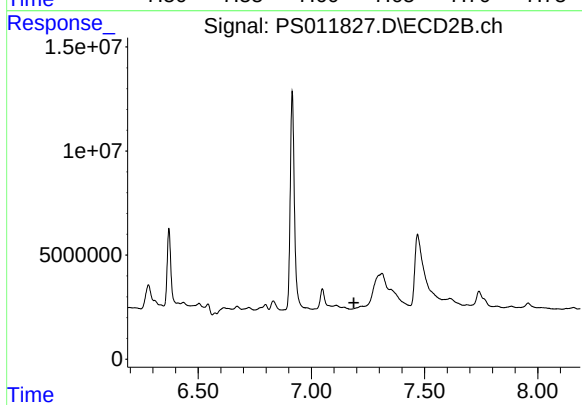

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

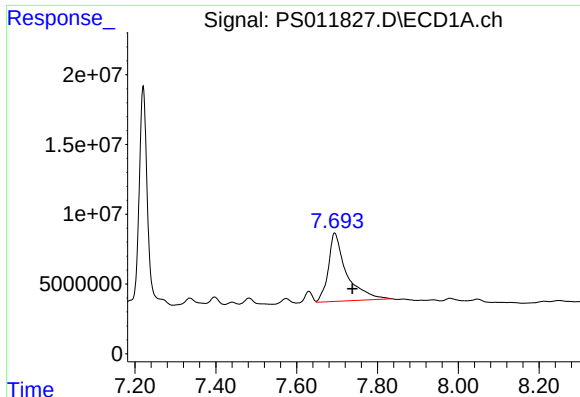

#7 MCPA


R.T.: 7.694 min
Delta R.T.: -0.044 min
Response: 152424097
Conc: 33.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

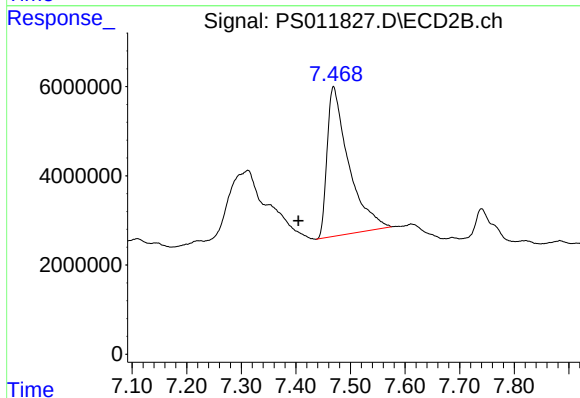


#7 MCPA

R.T.: 7.469 min
Delta R.T.: 0.064 min
Response: 91896920
Conc: 33.54 ug/ml

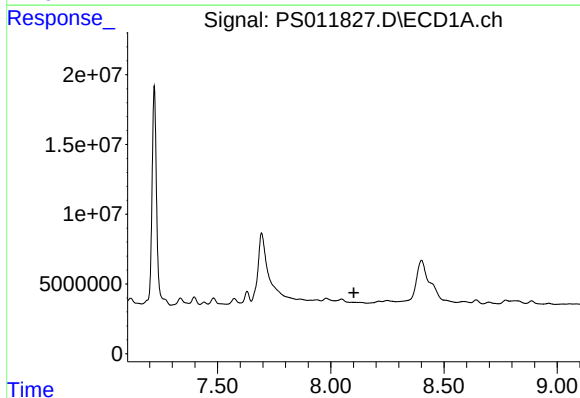


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

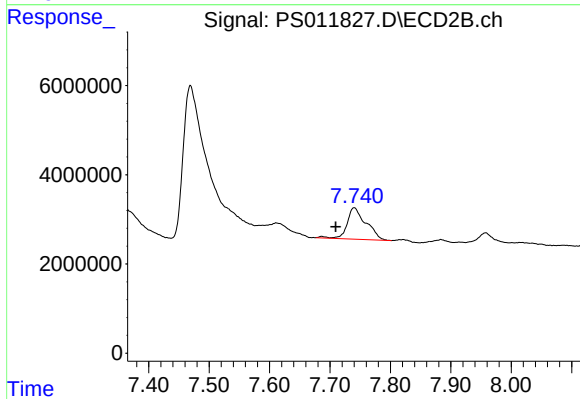

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.031 min
Response: 15324011
Conc: 27.14 ng/ml

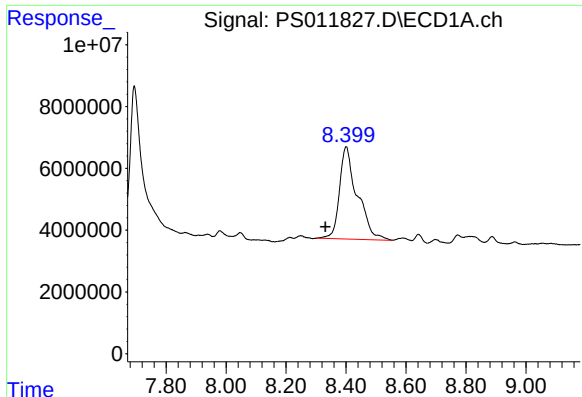

#9 2,4-D


R.T.: 8.401 min
Delta R.T.: 0.069 min
Response: 123310626
Conc: 109.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

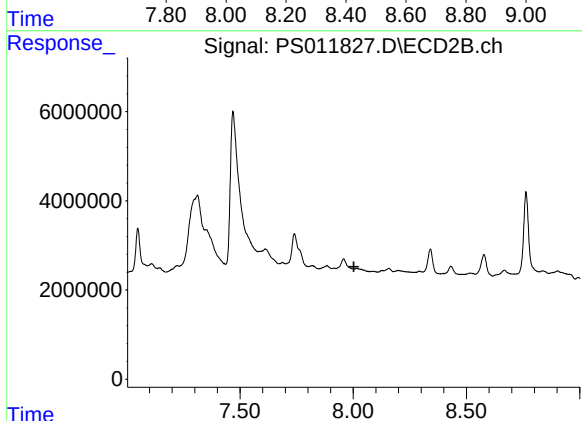


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

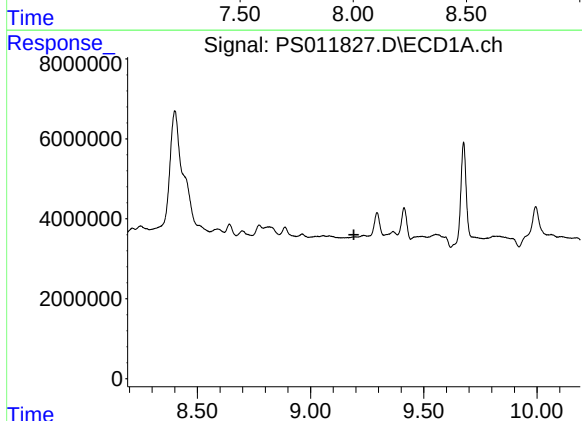


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

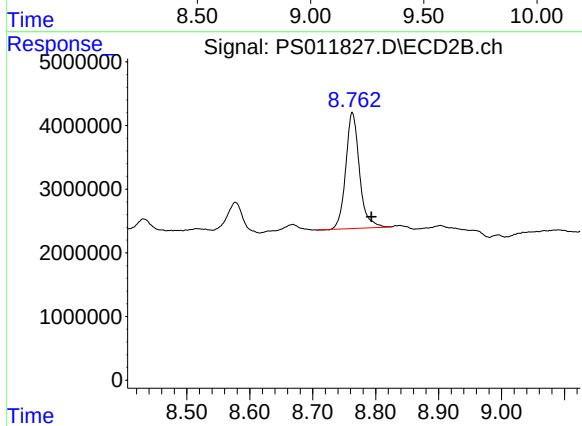

#11 2,4,5-TP (SILVEX)


R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 27510869
Conc: 9.41 ng/ml

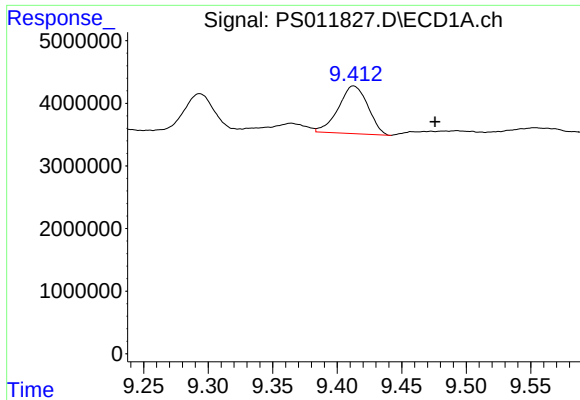

#12 2,4,5-T


R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 12105701
Conc: 2.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

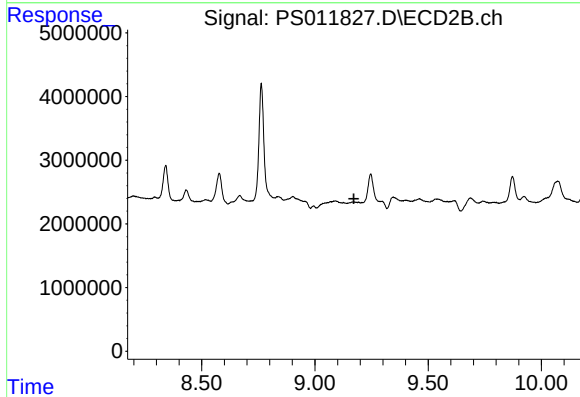


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

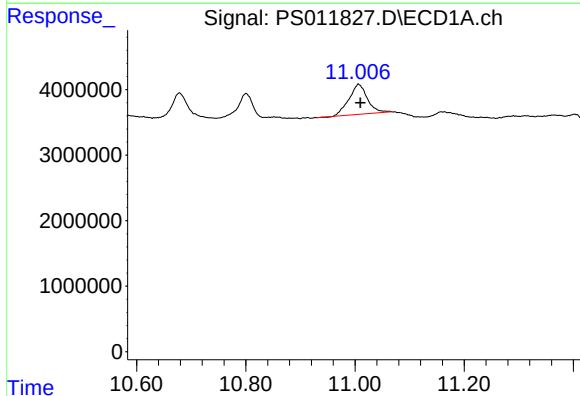

#15 Picloram

R.T.: 11.006 min
Delta R.T.: -0.003 min
Response: 10672448
Conc: 1.37 ng/ml

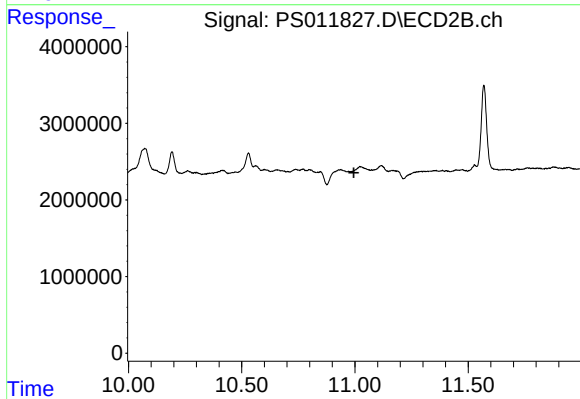

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.