

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 19:44
 Operator : DD\AJ
 Sample : L3508-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:47:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	251.2E6	157.4E6	230.288	294.250 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	27214638	N.D.	33.083
5) T	DICAMBA	0.000	7.049	0	7137141	N.D.	3.303
6) T	MCP	7.629	0.000	4704466	0	1.472	N.D. #
7) T	MCPA	7.689	7.463	210.5E6	154.3E6	46.281	56.309
8) T	DICHLORPROP	0.000	7.739	0	11552684	N.D.	20.460
9) T	2,4-D	8.399	0.000	129.7E6	0	114.878	N.D. #
11) T	2,4,5-TP ...	0.000	8.786	0	145.1E6	N.D.	49.646
12) T	2,4,5-T	9.411	0.000	13143549	0	2.218	N.D. #
14) T	DINOSEB	0.000	10.058	0	14962233	N.D.	7.038
15) T	Picloram	11.005	0.000	20587200	0	2.634	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 19:44
Operator : DD\AJ
Sample : L3508-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:47:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

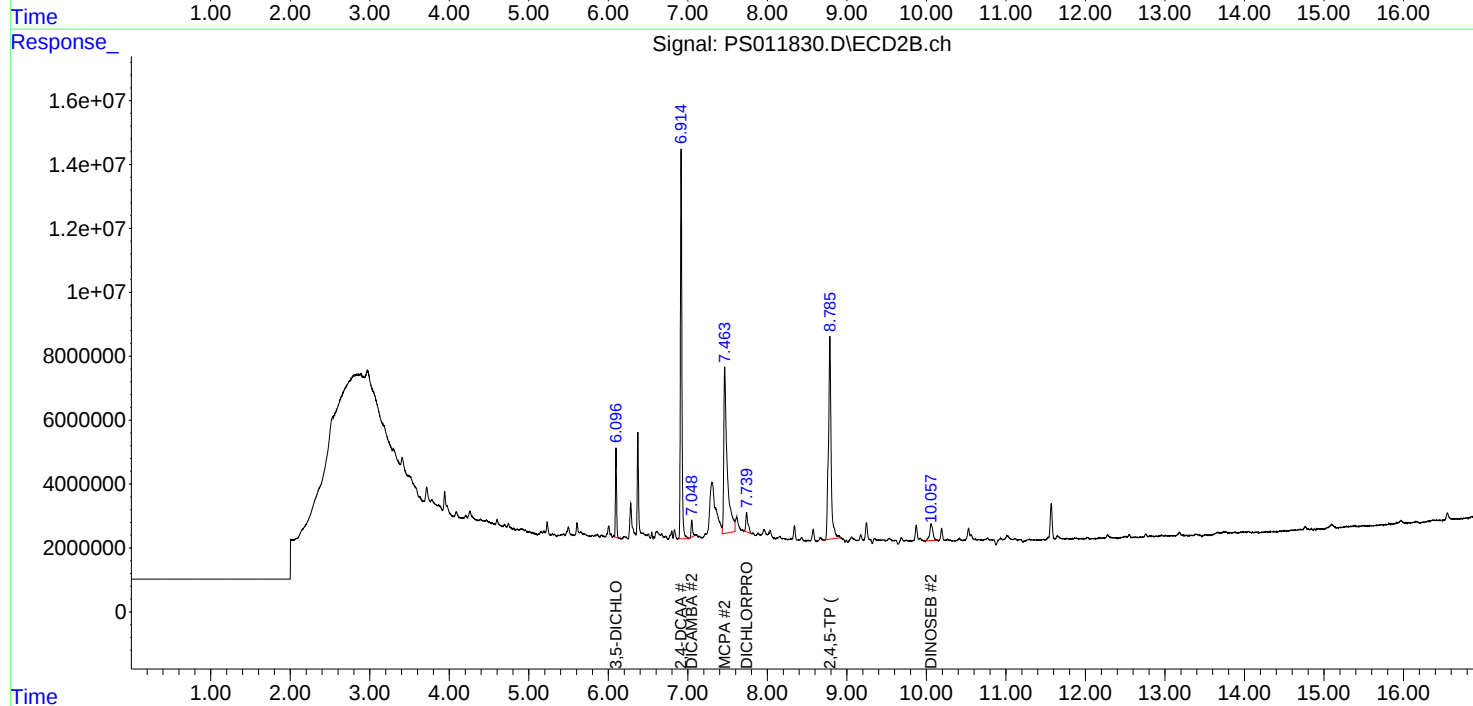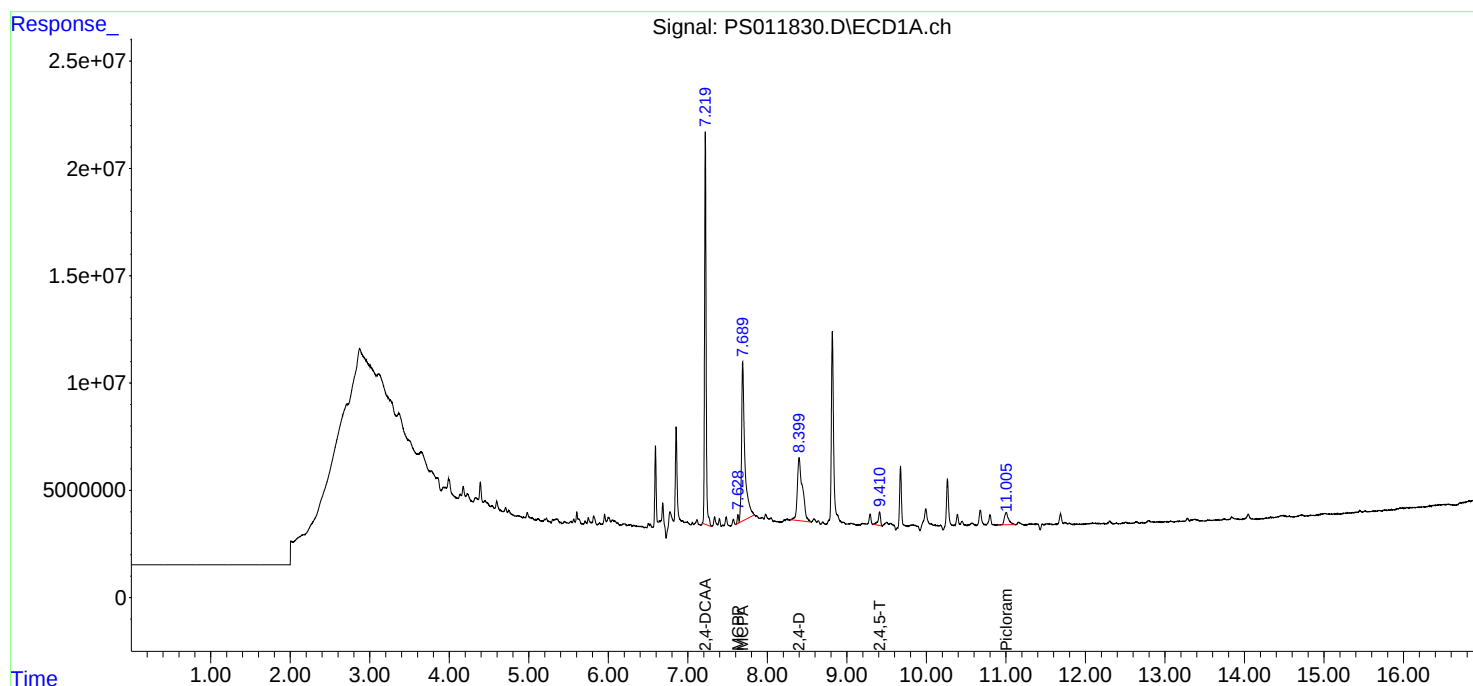


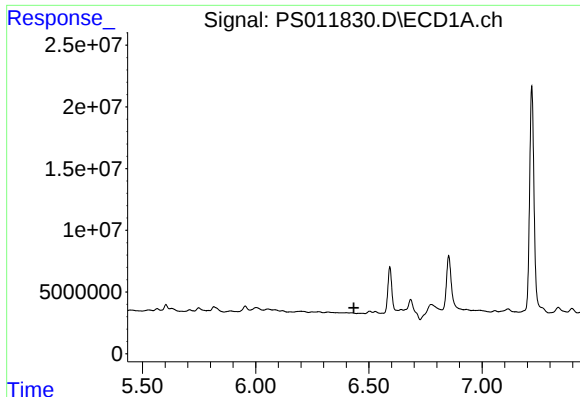

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

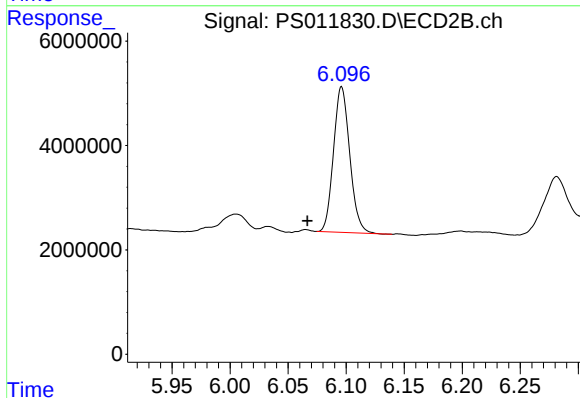


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 27214638
Conc: 33.08 ng/ml

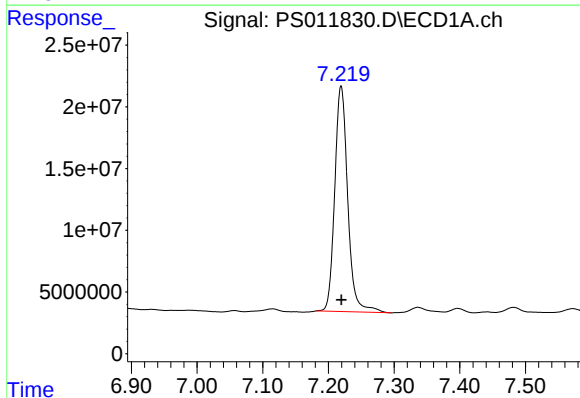


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 251191065
Conc: 230.29 ng/ml

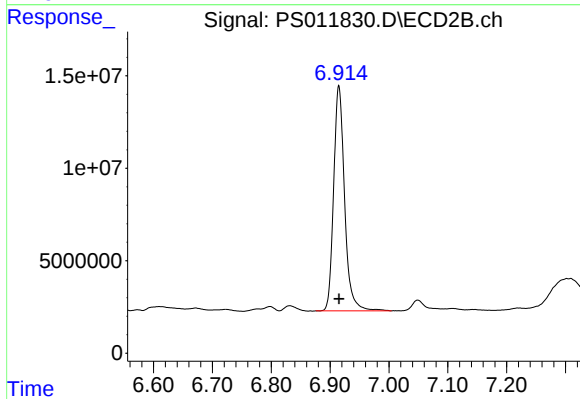

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 157361140
Conc: 294.25 ng/ml

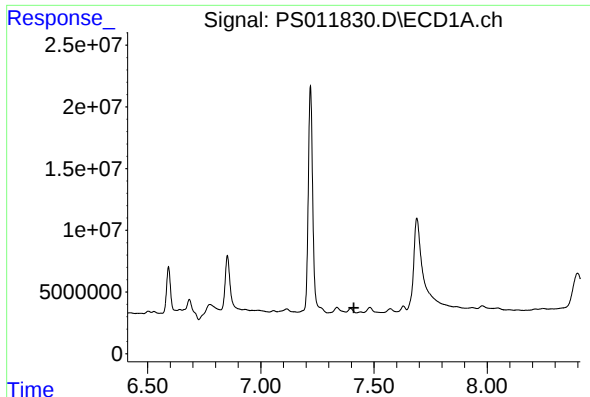

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

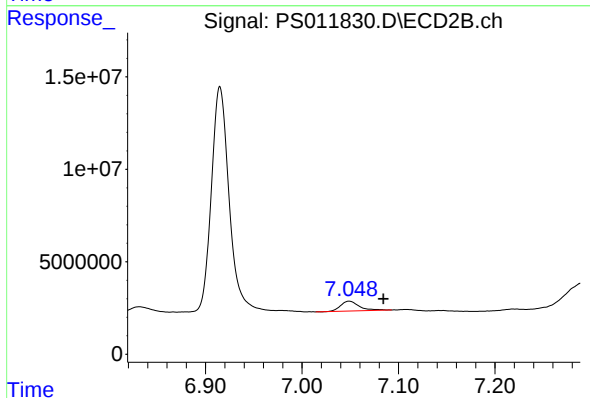


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 7137141
Conc: 3.30 ng/ml

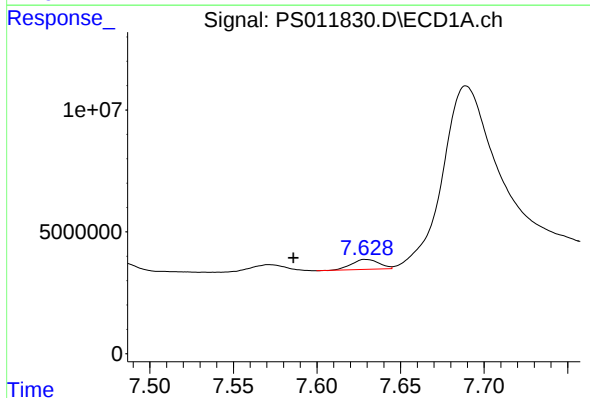


#6 MCP

R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 4704466
Conc: 1.47 ug/ml

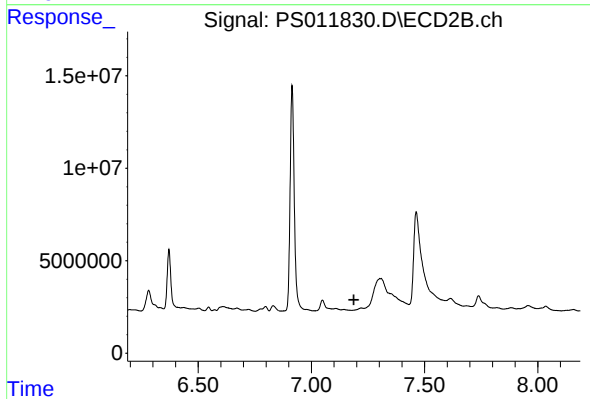

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

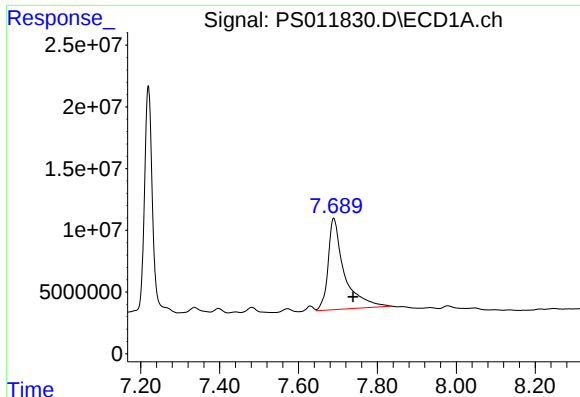

#7 MCPA


R.T.: 7.689 min
Delta R.T.: -0.049 min
Response: 210506259
Conc: 46.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

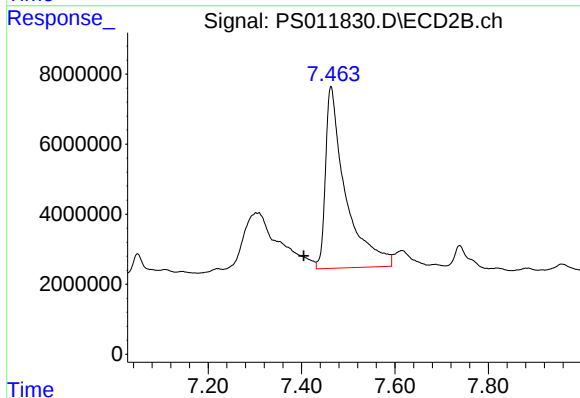


#7 MCPA

R.T.: 7.463 min
Delta R.T.: 0.058 min
Response: 154293825
Conc: 56.31 ug/ml

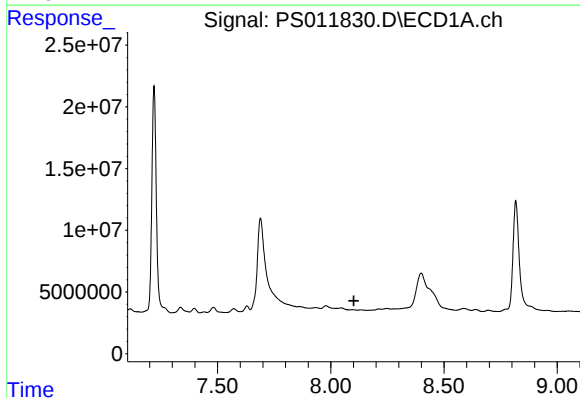


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

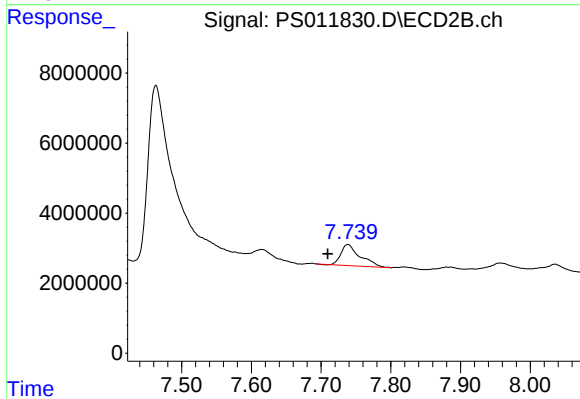

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 11552684
Conc: 20.46 ng/ml

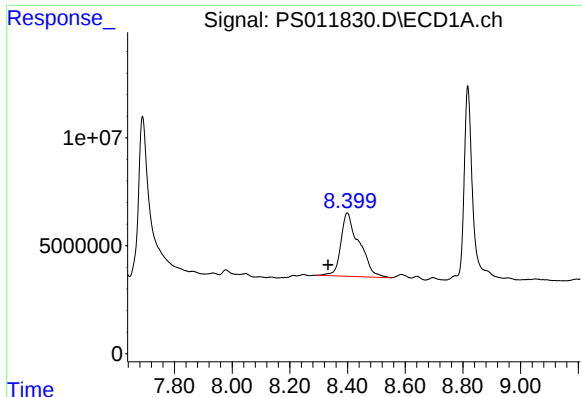

#9 2,4-D


R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 129707497
Conc: 114.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

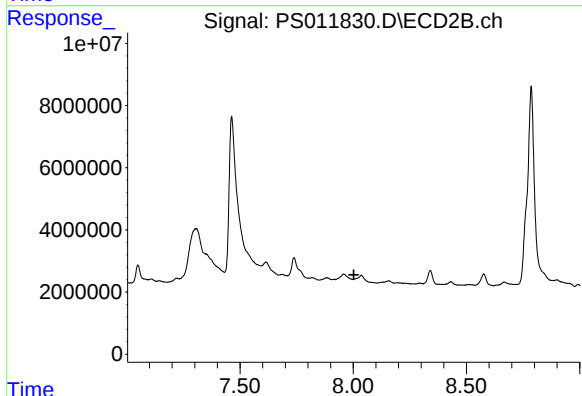


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

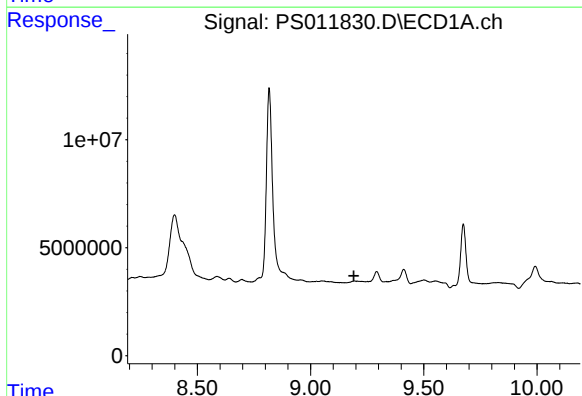


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

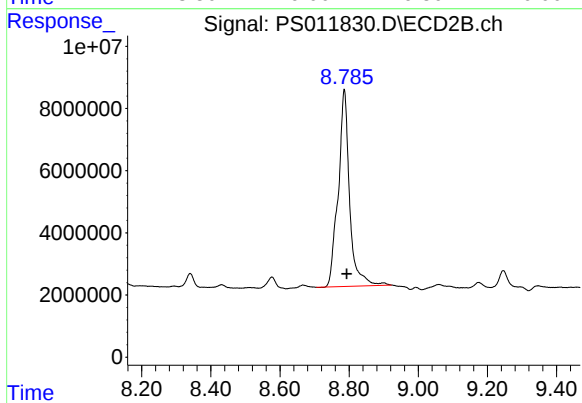

#11 2,4,5-TP (SILVEX)


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 145145956
Conc: 49.65 ng/ml

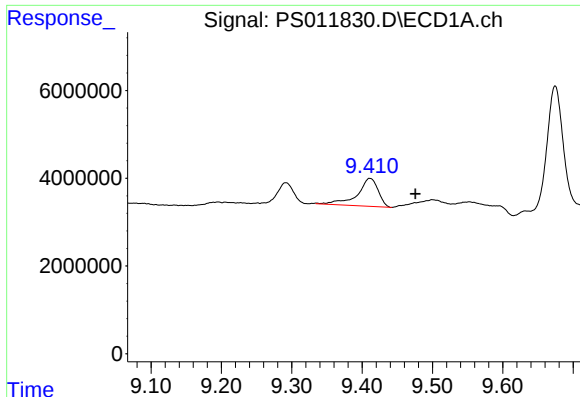

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 13143549
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

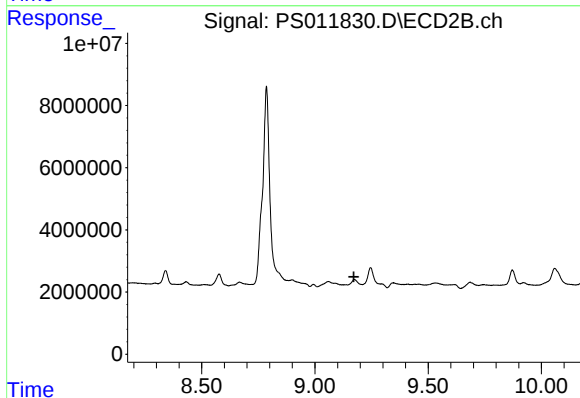


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

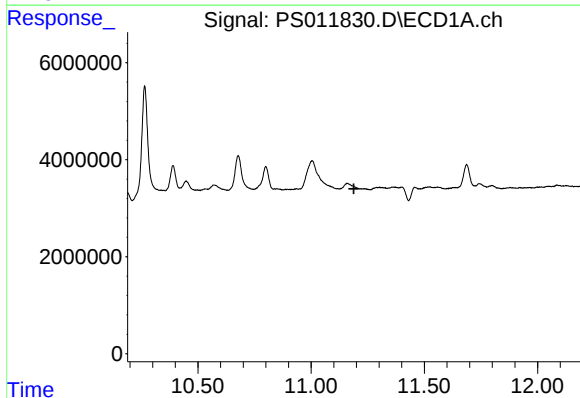


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

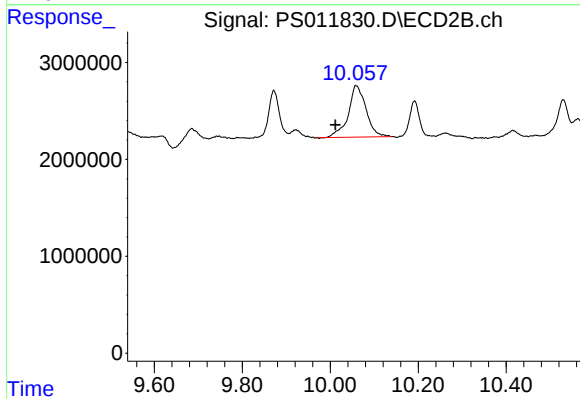

#14 DINOSEB


R.T.: 10.058 min
Delta R.T.: 0.047 min
Response: 14962233
Conc: 7.04 ng/ml

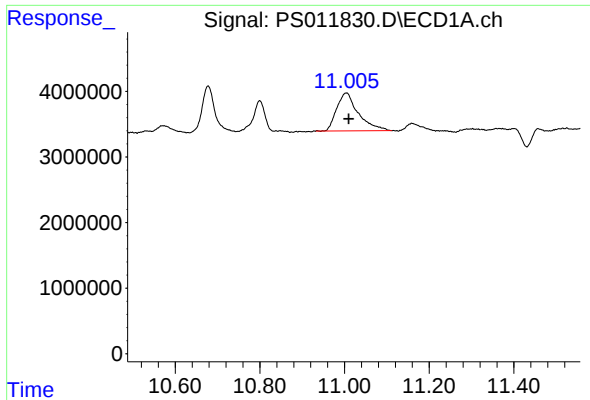

#15 Picloram

R.T.: 11.005 min
Delta R.T.: -0.005 min
Response: 20587200
Conc: 2.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

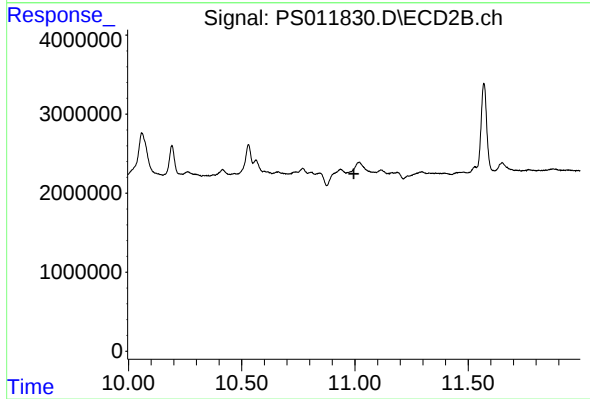

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.