

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
 Data File : PS011831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 20:07
 Operator : DD\AJ
 Sample : PB131039BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:47:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	508.4E6	309.4E6	466.105	578.576
Target Compounds							
2) T	3,5-DICHL...	0.000	6.097	0	61065455	N.D.	74.233
5) T	DICAMBA	7.397	7.049	8981500	10209373	2.193	4.725 #
6) T	MCP	7.630	0.000	11018067	0	3.448	N.D. #
7) T	MCPA	7.766	7.376	31382967	38375757	6.900	14.005 #
9) T	2,4-D	8.400	0.000	132.0E6	0	116.870	N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	25071098	N.D.	8.575
12) T	2,4,5-T	9.495	0.000	10468653	0	1.767	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081820\
Data File : PS011831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 20:07
Operator : DD\AJ
Sample : PB131039BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:47:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

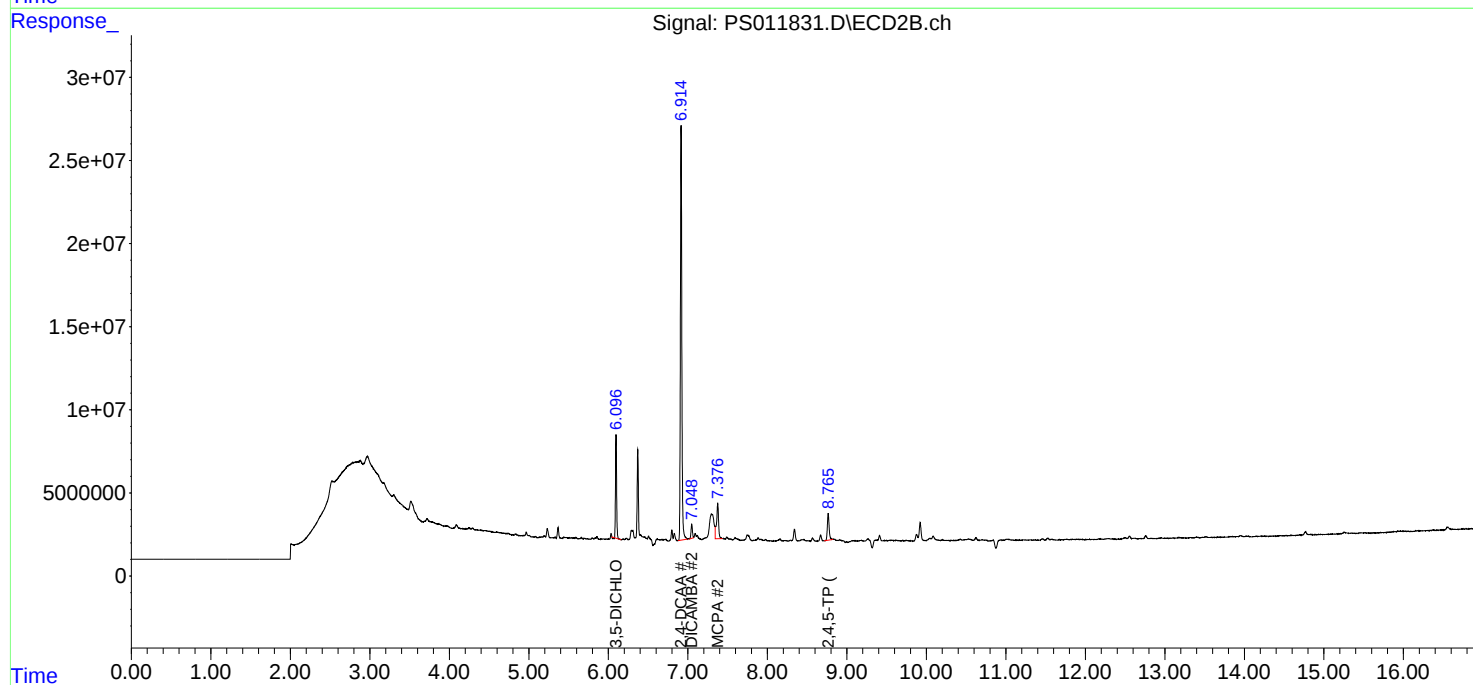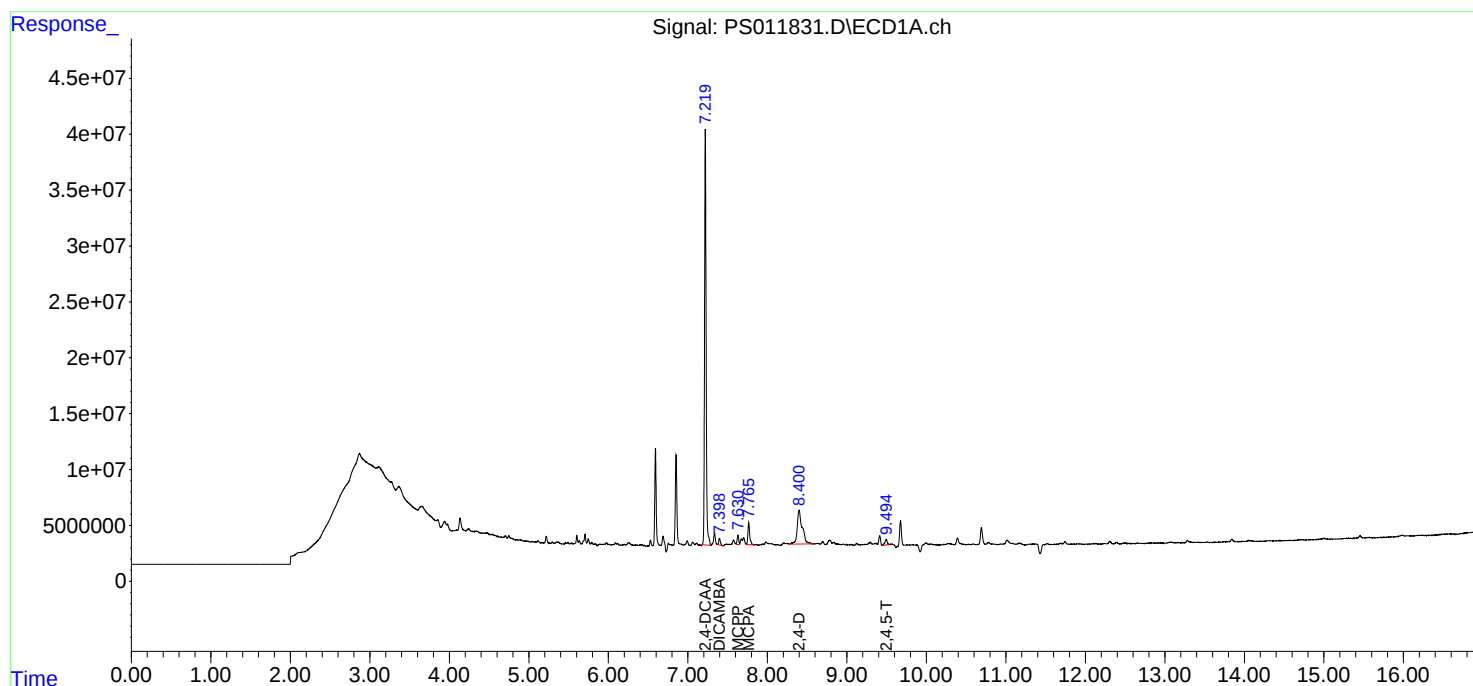


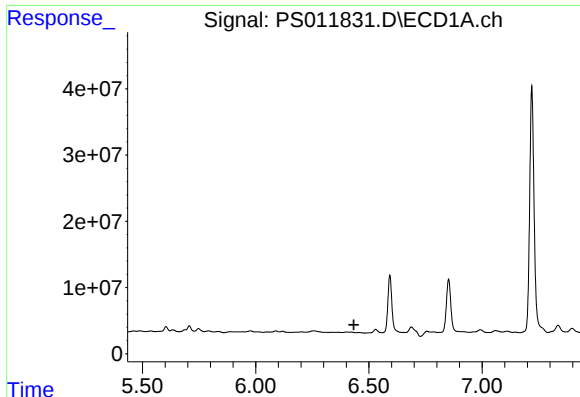

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

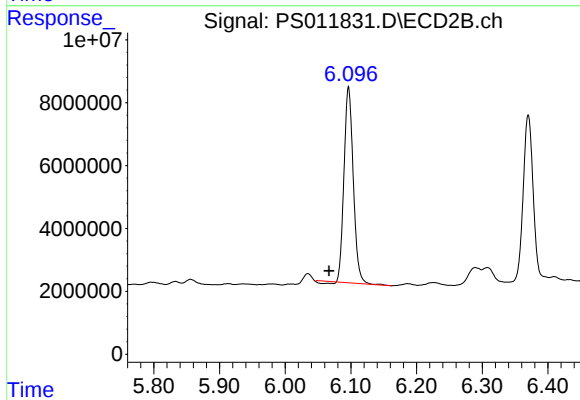


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.097 min
Delta R.T.: 0.030 min
Response: 61065455
Conc: 74.23 ng/ml

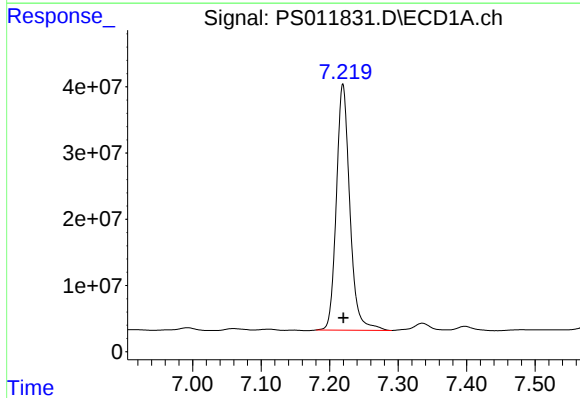


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 508412297
Conc: 466.10 ng/ml

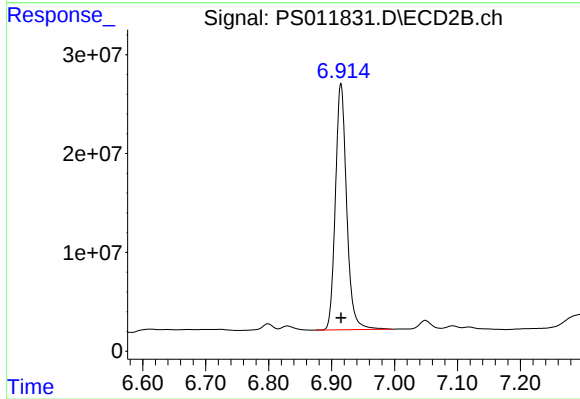

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 309414659
Conc: 578.58 ng/ml

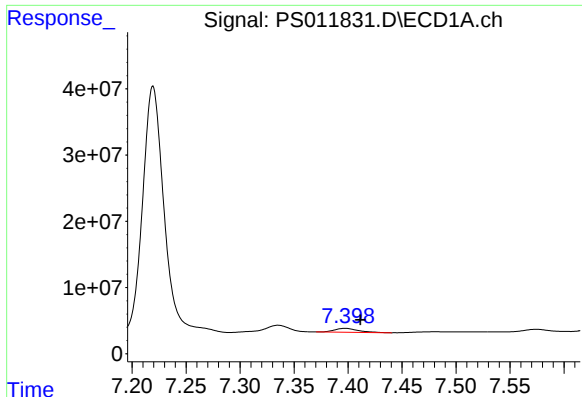

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: -0.014 min
Response: 8981500
Conc: 2.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

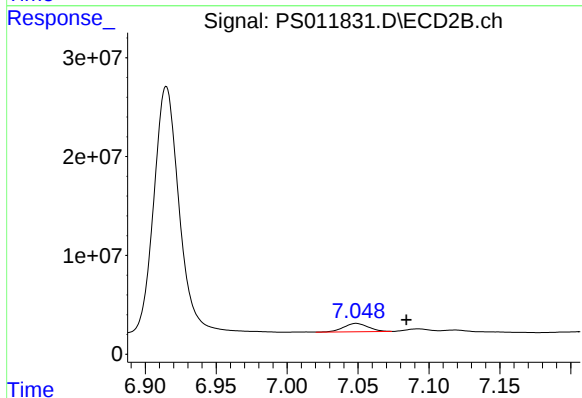


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 10209373
Conc: 4.73 ng/ml

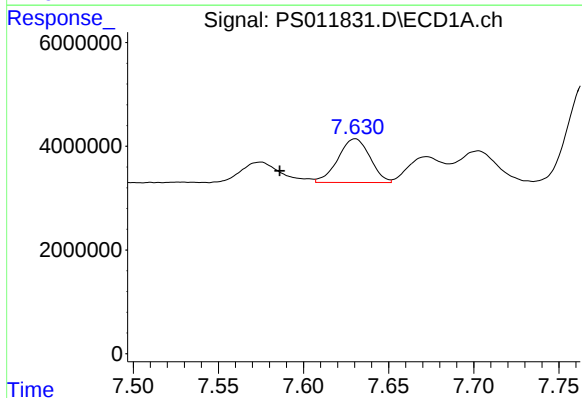


#6 MCP

R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 11018067
Conc: 3.45 ug/ml

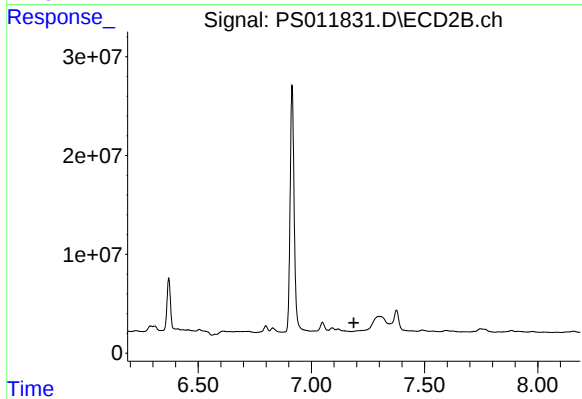

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

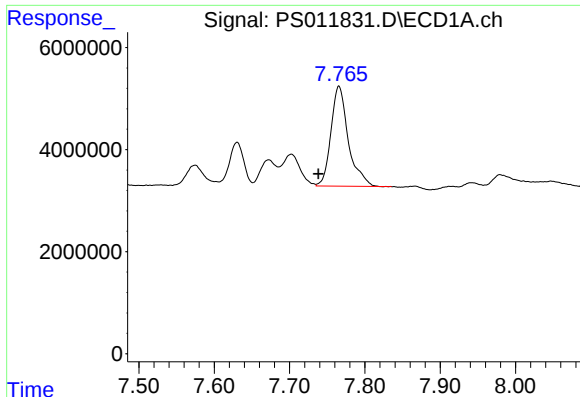

#7 MCPA


R.T.: 7.766 min
Delta R.T.: 0.027 min
Response: 31382967
Conc: 6.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

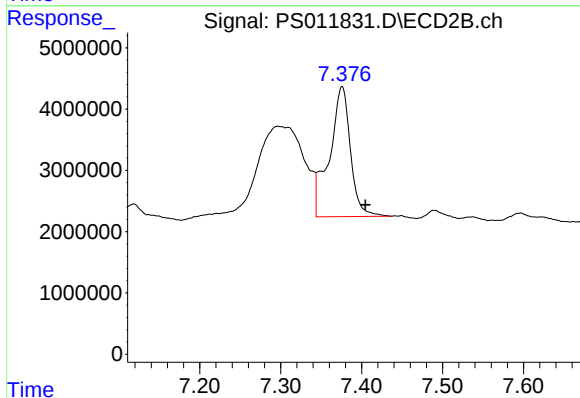


#7 MCPA

R.T.: 7.376 min
Delta R.T.: -0.029 min
Response: 38375757
Conc: 14.01 ug/ml

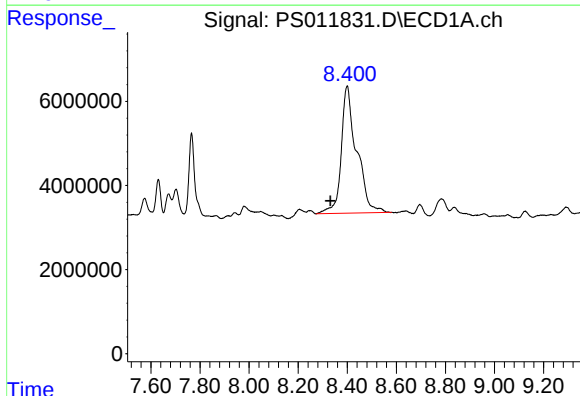


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 131957529
Conc: 116.87 ng/ml

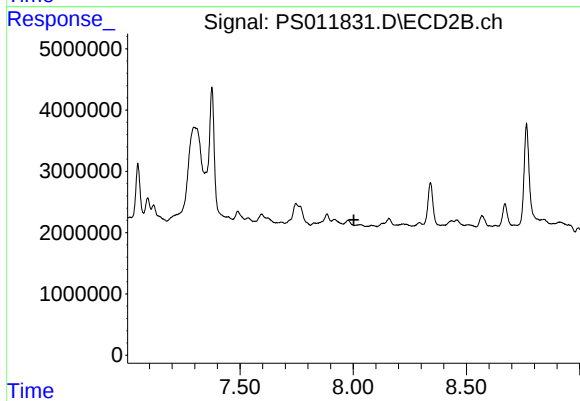

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

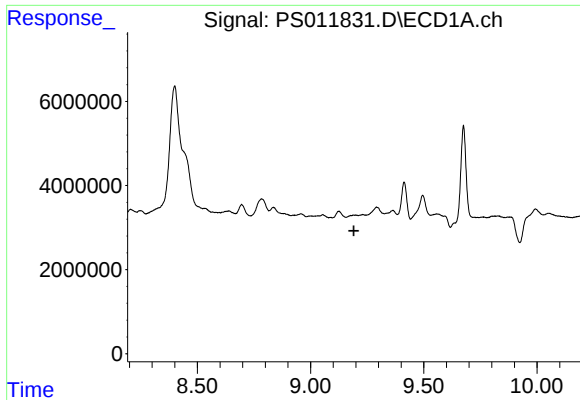

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

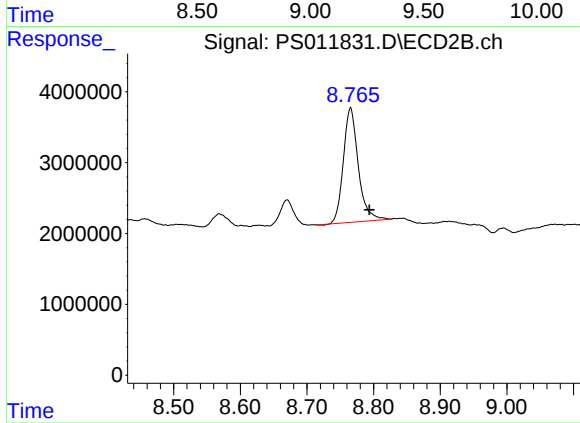


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: -0.028 min
Response: 25071098
Conc: 8.58 ng/ml

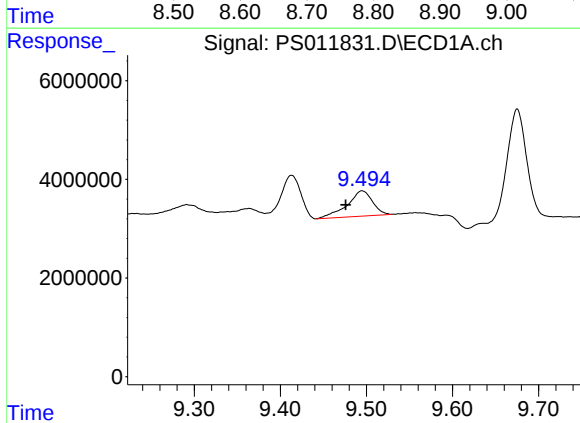

#12 2,4,5-T

R.T.: 9.495 min
Delta R.T.: 0.019 min
Response: 10468653
Conc: 1.77 ng/ml

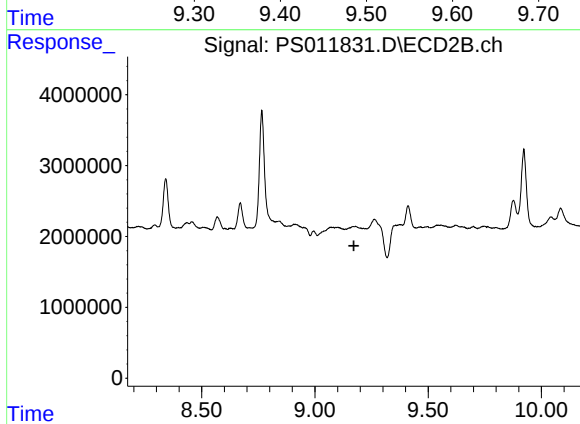

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.