

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081821\
 Data File : PS016476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 12:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 00:48:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	0.000	6.925	0	4620187	N.D.	2.120
6) T	MCP	0.000	7.050	0	1573200	N.D.	<MDL
7) T	MCPA	7.643f	0.000	10848218	0	1.761	N.D. #
10) T	Pentachlo...	8.606	8.262	9719172	4153115	<MDL	<MDL #
11) T	2,4,5-TP ...	9.159	8.624	7445076	3244637	1.030	1.112
12) T	2,4,5-T	9.447	9.005	10603949	4790550	1.391	1.654
14) T	DINOSEB	0.000	9.834	0	2742635	N.D.	1.346
15) T	Picloram	10.978	10.817	175.8E6	77331292	17.617	19.205
16) T	DCPA	11.414	10.762	13895798	6890173	1.315	1.533


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081821\
Data File : PS016476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 12:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 00:48:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

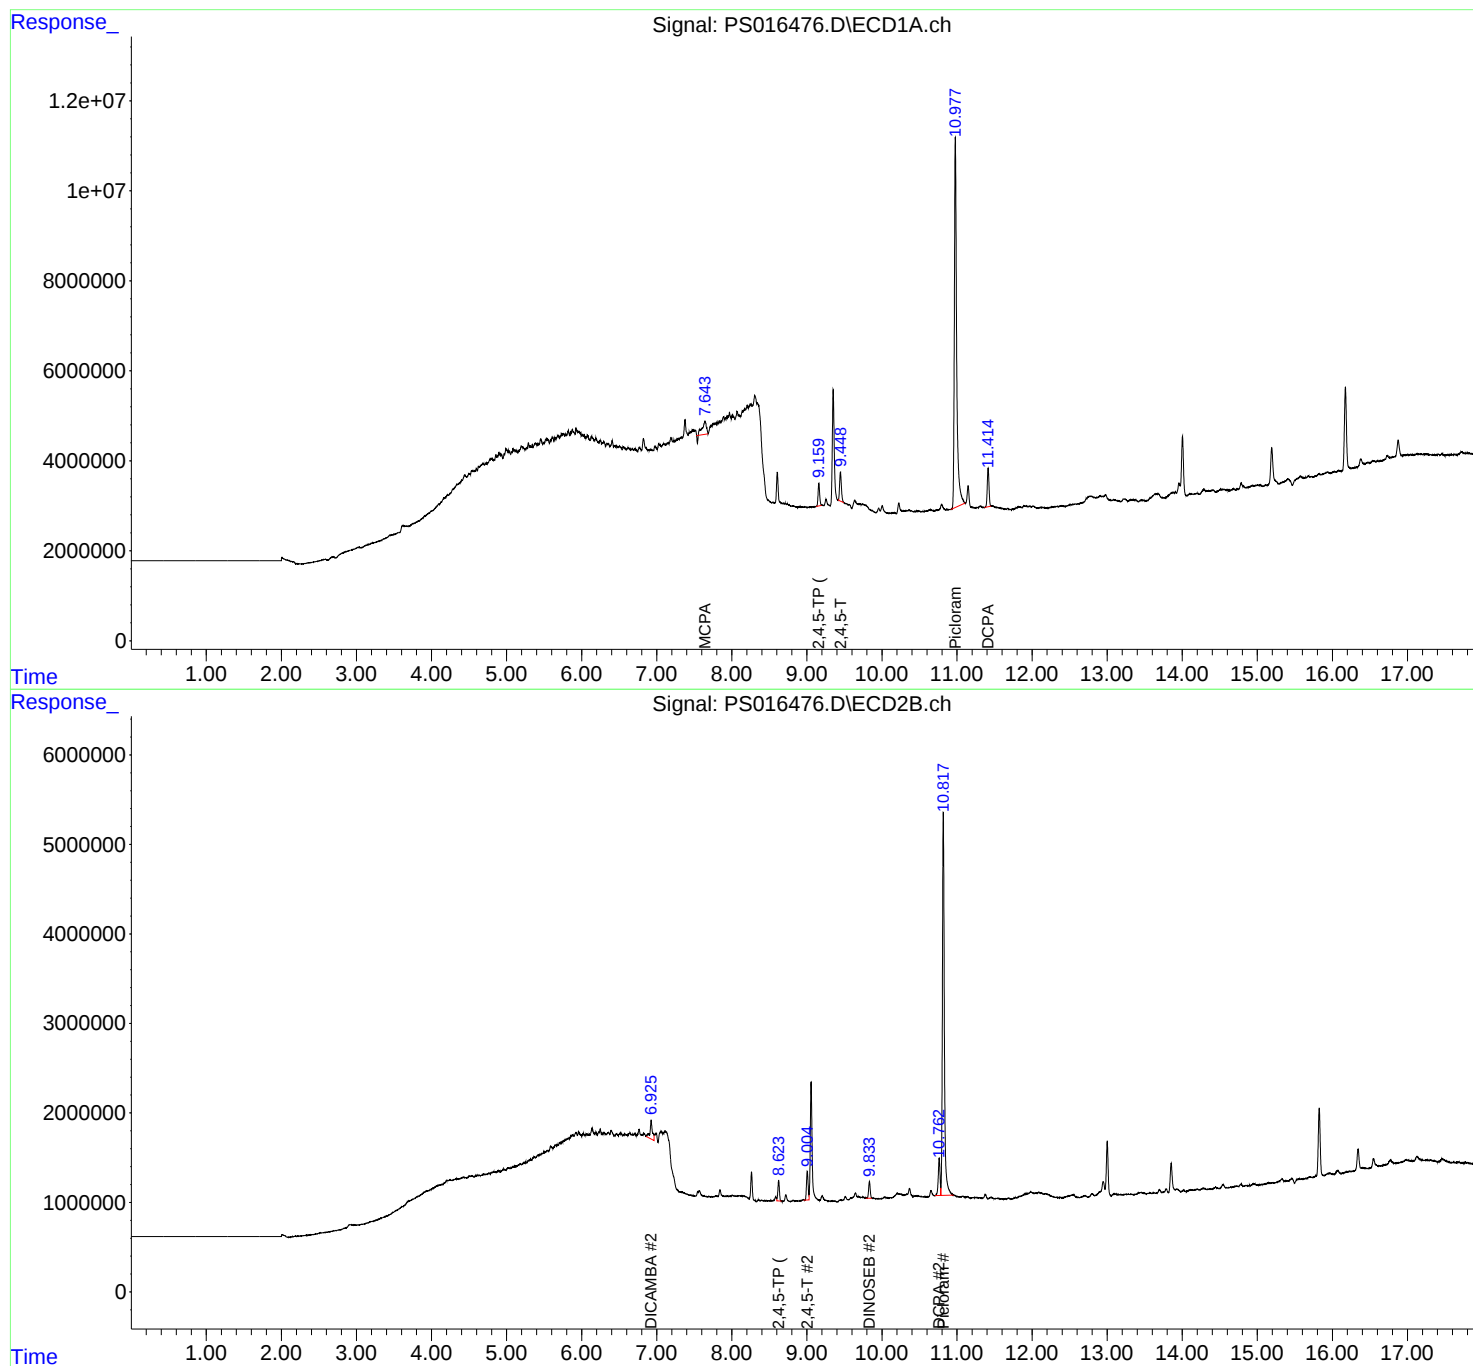


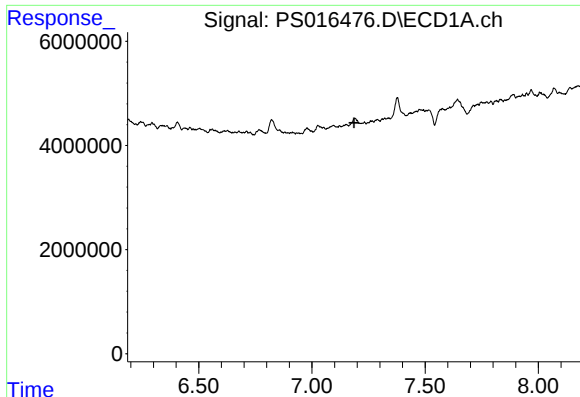

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

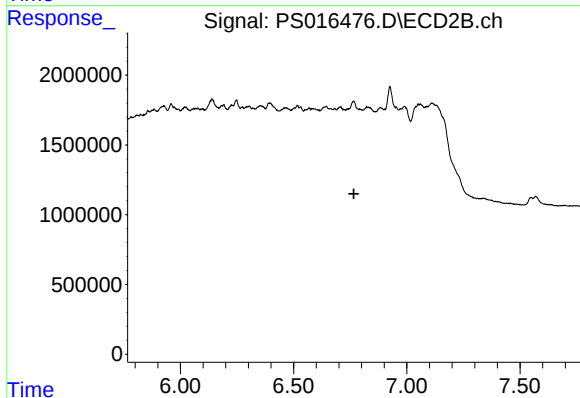


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.766 min
Response: 0
Conc: N.D.

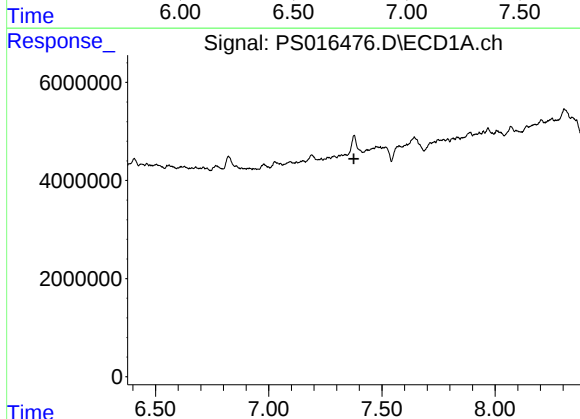


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

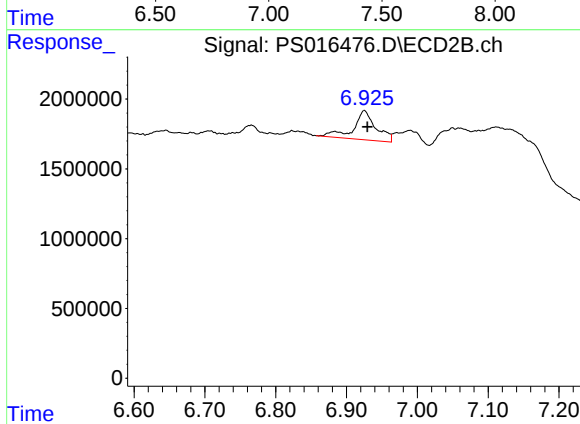

#5 DICAMBA


R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 4620187
Conc: 2.12 ng/ml

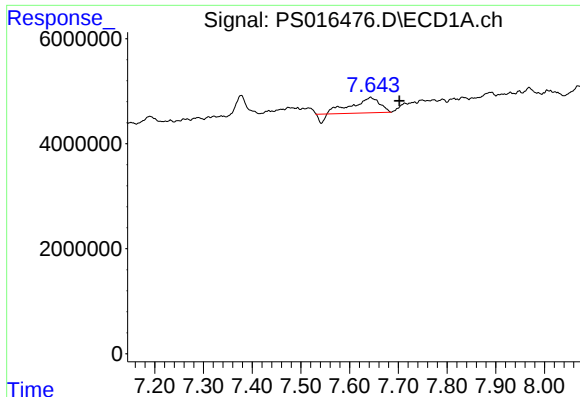

#7 MCPA


R.T.: 7.643 min
Delta R.T.: -0.059 min
Response: 10848218
Conc: 1.76 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

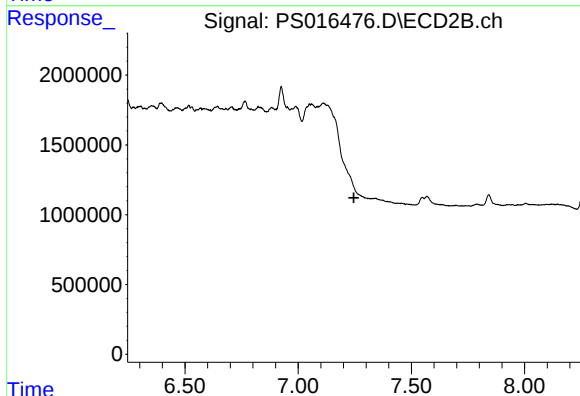


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.246 min
Response: 0
Conc: N.D.

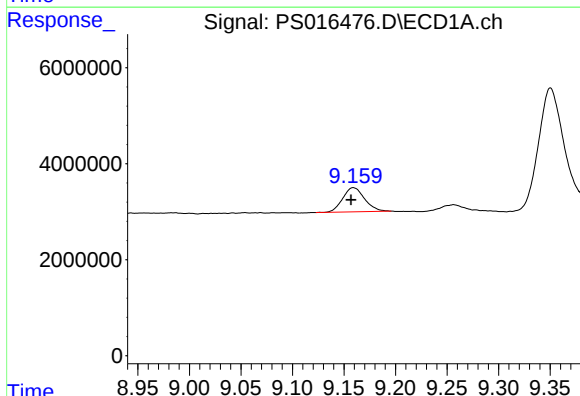


#11 2,4,5-TP (SILVEX)

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 7445076
Conc: 1.03 ng/ml

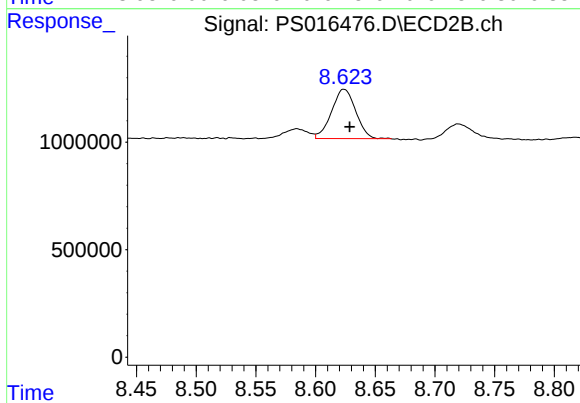

#11 2,4,5-TP (SILVEX)


R.T.: 8.624 min
Delta R.T.: -0.005 min
Response: 3244637
Conc: 1.11 ng/ml

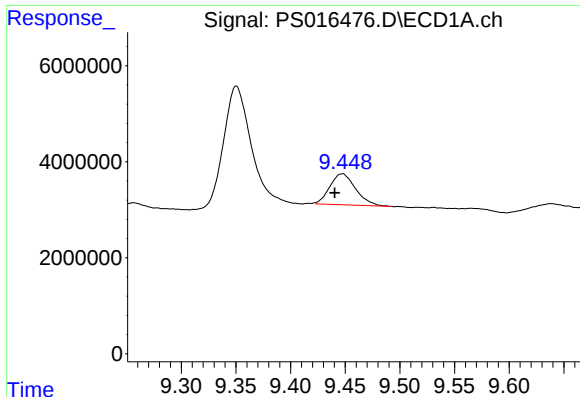

#12 2,4,5-T


R.T.: 9.447 min
Delta R.T.: 0.007 min
Response: 10603949
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

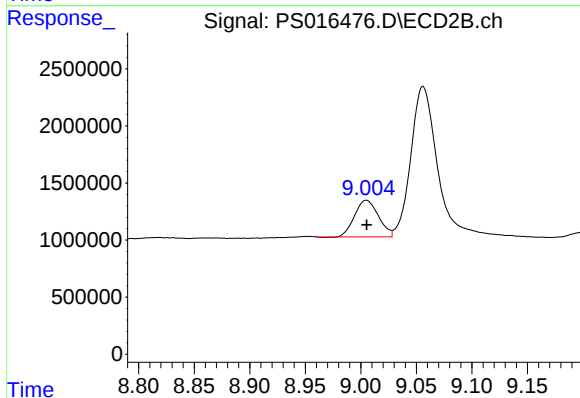


#12 2,4,5-T

R.T.: 9.005 min
Delta R.T.: 0.000 min
Response: 4790550
Conc: 1.65 ng/ml

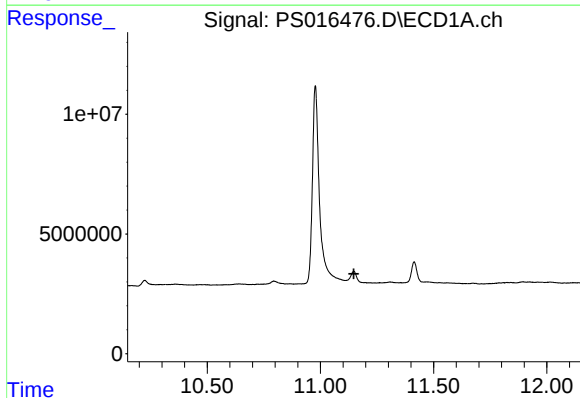


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.148 min
Response: 0
Conc: N.D.

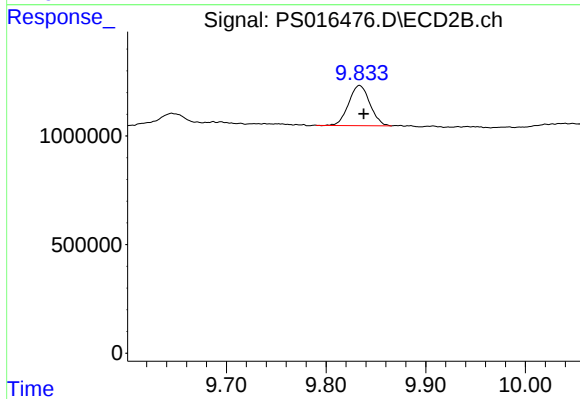

#14 DINOSEB


R.T.: 9.834 min
Delta R.T.: -0.004 min
Response: 2742635
Conc: 1.35 ng/ml

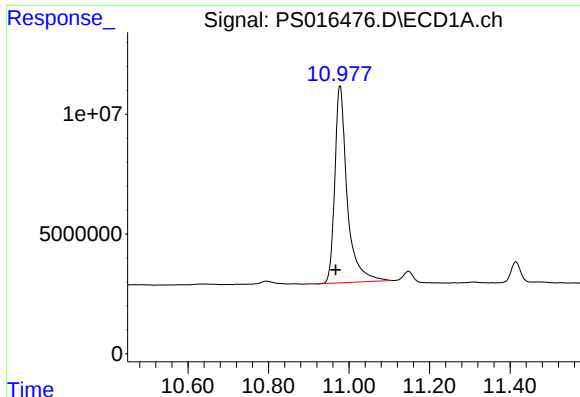

#15 Picloram


R.T.: 10.978 min
Delta R.T.: 0.011 min
Response: 175831969
Conc: 17.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

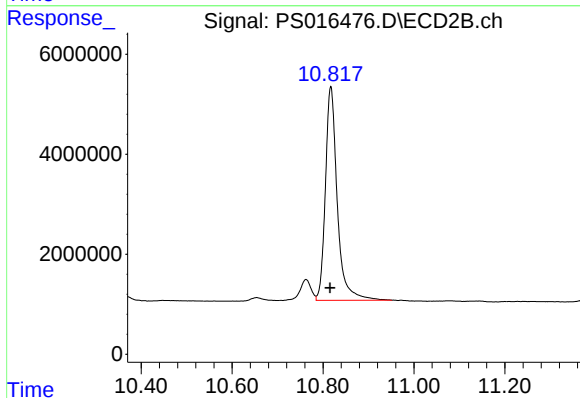


#15 Picloram

R.T.: 10.817 min
Delta R.T.: 0.002 min
Response: 77331292
Conc: 19.20 ng/ml

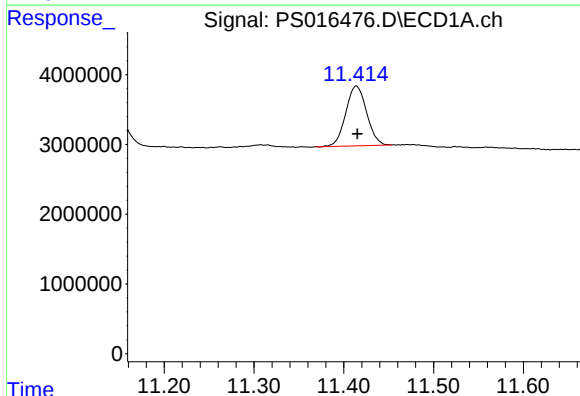

#16 DCPA

R.T.: 11.414 min
Delta R.T.: -0.001 min
Response: 13895798
Conc: 1.31 ng/ml

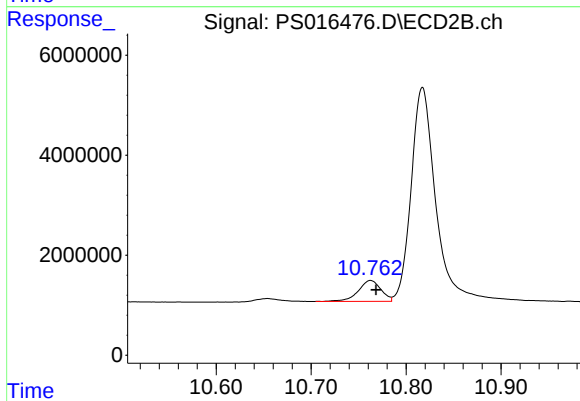

#16 DCPA

R.T.: 10.762 min
Delta R.T.: -0.006 min
Response: 6890173
Conc: 1.53 ng/ml