

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081825\
 Data File : PS031475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 09:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 11:50:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.291	7.745	1546.9E6	425.9E6	487.357	503.874
Target Compounds							
1) T	Dalapon	2.718f	0.000	27696620	0	5.277	N.D. #
2) T	3,5-DICHL...	6.462	0.000	335849	0	<MDL	N.D. #
6) T	MCP	7.623f	0.000	787640	0	<MDL	N.D. #
7) T	MCPA	7.830	8.250f	1389050	43460887	<MDL	15.491 #
8) T	DICHLORPROP	8.186	0.000	2438064	0	<MDL	N.D. #
10) T	Pentachlo...	8.716	9.513	7316972	5884803	<MDL	<MDL #
11) T	2,4,5-TP ...	9.297	9.904	3622126	11078687	<MDL	<MDL #
12) T	2,4,5-T	9.612	0.000	3921739	0	<MDL	N.D. #
13) T	2,4-DB	10.174	0.000	1903596	0	<MDL	N.D. #
14) T	DINOSEB	11.365	0.000	3915270	0	<MDL	N.D. #
15) T	Picloram	11.182	0.000	1664757	0	<MDL	N.D. #
16) T	DCPA	11.665	12.314	6083992	2884062	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081825\
Data File : PS031475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 09:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 11:50:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

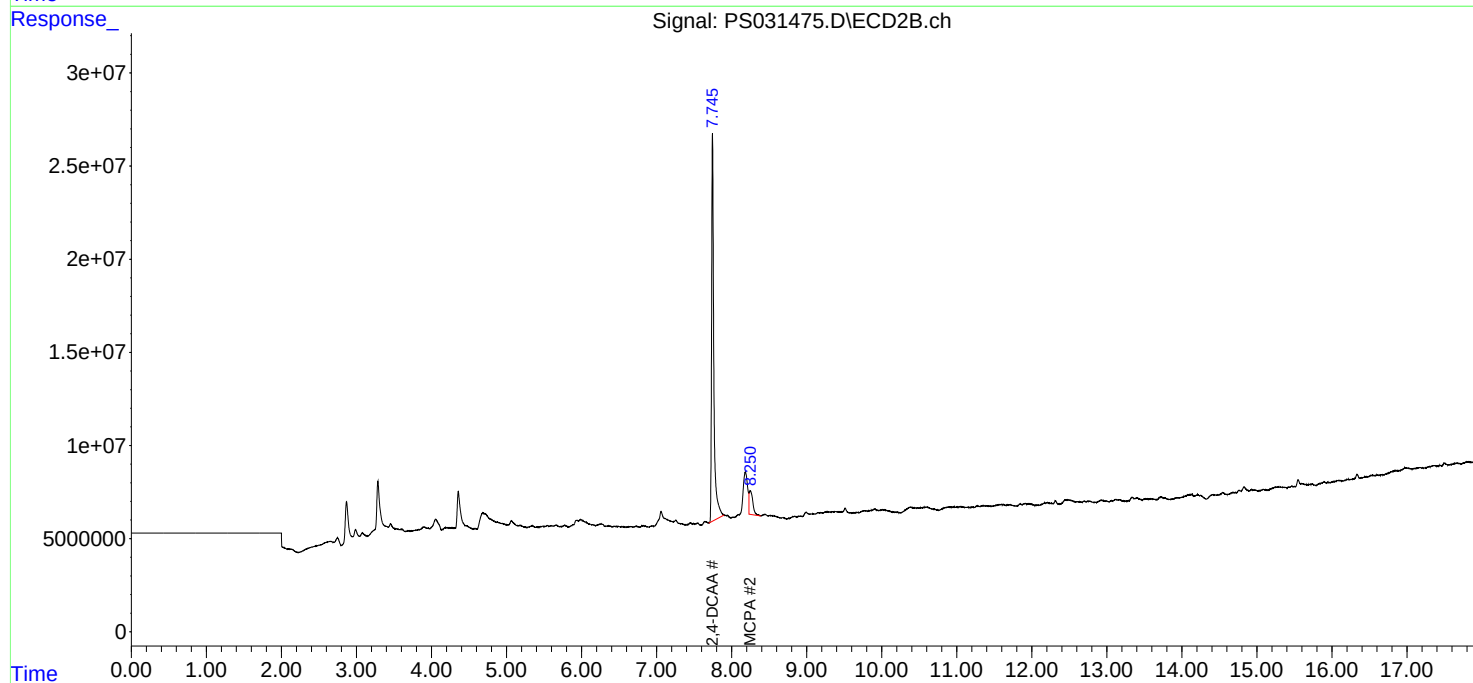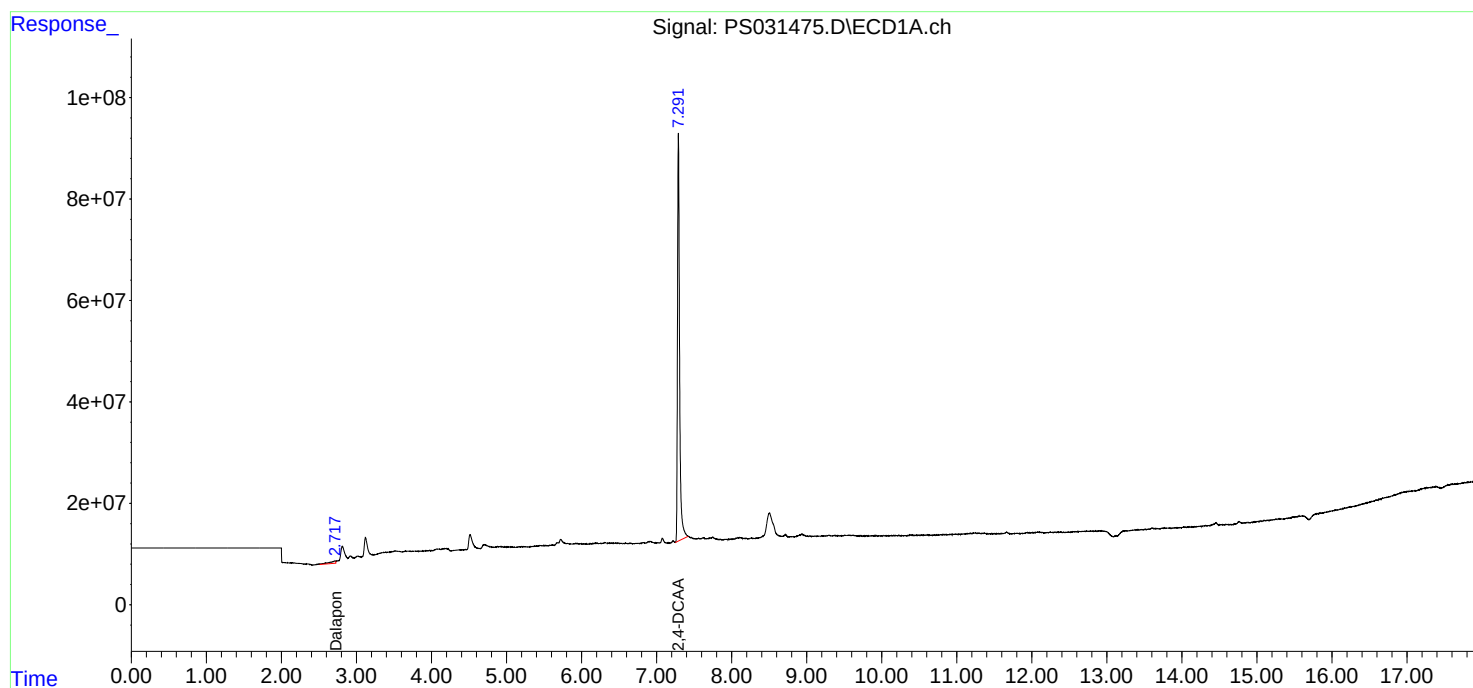


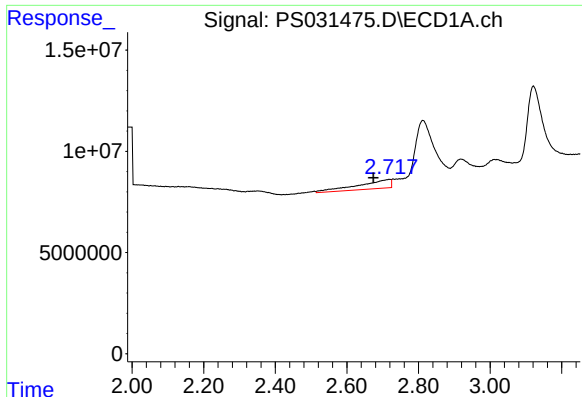

#1 Dalapon


R.T.: 2.718 min
Delta R.T.: 0.044 min
Response: 27696620
Conc: 5.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

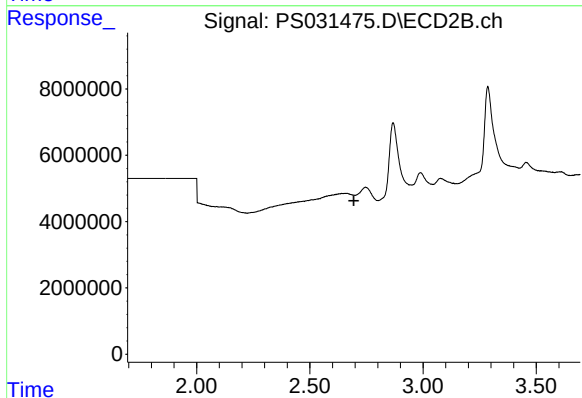


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.695 min
Response: 0
Conc: N.D.

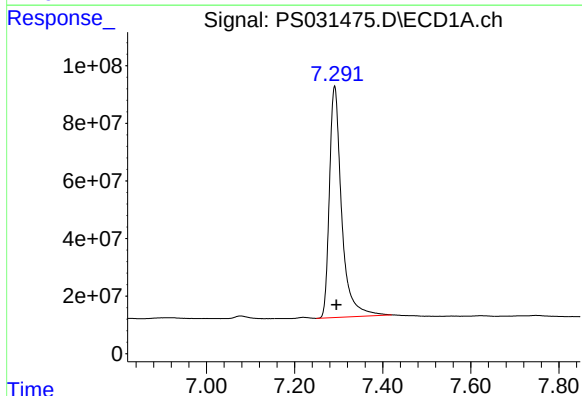


#4 2,4-DCAA

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 1546864460
Conc: 487.36 ng/ml

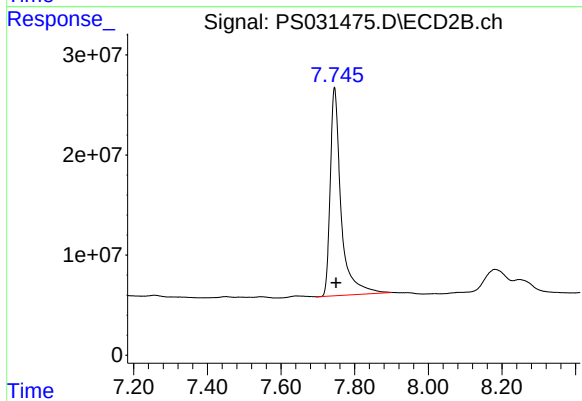

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: -0.004 min
Response: 425944505
Conc: 503.87 ng/ml

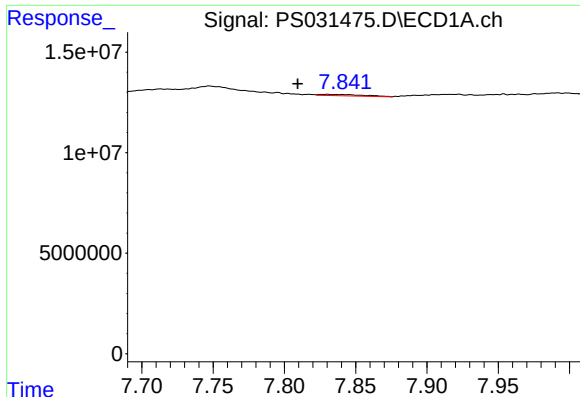

#7 MCPA

R.T.: 7.830 min
Delta R.T.: 0.020 min
Response: 1389050
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

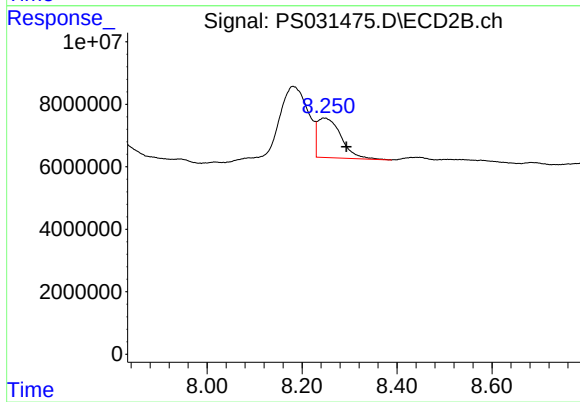

#7 MCPA

R.T.: 8.250 min
Delta R.T.: -0.044 min
Response: 43460887
Conc: 15.49 ug/ml