

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
 Data File : PS006201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 10:41
 Operator : SM\AJ
 Sample : K4272-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:02:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.509	5.235	582.9E6	363.0E6	675.238	738.027
Target Compounds							
1) T	Dalapon	2.047	1.761	74987314	89933242	68.819	143.321 #
7) T	MCPA	5.909	5.558	75446849	171.1E6	23.898	83.742 #
8) T	DICHLORPROP	0.000	5.909	0	53657986	N.D.	120.687
9) T	2,4-D	6.567	0.000	345.2E6	0	423.710	N.D. #
12) T	2,4,5-T	0.000	7.322	0	41578468	N.D.	16.725
15) T	Picloram	9.056	9.012	250.3E6	165.4E6	33.637	36.669
16) T	DCPA	0.000	9.012	0	165.4E6	N.D.	47.434



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
Data File : PS006201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 10:41
Operator : SM\AJ
Sample : K4272-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:02:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

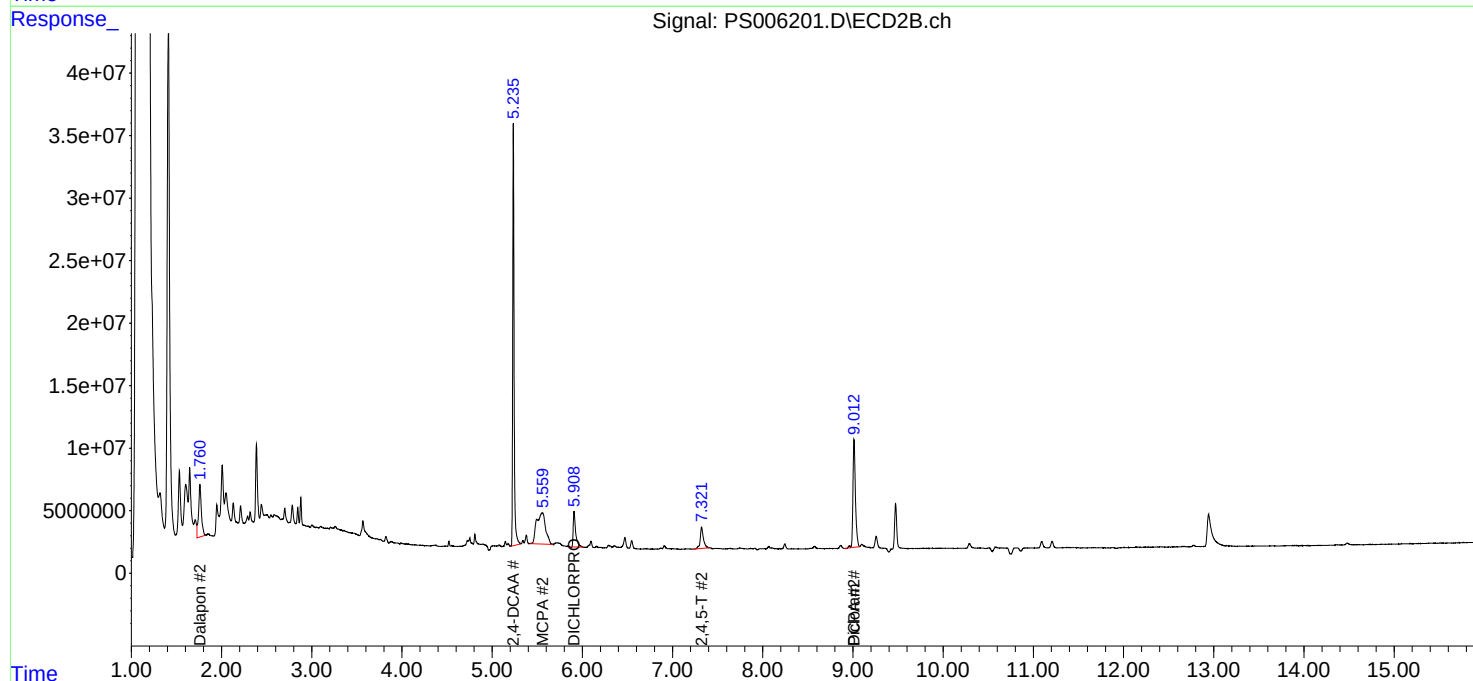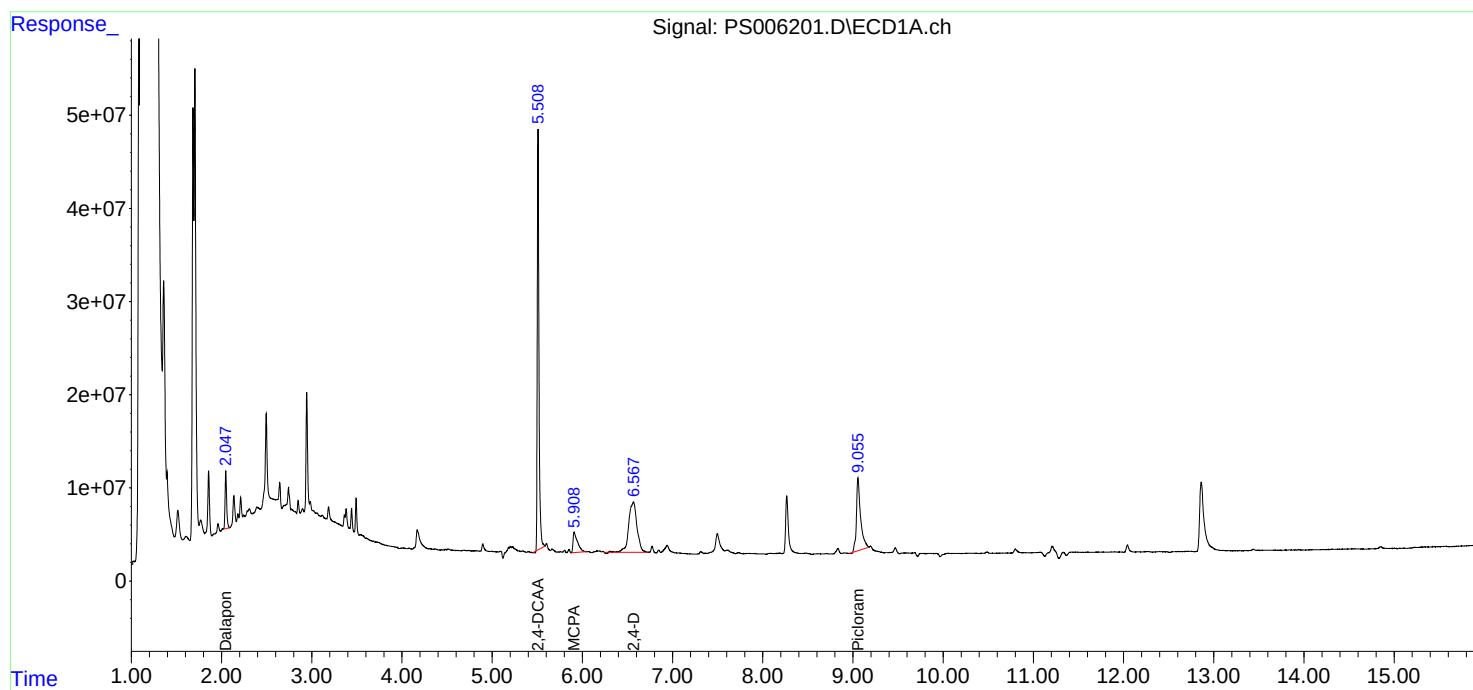


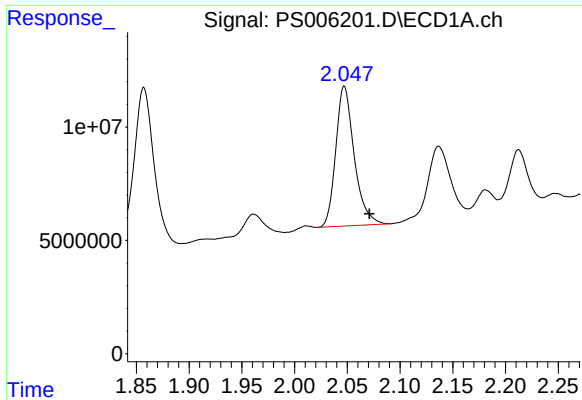

#1 Dalapon


R.T.: 2.047 min
Delta R.T.: -0.024 min
Response: 74987314
Conc: 68.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

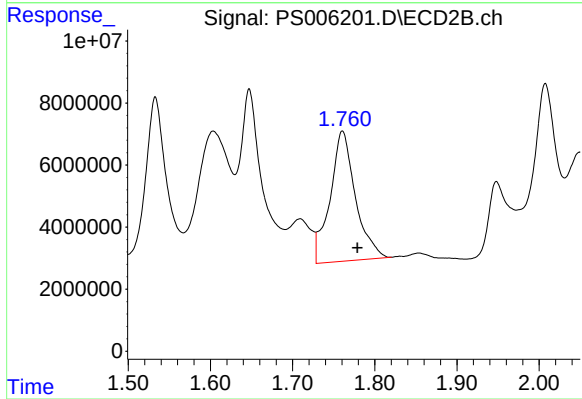


#1 Dalapon

R.T.: 1.761 min
Delta R.T.: -0.018 min
Response: 89933242
Conc: 143.32 ng/ml

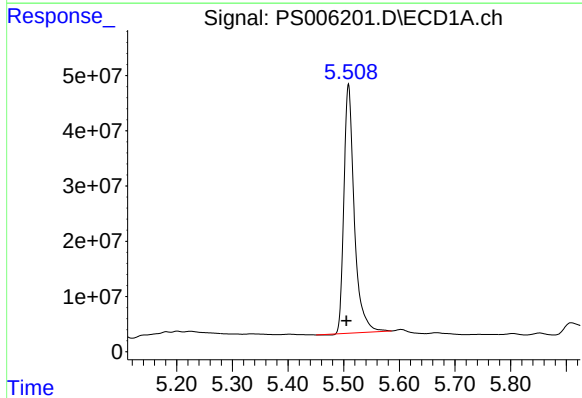


#4 2,4-DCAA

R.T.: 5.509 min
Delta R.T.: 0.004 min
Response: 582866066
Conc: 675.24 ng/ml

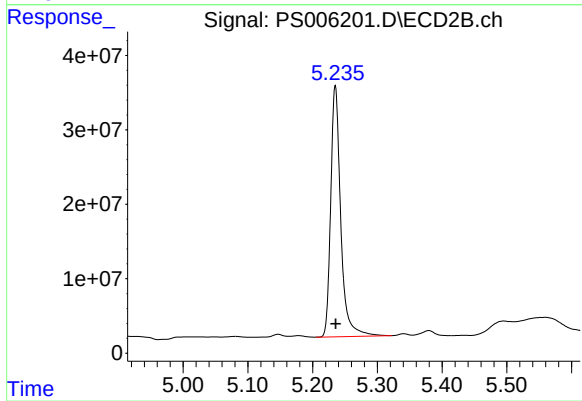

#4 2,4-DCAA


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 362999975
Conc: 738.03 ng/ml

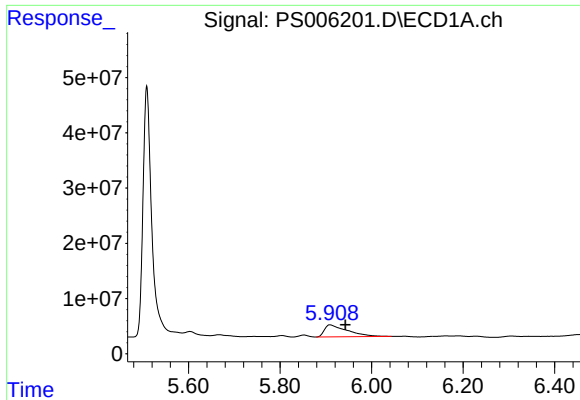

#7 MCPA


R.T.: 5.909 min
Delta R.T.: -0.033 min
Response: 75446849
Conc: 23.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

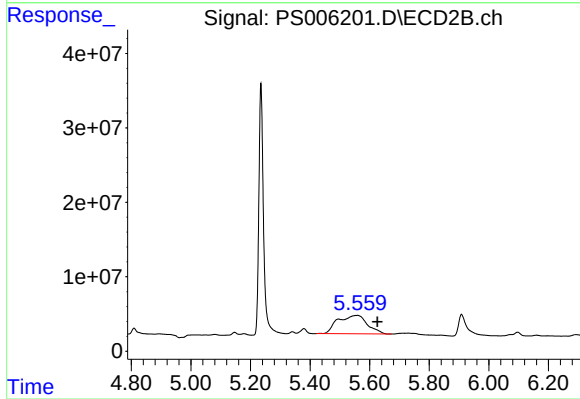


#7 MCPA

R.T.: 5.558 min
Delta R.T.: -0.069 min
Response: 171144553
Conc: 83.74 ug/ml

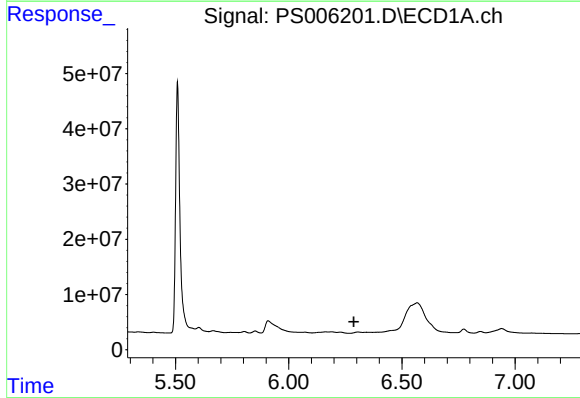


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

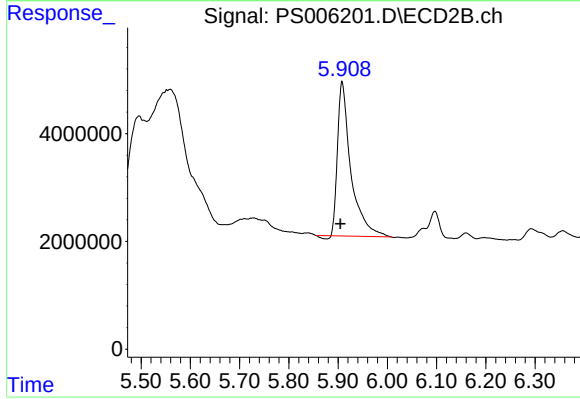

#8 DICHLORPROP


R.T.: 5.909 min
Delta R.T.: 0.004 min
Response: 53657986
Conc: 120.69 ng/ml

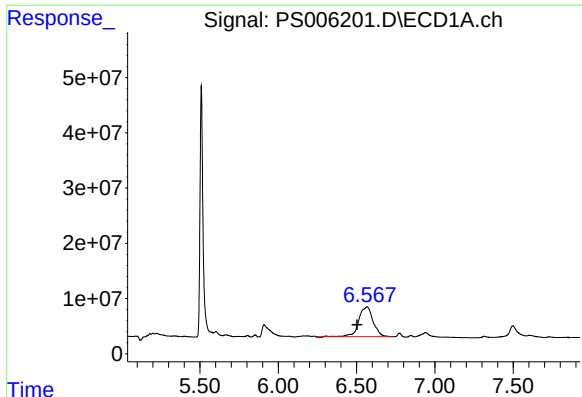

#9 2,4-D


R.T.: 6.567 min
Delta R.T.: 0.064 min
Response: 345232416
Conc: 423.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

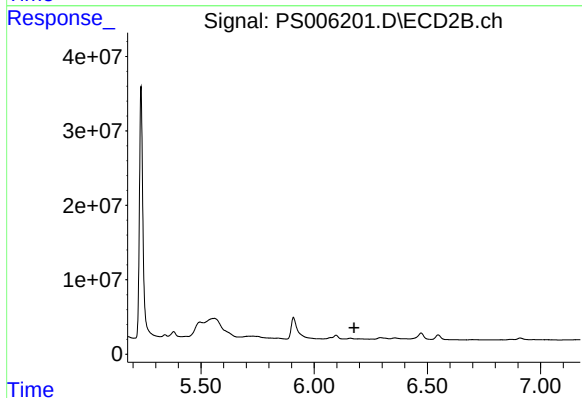


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

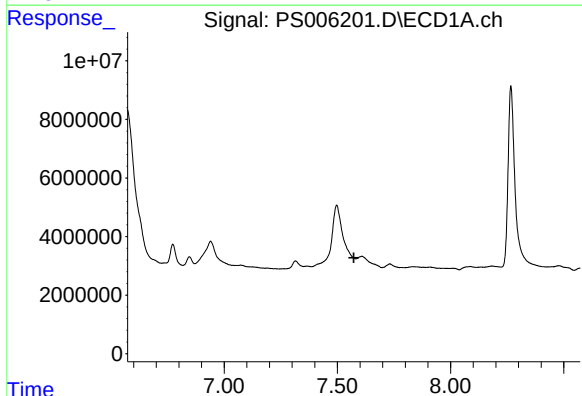


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

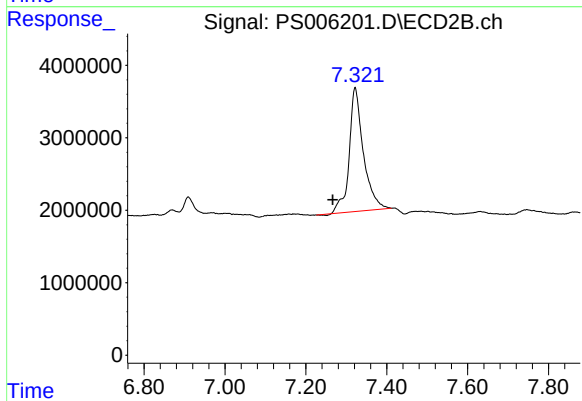

#12 2,4,5-T


R.T.: 7.322 min
Delta R.T.: 0.056 min
Response: 41578468
Conc: 16.72 ng/ml

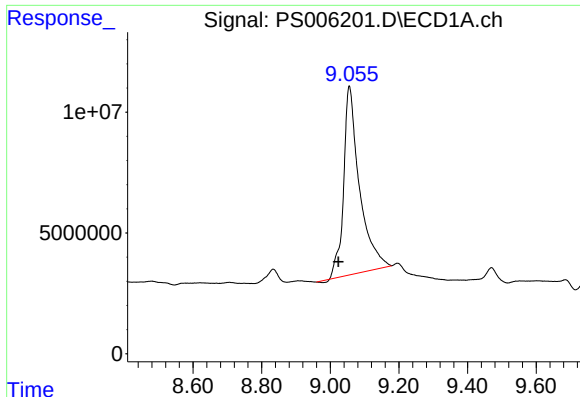

#15 Picloram


R.T.: 9.056 min
Delta R.T.: 0.032 min
Response: 250280129
Conc: 33.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

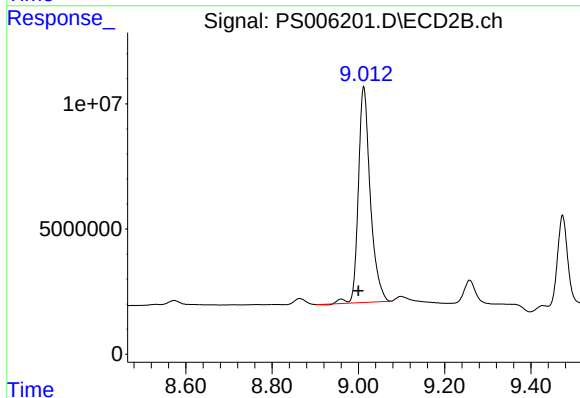


#15 Picloram

R.T.: 9.012 min
Delta R.T.: 0.012 min
Response: 165410064
Conc: 36.67 ng/ml

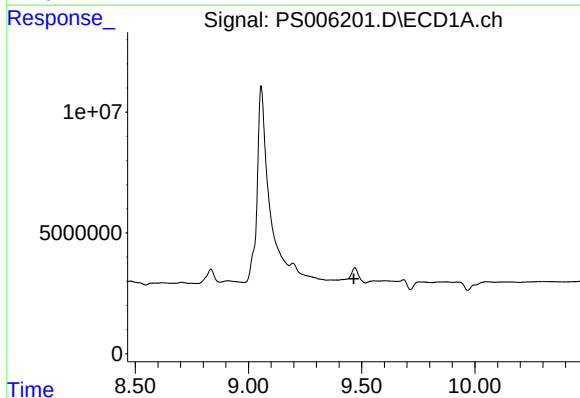

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

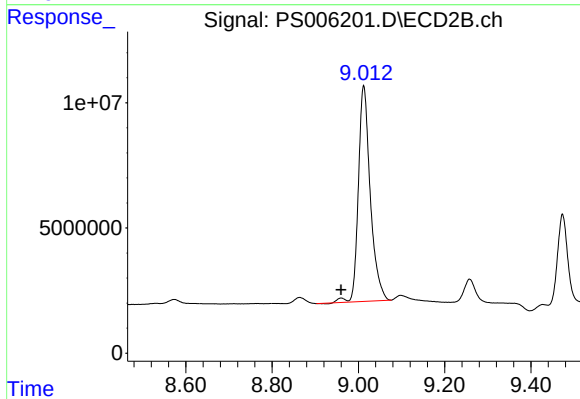

#16 DCPA

R.T.: 9.012 min
Delta R.T.: 0.053 min
Response: 165410064
Conc: 47.43 ng/ml