

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
 Data File : PS006204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 11:48
 Operator : SM\AJ
 Sample : K4356-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:16:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.216	535.8E6	291.2E6	620.670	592.102
Target Compounds							
1) T	Dalapon	2.027	1.742	201.8E6	80551518	185.193	128.370 #
2) T	3,5-DICHL...	4.872	0.000	54908862	0	50.930	N.D. #
3) T	4-Nitroph...	5.382	0.000	32820568	0	87.424	N.D. #
5) T	DICAMBA	5.667	5.360	17044630	19120642	5.307	10.366 #
6) T	MCPD	5.828	0.000	17557340	0	7.802	N.D. #
7) T	MCPA	5.893	0.000	69992457	0	22.170	N.D. #
8) T	DICHLORPROP	6.333	5.894	7825275	23697324	10.318	53.300 #
9) T	2,4-D	6.550	0.000	277.7E6	0	340.796	N.D. #
10) T	Pentachlo...	6.712	0.000	8964573	0	<MDL	N.D. #
13) T	2,4-DB	8.035	0.000	4181055	0	6.713	N.D. #
15) T	Picloram	9.070	0.000	769098	0	<MDL	N.D. #
16) T	DCPA	9.438	0.000	8168150	0	1.409	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
Data File : PS006204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 11:48
Operator : SM\AJ
Sample : K4356-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:16:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

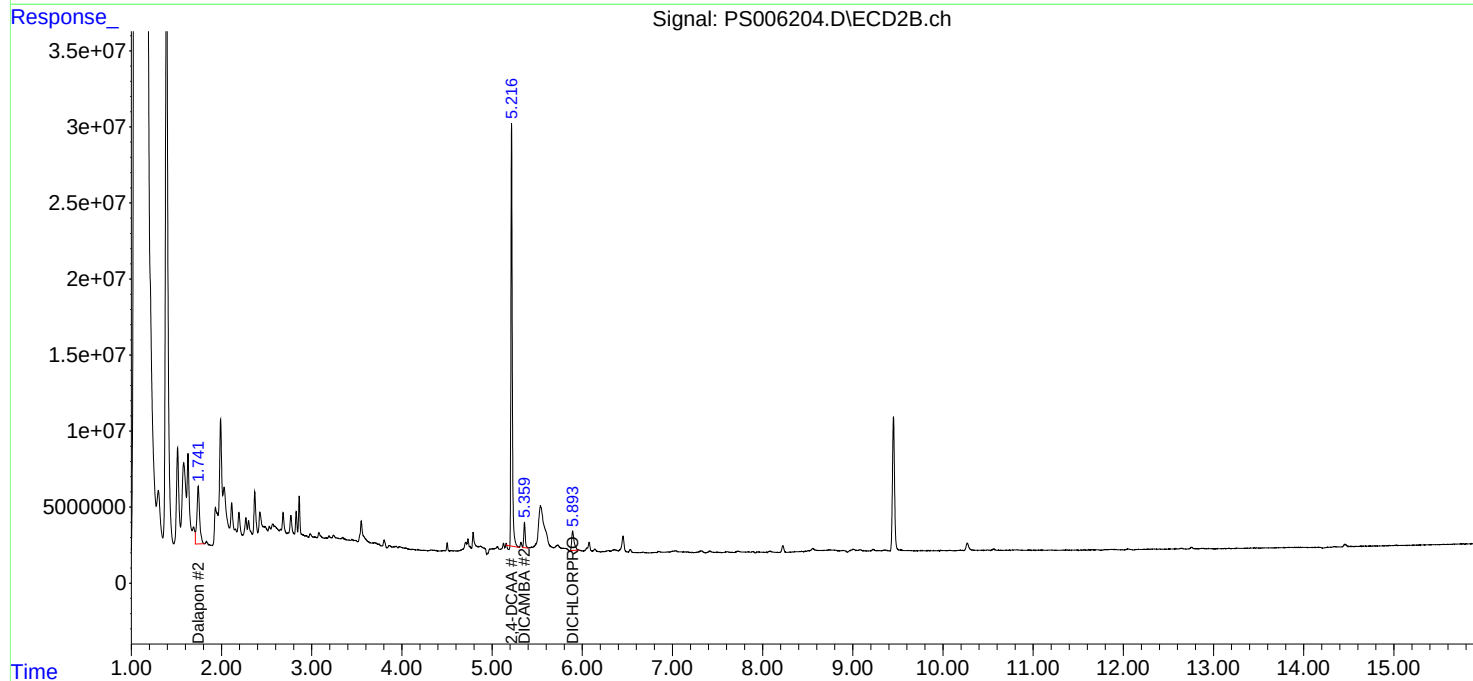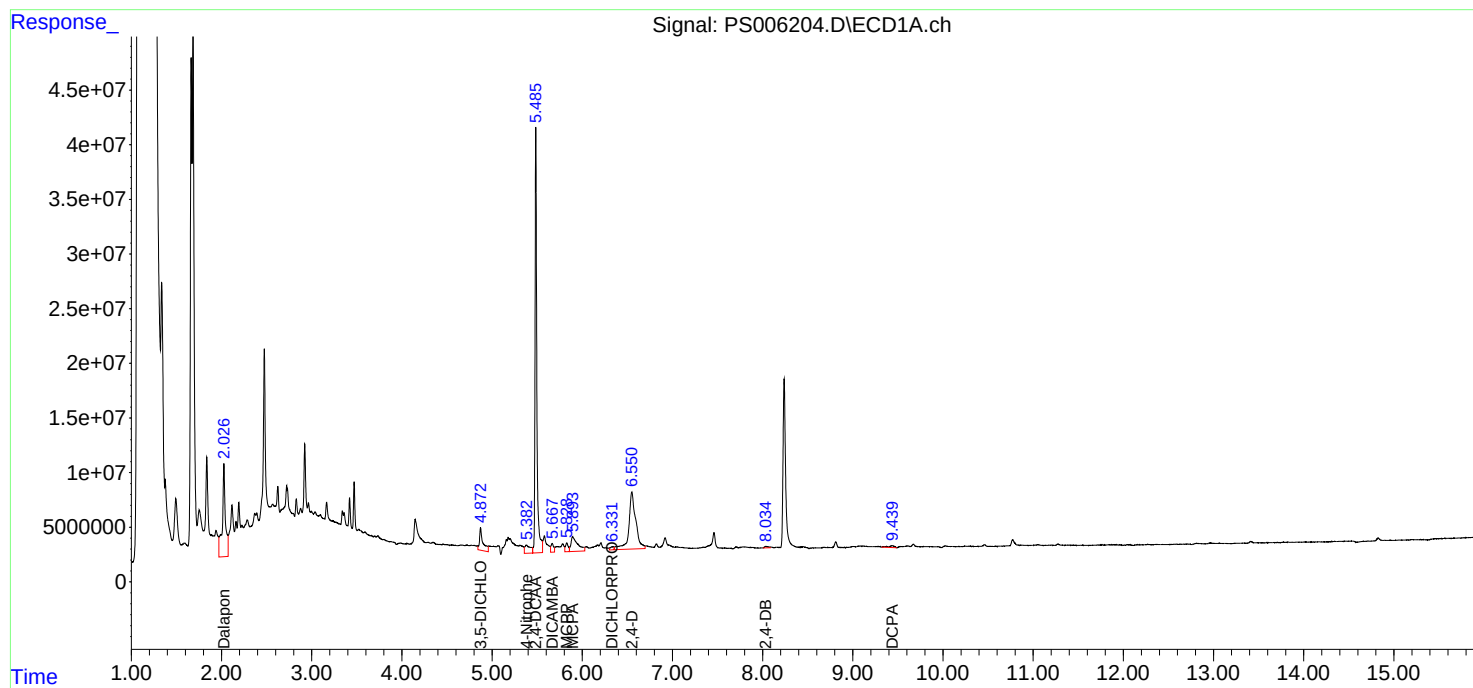


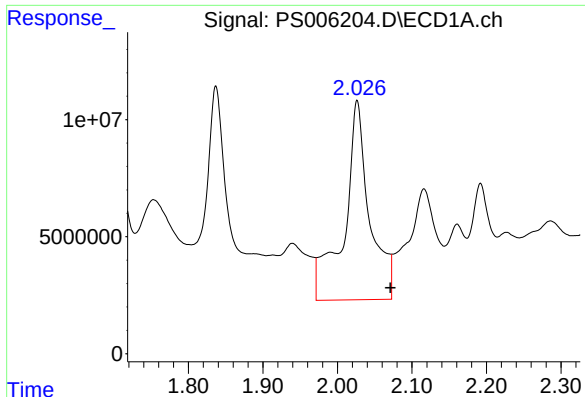

#1 Dalapon


R.T.: 2.027 min
Delta R.T.: -0.044 min
Response: 201790606
Conc: 185.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

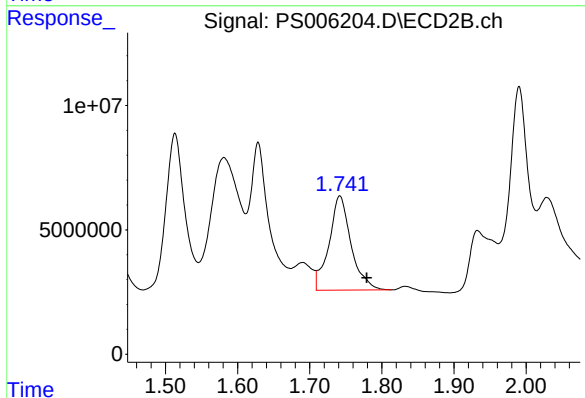


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.037 min
Response: 80551518
Conc: 128.37 ng/ml

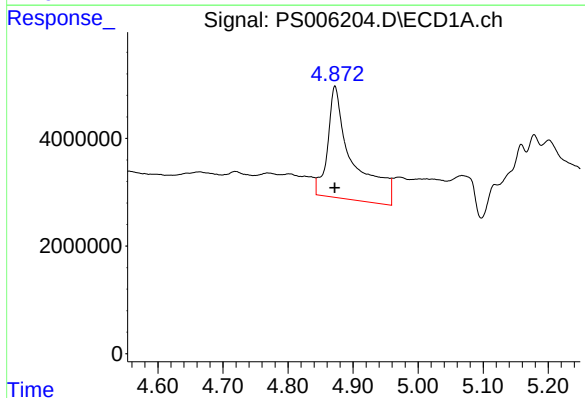


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 54908862
Conc: 50.93 ng/ml

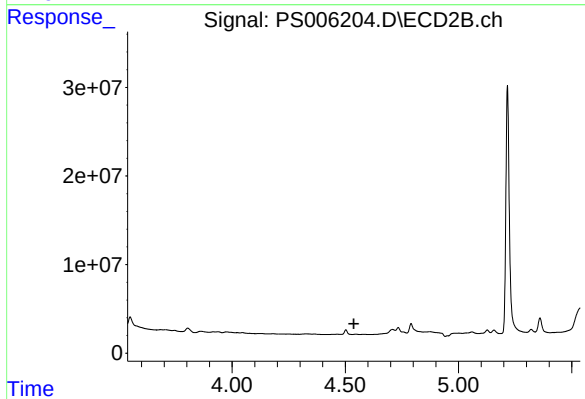

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

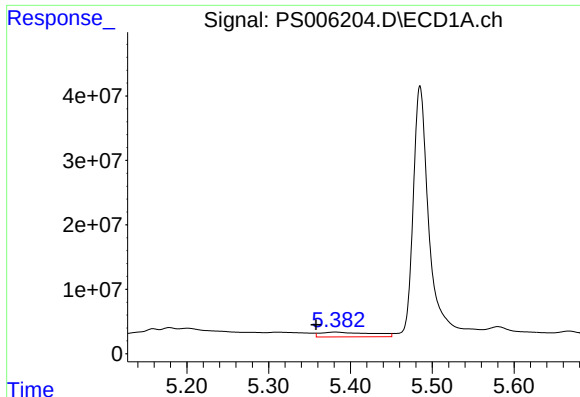

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: 0.024 min
Response: 32820568
Conc: 87.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

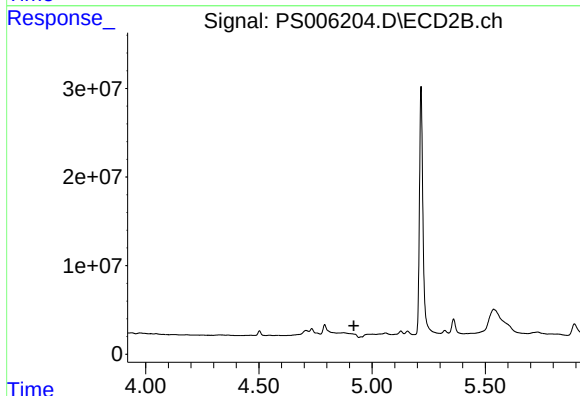


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

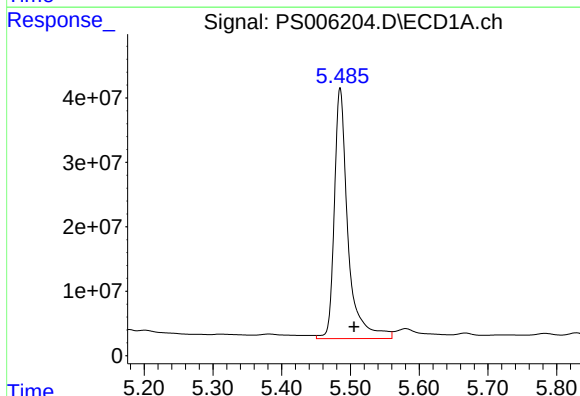


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 535762692
Conc: 620.67 ng/ml

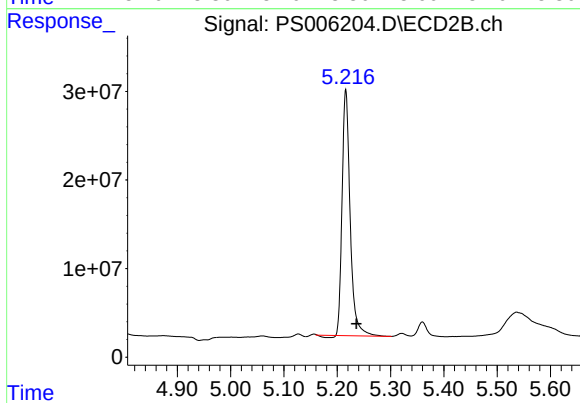

#4 2,4-DCAA


R.T.: 5.216 min
Delta R.T.: -0.019 min
Response: 291226631
Conc: 592.10 ng/ml

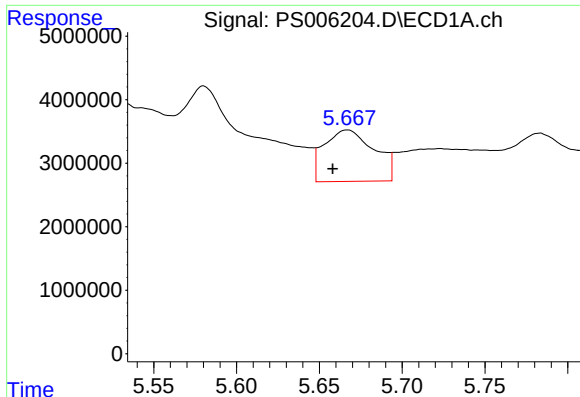

#5 DICAMBA


R.T.: 5.667 min
Delta R.T.: 0.009 min
Response: 17044630
Conc: 5.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

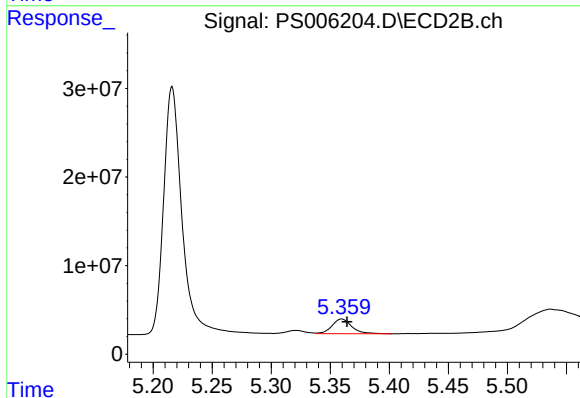


#5 DICAMBA

R.T.: 5.360 min
Delta R.T.: -0.004 min
Response: 19120642
Conc: 10.37 ng/ml

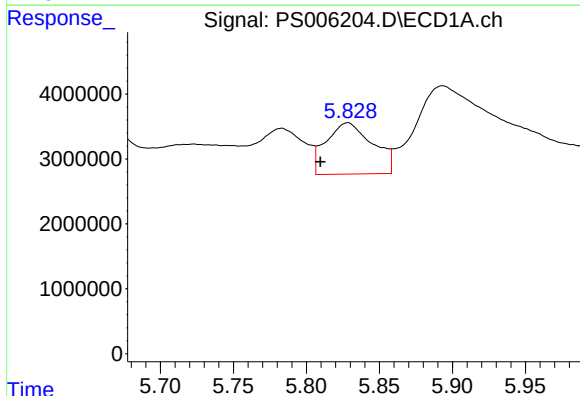


#6 MCP

R.T.: 5.828 min
Delta R.T.: 0.019 min
Response: 17557340
Conc: 7.80 ug/ml

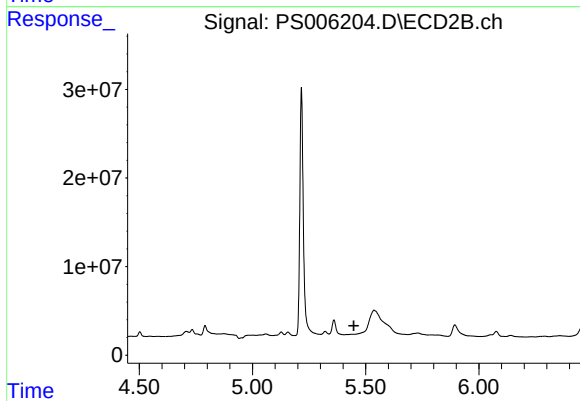

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

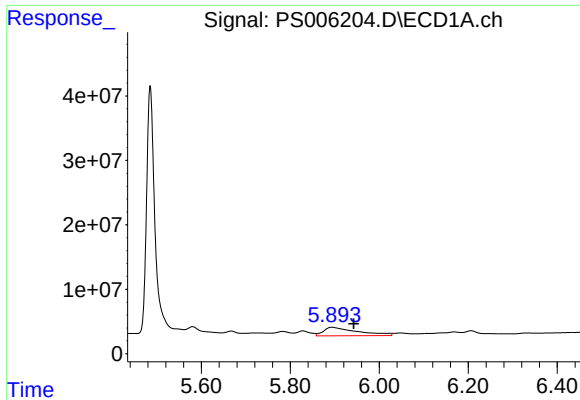

#7 MCPA


R.T.: 5.893 min
Delta R.T.: -0.049 min
Response: 69992457
Conc: 22.17 ug/ml

Instrument :
ECD_S
ClientSampleId :

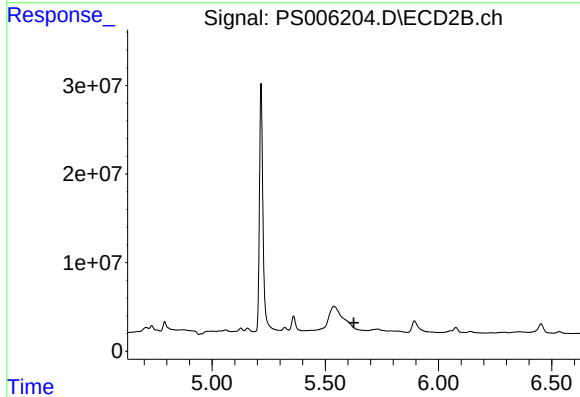


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.626 min
Response: 0
Conc: N.D.

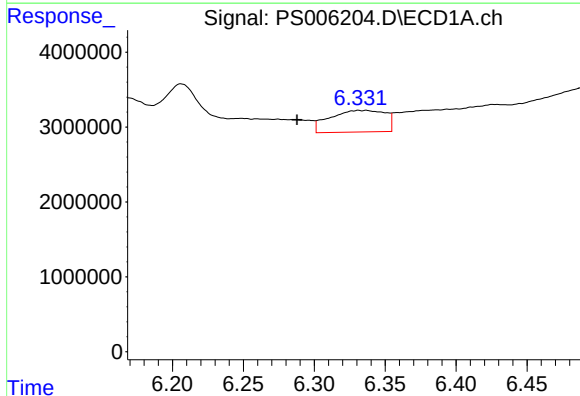


#8 DICHLORPROP

R.T.: 6.333 min
Delta R.T.: 0.045 min
Response: 7825275
Conc: 10.32 ng/ml

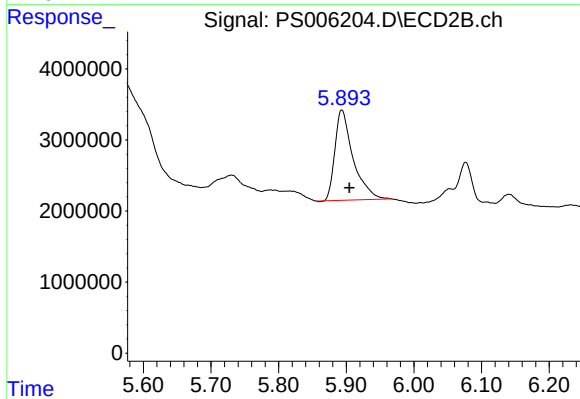

#8 DICHLORPROP


R.T.: 5.894 min
Delta R.T.: -0.011 min
Response: 23697324
Conc: 53.30 ng/ml

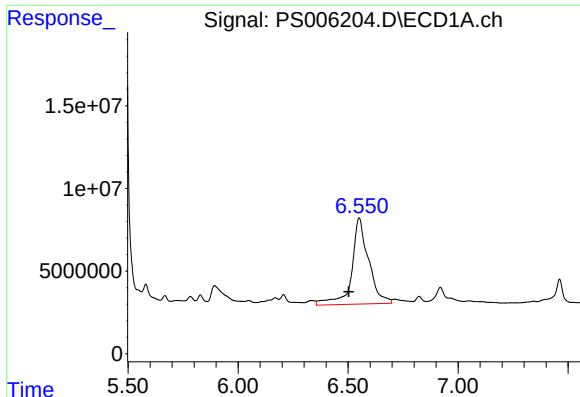

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 277675172
Conc: 340.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

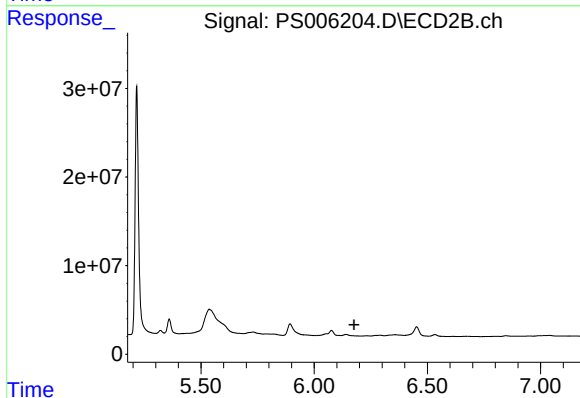


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

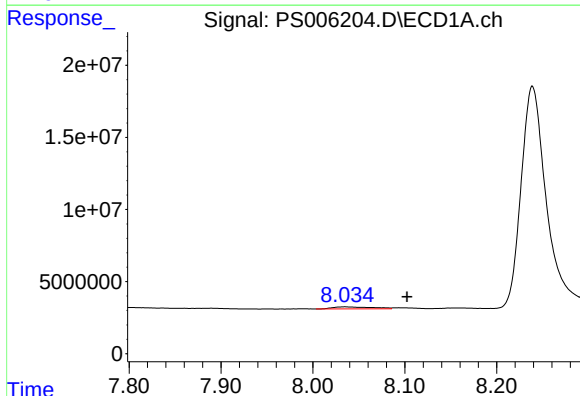


#13 2,4-DB

R.T.: 8.035 min
Delta R.T.: -0.068 min
Response: 4181055
Conc: 6.71 ng/ml

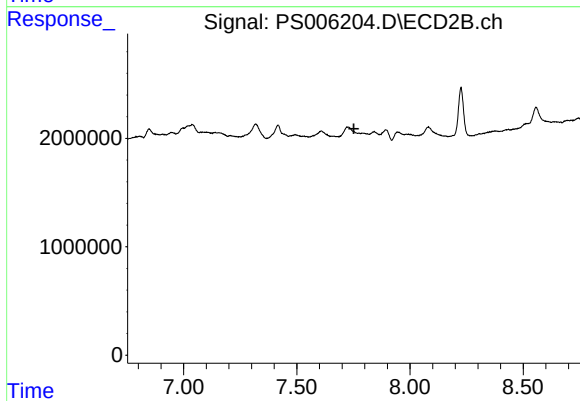

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

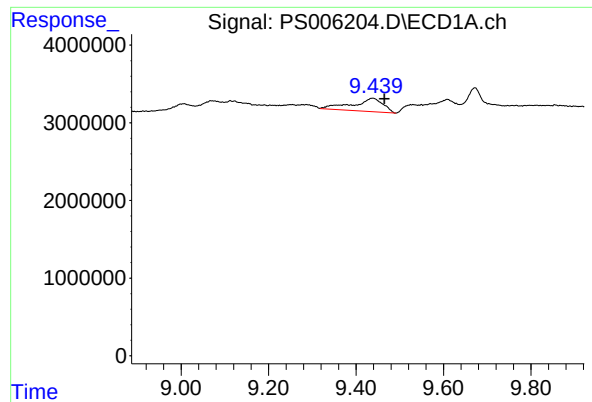

#16 DCPA

R.T.: 9.438 min
Delta R.T.: -0.027 min
Response: 8168150
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

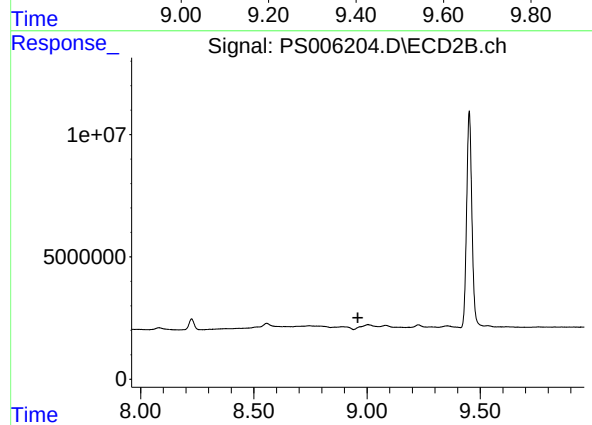

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.