

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
 Data File : PS006208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 13:16
 Operator : SM\AJ
 Sample : K4356-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:17:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.215	520.0E6	290.0E6	602.447	589.691
Target Compounds							
1) T	Dalapon	2.115	1.740	120.5E6	65437818	110.575	104.285
2) T	3,5-DICHL...	4.875	0.000	59313350	0	55.015	N.D. #
3) T	4-Nitroph...	5.379	0.000	31160586	0	83.003	N.D. #
6) T	MCP	5.829	0.000	17702891	0	7.866	N.D. #
7) T	MCPA	5.912	0.000	46523148	0	14.736	N.D. #
9) T	2,4-D	6.550	0.000	302.2E6	0	370.882	N.D. #
10) T	Pentachlo...	6.822	0.000	7144150	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.344	0.000	2883108	0	<MDL	N.D. #
13) T	2,4-DB	8.050	0.000	5862933	0	9.414	N.D. #
16) T	DCPA	9.436	0.000	7501744	0	1.294	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
Data File : PS006208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 13:16
Operator : SM\AJ
Sample : K4356-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:17:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

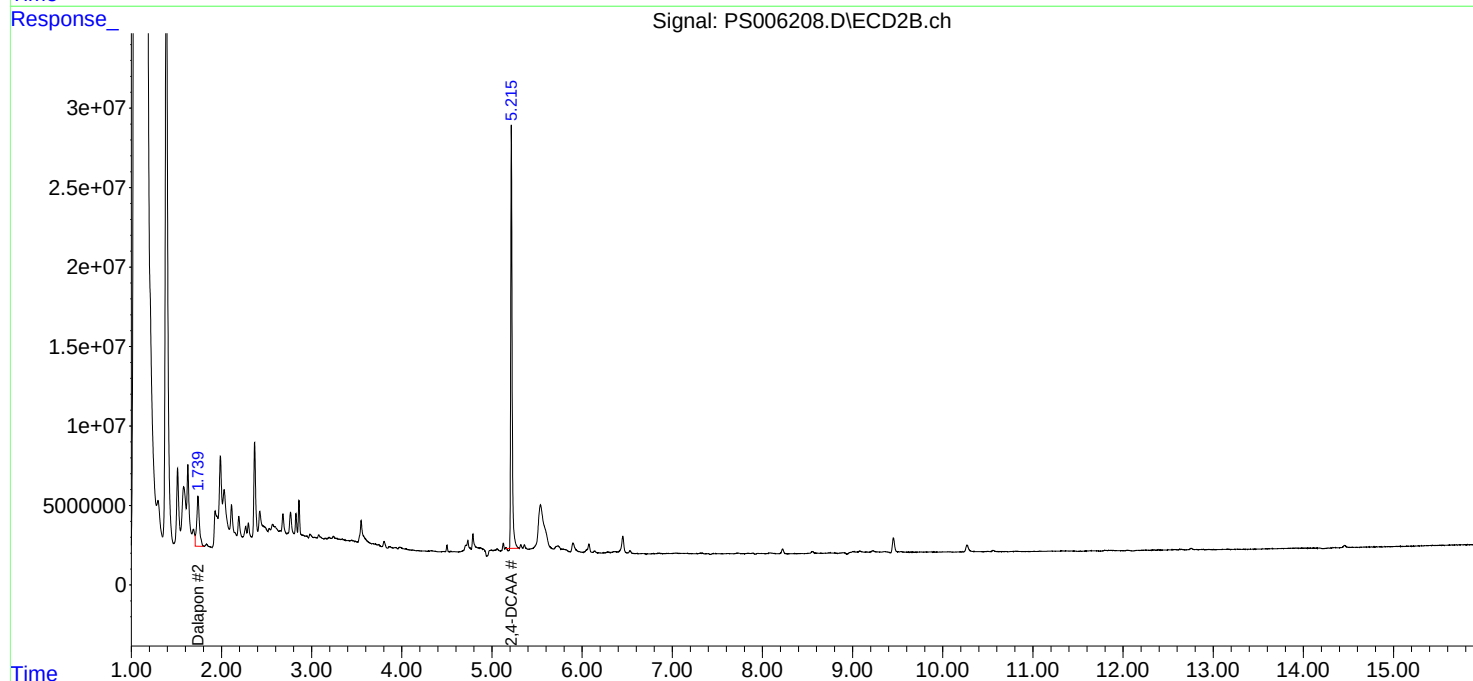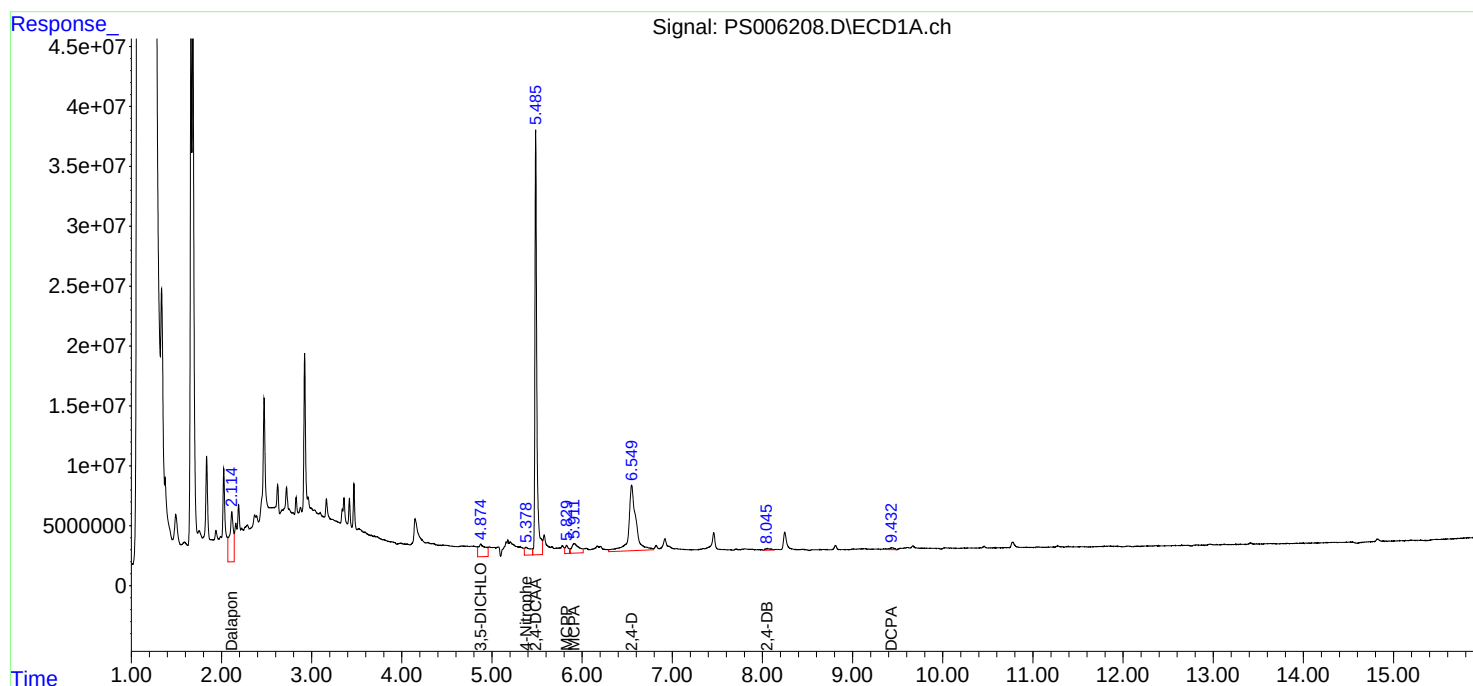


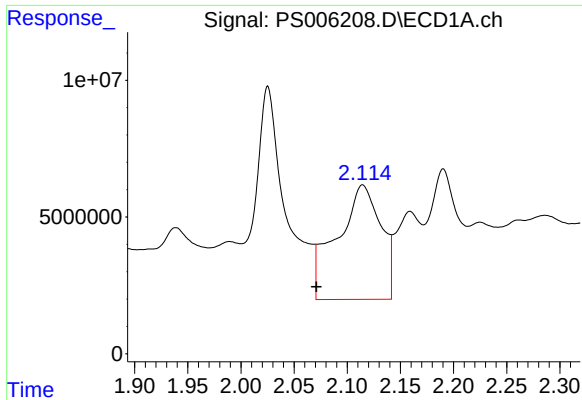

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: 120484841
Conc: 110.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

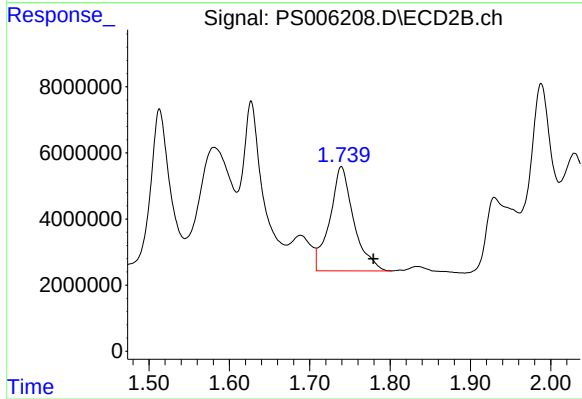


#1 Dalapon

R.T.: 1.740 min
Delta R.T.: -0.040 min
Response: 65437818
Conc: 104.28 ng/ml

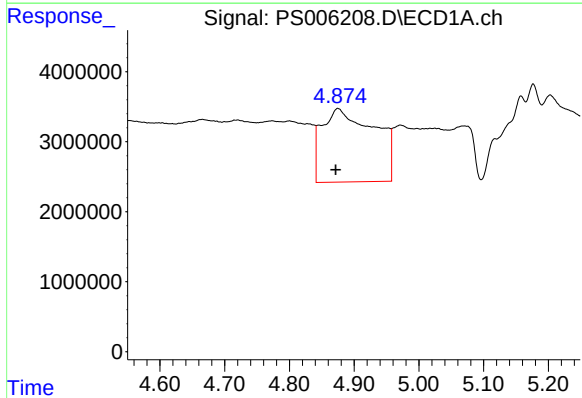


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.875 min
Delta R.T.: 0.003 min
Response: 59313350
Conc: 55.01 ng/ml

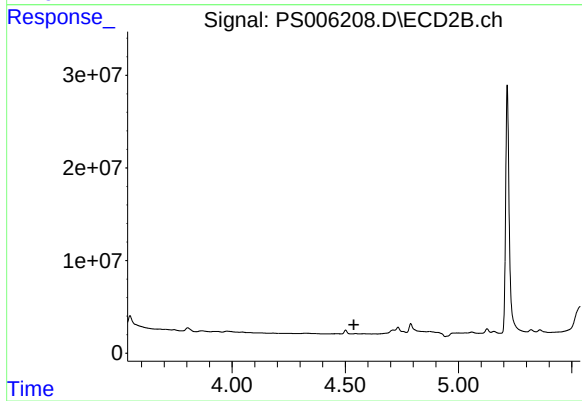

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

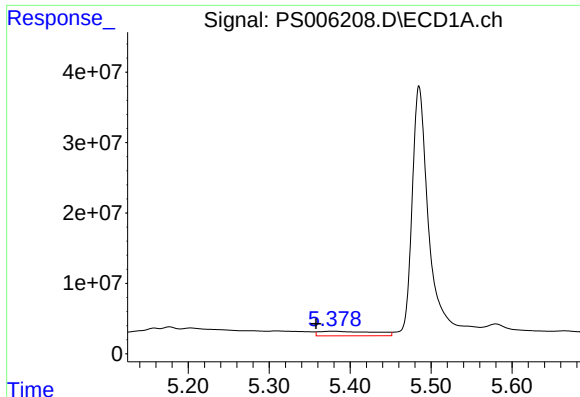

#3 4-Nitrophenol


R.T.: 5.379 min
Delta R.T.: 0.021 min
Response: 31160586
Conc: 83.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

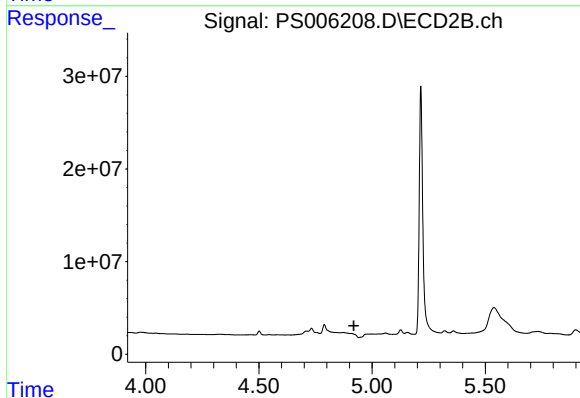


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

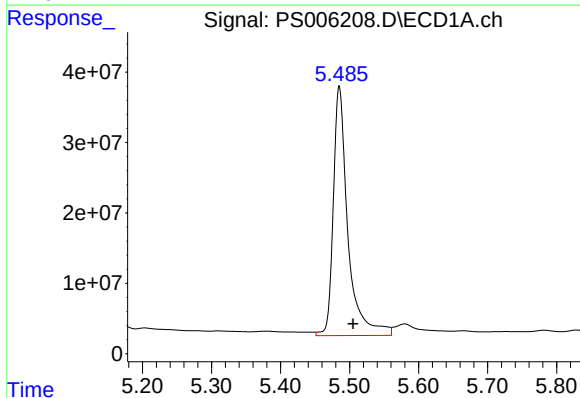


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 520032517
Conc: 602.45 ng/ml

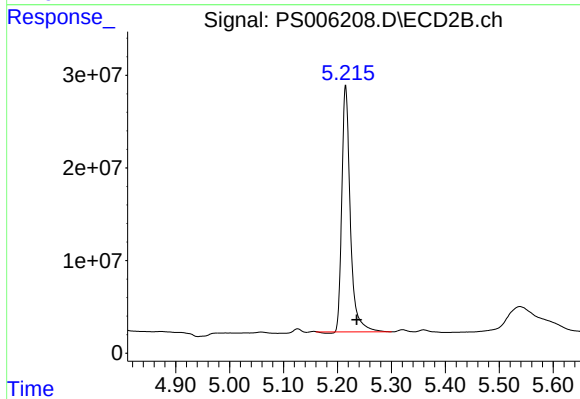

#4 2,4-DCAA


R.T.: 5.215 min
Delta R.T.: -0.020 min
Response: 290040579
Conc: 589.69 ng/ml

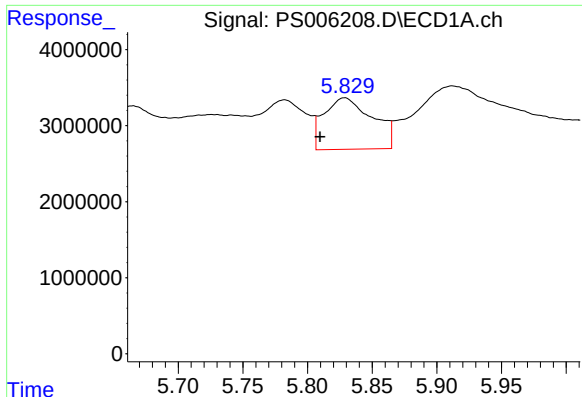

#6 MCPP


R.T.: 5.829 min
Delta R.T.: 0.019 min
Response: 17702891
Conc: 7.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

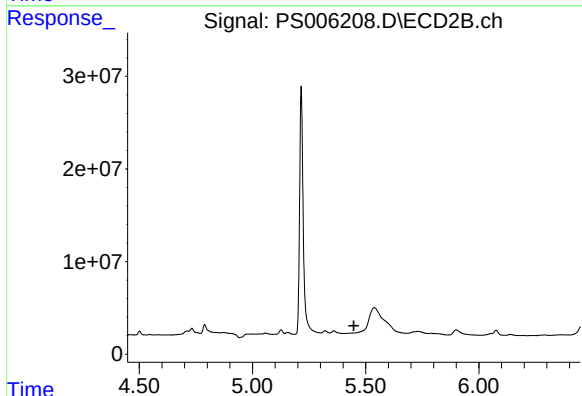


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.448 min
Response: 0
Conc: N.D.

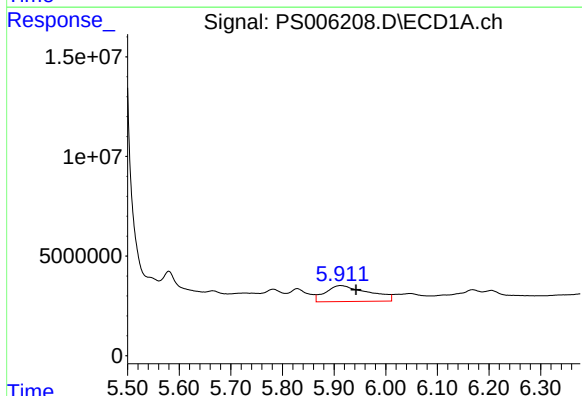


#7 MCPA

R.T.: 5.912 min
Delta R.T.: -0.030 min
Response: 46523148
Conc: 14.74 ug/ml

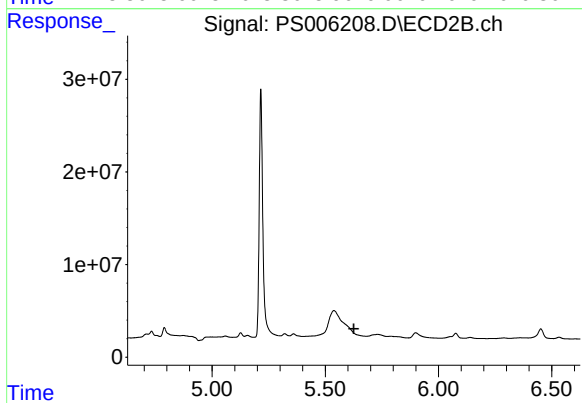

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

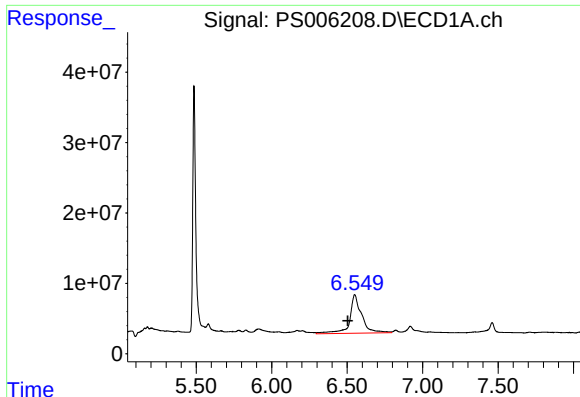

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 302188656
Conc: 370.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

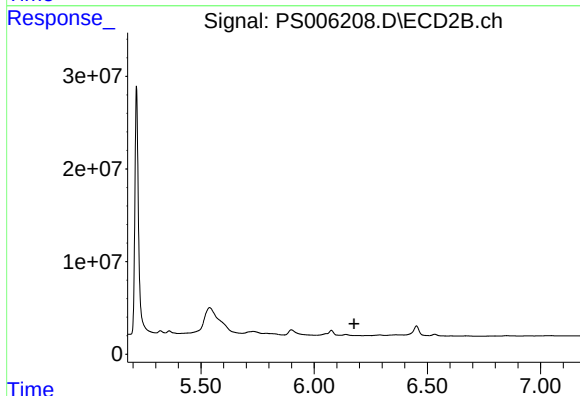


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

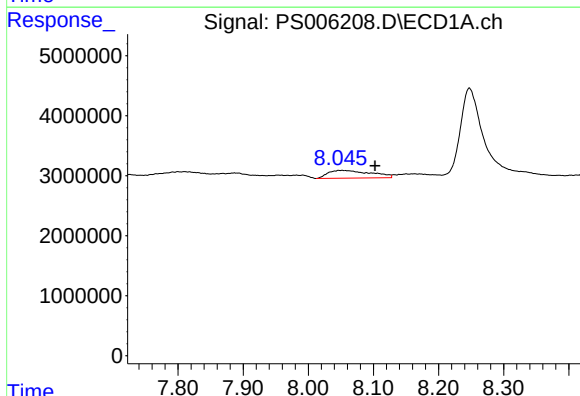


#13 2,4-DB

R.T.: 8.050 min
Delta R.T.: -0.052 min
Response: 5862933
Conc: 9.41 ng/ml

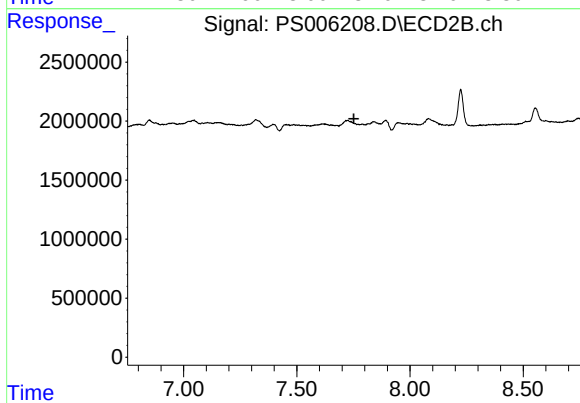

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

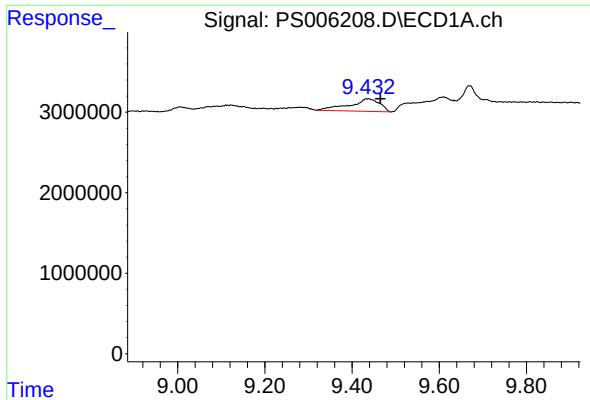

#16 DCPA

R.T.: 9.436 min
Delta R.T.: -0.029 min
Response: 7501744
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

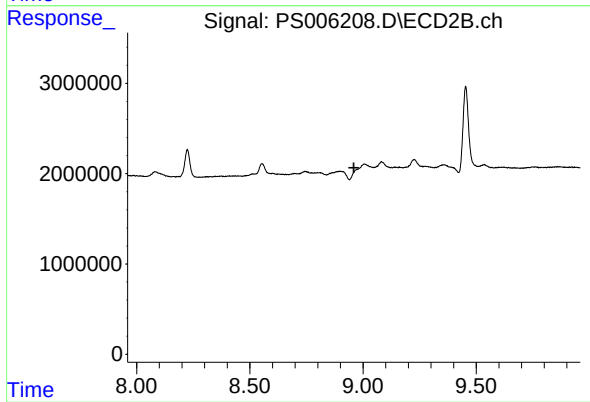

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.