

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
 Data File : PS006209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 13:38
 Operator : SM\AJ
 Sample : K4372-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:17:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.481	5.228	496.2E6	297.6E6	574.824	605.052
Target Compounds							
1) T	Dalapon	2.111	1.754	89812425	60811465	82.425	96.912
2) T	3,5-DICHL...	4.865	0.000	108.7E6	0	100.787	N.D. #
3) T	4-Nitroph...	5.375	0.000	6291678	0	16.759	N.D. #
5) T	DICAMBA	0.000	5.372	0	42211432	N.D.	22.885
6) T	MCPD	5.822	0.000	5842233	0	2.596	N.D. #
7) T	MCPA	5.901	0.000	17862116	0	5.658	N.D. #
8) T	DICHLORPROP	6.317	0.000	3794257	0	5.003	N.D. #
9) T	2,4-D	6.546	0.000	319.7E6	0	392.399	N.D. #
10) T	Pentachlo...	6.816	0.000	10619523	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.288	0.000	7347213	0	1.611	N.D. #
15) T	Picloram	9.051	0.000	17449671	0	2.345	N.D. #
16) T	DCPA	9.508	0.000	3826210	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
Data File : PS006209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 13:38
Operator : SM\AJ
Sample : K4372-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:17:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

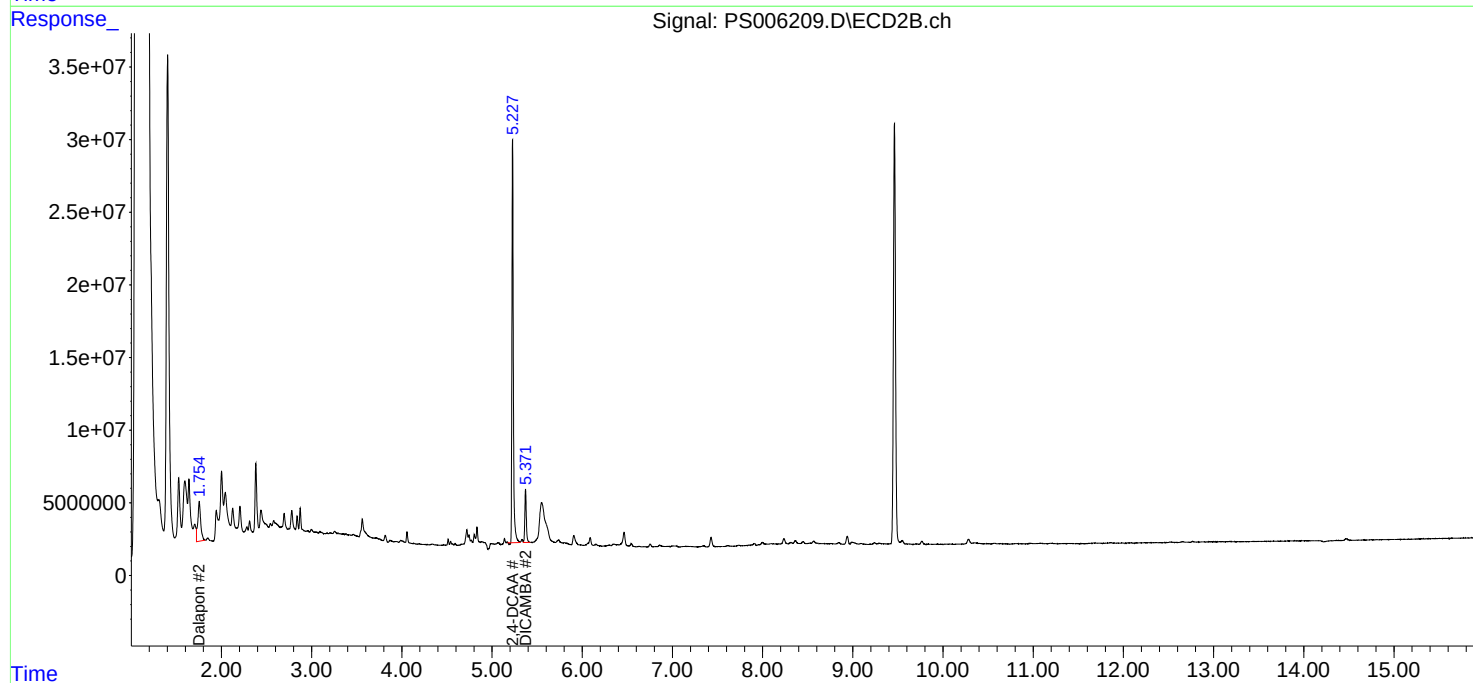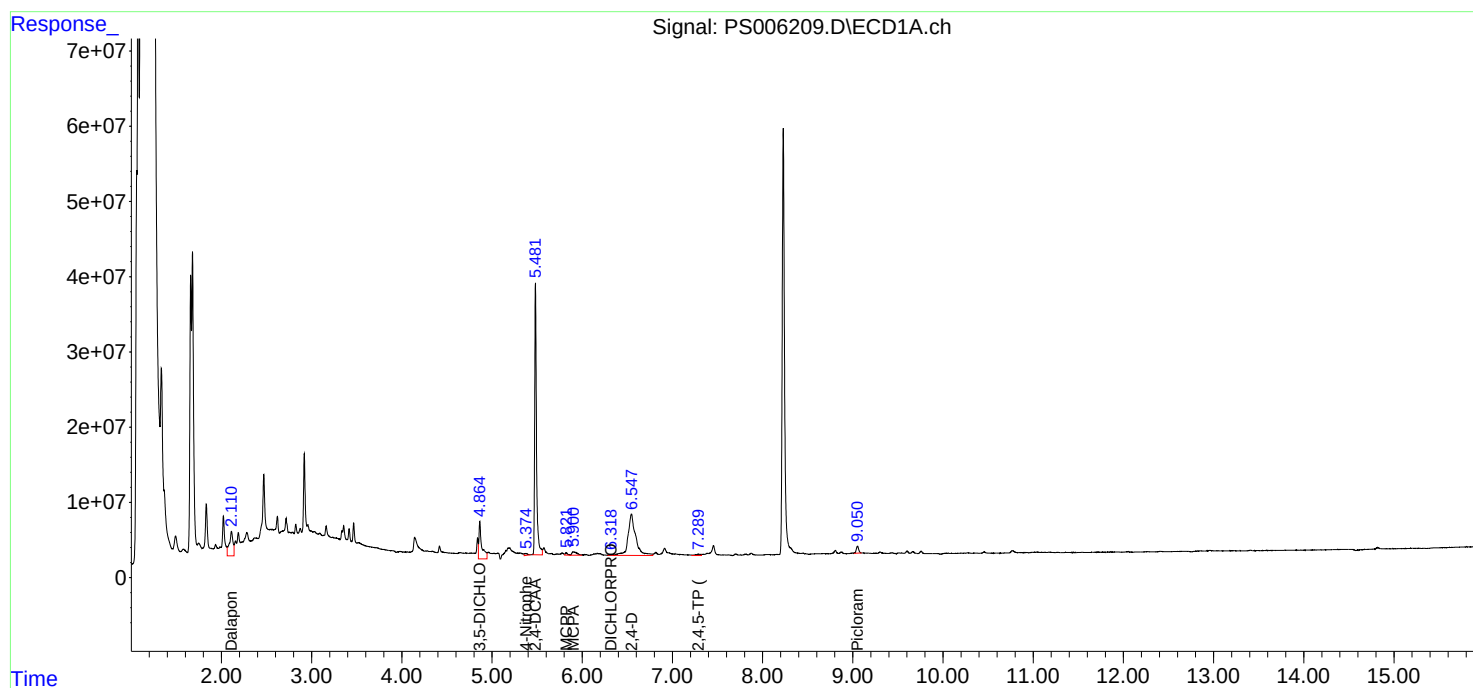


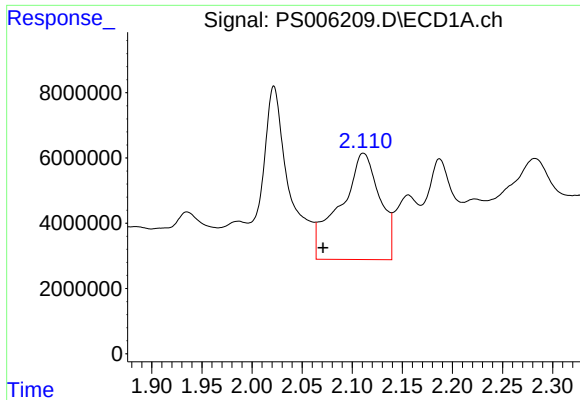

#1 Dalapon


R.T.: 2.111 min
Delta R.T.: 0.040 min
Response: 89812425
Conc: 82.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

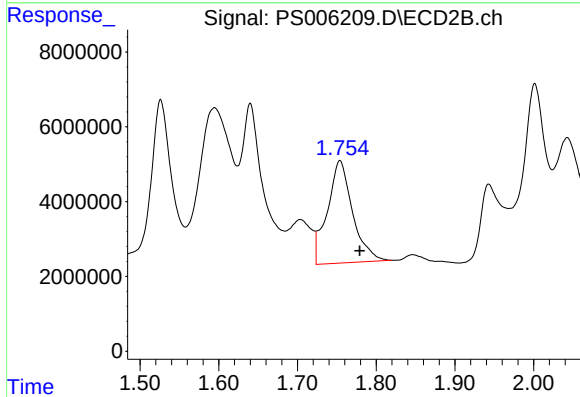


#1 Dalapon

R.T.: 1.754 min
Delta R.T.: -0.025 min
Response: 60811465
Conc: 96.91 ng/ml

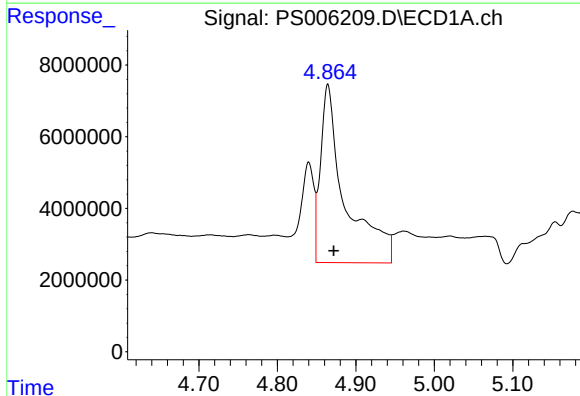


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.865 min
Delta R.T.: -0.007 min
Response: 108661769
Conc: 100.79 ng/ml

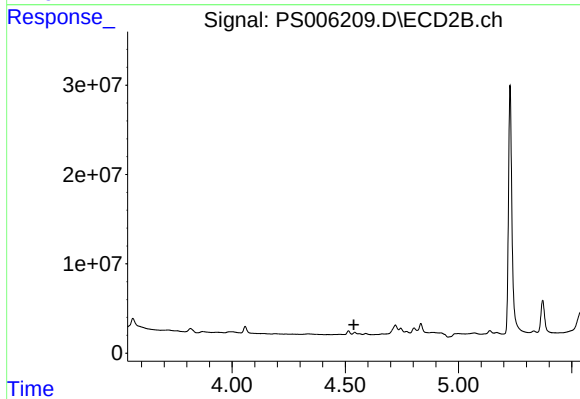

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

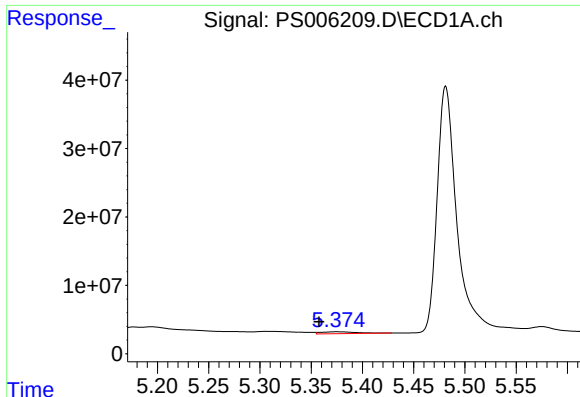

#3 4-Nitrophenol


R.T.: 5.375 min
Delta R.T.: 0.018 min
Response: 6291678
Conc: 16.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

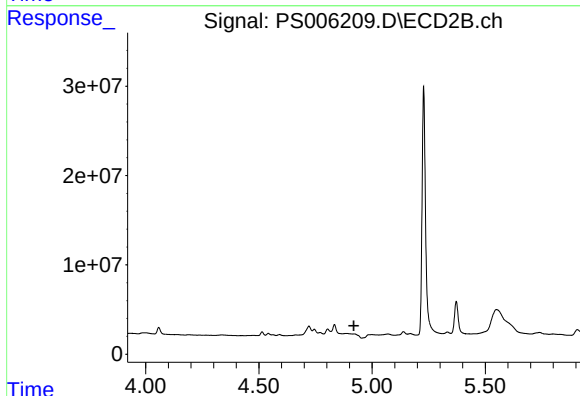


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

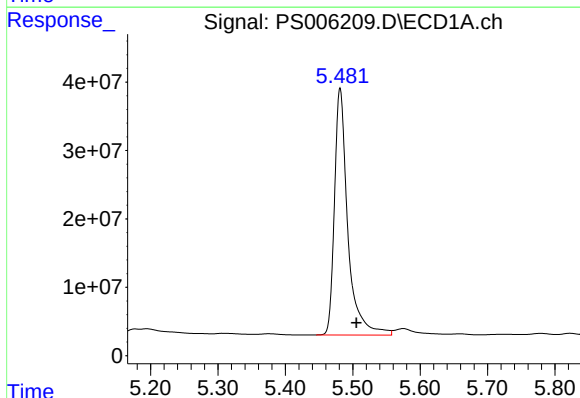


#4 2,4-DCAA

R.T.: 5.481 min
Delta R.T.: -0.024 min
Response: 496188531
Conc: 574.82 ng/ml

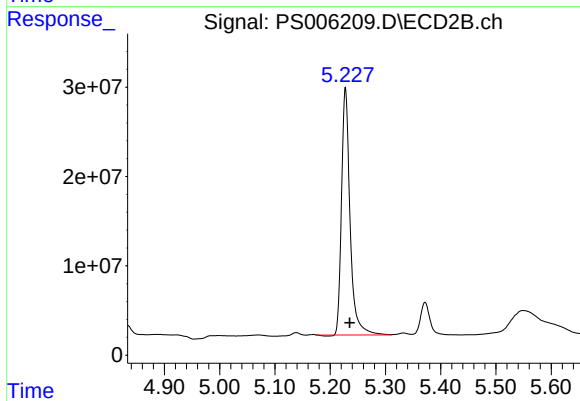

#4 2,4-DCAA


R.T.: 5.228 min
Delta R.T.: -0.008 min
Response: 297596161
Conc: 605.05 ng/ml

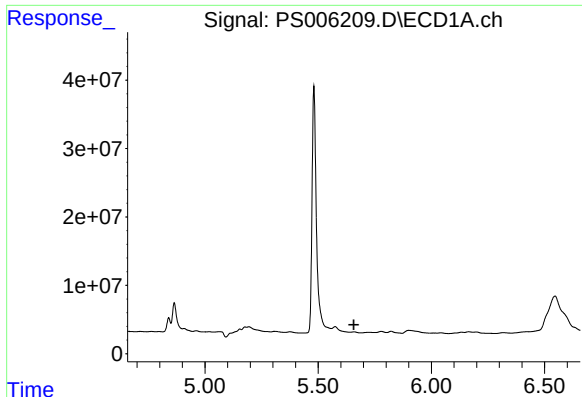

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

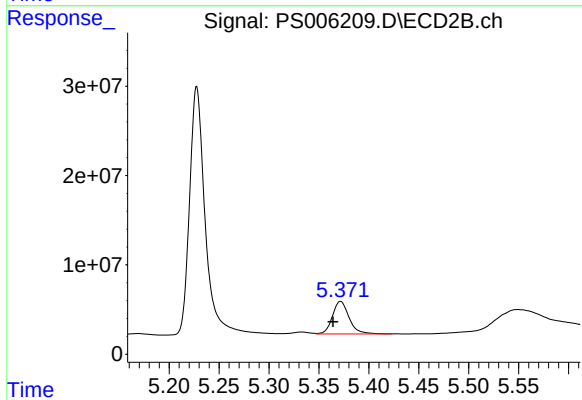


#5 DICAMBA

R.T.: 5.372 min
Delta R.T.: 0.008 min
Response: 42211432
Conc: 22.88 ng/ml

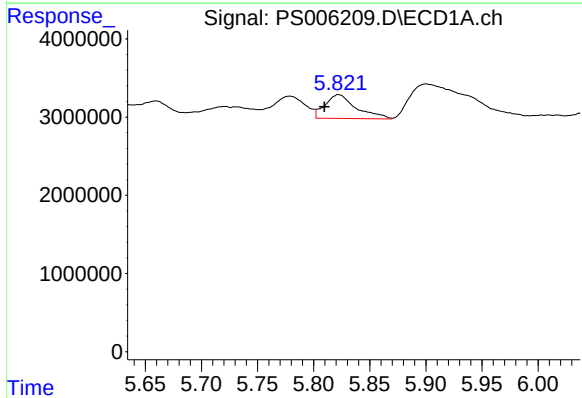


#6 MCP

R.T.: 5.822 min
Delta R.T.: 0.013 min
Response: 5842233
Conc: 2.60 ug/ml

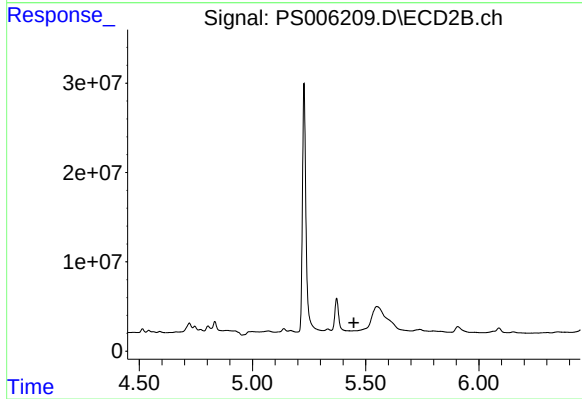

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

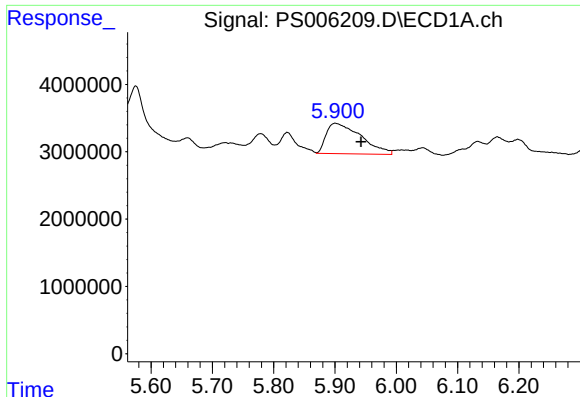

#7 MCPA


R.T.: 5.901 min
Delta R.T.: -0.042 min
Response: 17862116
Conc: 5.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

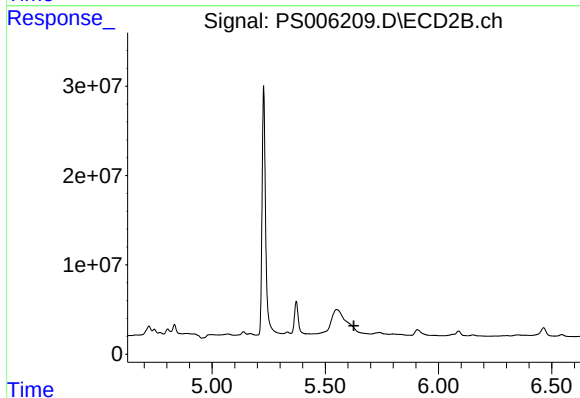


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

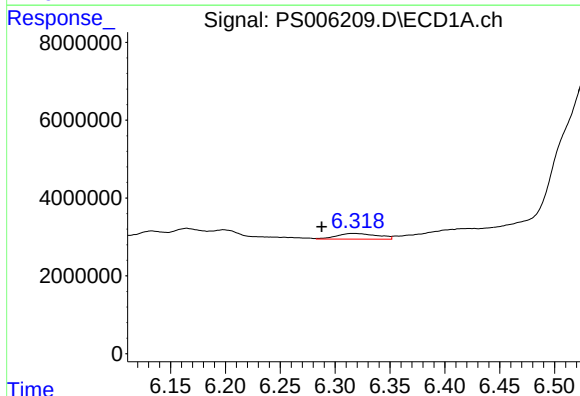


#8 DICHLORPROP

R.T.: 6.317 min
Delta R.T.: 0.029 min
Response: 3794257
Conc: 5.00 ng/ml

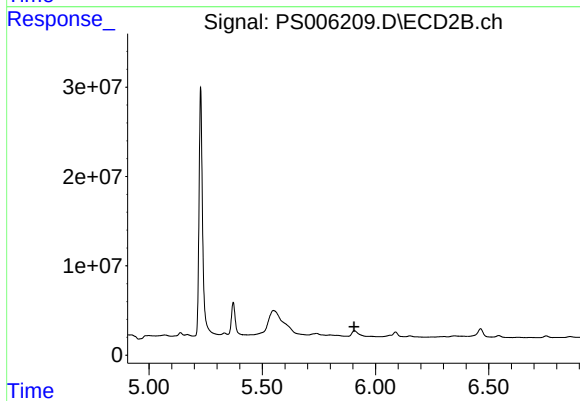

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.905 min
Response: 0
Conc: N.D.

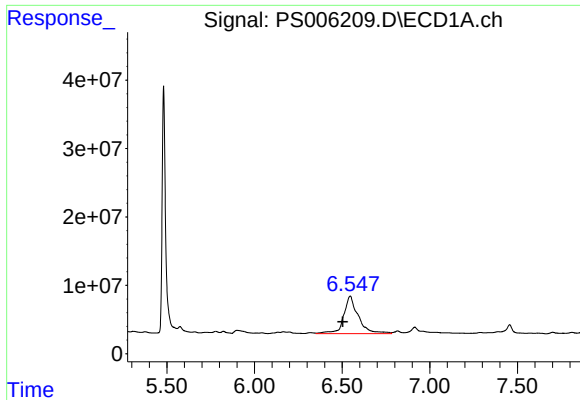

#9 2,4-D


R.T.: 6.546 min
Delta R.T.: 0.043 min
Response: 319720542
Conc: 392.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

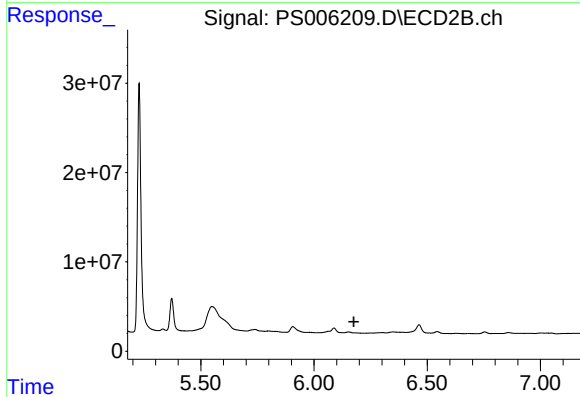


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

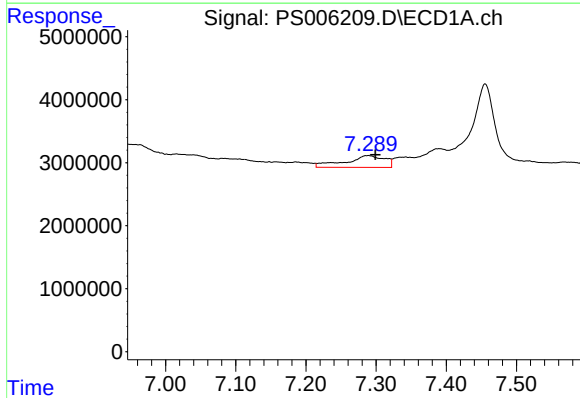


#11 2,4,5-TP (SILVEX)

R.T.: 7.288 min
Delta R.T.: -0.011 min
Response: 7347213
Conc: 1.61 ng/ml

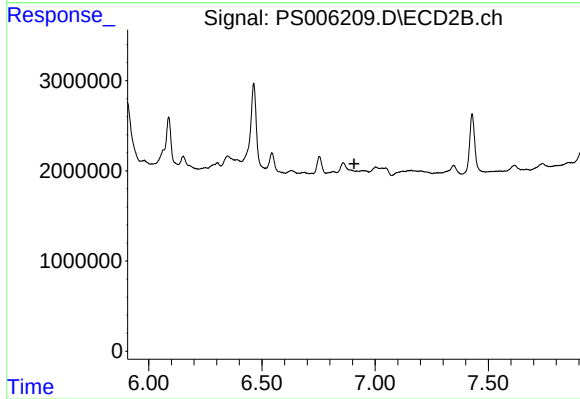

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

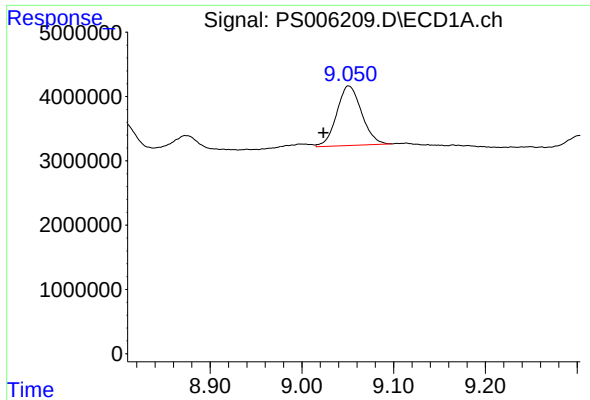

#15 Picloram

R.T.: 9.051 min
Delta R.T.: 0.028 min
Response: 17449671
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

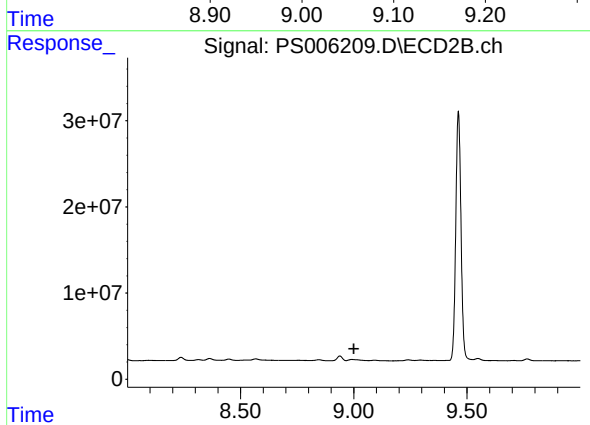

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.