

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
 Data File : PS006210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 14:00
 Operator : SM\AJ
 Sample : K4383-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:18:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.487	5.217	586.4E6	324.4E6	679.275	659.599
Target Compounds							
1) T	Dalapon	2.028	1.742	113.7E6	39480344	104.311	62.918 #
2) T	3,5-DICHL...	4.874	0.000	16338586	0	15.155	N.D. #
3) T	4-Nitroph...	5.382	0.000	30569389	0	81.428	N.D. #
5) T	DICAMBA	5.668	5.362	18893080	11318098	5.883	6.136
6) T	MCPD	5.829	0.000	16025620	0	7.121	N.D. #
7) T	MCPA	5.898	0.000	88299117	0	27.969	N.D. #
8) T	DICHLORPROP	0.000	5.893	0	37603909	N.D.	84.578
9) T	2,4-D	6.552	0.000	313.9E6	0	385.271	N.D. #
10) T	Pentachlo...	6.823	0.000	6998095	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.346	0.000	4081258	0	<MDL	N.D. #
15) T	Picloram	9.009	0.000	3091255	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081919\
Data File : PS006210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 14:00
Operator : SM\AJ
Sample : K4383-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:18:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

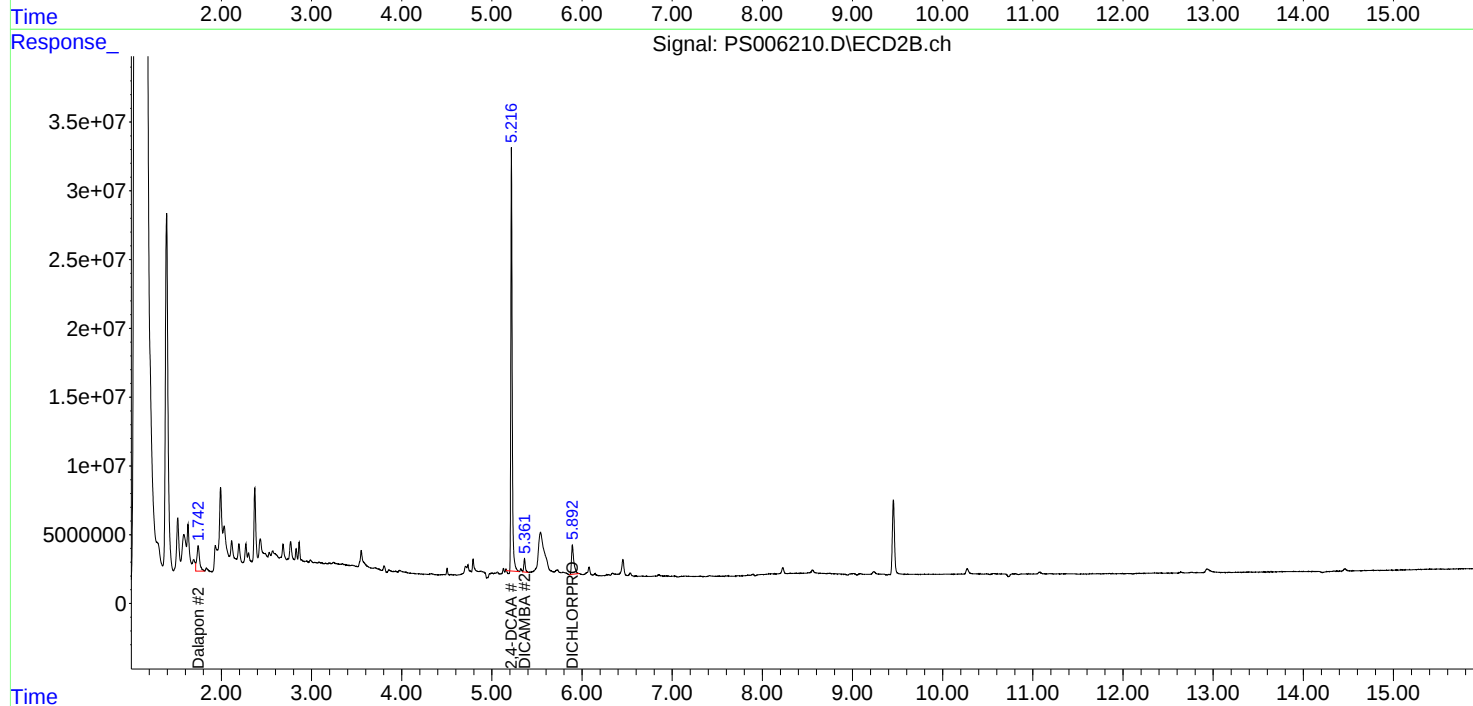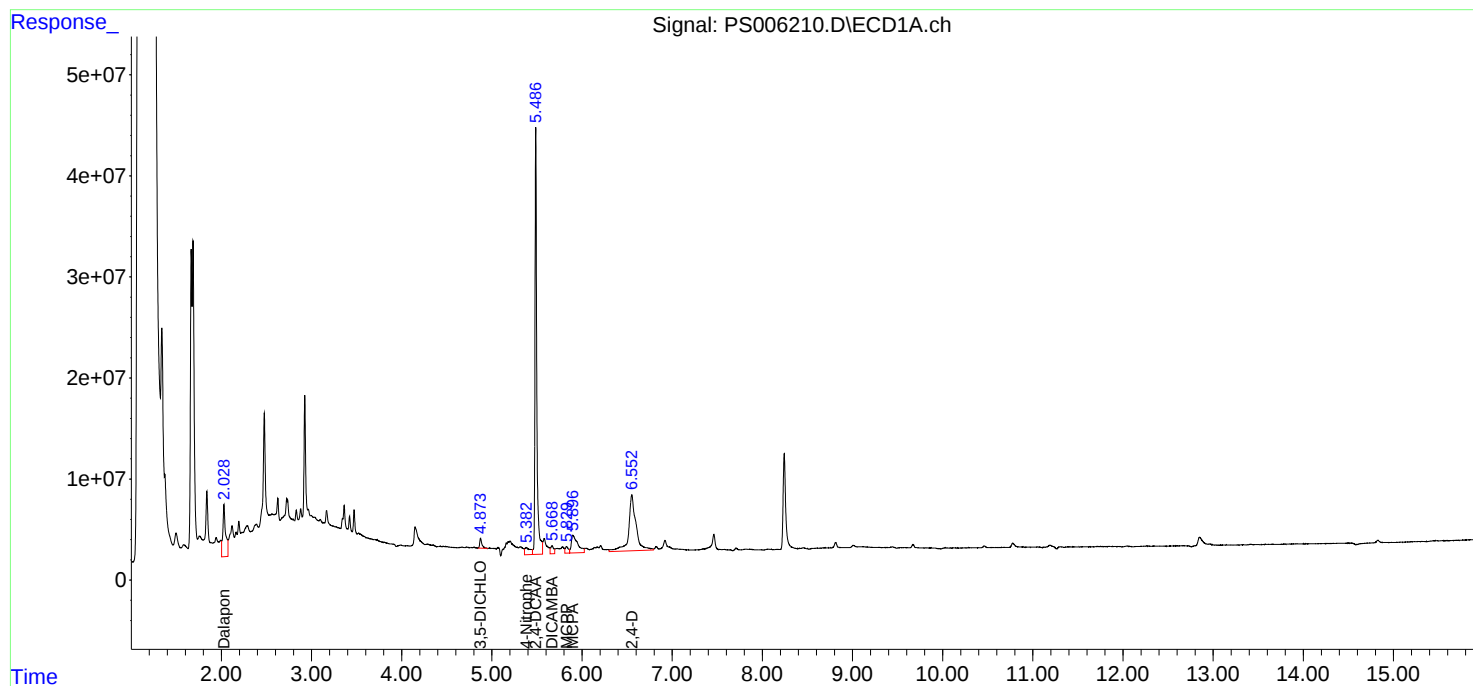


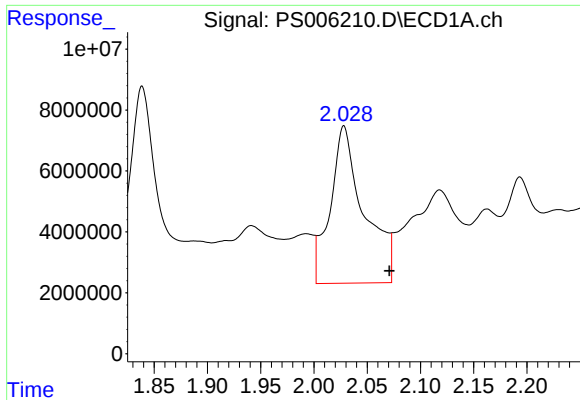

#1 Dalapon


R.T.: 2.028 min
Delta R.T.: -0.043 min
Response: 113660202
Conc: 104.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

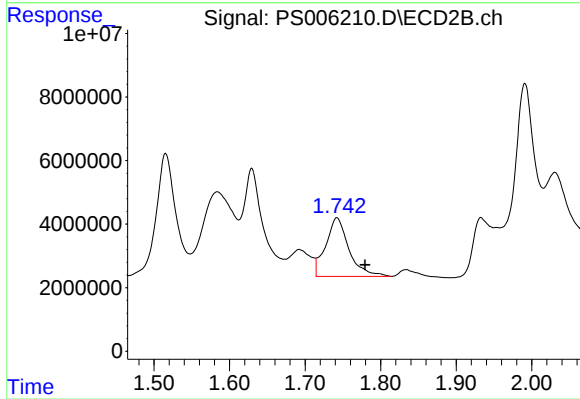


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.037 min
Response: 39480344
Conc: 62.92 ng/ml

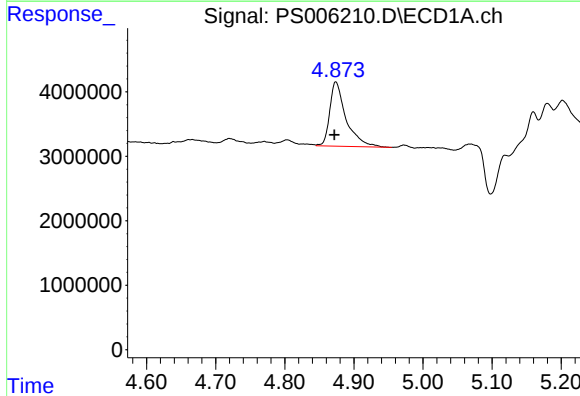


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.874 min
Delta R.T.: 0.003 min
Response: 16338586
Conc: 15.15 ng/ml

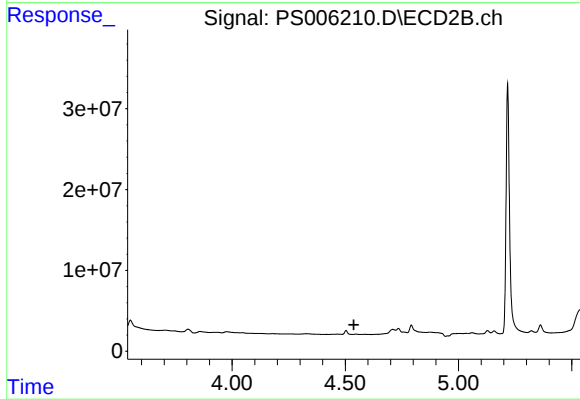

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

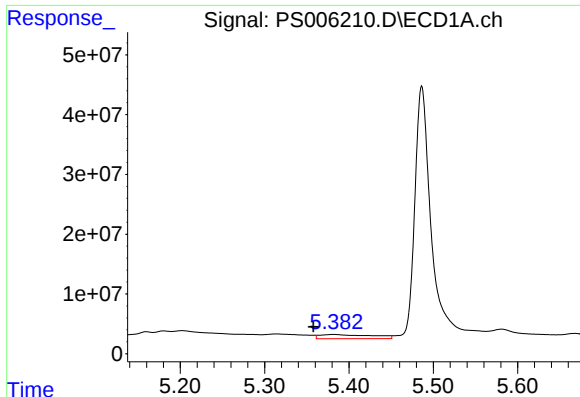

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: 0.024 min
Response: 30569389
Conc: 81.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

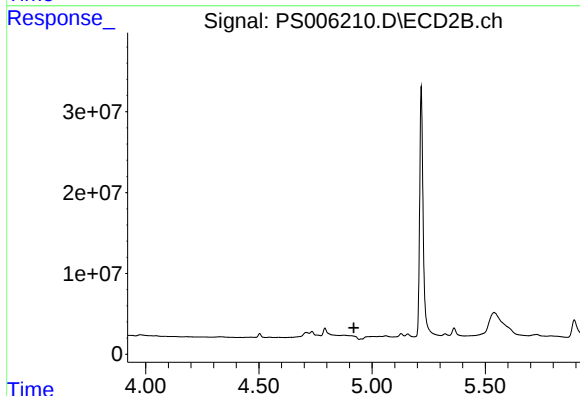


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

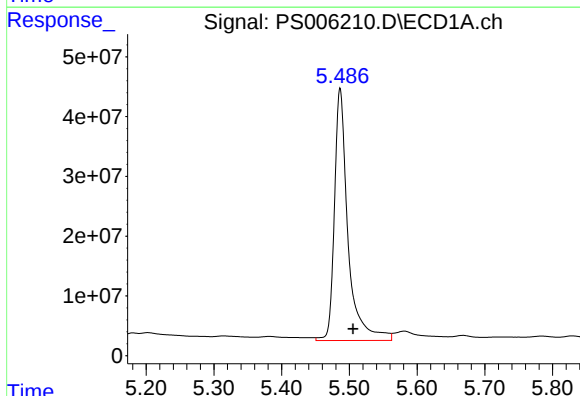


#4 2,4-DCAA

R.T.: 5.487 min
Delta R.T.: -0.019 min
Response: 586350928
Conc: 679.28 ng/ml

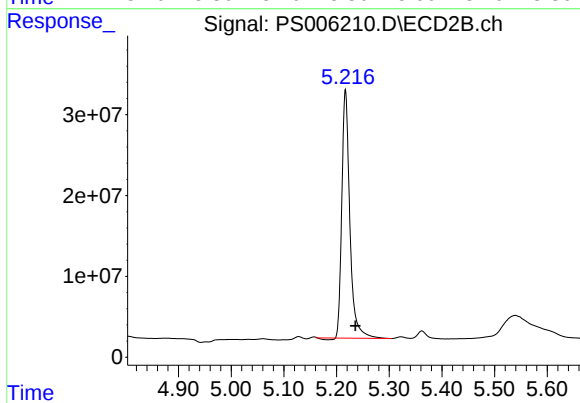

#4 2,4-DCAA


R.T.: 5.217 min
Delta R.T.: -0.019 min
Response: 324424806
Conc: 659.60 ng/ml

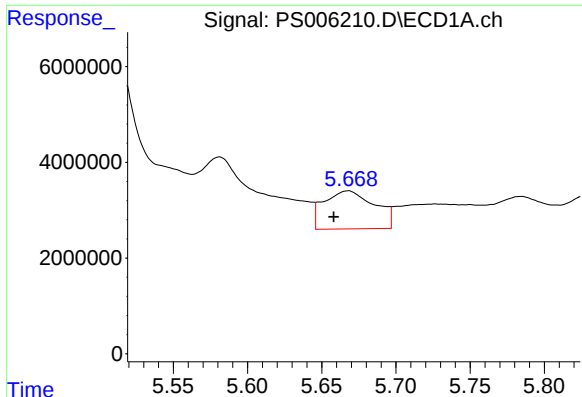

#5 DICAMBA


R.T.: 5.668 min
Delta R.T.: 0.010 min
Response: 18893080
Conc: 5.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

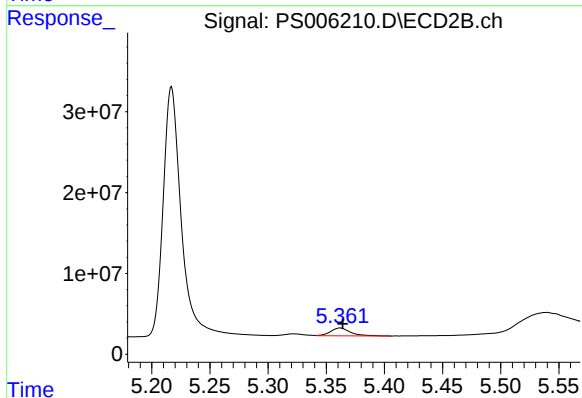


#5 DICAMBA

R.T.: 5.362 min
Delta R.T.: -0.002 min
Response: 11318098
Conc: 6.14 ng/ml

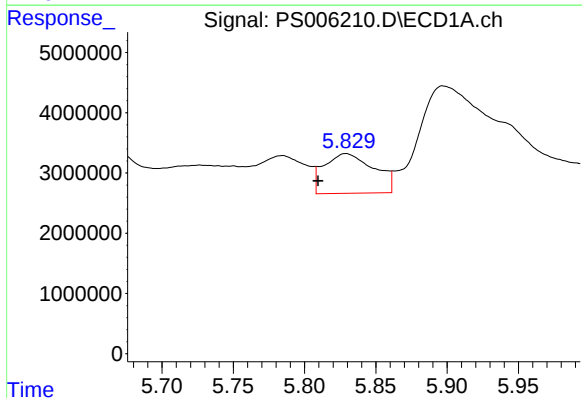


#6 MCP

R.T.: 5.829 min
Delta R.T.: 0.020 min
Response: 16025620
Conc: 7.12 ug/ml

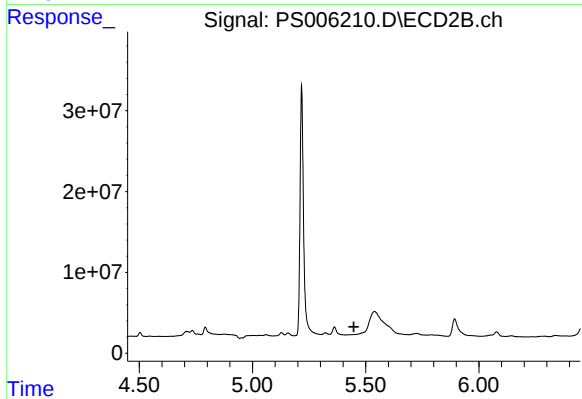

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

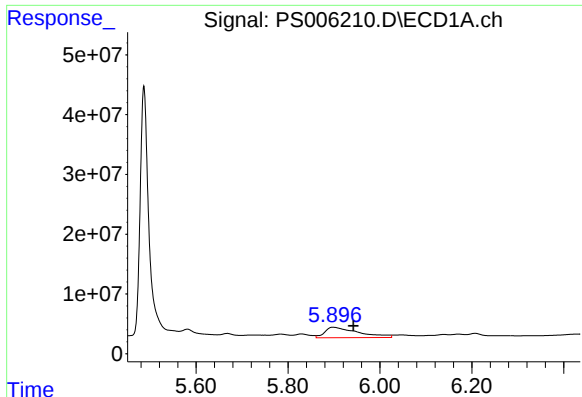

#7 MCPA


R.T.: 5.898 min
Delta R.T.: -0.044 min
Response: 88299117
Conc: 27.97 ug/ml

Instrument :
ECD_S
ClientSampleId :

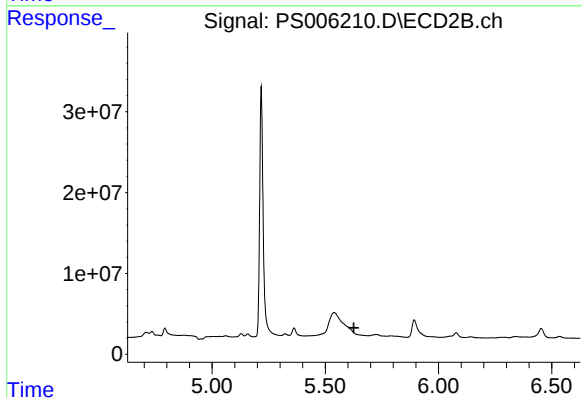


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

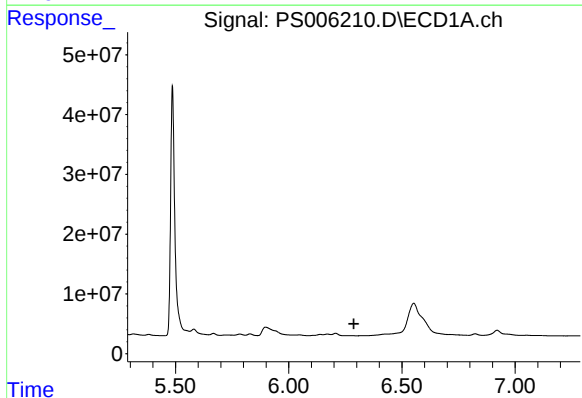


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

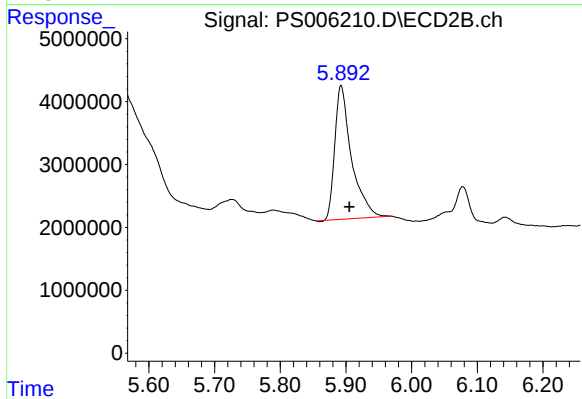

#8 DICHLORPROP


R.T.: 5.893 min
Delta R.T.: -0.012 min
Response: 37603909
Conc: 84.58 ng/ml

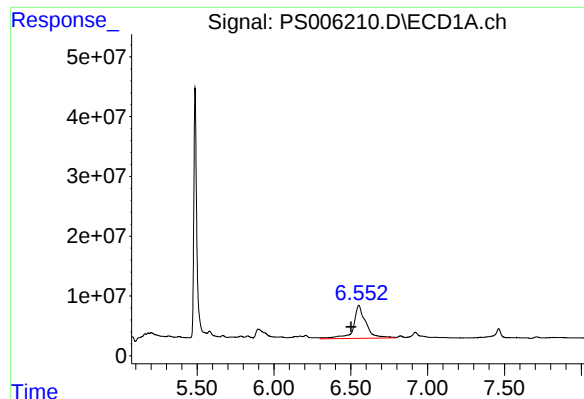

#9 2,4-D

R.T.: 6.552 min
Delta R.T.: 0.049 min
Response: 313912636
Conc: 385.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

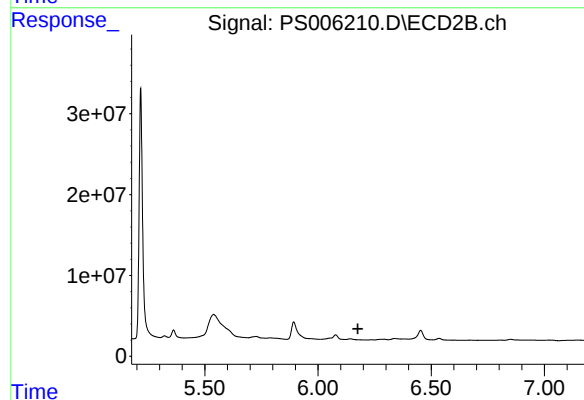

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.