

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081921\
 Data File : PS016501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 16:21
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 04:05:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.764	659.6E6	276.5E6	448.365	529.993
Target Compounds							
7) T	MCPA	7.649f	0.000	14281432	0	2.318	N.D. #
8) T	DICHLORPROP	0.000	7.577	0	7050576	N.D.	13.014
15) T	Picloram	10.995	10.828	11867836	7262098	1.189	1.804 #
16) T	DCPA	0.000	10.828f	0	7262098	N.D.	1.616



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081921\
Data File : PS016501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 16:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 04:05:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

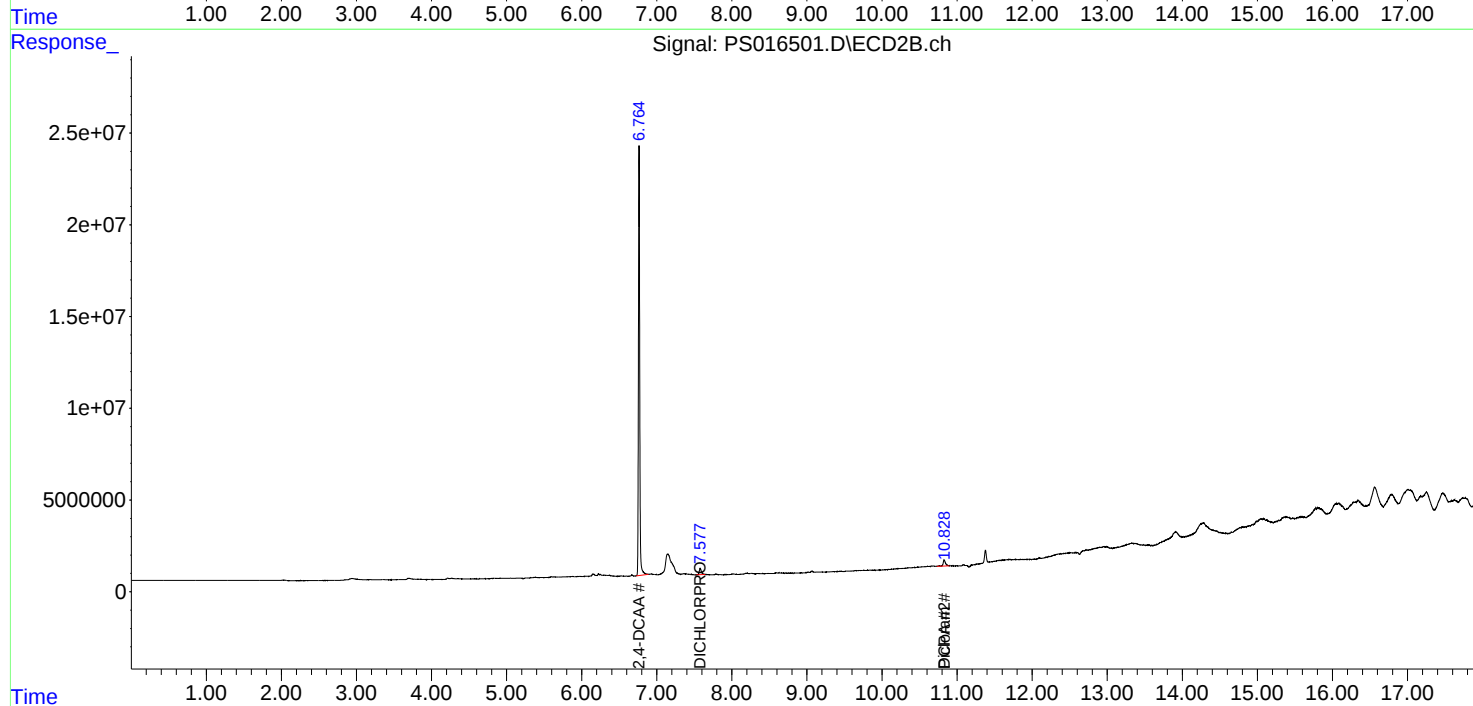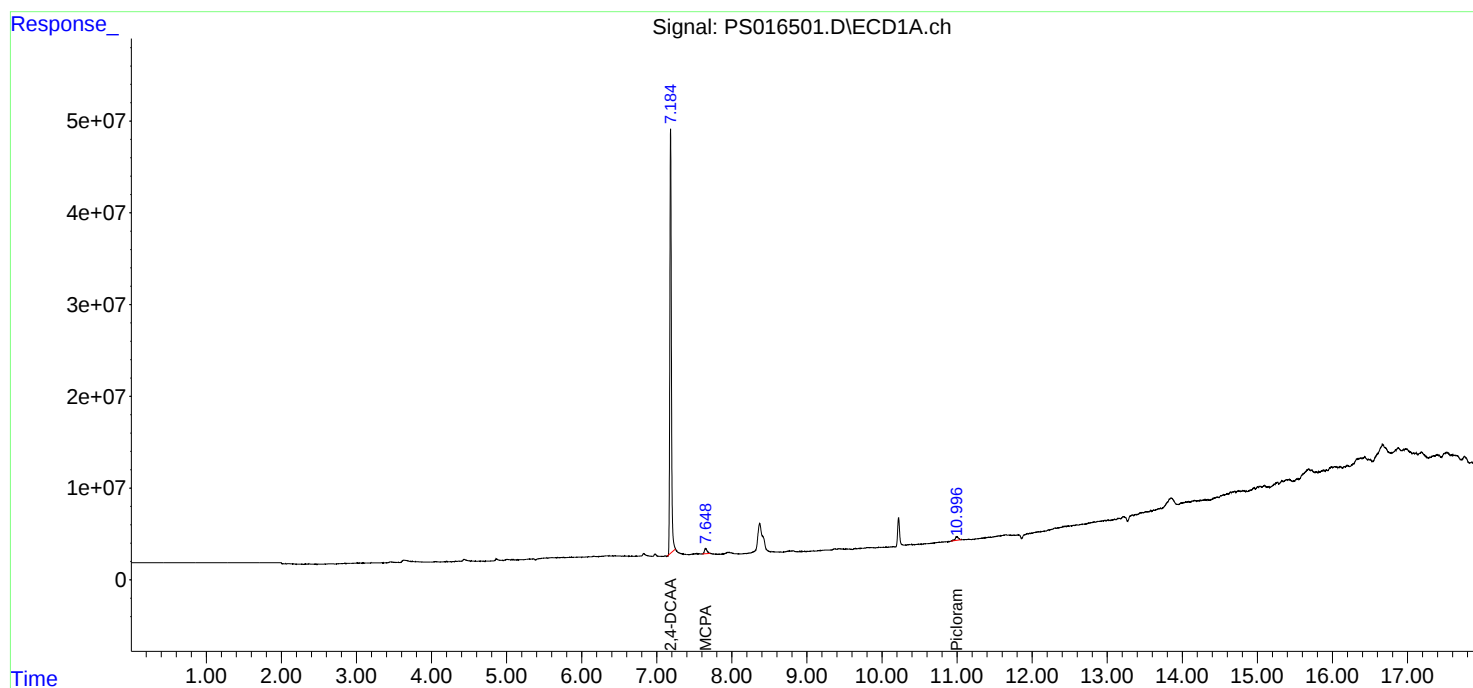


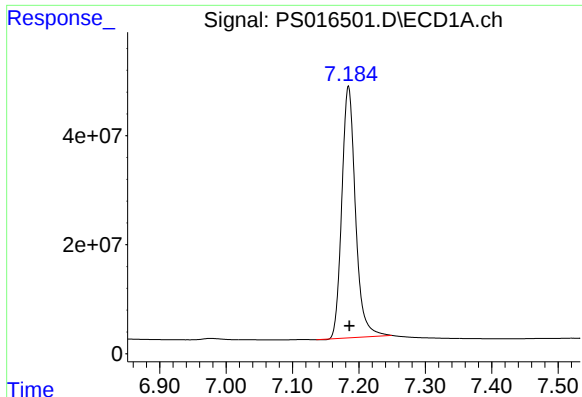

#4 2,4-DCAA


R.T.: 7.184 min
Delta R.T.: -0.001 min
Response: 659592651
Conc: 448.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

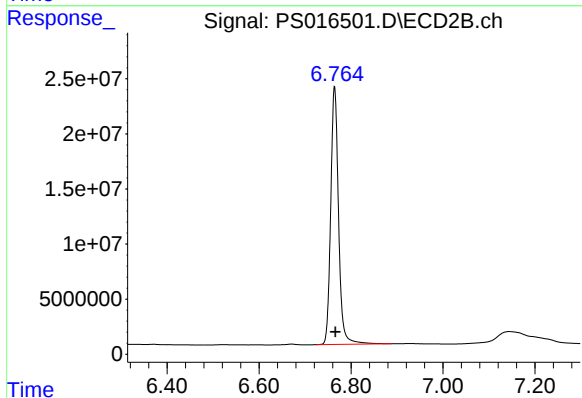


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 276457383
Conc: 529.99 ng/ml

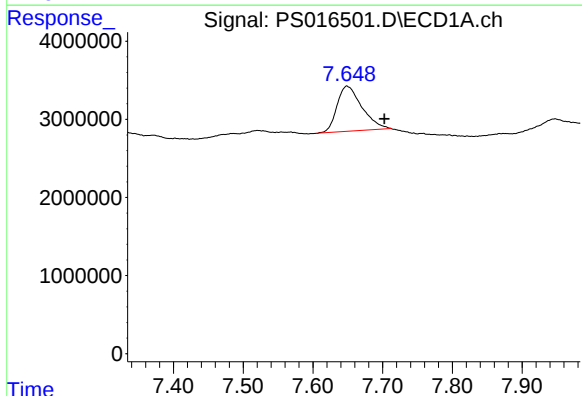


#7 MCPA

R.T.: 7.649 min
Delta R.T.: -0.054 min
Response: 14281432
Conc: 2.32 ug/ml

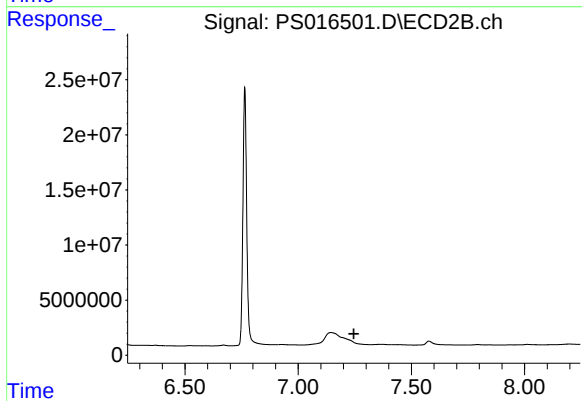

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.246 min
Response: 0
Conc: N.D.

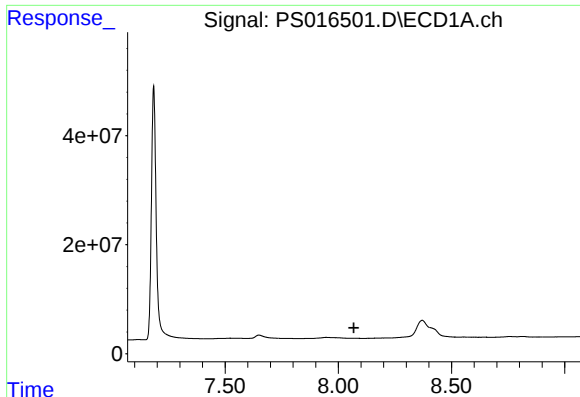

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

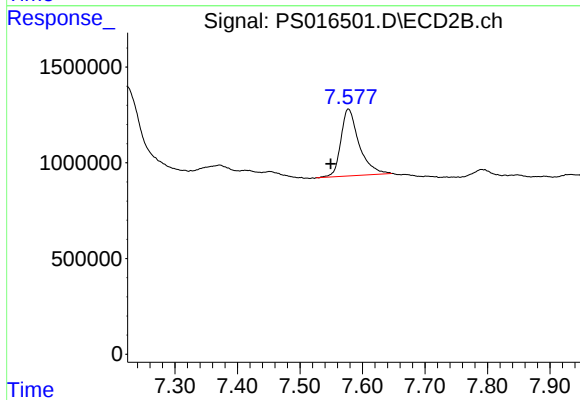


#8 DICHLORPROP

R.T.: 7.577 min
Delta R.T.: 0.028 min
Response: 7050576
Conc: 13.01 ng/ml

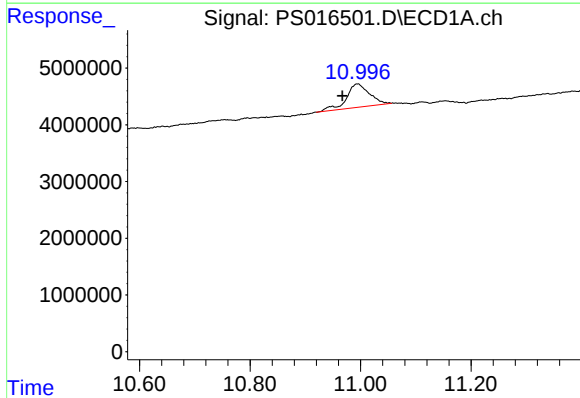


#15 Picloram

R.T.: 10.995 min
Delta R.T.: 0.028 min
Response: 11867836
Conc: 1.19 ng/ml

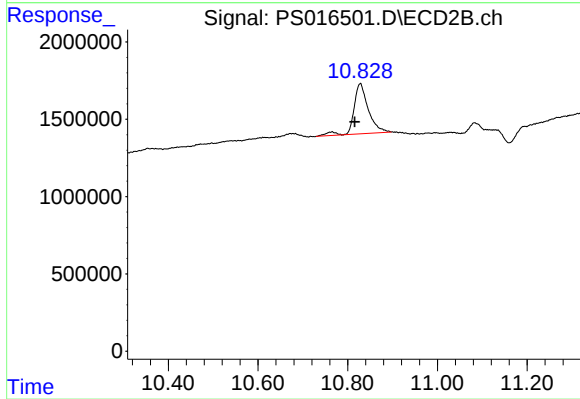

#15 Picloram


R.T.: 10.828 min
Delta R.T.: 0.013 min
Response: 7262098
Conc: 1.80 ng/ml

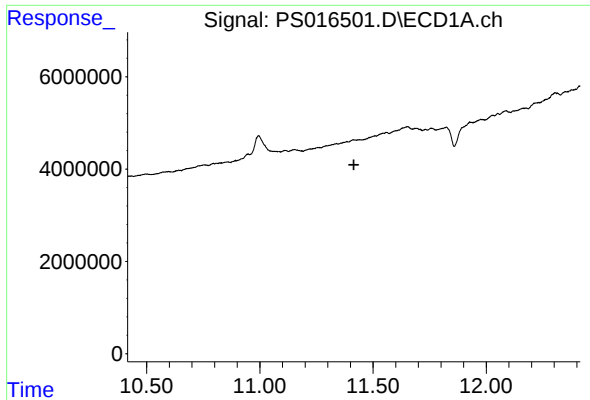

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

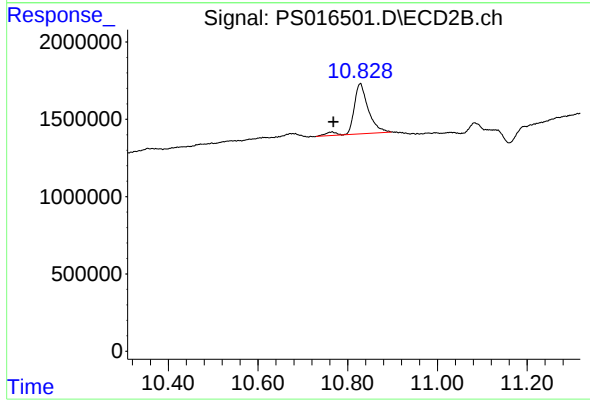

#16 DCPA

R.T.: 10.828 min
Delta R.T.: 0.060 min
Response: 7262098
Conc: 1.62 ng/ml