

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081922\
 Data File : PS020310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2022 13:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 22:21:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.760	1336.4E6	429.8E6	453.197	527.368
Target Compounds							
1) T	Dalapon	3.012	0.000	632974	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.432	0.000	329649	0	<MDL	N.D. #
3) T	4-Nitroph...	6.996	0.000	1680908	0	1.210	N.D. #
7) T	MCPA	7.654	7.155f	-109288	25398665	N.D.	6.033
10) T	Pentachlo...	8.603	0.000	1746844	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.171	0.000	3073158	0	<MDL	N.D. #
12) T	2,4,5-T	9.446	0.000	6605013	0	<MDL	N.D. #
13) T	2,4-DB	10.014	0.000	553718	0	<MDL	N.D. #
14) T	DINOSEB	11.133	0.000	19970121	0	1.255	N.D. #
15) T	Picloram	10.987	0.000	366470	0	<MDL	N.D. #
16) T	DCPA	11.407	0.000	3420207	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081922\
Data File : PS020310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2022 13:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 22:21:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

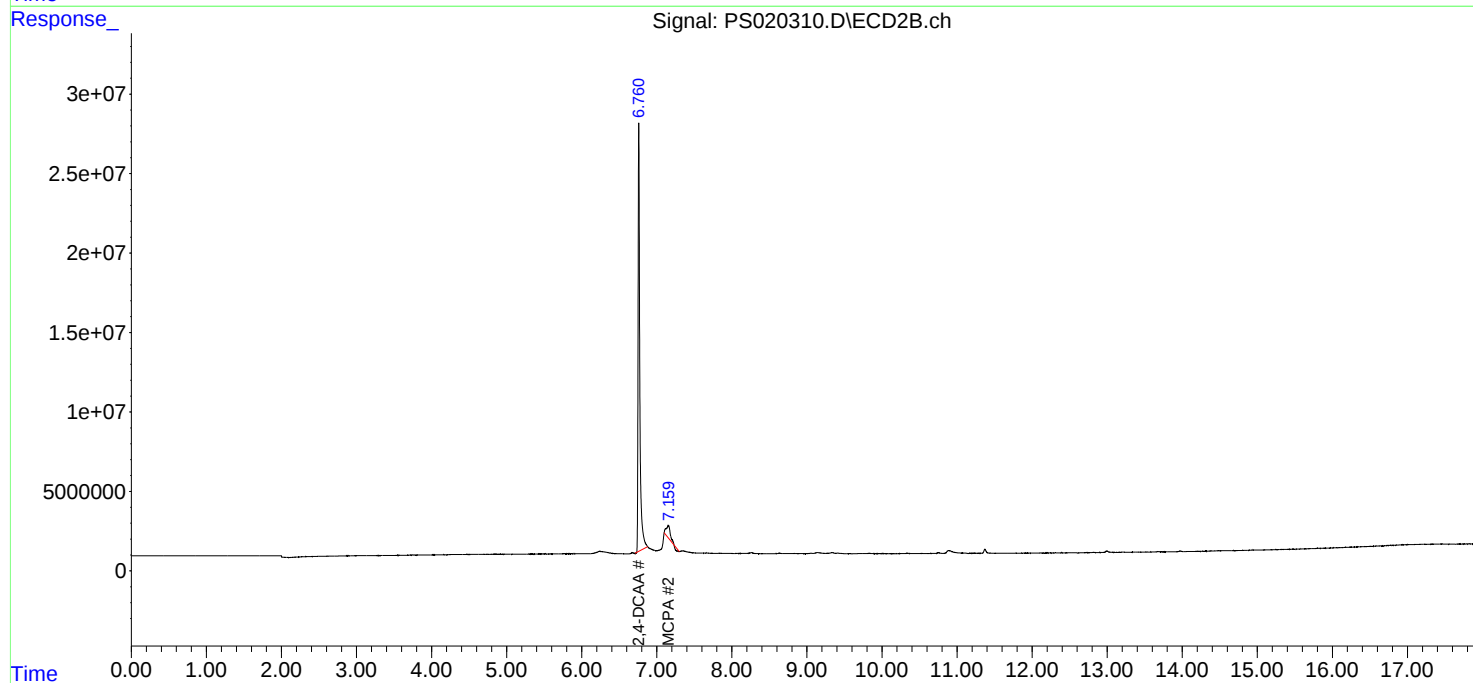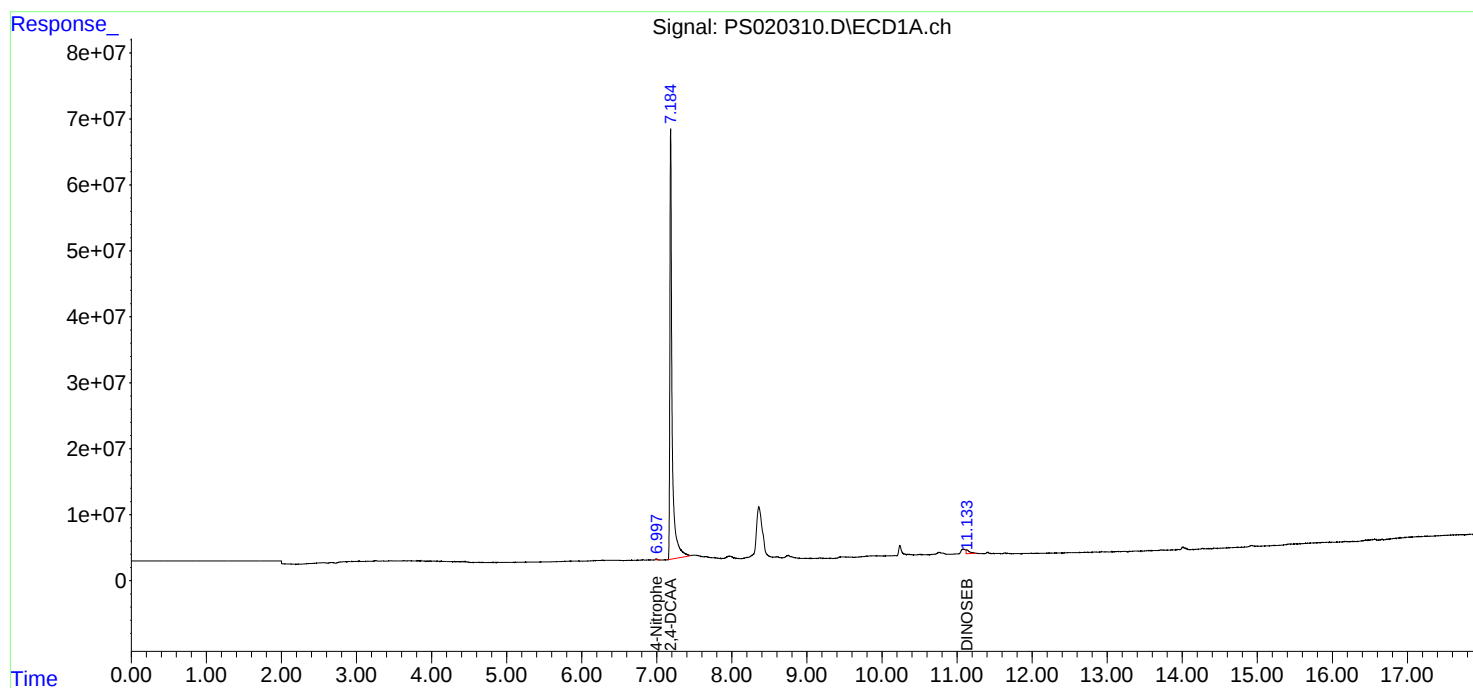


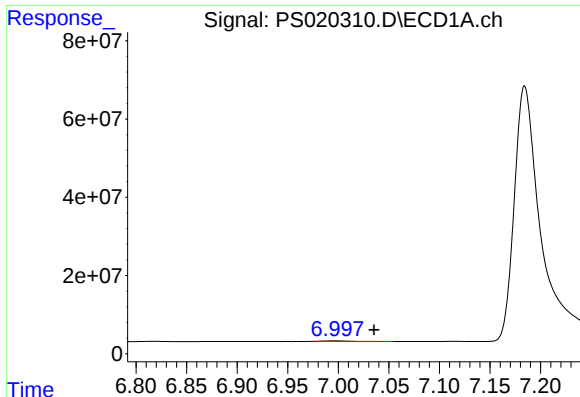

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.039 min
Response: 1680908
Conc: 1.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

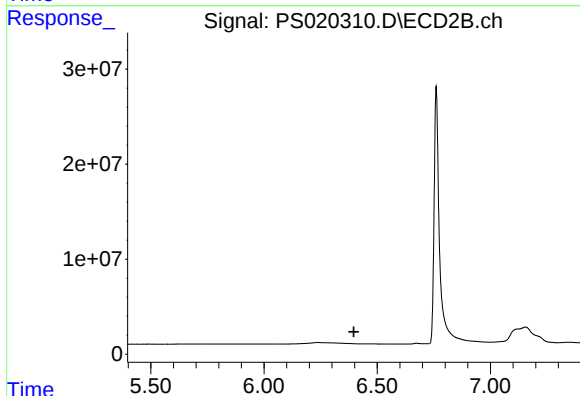


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.397 min
Response: 0
Conc: N.D.

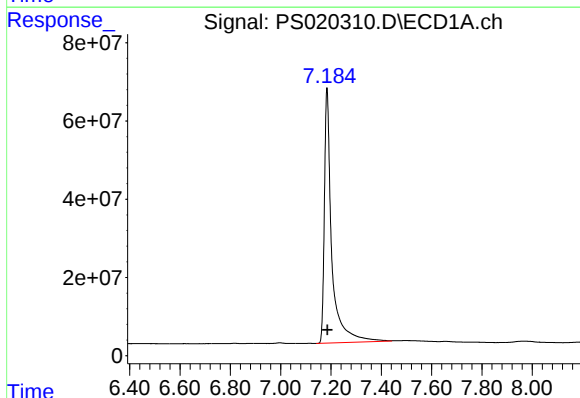


#4 2,4-DCAA

R.T.: 7.184 min
Delta R.T.: -0.001 min
Response: 1336353053
Conc: 453.20 ng/ml

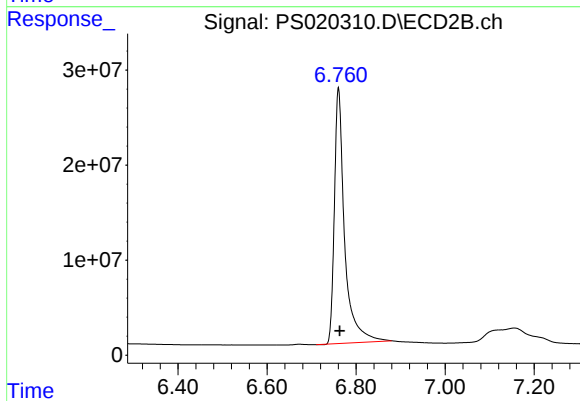

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: -0.003 min
Response: 429781632
Conc: 527.37 ng/ml

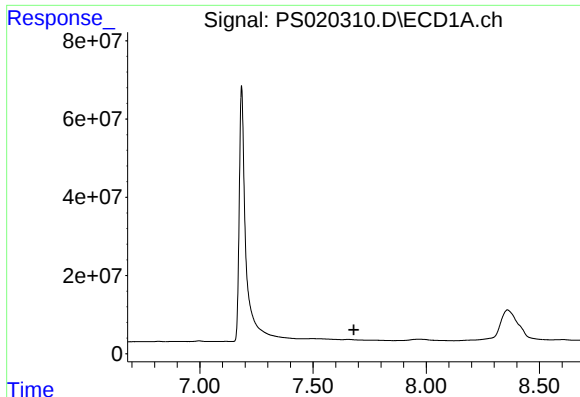

#7 MCPA


R.T.: 7.654 min
Delta R.T.: -0.026 min
Response: -109288
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

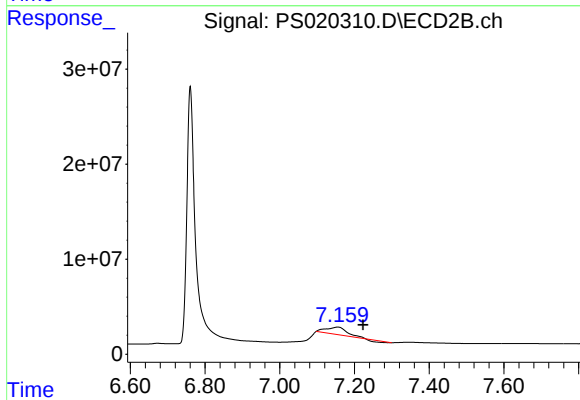


#7 MCPA

R.T.: 7.155 min
Delta R.T.: -0.068 min
Response: 25398665
Conc: 6.03 ug/ml

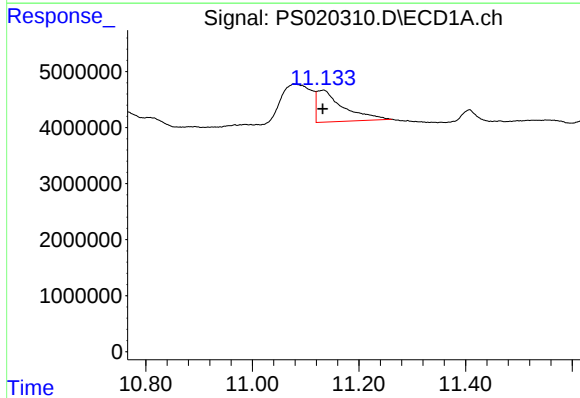

#14 DINOSEB

R.T.: 11.133 min
Delta R.T.: 0.000 min
Response: 19970121
Conc: 1.26 ng/ml

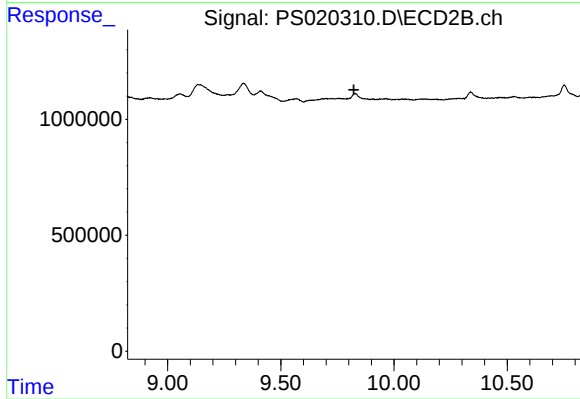

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.823 min
Response: 0
Conc: N.D.