

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
 Data File : PS027457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 11:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 14:53:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.166	7.738	1156.5E6	929.1E6	447.182	470.624
Target Compounds							
3) T	4-Nitroph...	6.966	0.000	6117070	0	3.928	N.D. #
5) T	DICAMBA	0.000	7.932	0	1033196	N.D.	<MDL
7) T	MCPA	0.000	8.270	0	5334195	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.651	0	50500	N.D.	<MDL
10) T	Pentachlo...	8.597f	9.462f	2195651	282497	<MDL	<MDL #
12) T	2,4,5-T	9.445f	10.297	301068	1249433	<MDL	<MDL #
13) T	2,4-DB	9.993	10.883	168777	104086	<MDL	<MDL #
14) T	DINOSEB	0.000	11.242	0	355054	N.D.	<MDL
15) T	Picloram	11.026f	12.337	9997071	9529795	<MDL	<MDL #
16) T	DCPA	0.000	12.239f	0	5013181	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
Data File : PS027457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 11:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 14:53:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

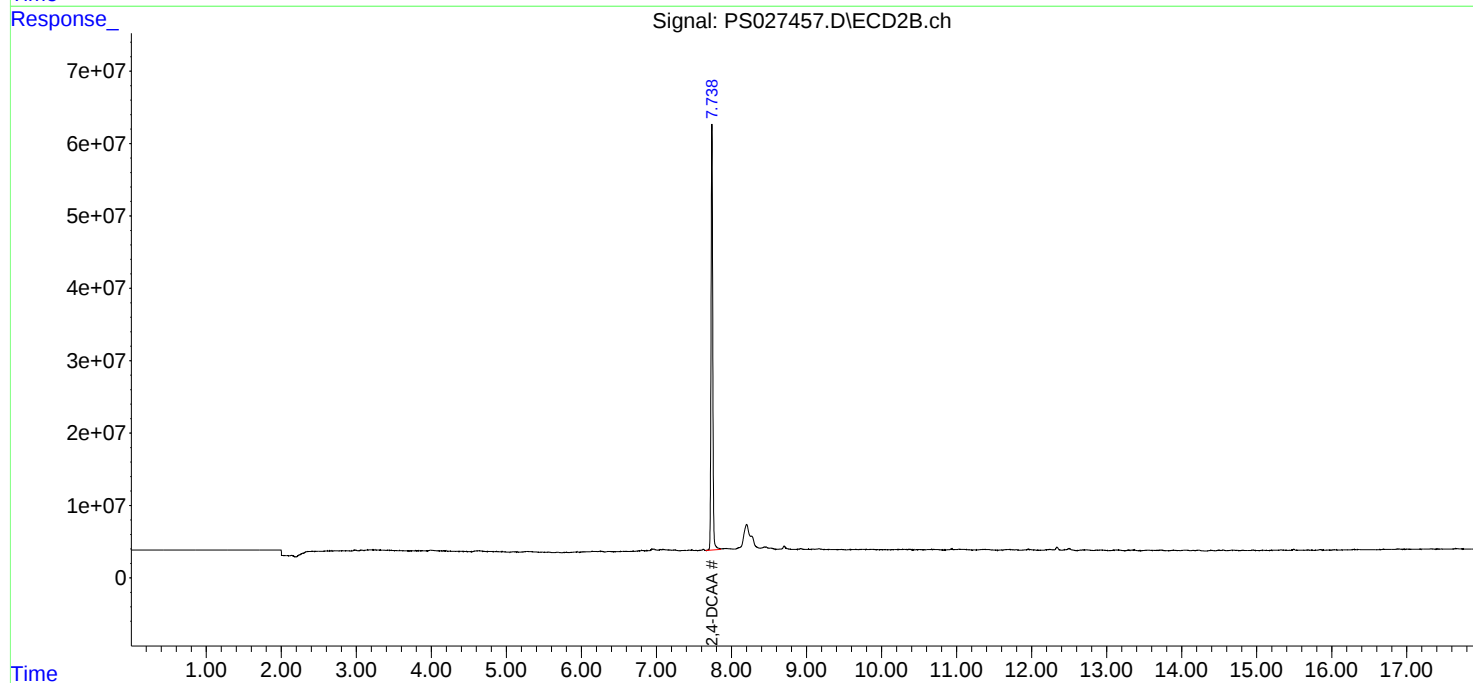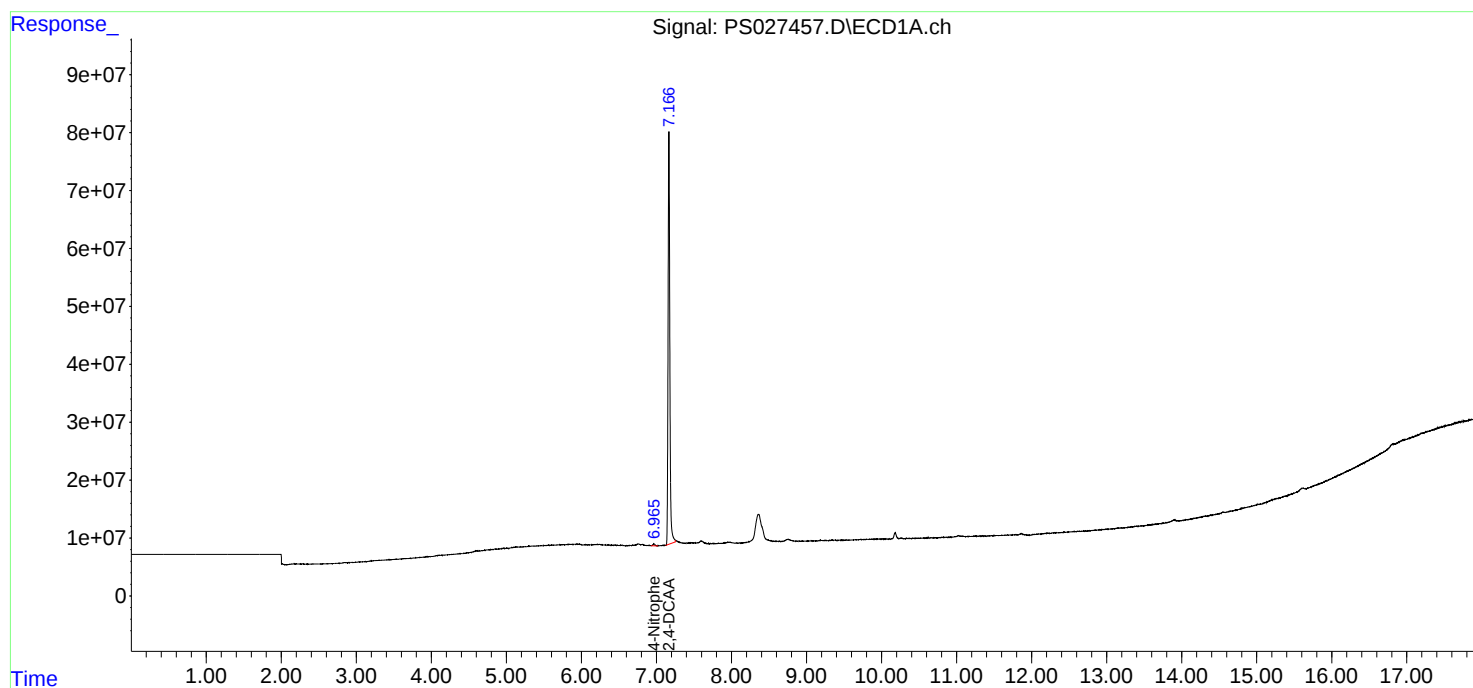


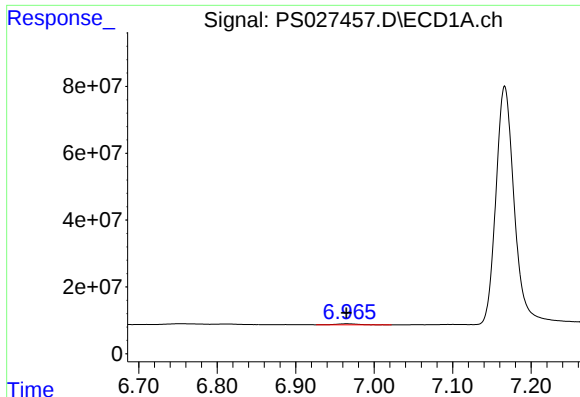

#3 4-Nitrophenol


R.T.: 6.966 min
Delta R.T.: 0.001 min
Response: 6117070
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

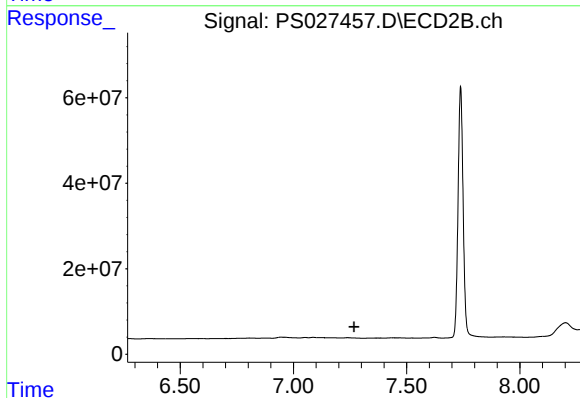


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.267 min
Response: 0
Conc: N.D.

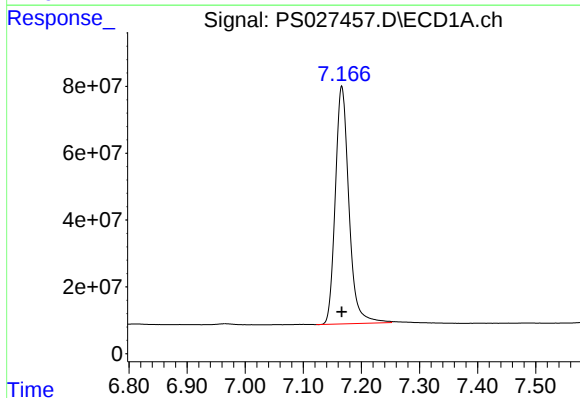

#4 2,4-DCAA

R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 1156529344
Conc: 447.18 ng/ml

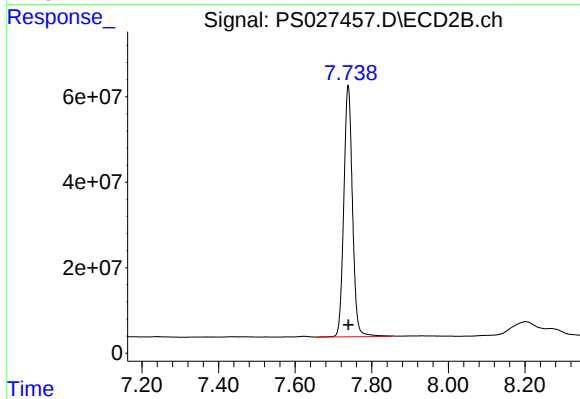

#4 2,4-DCAA

R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 929122982
Conc: 470.62 ng/ml