

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
 Data File : PS027464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 14:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:28:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.166	7.738	1164.6E6	946.8E6	450.309	479.567
Target Compounds							
2) T	3,5-DICHL...	0.000	6.694	0	211863	N.D.	<MDL
3) T	4-Nitroph...	6.962	7.243	13063941	550986	8.389	<MDL #
5) T	DICAMBA	0.000	7.935	0	6290337	N.D.	<MDL
6) T	MCP	7.483f	8.038	1617857	1222836	<MDL	<MDL #
8) T	DICHLORPROP	8.044	8.651	804659	118468	<MDL	<MDL #
10) T	Pentachlo...	8.557	9.502	3029096	2006057	<MDL	<MDL #
11) T	2,4,5-TP ...	9.128	9.880	6518522	2749554	<MDL	<MDL #
12) T	2,4,5-T	9.427	10.302	11544621	1848311	<MDL	<MDL #
13) T	2,4-DB	9.985	10.863	7426011	99694	3.473	<MDL #
14) T	DINOSEB	11.158	11.240	17962188	661149	1.498	<MDL #
15) T	Picloram	10.969	12.338	34344082	32394292	1.709	1.655
16) T	DCPA	11.431f	12.242f	9617291	792564	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
Data File : PS027464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 14:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:28:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

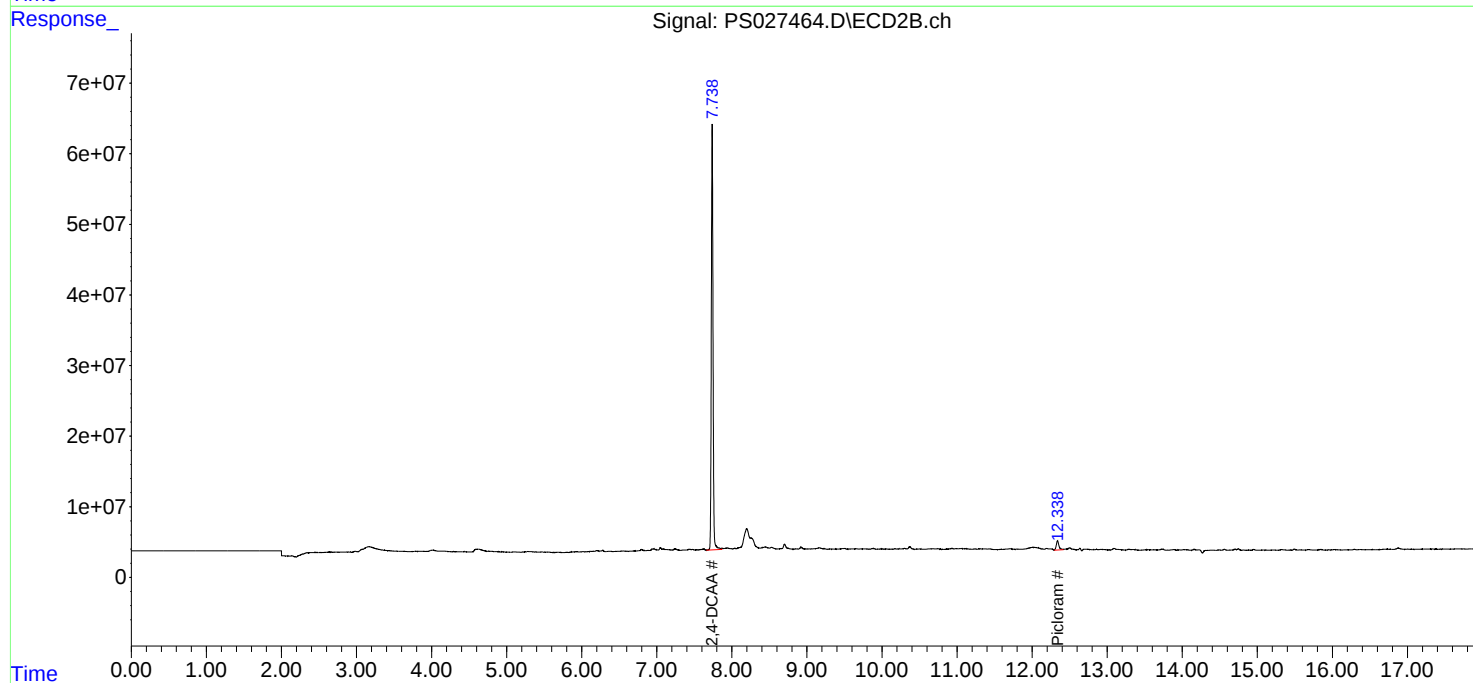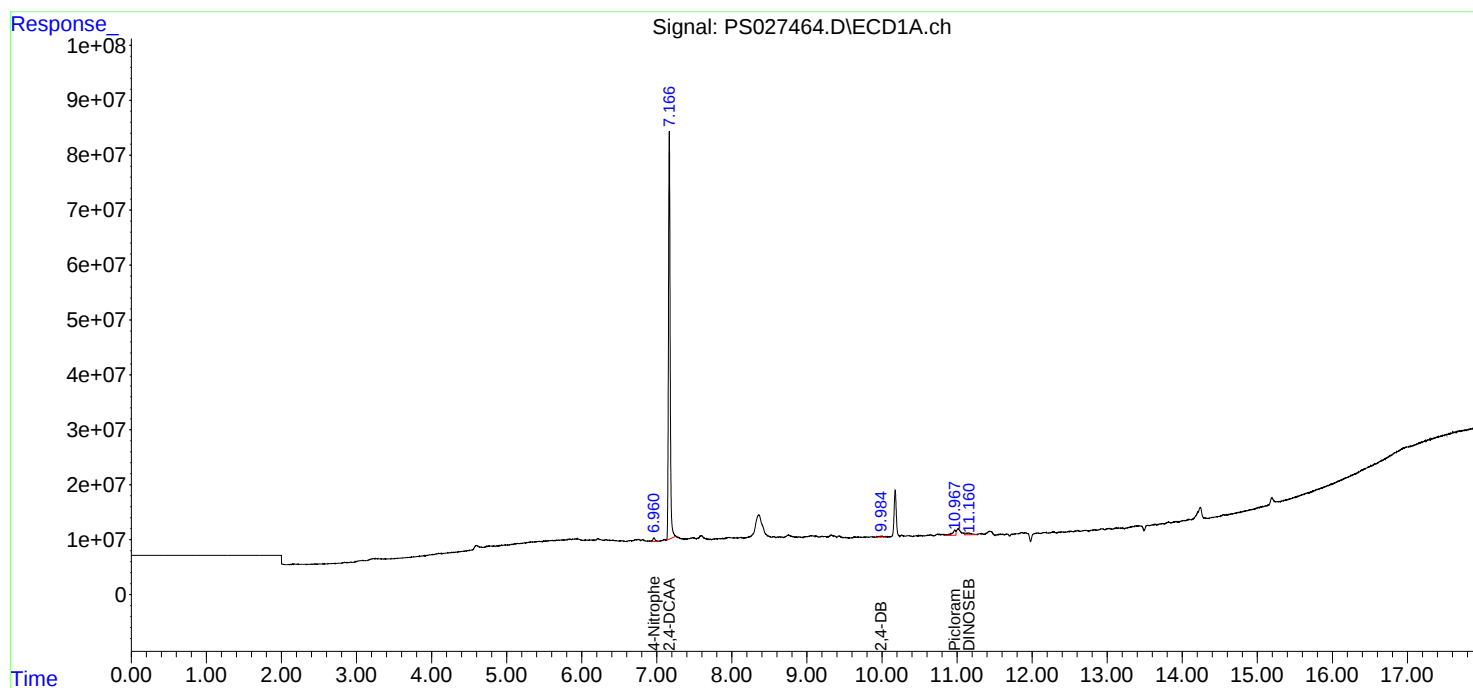


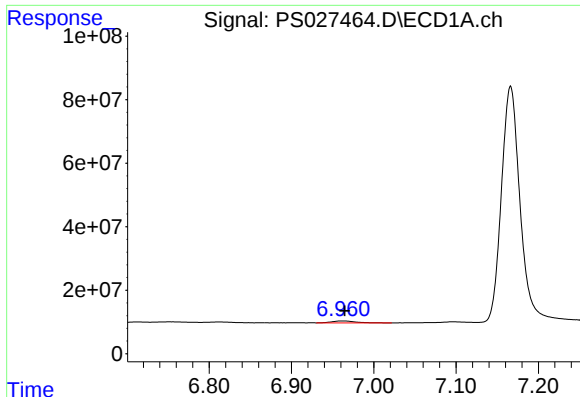

#3 4-Nitrophenol


R.T.: 6.962 min
Delta R.T.: -0.003 min
Response: 13063941
Conc: 8.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

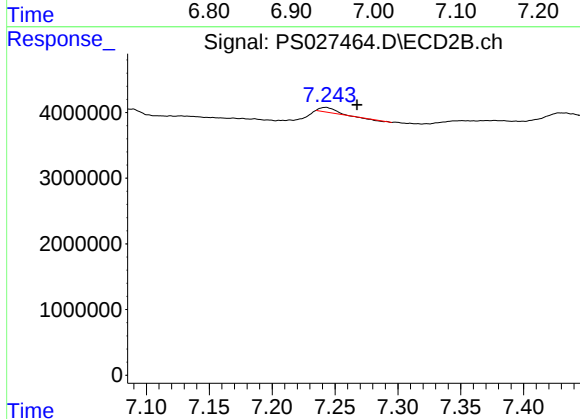


#3 4-Nitrophenol

R.T.: 7.243 min
Delta R.T.: -0.024 min
Response: 550986
Conc: N.D.

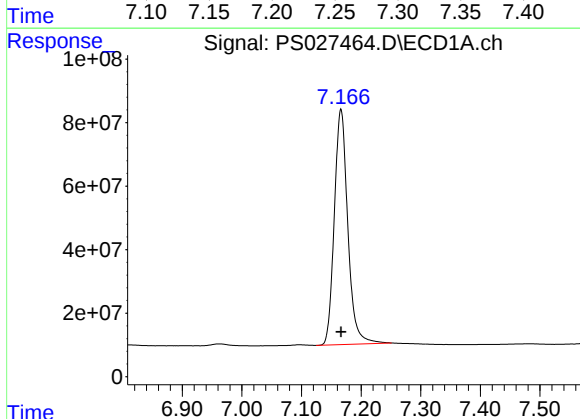


#4 2,4-DCAA

R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 1164616493
Conc: 450.31 ng/ml

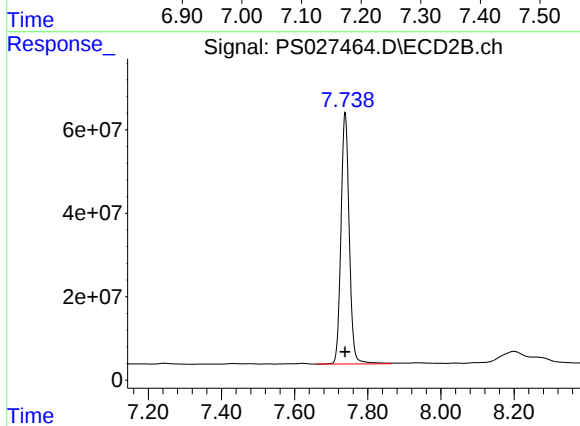

#4 2,4-DCAA


R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 946778445
Conc: 479.57 ng/ml

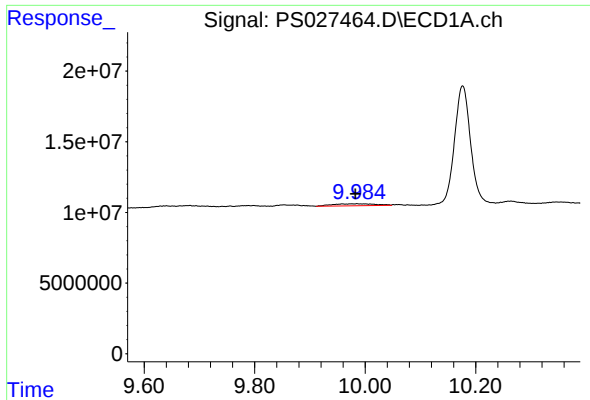

#13 2,4-DB


R.T.: 9.985 min
Delta R.T.: 0.003 min
Response: 7426011
Conc: 3.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

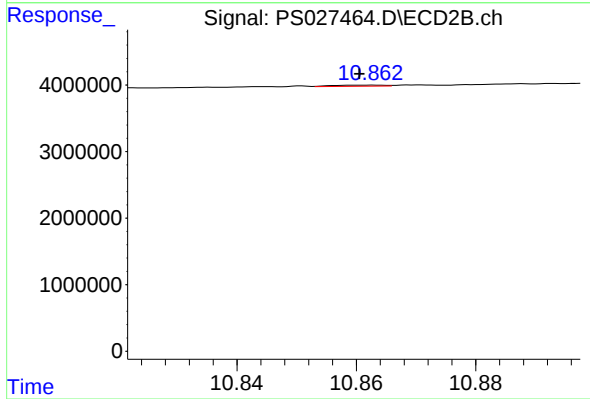


#13 2,4-DB

R.T.: 10.863 min
Delta R.T.: 0.002 min
Response: 99694
Conc: N.D.

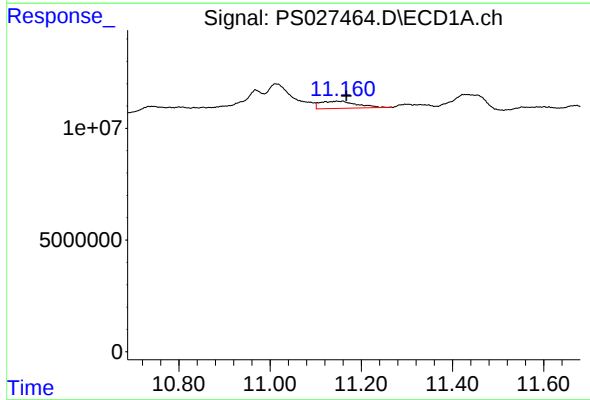


#14 DINOSEB

R.T.: 11.158 min
Delta R.T.: -0.009 min
Response: 17962188
Conc: 1.50 ng/ml

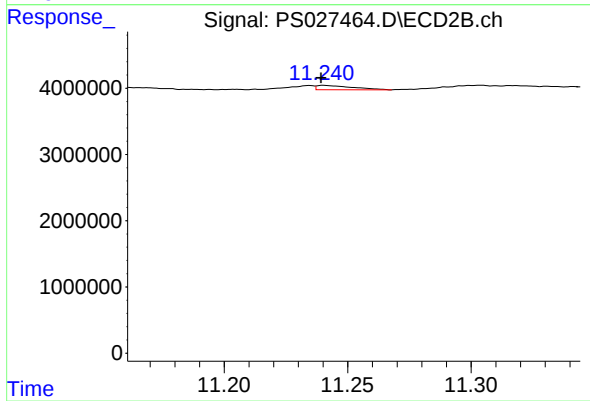

#14 DINOSEB


R.T.: 11.240 min
Delta R.T.: 0.000 min
Response: 661149
Conc: N.D.

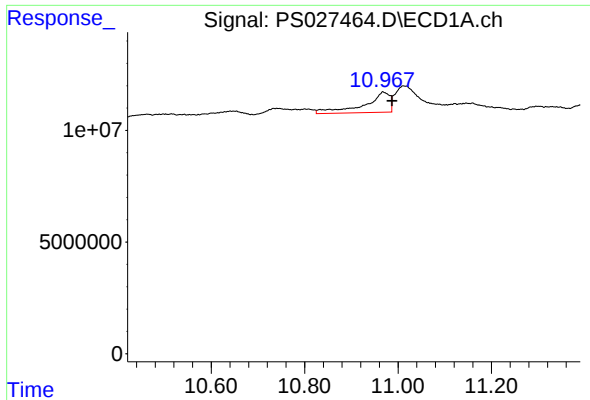

#15 Picloram

R.T.: 10.969 min
Delta R.T.: -0.018 min
Response: 34344082
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

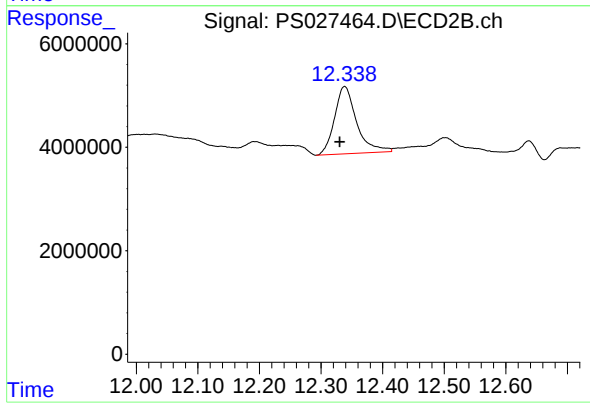

#15 Picloram

R.T.: 12.338 min
Delta R.T.: 0.008 min
Response: 32394292
Conc: 1.65 ng/ml