

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
 Data File : PS027476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 19:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:34:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.165	7.738	1220.4E6	961.8E6	471.870	487.159
Target Compounds							
1) T	Dalapon	0.000	2.665f	0	6542076	N.D.	1.791
3) T	4-Nitroph...	6.961	0.000	6104576	0	3.920	N.D. #
5) T	DICAMBA	0.000	7.930	0	7062372	N.D.	<MDL
6) T	MCP	0.000	8.040	0	697080	N.D.	<MDL
8) T	DICHLORPROP	8.049	0.000	163385	0	<MDL	N.D. #
10) T	Pentachlo...	8.563	9.495	1826570	824219	<MDL	<MDL #
11) T	2,4,5-TP ...	9.125	9.903	460370	3793760	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.301	0	994674	N.D.	<MDL
14) T	DINOSEB	11.198f	11.249	6092813	1348320	<MDL	<MDL #
15) T	Picloram	10.965	12.341	28200688	15903287	1.404	<MDL #
16) T	DCPA	0.000	12.253f	0	12311489	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
Data File : PS027476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 19:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:34:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

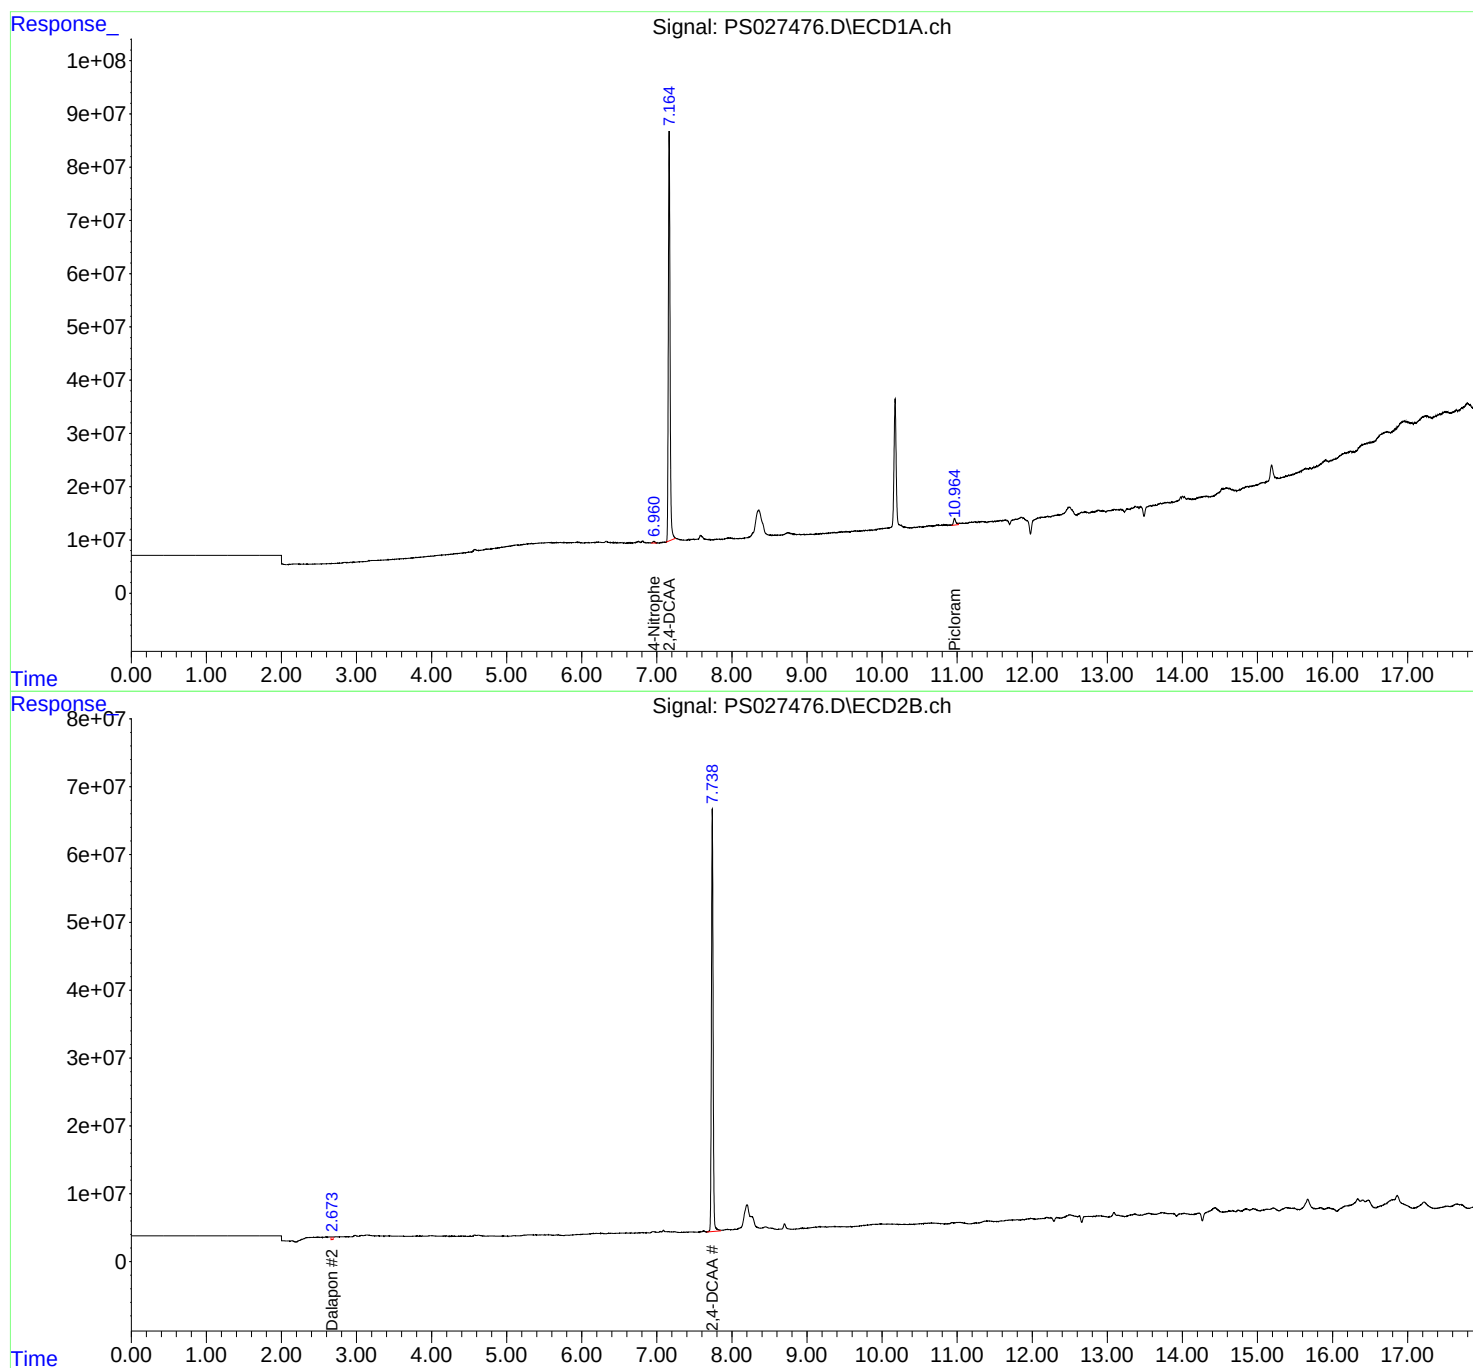


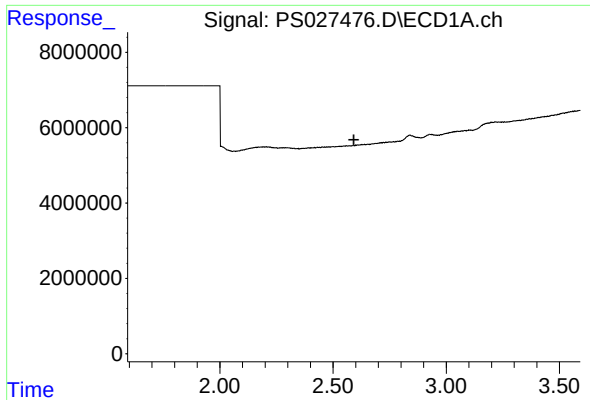

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

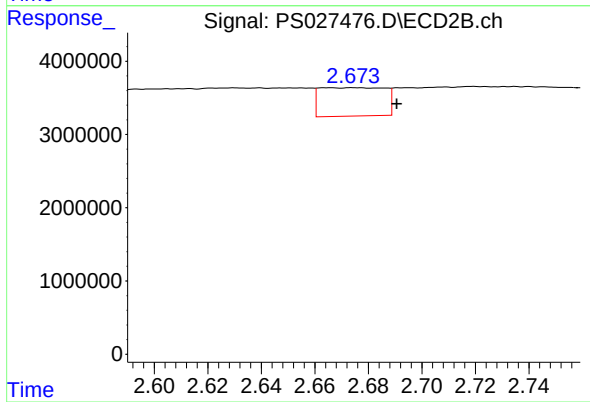


#1 Dalapon

R.T.: 2.665 min
Delta R.T.: -0.025 min
Response: 6542076
Conc: 1.79 ng/ml

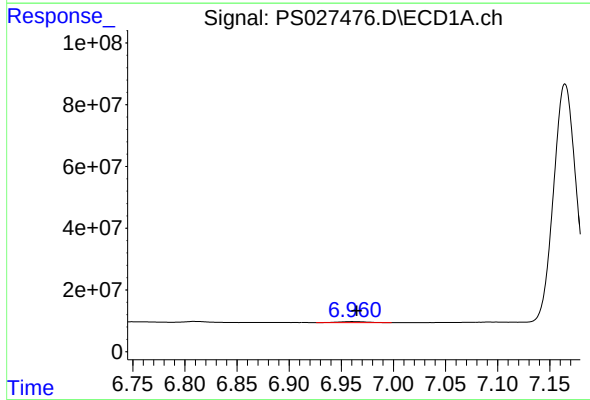


#3 4-Nitrophenol

R.T.: 6.961 min
Delta R.T.: -0.003 min
Response: 6104576
Conc: 3.92 ng/ml

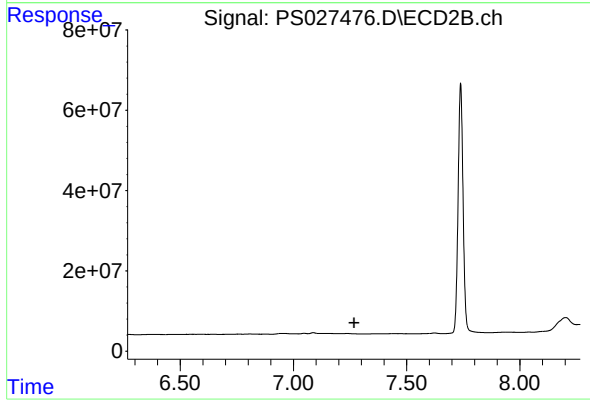

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

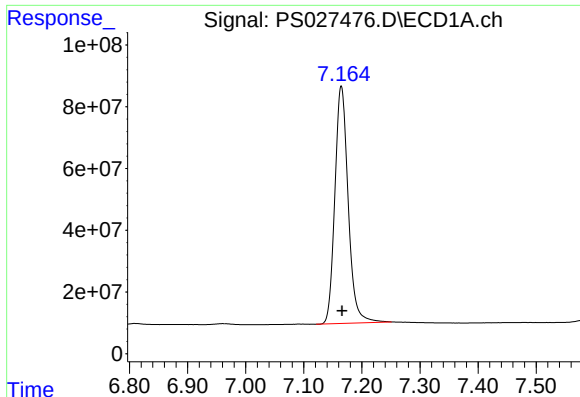

#4 2,4-DCAA


R.T.: 7.165 min
Delta R.T.: -0.001 min
Response: 1220379228
Conc: 471.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

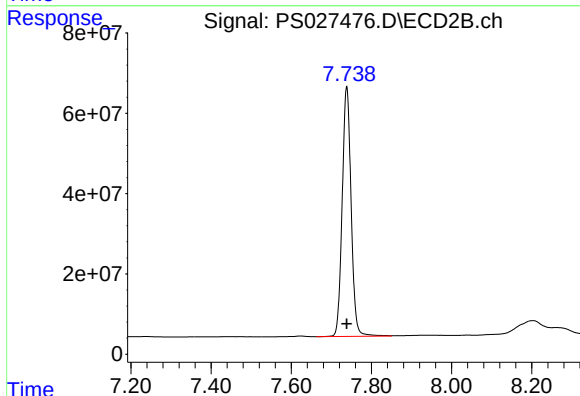


#4 2,4-DCAA

R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 961766419
Conc: 487.16 ng/ml

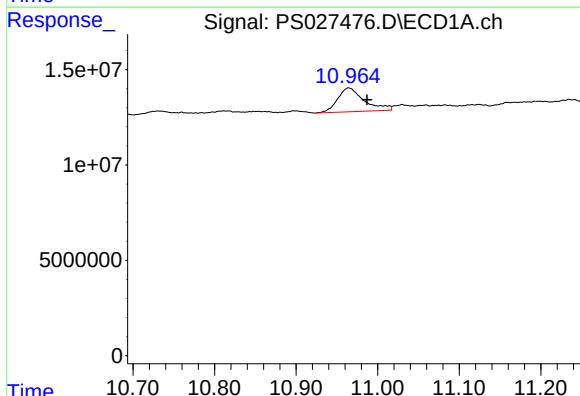

#15 Picloram

R.T.: 10.965 min
Delta R.T.: -0.022 min
Response: 28200688
Conc: 1.40 ng/ml

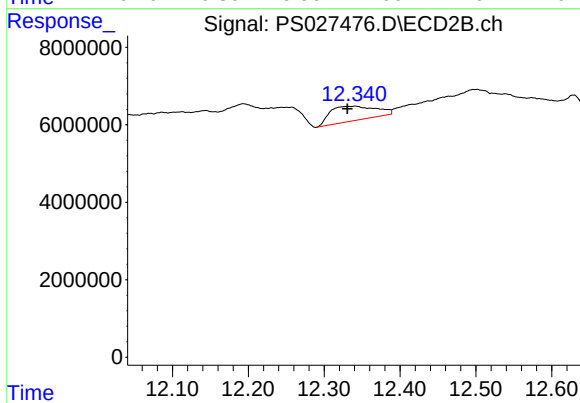

#15 Picloram

R.T.: 12.341 min
Delta R.T.: 0.010 min
Response: 15903287
Conc: N.D.