

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
 Data File : PS027486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2024 00:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:38:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.164	7.738	1220.8E6	962.9E6	472.019	487.732
Target Compounds							
1) T	Dalapon	0.000	2.723f	0	10838206	N.D.	2.967
2) T	3,5-DICHL...	0.000	6.702	0	220038	N.D.	<MDL
3) T	4-Nitroph...	6.959	0.000	14216522	0	9.130	N.D. #
5) T	DICAMBA	0.000	7.935	0	7472836	N.D.	<MDL
6) T	MCP	7.479f	8.040	1617354	1768518	<MDL	<MDL #
8) T	DICHLORPROP	8.066f	0.000	293218	0	<MDL	N.D. #
10) T	Pentachlo...	8.579	9.503	2523322	896957	<MDL	<MDL #
11) T	2,4,5-TP ...	9.113	9.886	2515489	1886494	<MDL	<MDL #
13) T	2,4-DB	9.982	0.000	2202882	0	1.030	N.D. #
14) T	DINOSEB	11.152	0.000	2569750	0	<MDL	N.D. #
15) T	Picloram	10.963	12.334	49962970	18063407	2.487	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
Data File : PS027486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2024 00:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:38:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

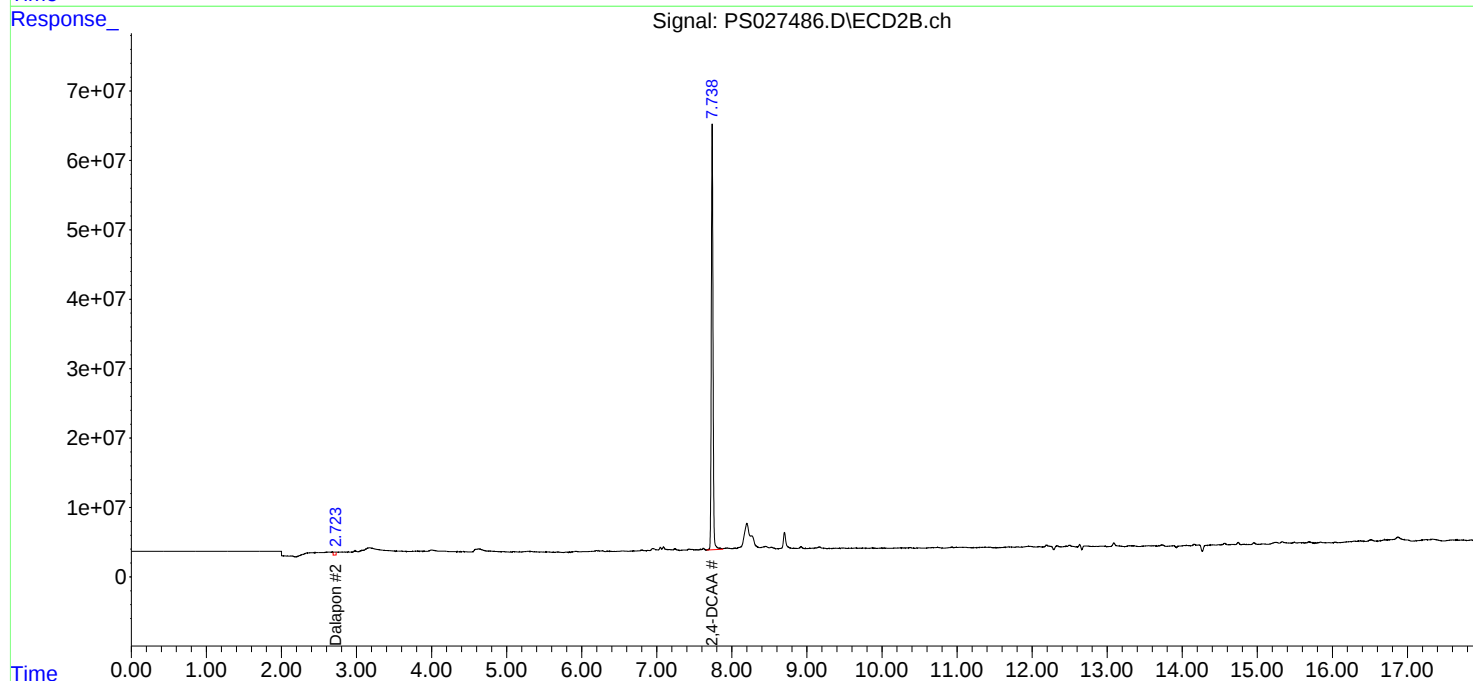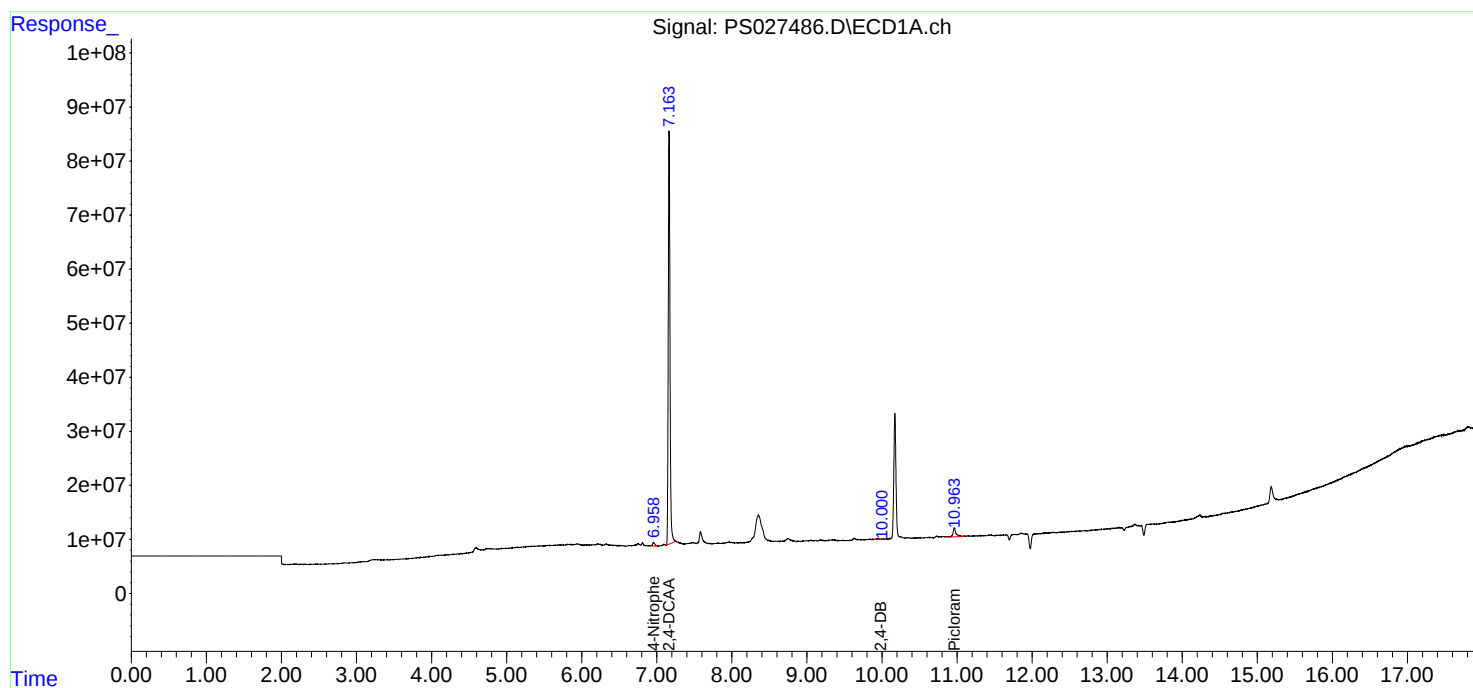


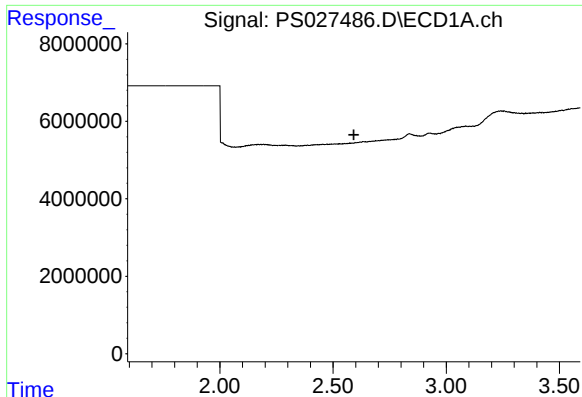

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

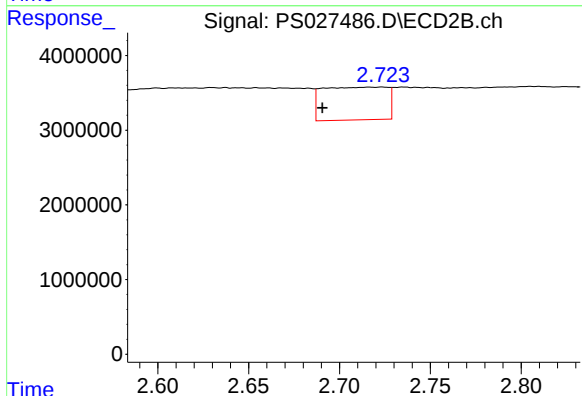


#1 Dalapon

R.T.: 2.723 min
Delta R.T.: 0.033 min
Response: 10838206
Conc: 2.97 ng/ml

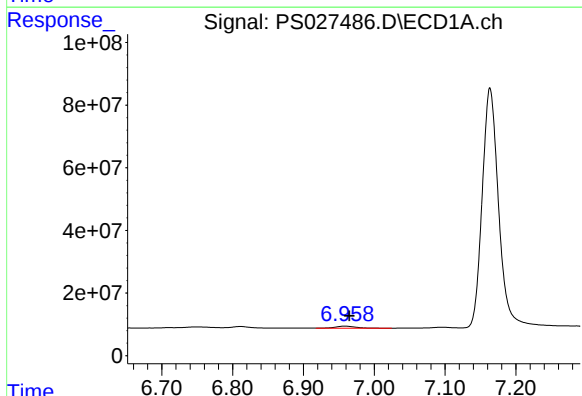


#3 4-Nitrophenol

R.T.: 6.959 min
Delta R.T.: -0.006 min
Response: 14216522
Conc: 9.13 ng/ml

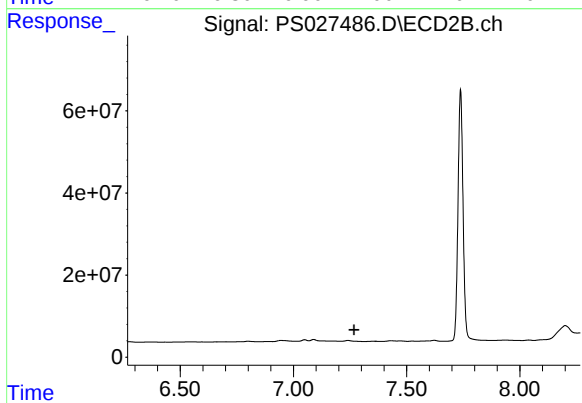

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

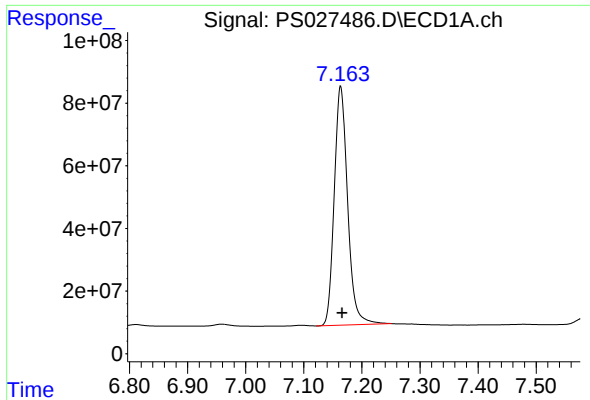

#4 2,4-DCAA


R.T.: 7.164 min
Delta R.T.: -0.002 min
Response: 1220763528
Conc: 472.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

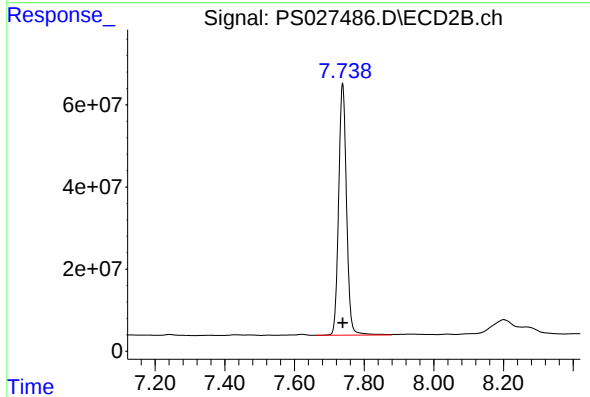


#4 2,4-DCAA

R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 962897754
Conc: 487.73 ng/ml

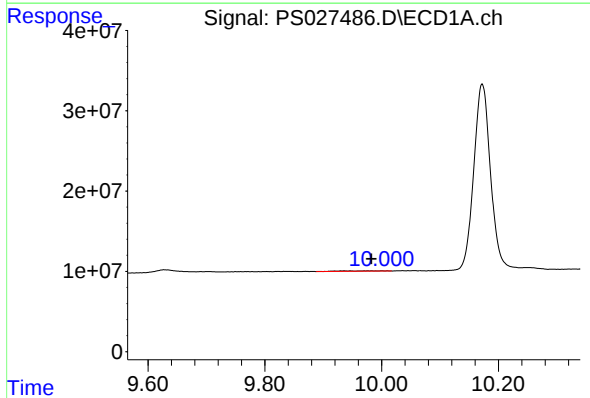


#13 2,4-DB

R.T.: 9.982 min
Delta R.T.: 0.000 min
Response: 2202882
Conc: 1.03 ng/ml

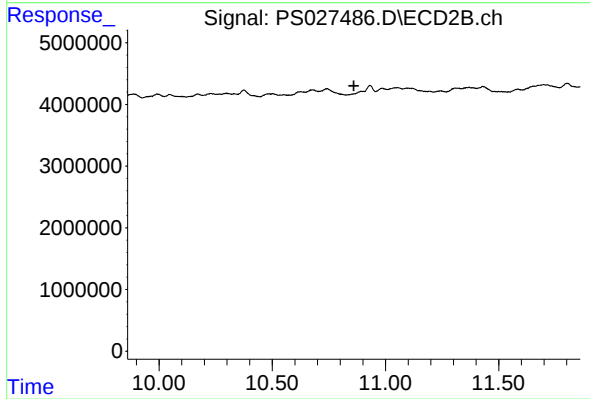

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.861 min
Response: 0
Conc: N.D.

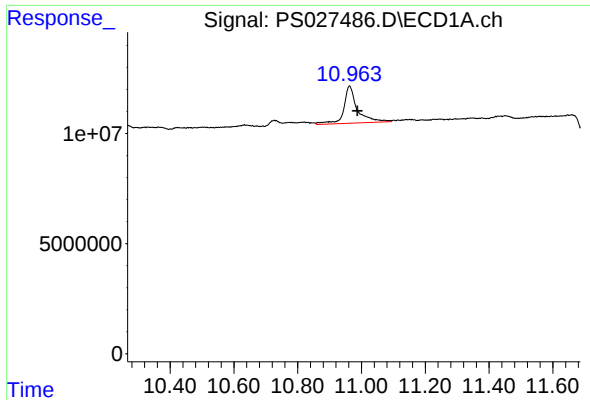

#15 Picloram

R.T.: 10.963 min
Delta R.T.: -0.024 min
Response: 49962970
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

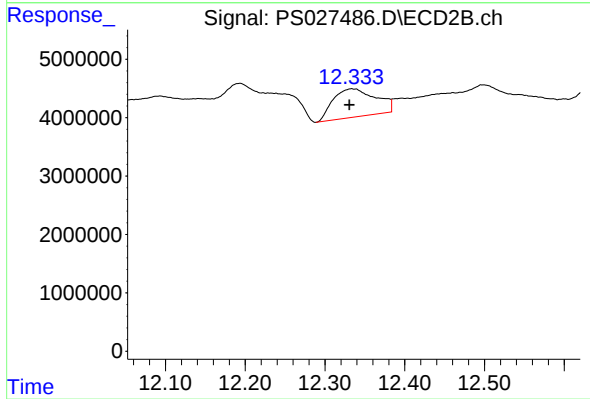

#15 Picloram

R.T.: 12.334 min
Delta R.T.: 0.004 min
Response: 18063407
Conc: N.D.