

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
 Data File : PS027471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 17:47
 Operator : AR\AJ
 Sample : P3597-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SP-1-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/20/2024
 Supervised By :Ankita Jodhani 08/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:31:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.164	7.738	756.0E6	451.0E6	292.307m	228.420
------	----------	-------	-------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081924\
Data File : PS027471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 17:47
Operator : AR\AJ
Sample : P3597-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SP-1-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/20/2024
Supervised By : Ankita Jodhani 08/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:31:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

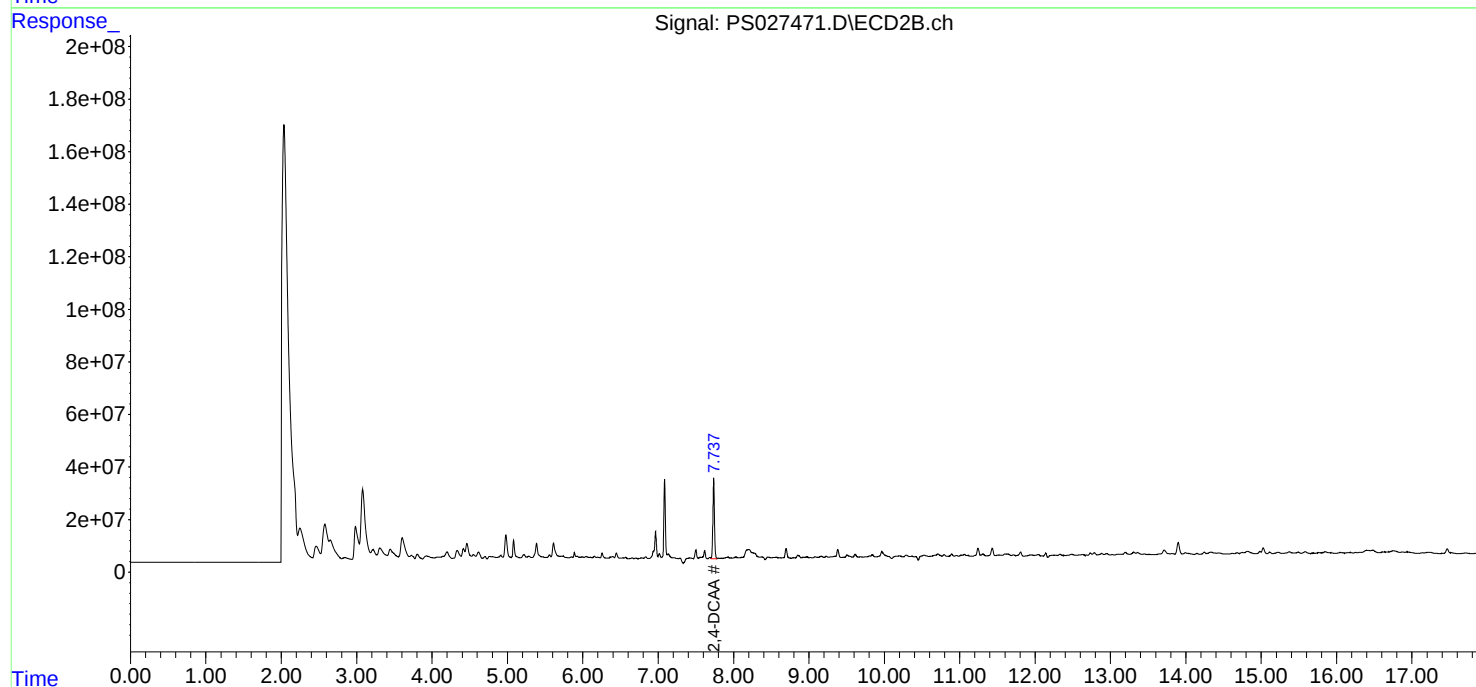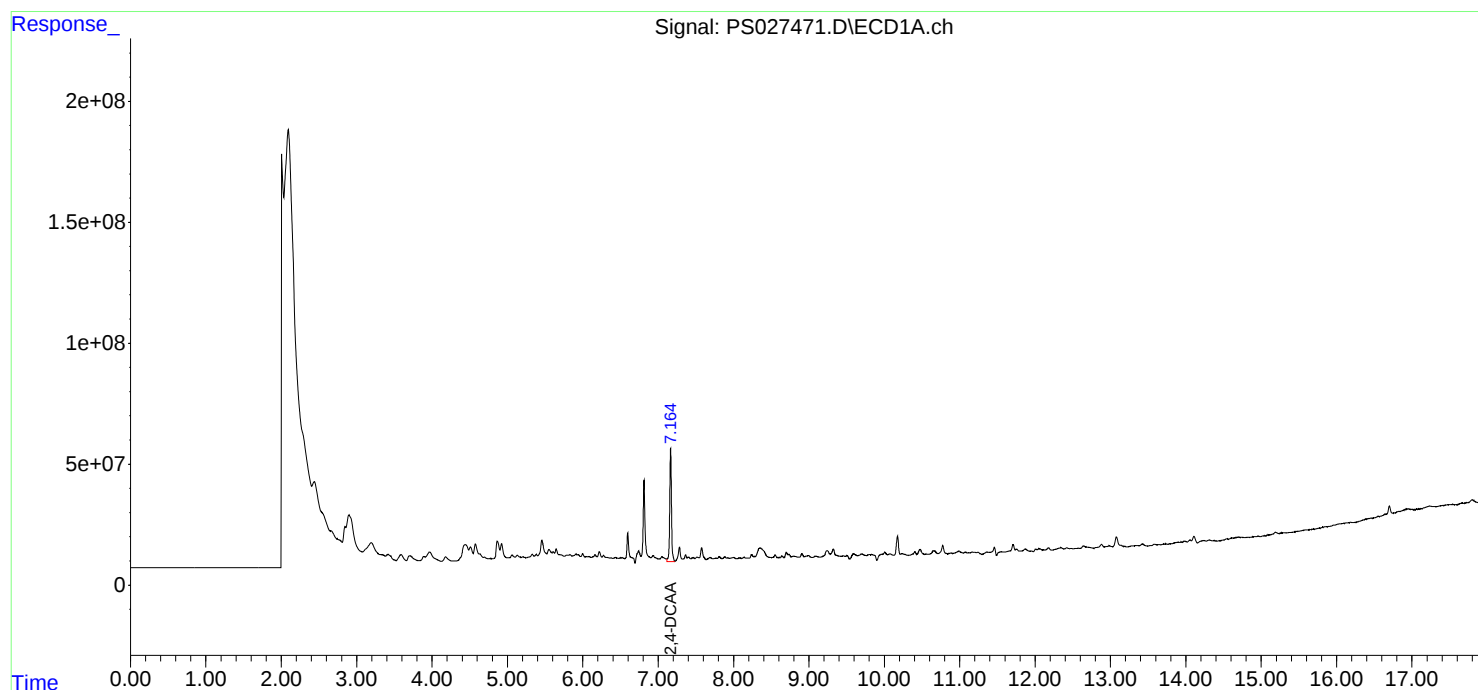

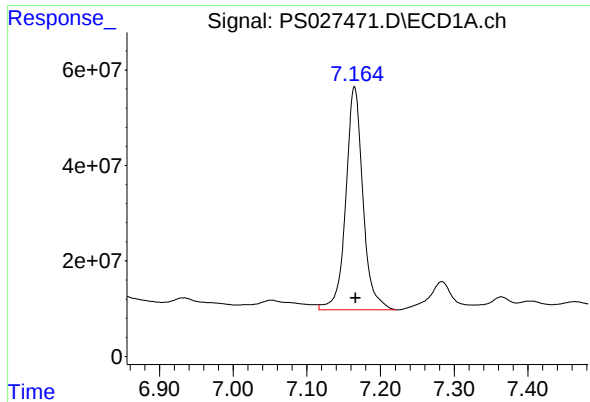


#4 2,4-DCAA

R.T.: 7.164 min
Delta R.T.: -0.002 min
Response: 755981470
Conc: 292.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-1-COMP

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/20/2024
Supervised By :Ankita Jodhani 08/20/2024

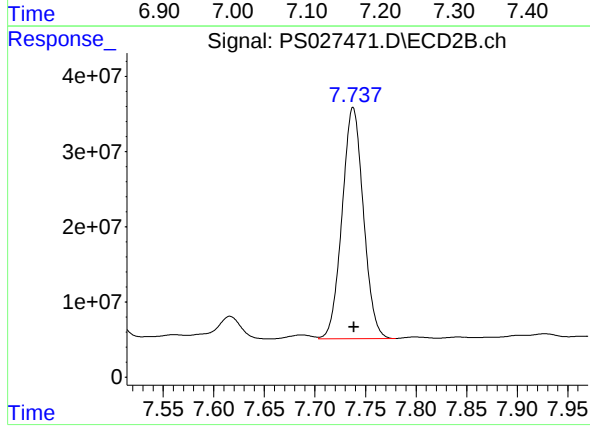

#4 2,4-DCAA

R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 450955439
Conc: 228.42 ng/ml