

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081925\
 Data File : PS031502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 19:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 06:24:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.743	1645.5E6	463.1E6	518.423	547.808
Target Compounds							
1) T	Dalapon	0.000	2.651f	0	60610375	N.D.	22.777
2) T	3,5-DICHL...	6.452	0.000	1904233	0	<MDL	N.D. #
5) T	DICAMBA	7.468	0.000	765977	0	<MDL	N.D. #
6) T	MCP	7.684	0.000	334162	0	<MDL	N.D. #
7) T	MCPA	7.829	8.247f	407882	54739401	<MDL	19.511 #
8) T	DICHLORPROP	8.193	0.000	1362441	0	<MDL	N.D. #
10) T	Pentachlo...	8.714	9.512	6732502	15178781	<MDL	<MDL #
11) T	2,4,5-TP ...	9.291	9.901	4258917	18576465	<MDL	1.416 #
12) T	2,4,5-T	9.600	0.000	1548182	0	<MDL	N.D. #
13) T	2,4-DB	10.156	0.000	331846	0	<MDL	N.D. #
14) T	DINOSEB	11.361	0.000	3397072	0	<MDL	N.D. #
15) T	Picloram	11.182	0.000	593810	0	<MDL	N.D. #
16) T	DCPA	11.664	0.000	2383463	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081925\
Data File : PS031502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 19:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 06:24:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

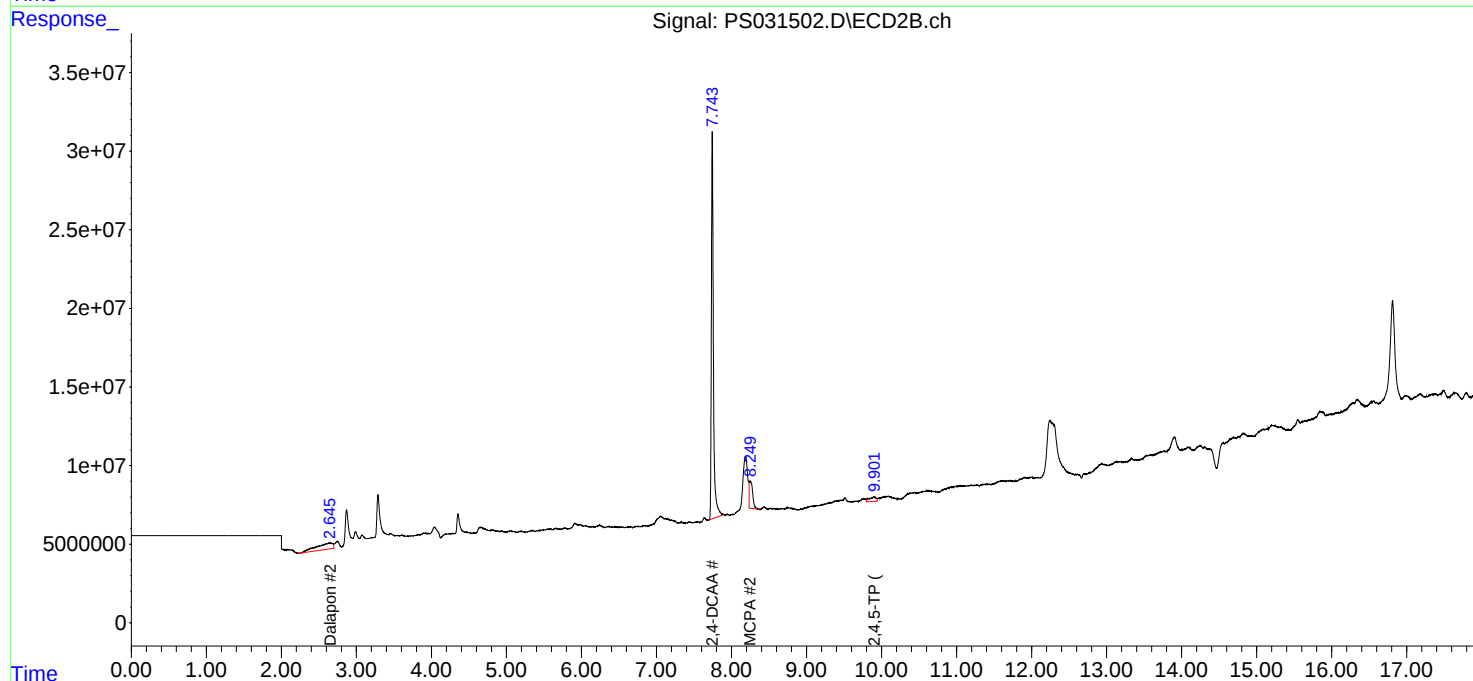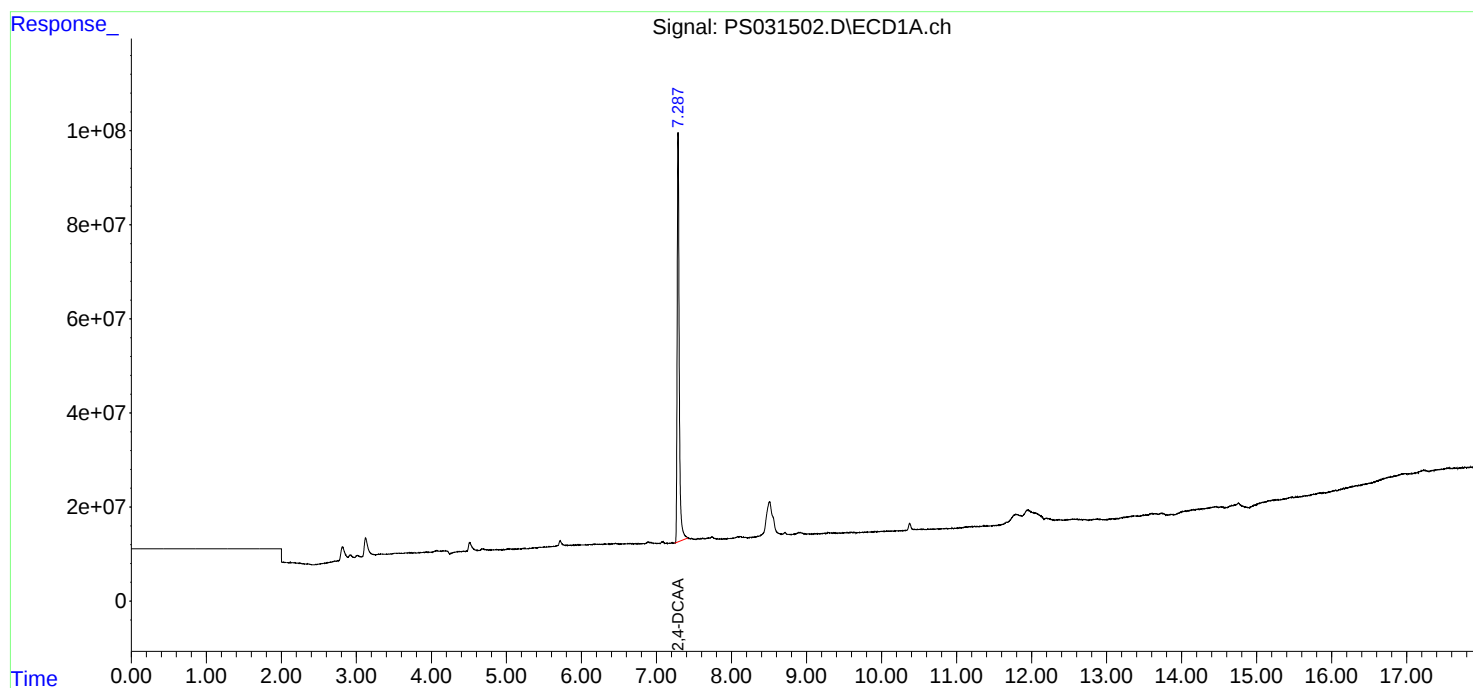


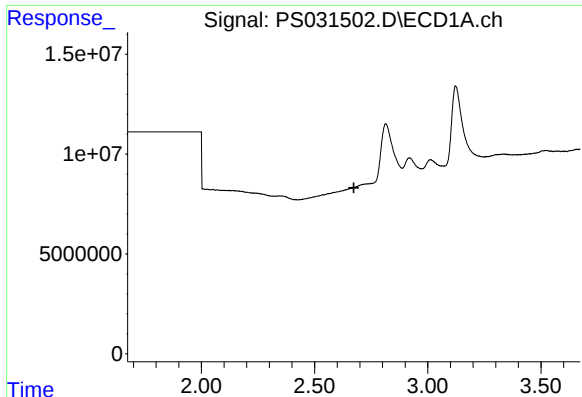

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

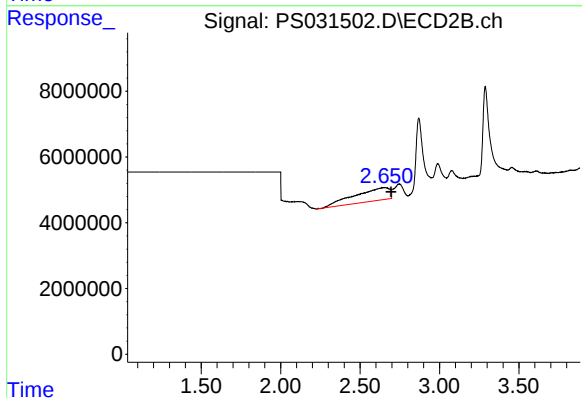


#1 Dalapon

R.T.: 2.651 min
Delta R.T.: -0.044 min
Response: 60610375
Conc: 22.78 ng/ml

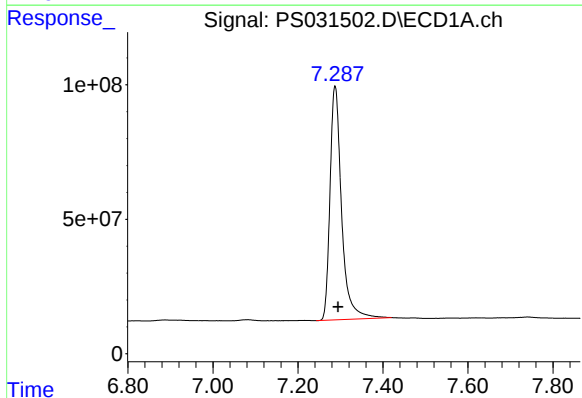


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.007 min
Response: 1645469039
Conc: 518.42 ng/ml

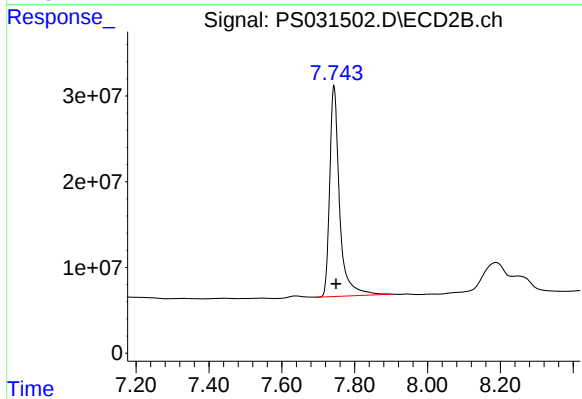

#4 2,4-DCAA


R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 463083626
Conc: 547.81 ng/ml

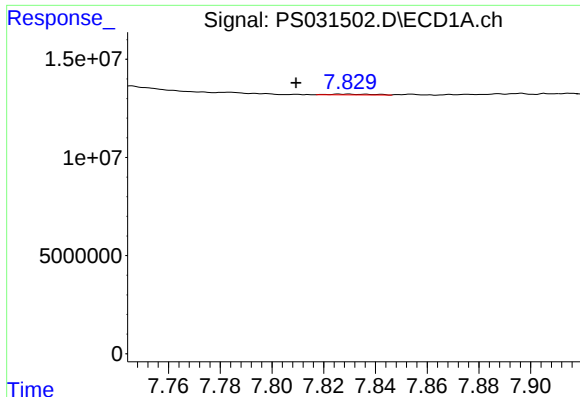

#7 MCPA


R.T.: 7.829 min
Delta R.T.: 0.019 min
Response: 407882
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

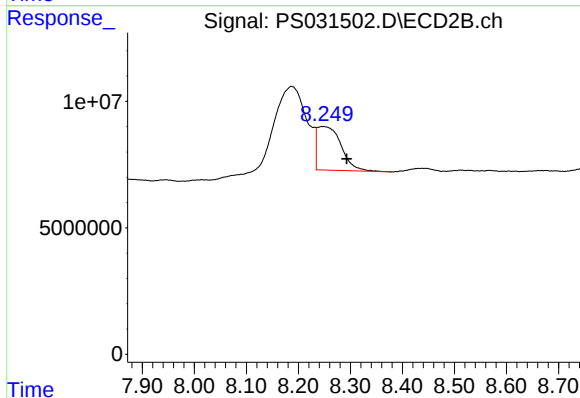


#7 MCPA

R.T.: 8.247 min
Delta R.T.: -0.046 min
Response: 54739401
Conc: 19.51 ug/ml

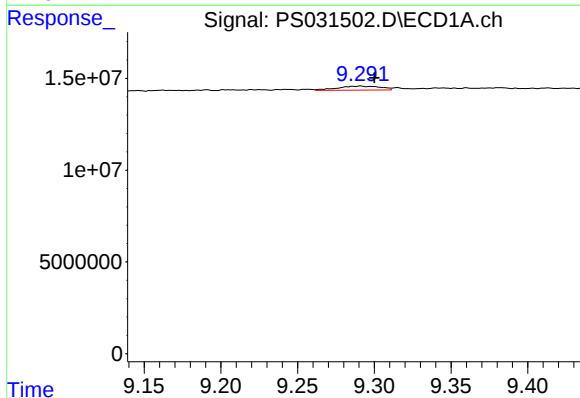

#11 2,4,5-TP (SILVEX)

R.T.: 9.291 min
Delta R.T.: -0.009 min
Response: 4258917
Conc: N.D.

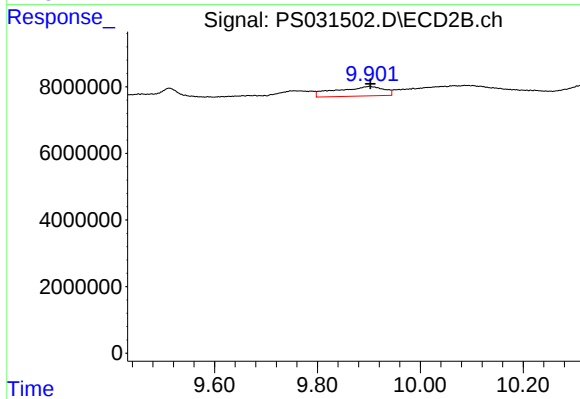

#11 2,4,5-TP (SILVEX)

R.T.: 9.901 min
Delta R.T.: -0.002 min
Response: 18576465
Conc: 1.42 ng/ml