

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081925\
 Data File : PS031512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 00:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 06:26:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.743	1668.7E6	474.7E6	525.732	561.580
Target Compounds							
1) T	Dalapon	0.000	2.654f	0	70344095	N.D.	26.435
2) T	3,5-DICHL...	6.441	0.000	2244170	0	<MDL	N.D. #
5) T	DICAMBA	7.471	0.000	152138	0	<MDL	N.D. #
6) T	MCP	7.620f	8.000f	1640856	1765475	<MDL	<MDL #
7) T	MCPA	7.826	8.243f	746795	44420818	<MDL	15.833 #
8) T	DICHLORPROP	8.179	8.668	3294251	1982565	1.038	1.485 #
10) T	Pentachlo...	8.711	9.512	6817671	10576930	<MDL	<MDL #
11) T	2,4,5-TP ...	9.291	9.900	8572843	8297980	<MDL	<MDL #
12) T	2,4,5-T	9.601	0.000	4088011	0	<MDL	N.D. #
13) T	2,4-DB	10.166	0.000	6362095	0	3.311	N.D. #
14) T	DINOSEB	11.364	0.000	3374719	0	<MDL	N.D. #
15) T	Picloram	11.180	0.000	6481725	0	<MDL	N.D. #
16) T	DCPA	11.662	0.000	3875439	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081925\
Data File : PS031512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 00:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 06:26:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

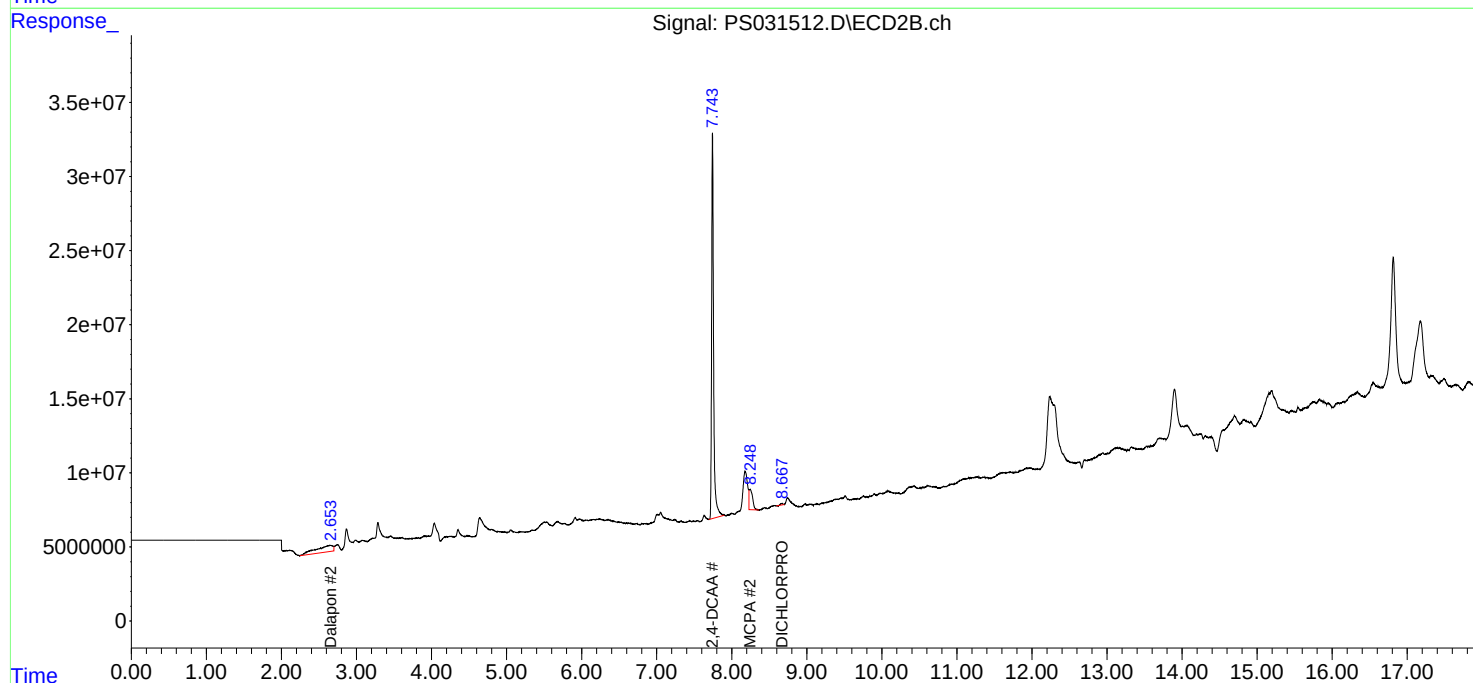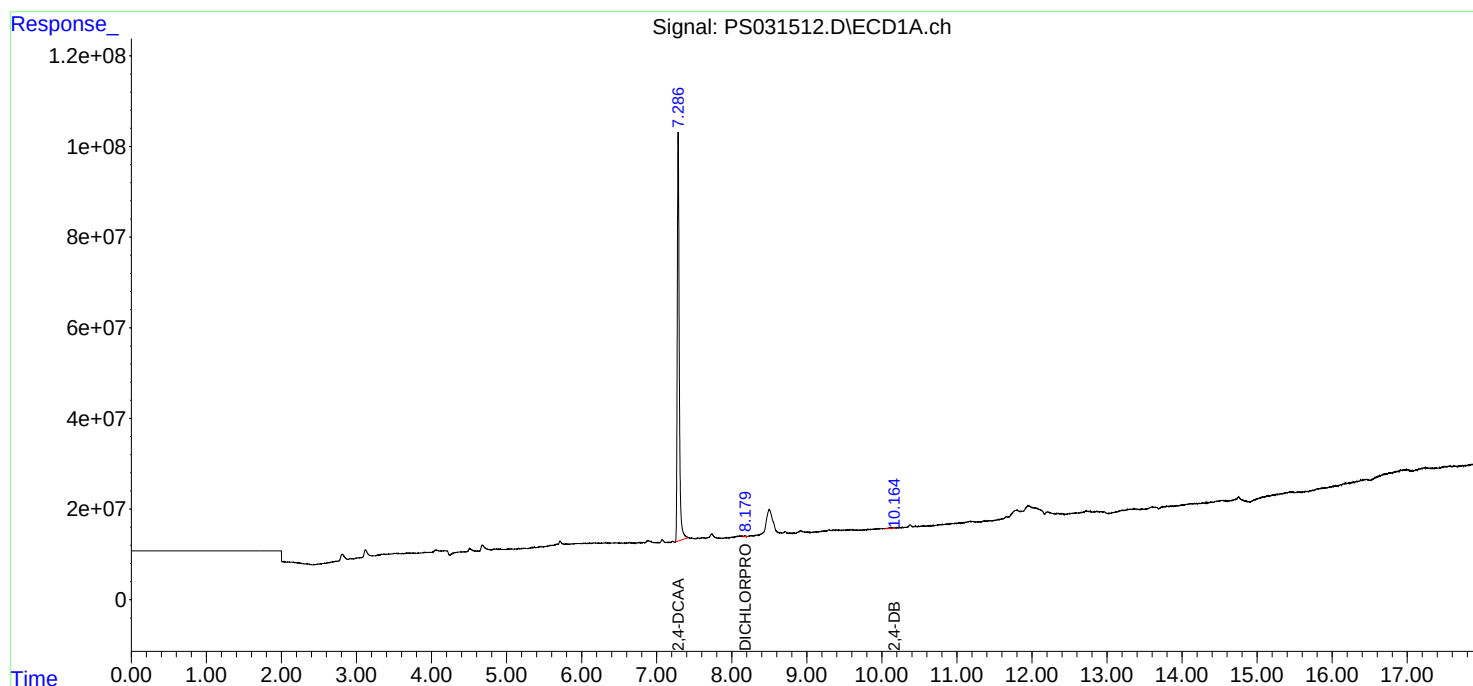


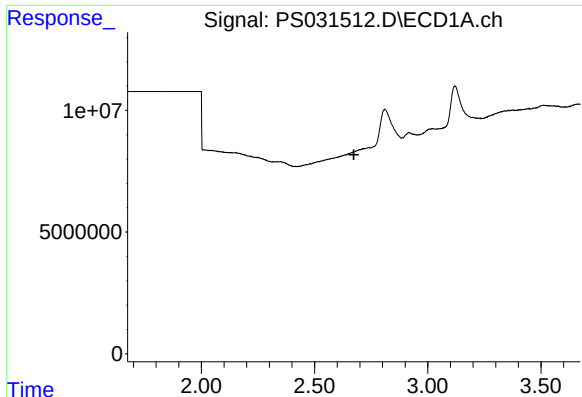

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

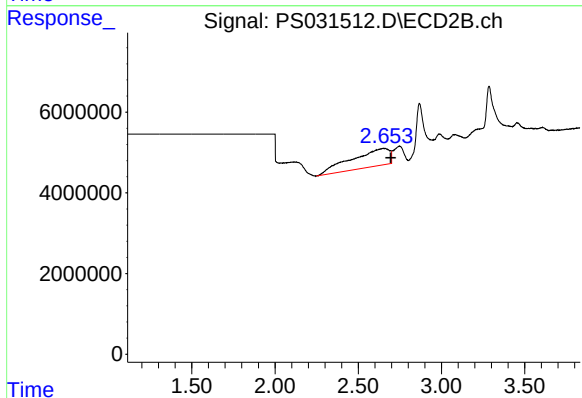


#1 Dalapon

R.T.: 2.654 min
Delta R.T.: -0.041 min
Response: 70344095
Conc: 26.44 ng/ml

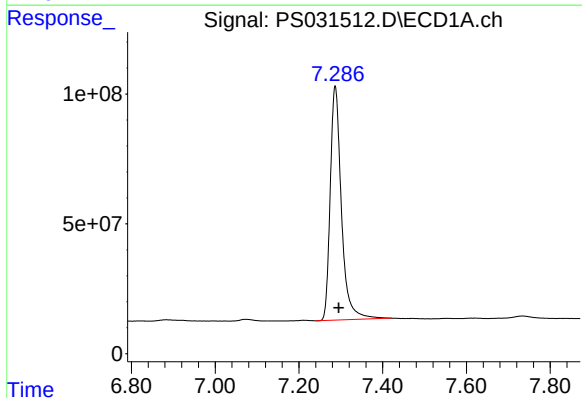


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1668668446
Conc: 525.73 ng/ml

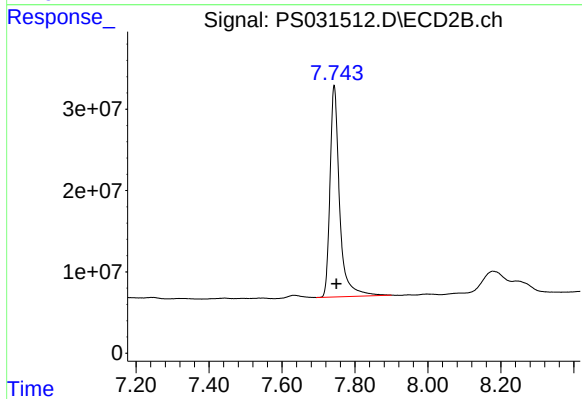

#4 2,4-DCAA


R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 474725804
Conc: 561.58 ng/ml

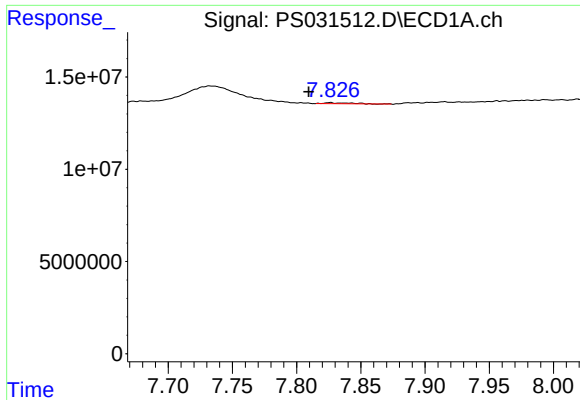

#7 MCPA


R.T.: 7.826 min
Delta R.T.: 0.017 min
Response: 746795
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

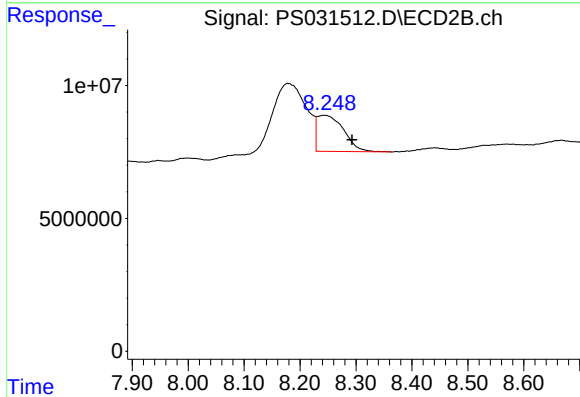


#7 MCPA

R.T.: 8.243 min
Delta R.T.: -0.050 min
Response: 44420818
Conc: 15.83 ug/ml

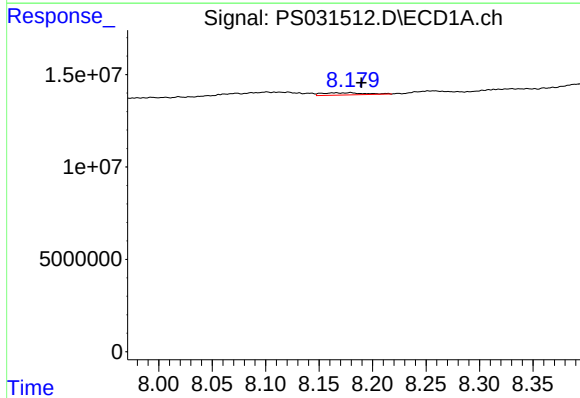


#8 DICHLORPROP

R.T.: 8.179 min
Delta R.T.: -0.011 min
Response: 3294251
Conc: 1.04 ng/ml

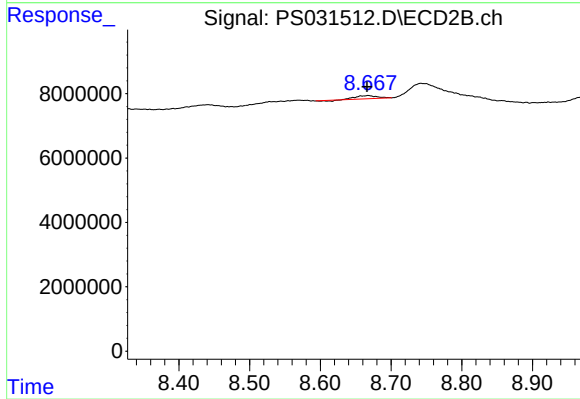

#8 DICHLORPROP


R.T.: 8.668 min
Delta R.T.: 0.002 min
Response: 1982565
Conc: 1.49 ng/ml

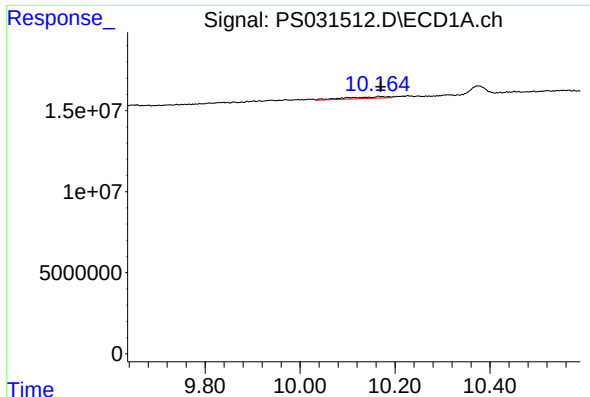

#13 2,4-DB

R.T.: 10.166 min
Delta R.T.: -0.005 min
Response: 6362095
Conc: 3.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

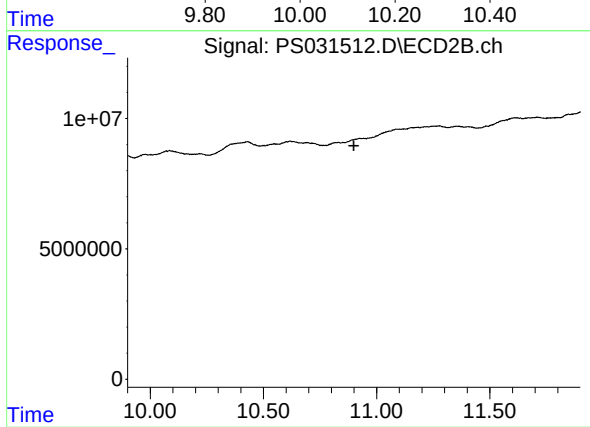

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.899 min
Response: 0
Conc: N.D.