

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
 Data File : PS011858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2020 17:35
 Operator : DD\AJ
 Sample : PB131123BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:36:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	518.2E6	317.3E6	475.038	593.412
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	60207171	N.D.	73.190
3) T	4-Nitroph...	6.993	0.000	387578	0	<MDL	N.D. #
5) T	DICAMBA	7.398	7.049	7857745	7564344	1.918	3.501 #
6) T	MCP	7.629	0.000	6493025	0	2.032	N.D. #
7) T	MCPA	7.765	7.376	30854590	38192818	6.783	13.938 #
9) T	2,4-D	8.400	0.000	127.3E6	0	112.782	N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	33388216	N.D.	11.420
12) T	2,4,5-T	9.495	0.000	13063173	0	2.204	N.D. #
15) T	Picloram	0.000	11.031	0	32712936	N.D.	7.217



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
Data File : PS011858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2020 17:35
Operator : DD\AJ
Sample : PB131123BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:36:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

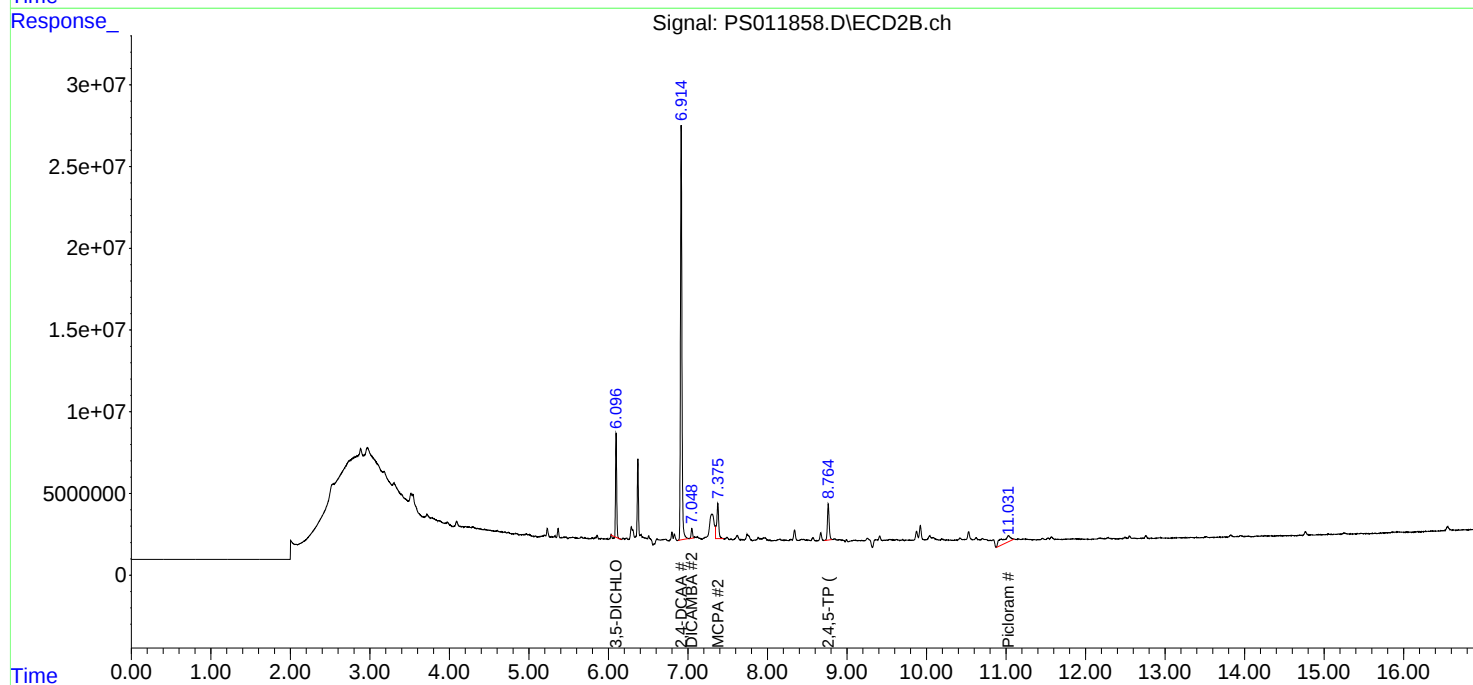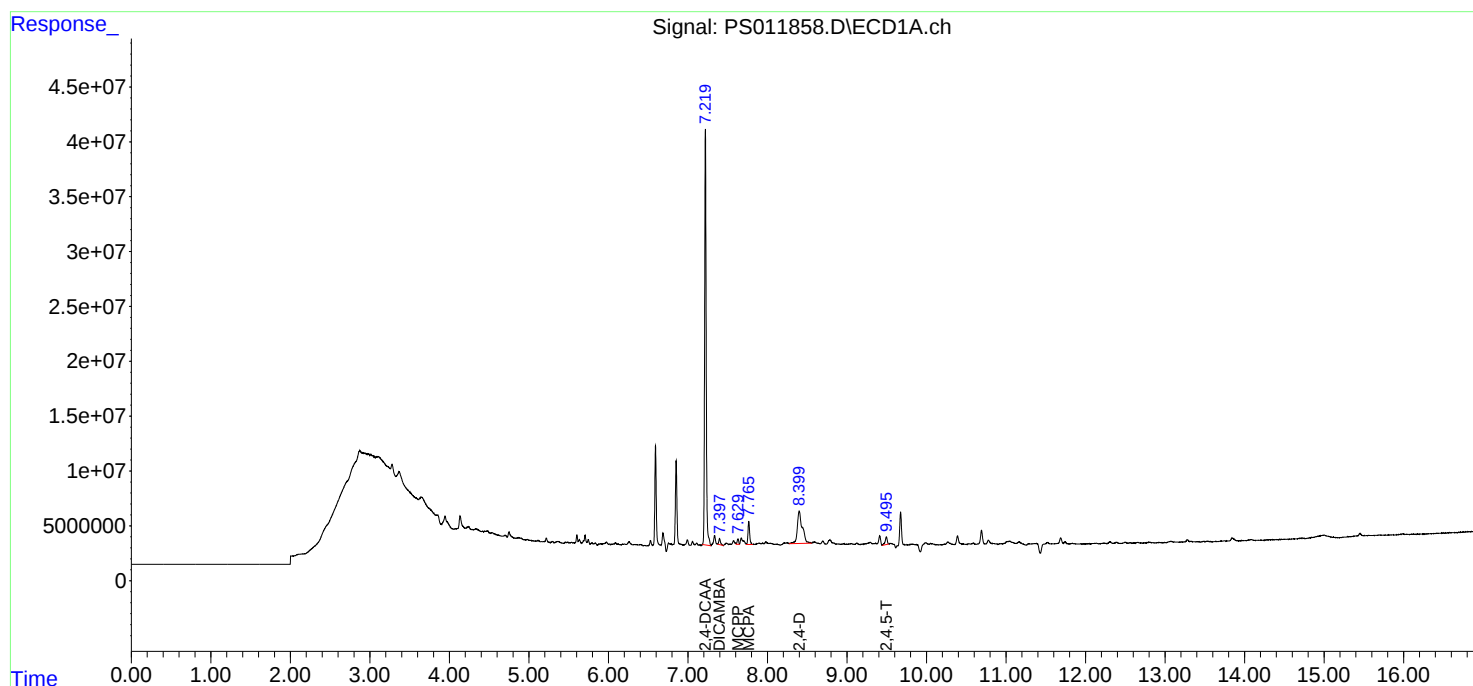


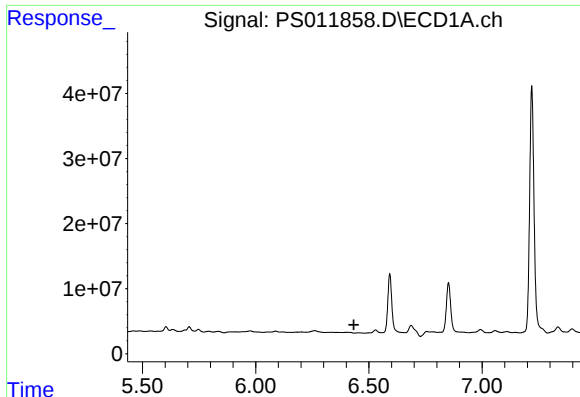

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

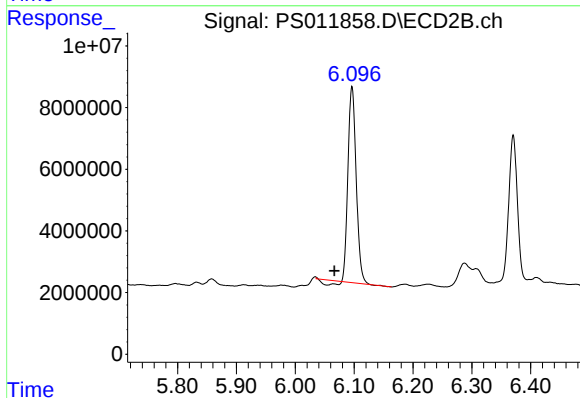


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 60207171
Conc: 73.19 ng/ml

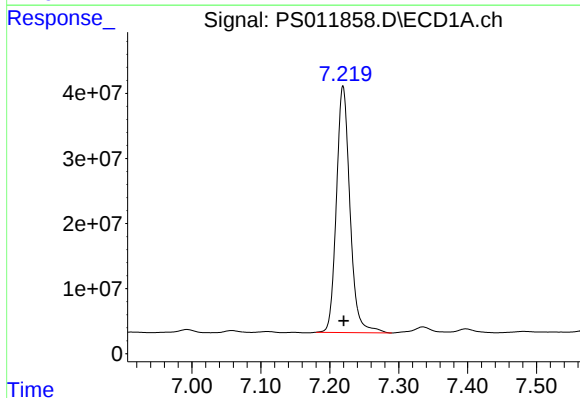


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 518156212
Conc: 475.04 ng/ml

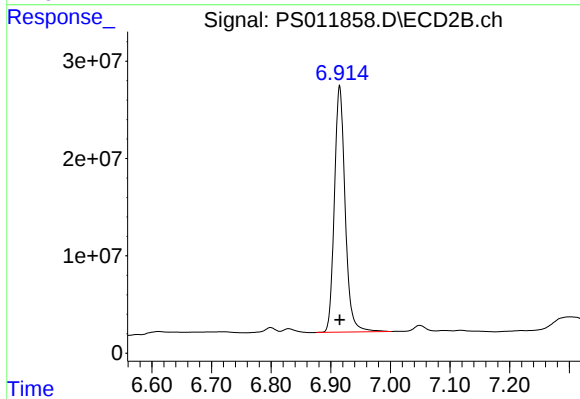

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 317348718
Conc: 593.41 ng/ml

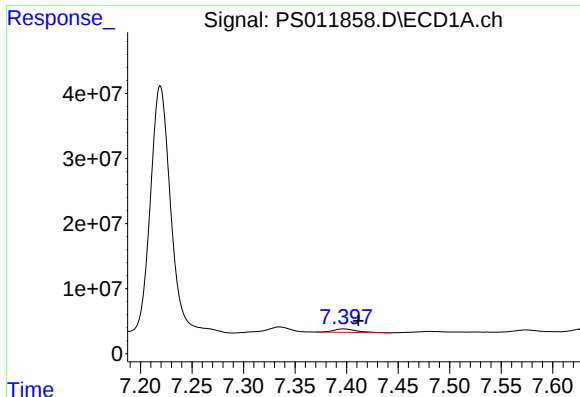

#5 DICAMBA


R.T.: 7.398 min
Delta R.T.: -0.014 min
Response: 7857745
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

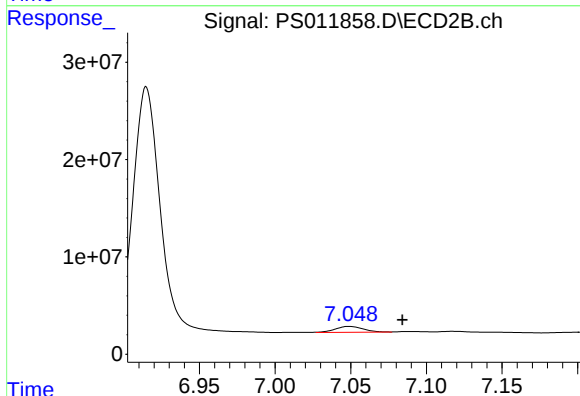


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 7564344
Conc: 3.50 ng/ml

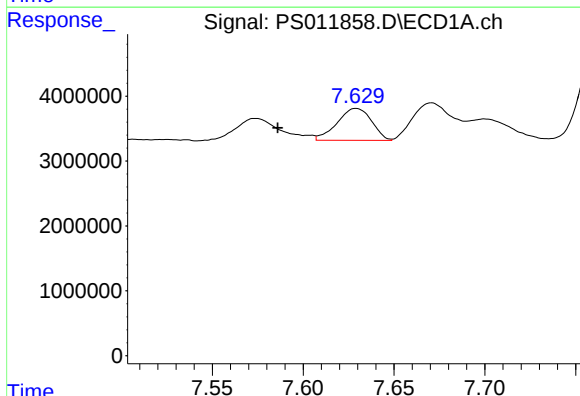


#6 MCP

R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 6493025
Conc: 2.03 ug/ml

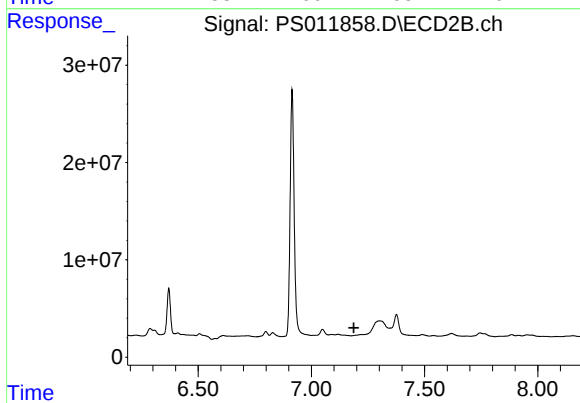

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

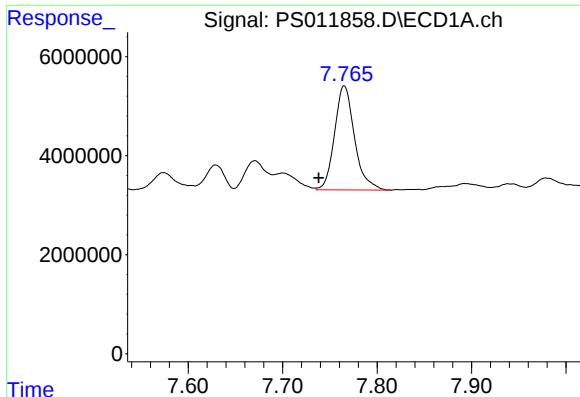

#7 MCPA


R.T.: 7.765 min
Delta R.T.: 0.027 min
Response: 30854590
Conc: 6.78 ug/ml

Instrument :
ECD_S
ClientSampleId :

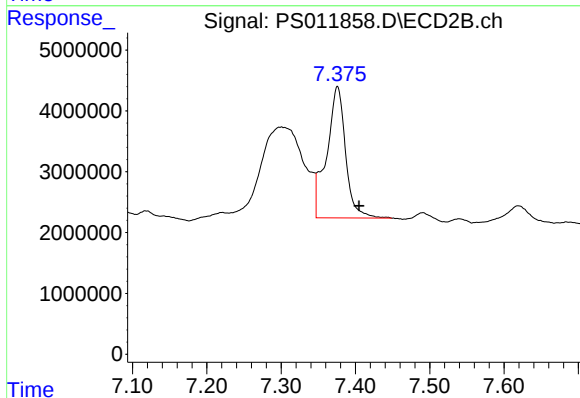


#7 MCPA

R.T.: 7.376 min
Delta R.T.: -0.029 min
Response: 38192818
Conc: 13.94 ug/ml

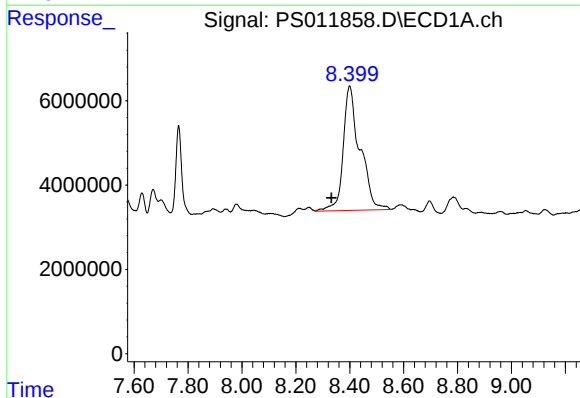


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.067 min
Response: 127341391
Conc: 112.78 ng/ml

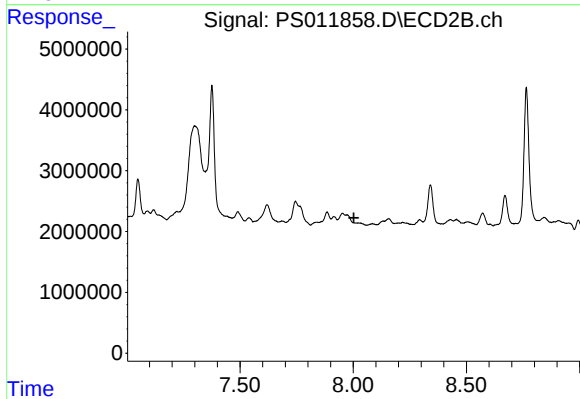

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

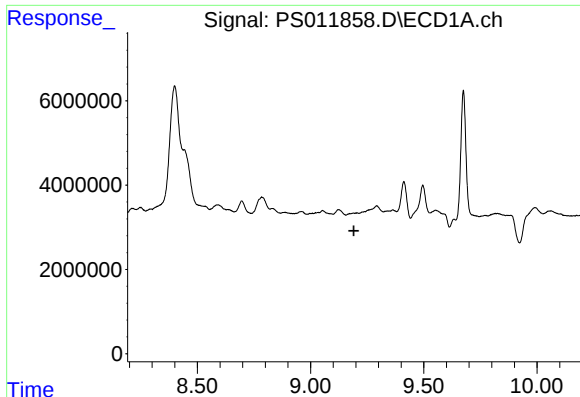

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

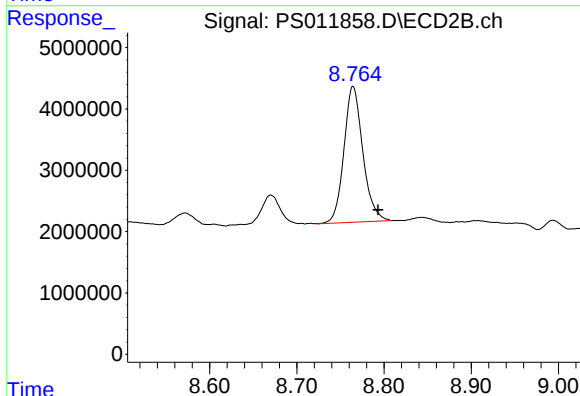


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: -0.029 min
Response: 33388216
Conc: 11.42 ng/ml

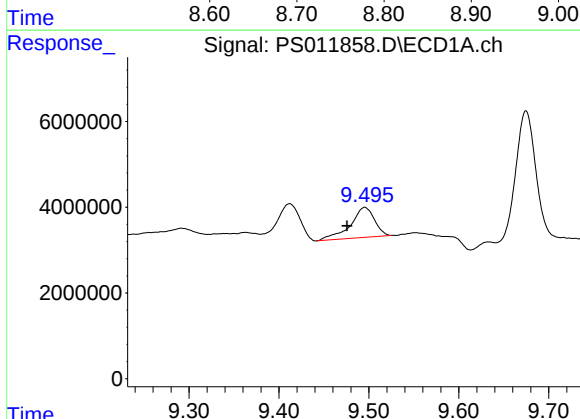


#12 2,4,5-T

R.T.: 9.495 min
Delta R.T.: 0.020 min
Response: 13063173
Conc: 2.20 ng/ml

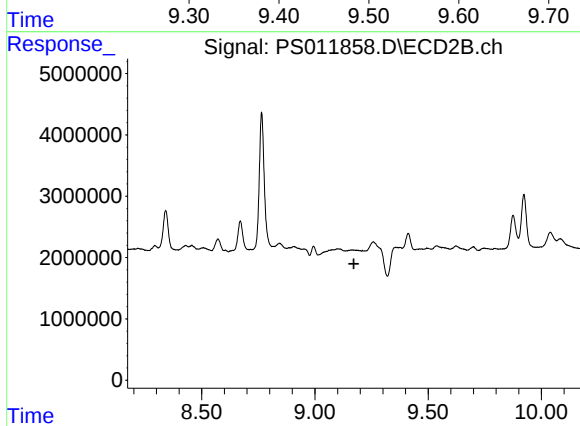

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

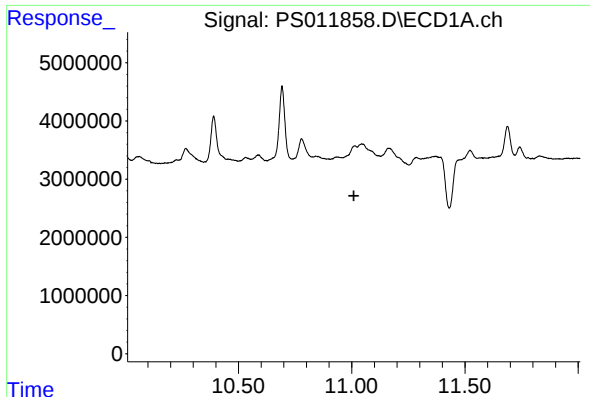

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

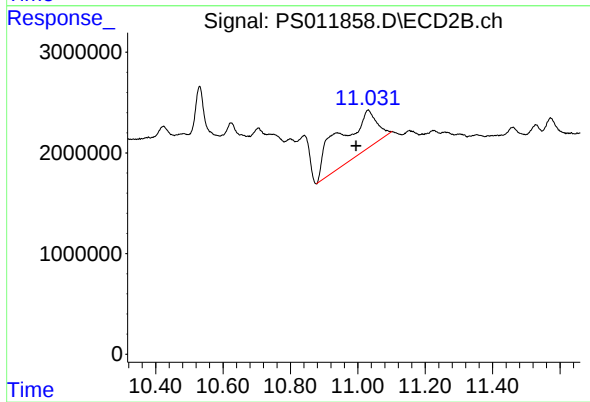

#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.036 min
Response: 32712936
Conc: 7.22 ng/ml