

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
 Data File : PS011860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2020 18:21
 Operator : DD\AJ
 Sample : PB131123TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:37:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	189.2E6	120.8E6	173.423	225.912 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	32558555	N.D.	39.579
5) T	DICAMBA	7.480	7.050	10136648	16094205	2.475	7.449 #
6) T	MCP	7.629	0.000	5270134	0	1.649	N.D. #
7) T	MCPA	7.691	7.395	128.4E6	11060168	28.225	4.036 #
8) T	DICHLORPROP	0.000	7.737	0	20301856	N.D.	35.956
9) T	2,4-D	8.398	0.000	121.0E6	0	107.136	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	16924877	N.D.	5.789
12) T	2,4,5-T	9.412	0.000	19058996	0	3.216	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
Data File : PS011860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2020 18:21
Operator : DD\AJ
Sample : PB131123TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:37:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

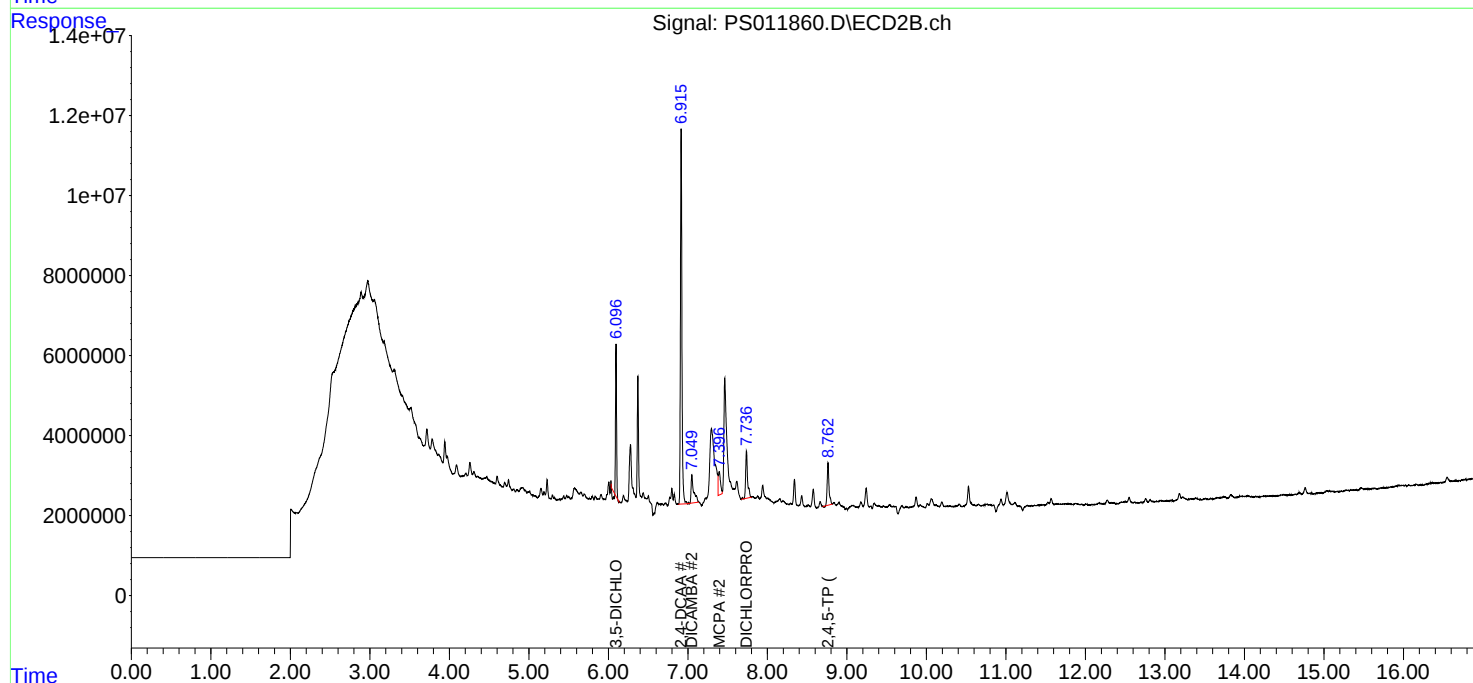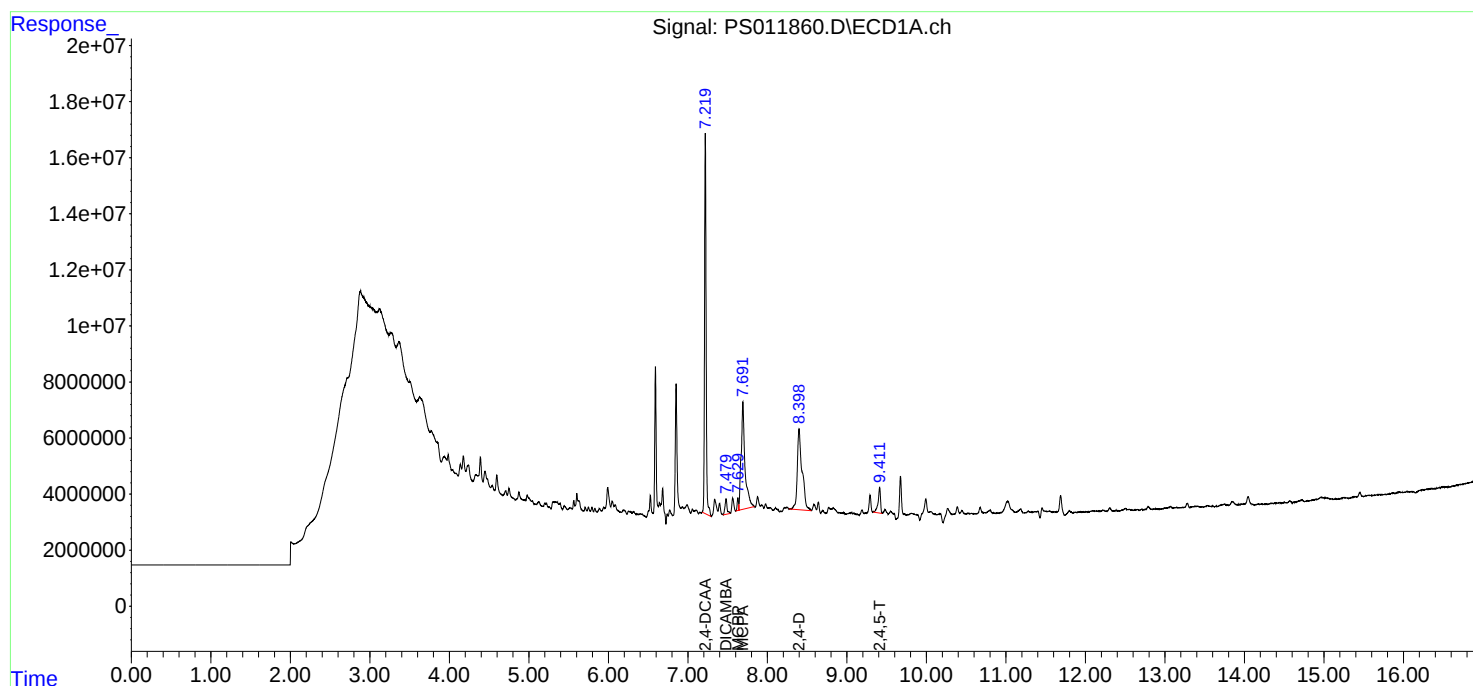


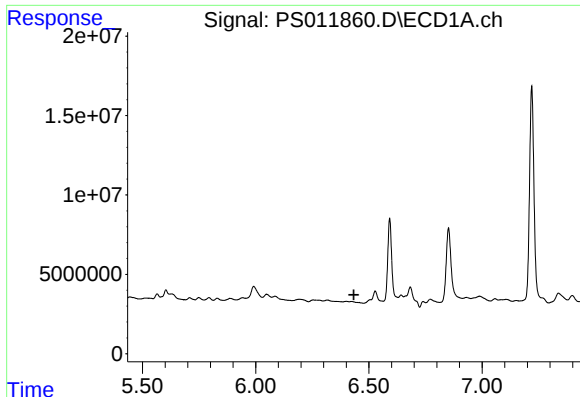

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

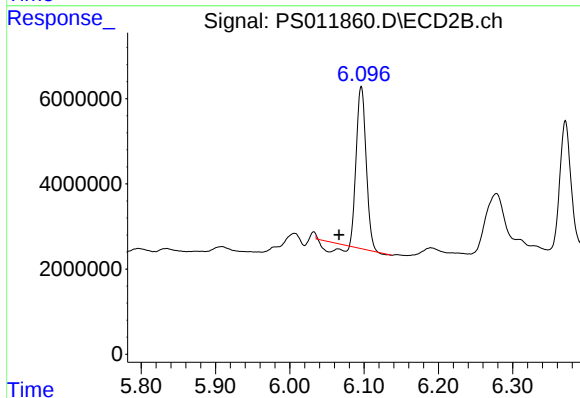


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 32558555
Conc: 39.58 ng/ml

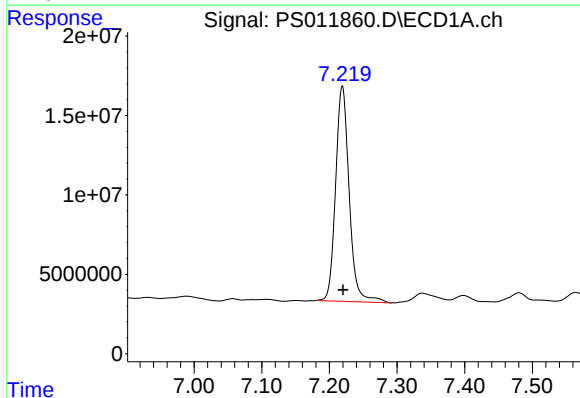


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 189164498
Conc: 173.42 ng/ml

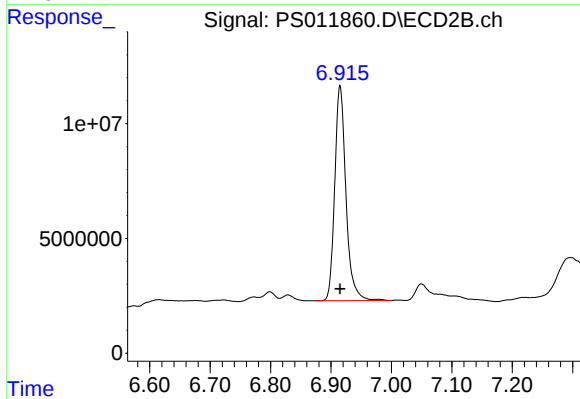

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 120814484
Conc: 225.91 ng/ml

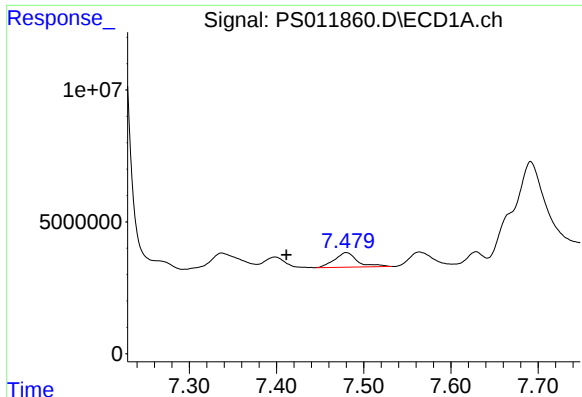

#5 DICAMBA


R.T.: 7.480 min
Delta R.T.: 0.068 min
Response: 10136648
Conc: 2.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

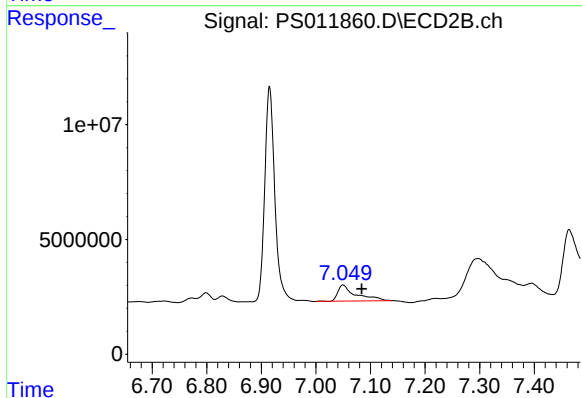


#5 DICAMBA

R.T.: 7.050 min
Delta R.T.: -0.034 min
Response: 16094205
Conc: 7.45 ng/ml

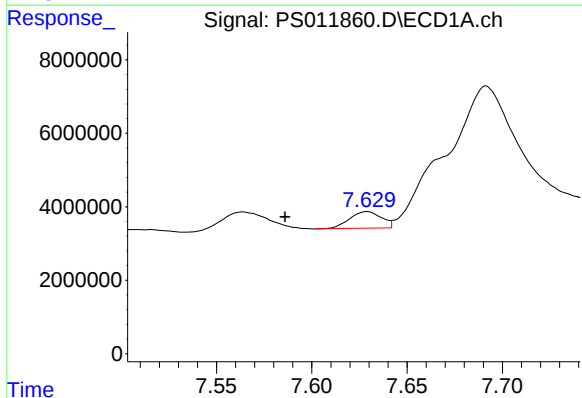


#6 MCP

R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 5270134
Conc: 1.65 ug/ml

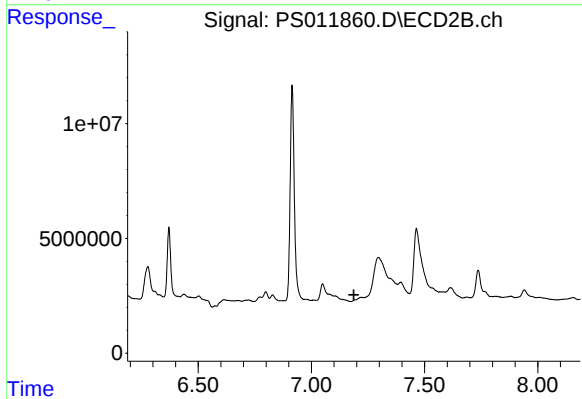

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

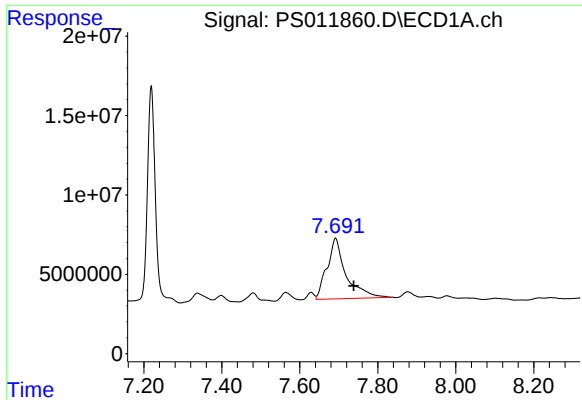

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.047 min
Response: 128381487
Conc: 28.23 ug/ml

Instrument :
ECD_S
ClientSampleId :

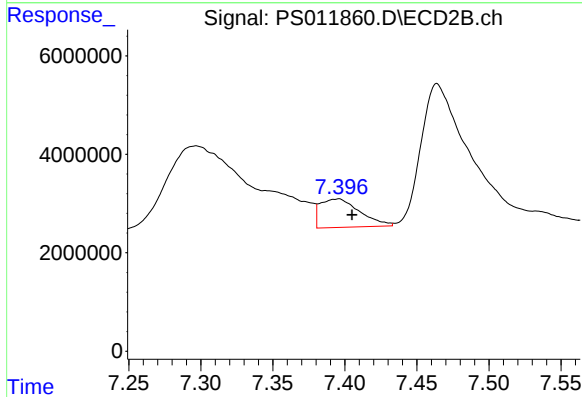


#7 MCPA

R.T.: 7.395 min
Delta R.T.: -0.010 min
Response: 11060168
Conc: 4.04 ug/ml

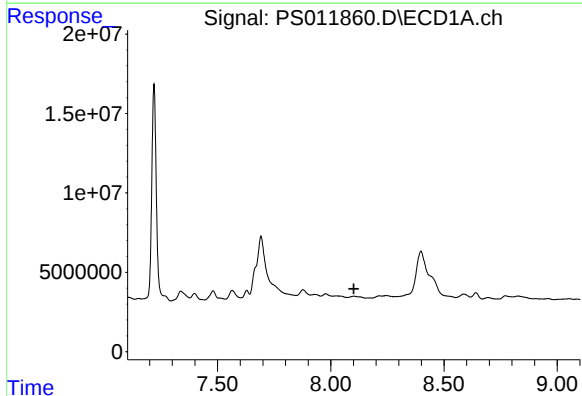


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

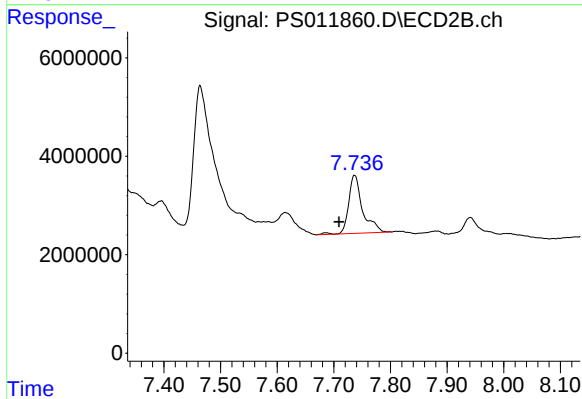

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.027 min
Response: 20301856
Conc: 35.96 ng/ml

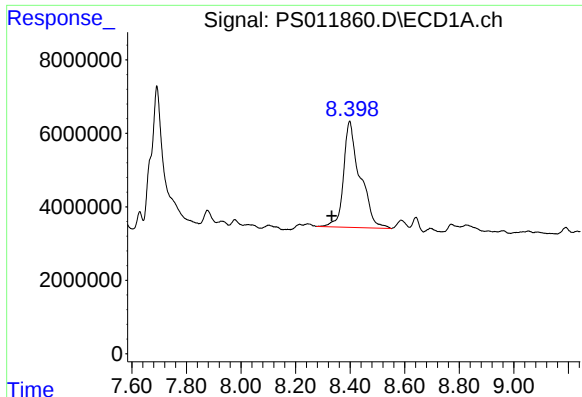

#9 2,4-D


R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 120967017
Conc: 107.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

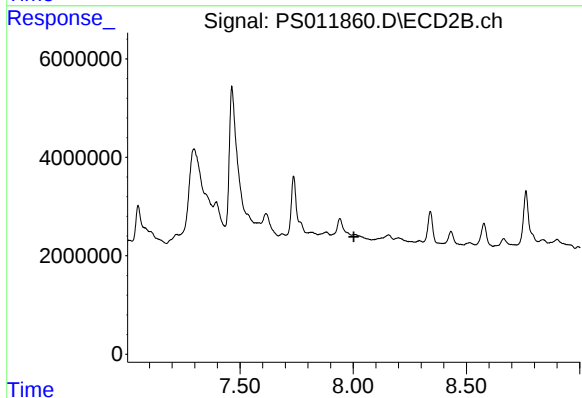


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

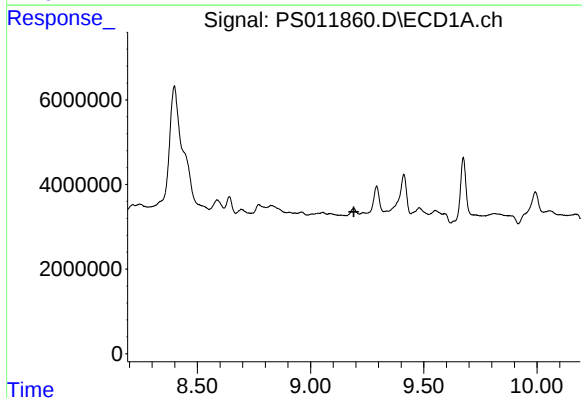


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

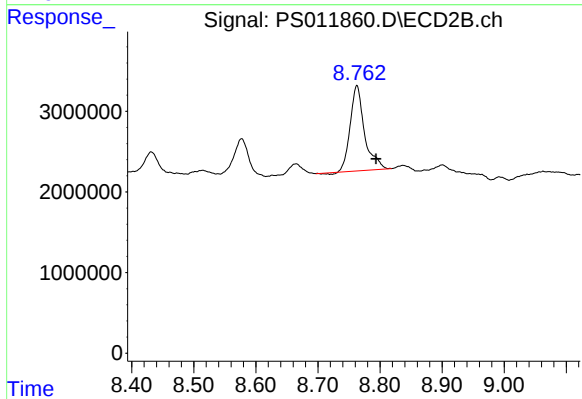

#11 2,4,5-TP (SILVEX)


R.T.: 8.763 min
Delta R.T.: -0.031 min
Response: 16924877
Conc: 5.79 ng/ml

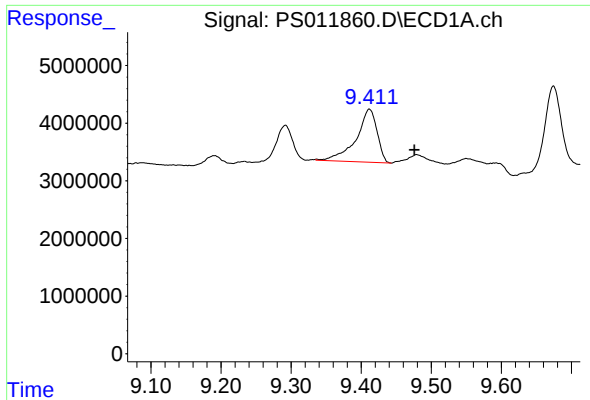

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 19058996
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

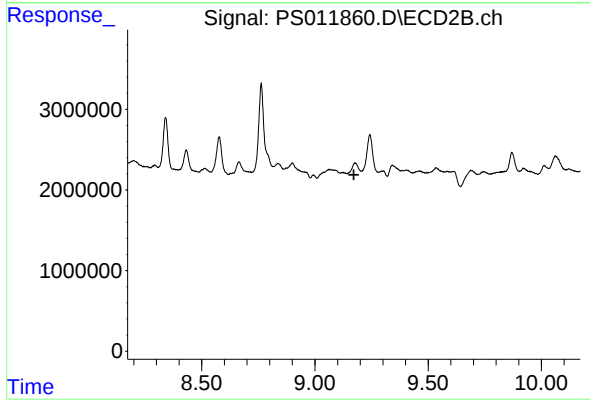

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.