

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
 Data File : PS011861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2020 18:44
 Operator : DD\AJ
 Sample : L3499-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:37:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	281.4E6	178.5E6	258.015	333.755 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	50716608	N.D.	61.653
3) T	4-Nitroph...	6.986	0.000	3193483	0	5.421	N.D. #
5) T	DICAMBA	7.397	7.048	6514681	14554737	1.591	6.737 #
6) T	MCP	7.630	0.000	10320784	0	3.230	N.D. #
7) T	MCPA	7.690	7.462	179.5E6	127.7E6	39.454	46.598
8) T	DICHLORPROP	0.000	7.736	0	19767153	N.D.	35.009
9) T	2,4-D	8.398	0.000	120.9E6	0	107.102	N.D. #
12) T	2,4,5-T	9.413	0.000	21573732	0	3.641	N.D. #
15) T	Picloram	11.004	0.000	8997745	0	1.151	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
Data File : PS011861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2020 18:44
Operator : DD\AJ
Sample : L3499-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:37:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

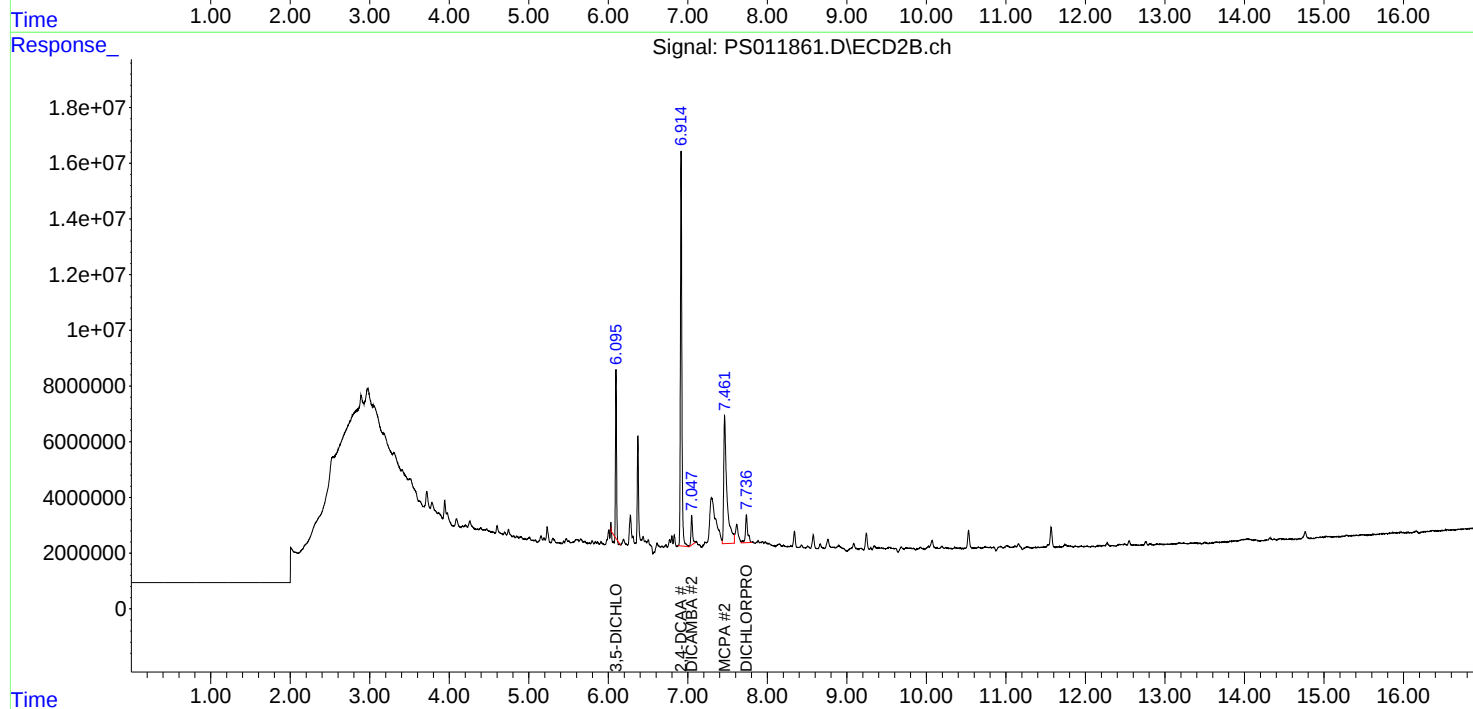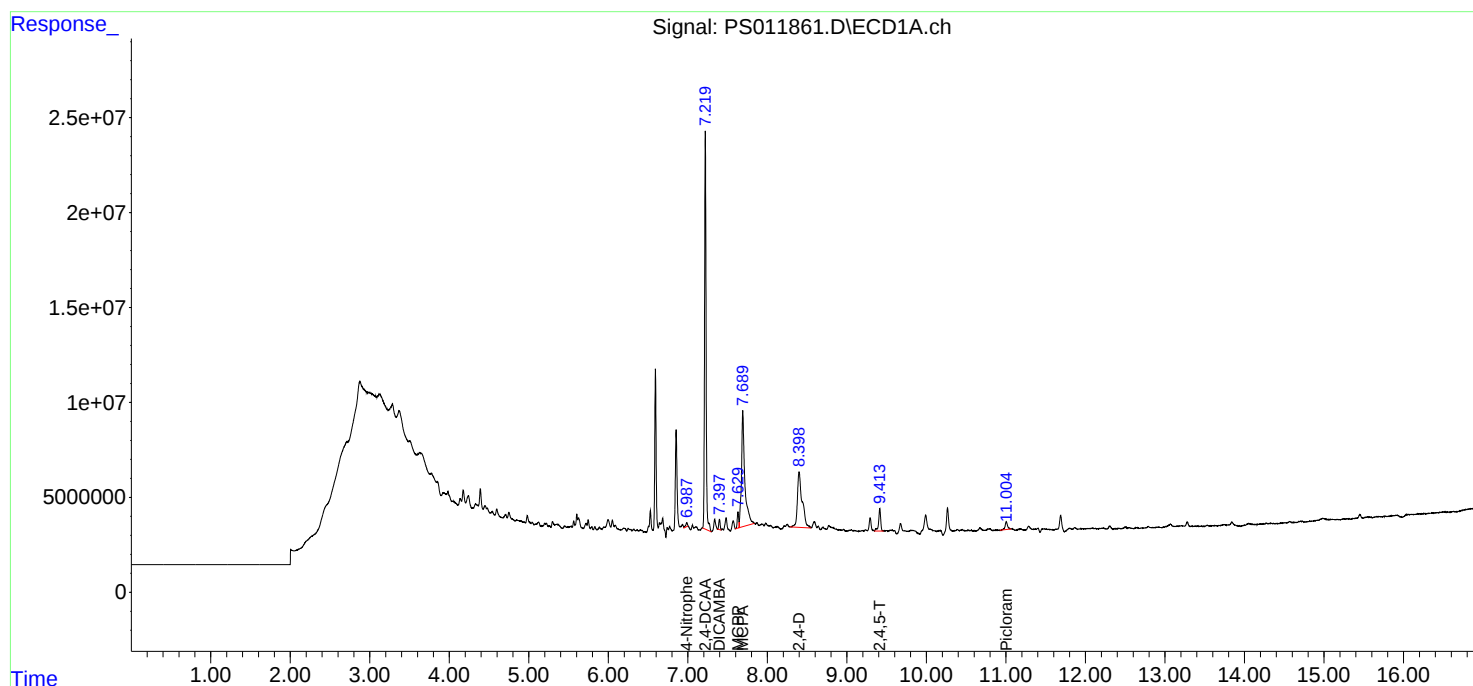


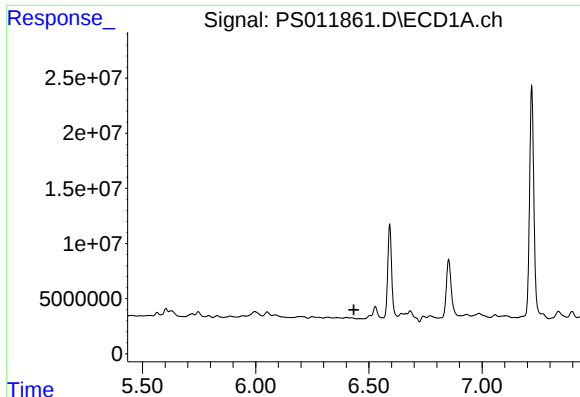

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

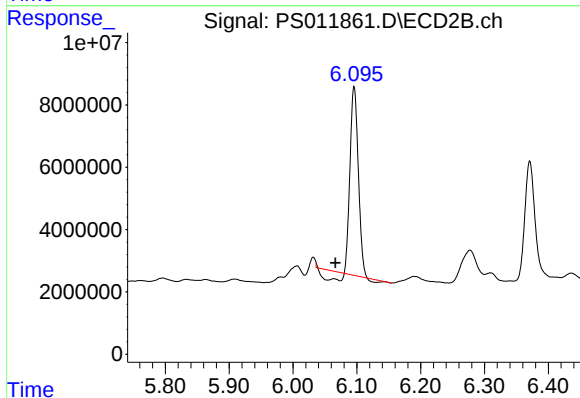


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 50716608
Conc: 61.65 ng/ml

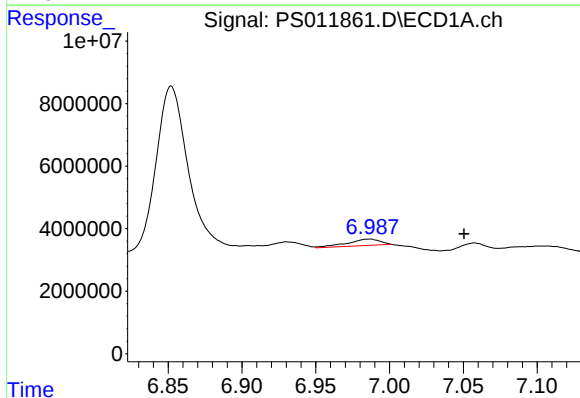


#3 4-Nitrophenol

R.T.: 6.986 min
Delta R.T.: -0.064 min
Response: 3193483
Conc: 5.42 ng/ml

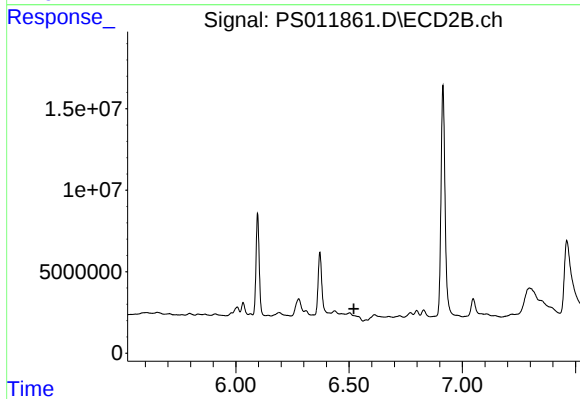

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

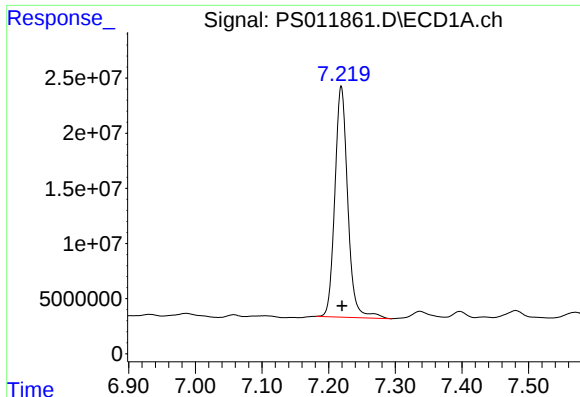

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 281434975
Conc: 258.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

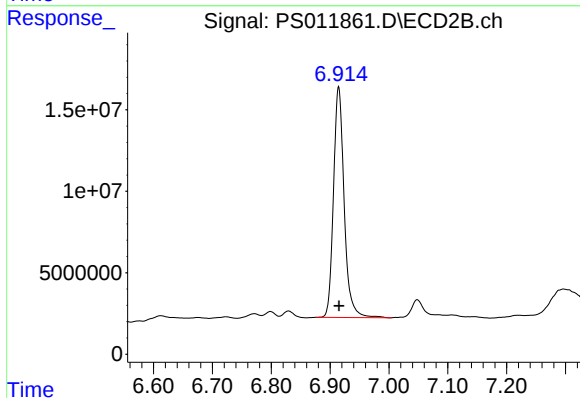


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 178487589
Conc: 333.75 ng/ml

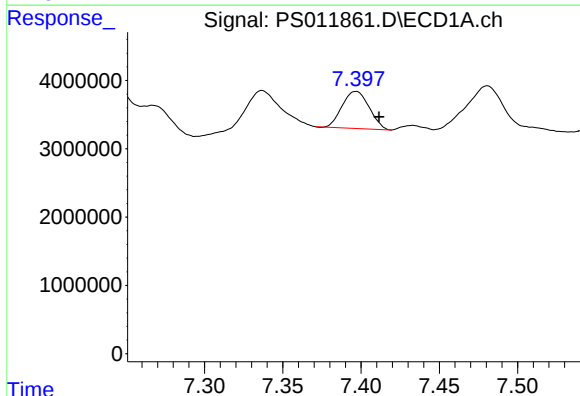


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 6514681
Conc: 1.59 ng/ml

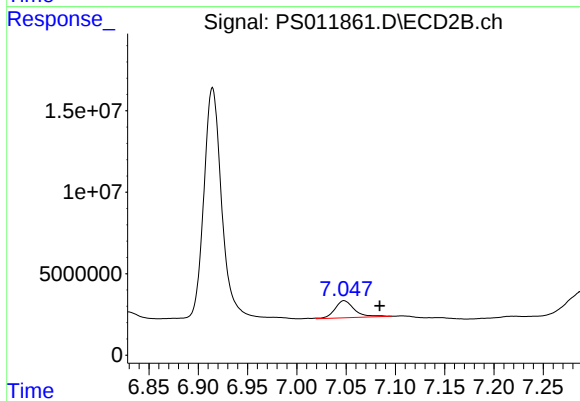

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 14554737
Conc: 6.74 ng/ml

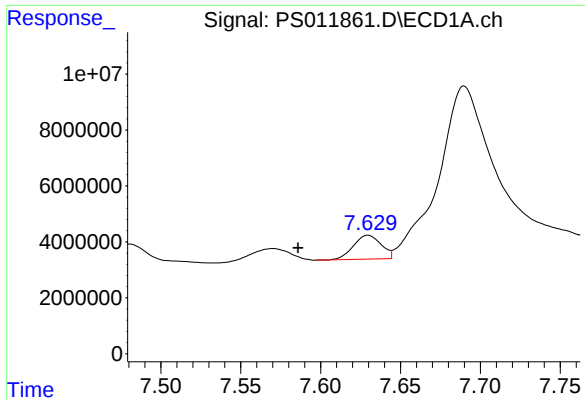

#6 MCPP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 10320784
Conc: 3.23 ug/ml

Instrument :
ECD_S
ClientSampleId :

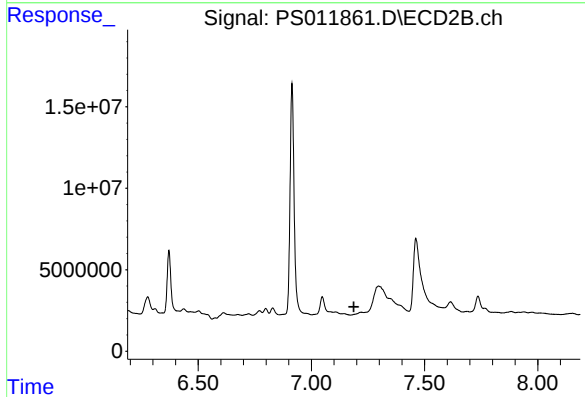


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

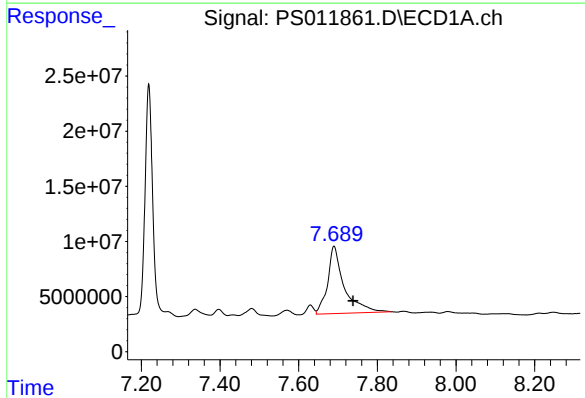


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.048 min
Response: 179455410
Conc: 39.45 ug/ml

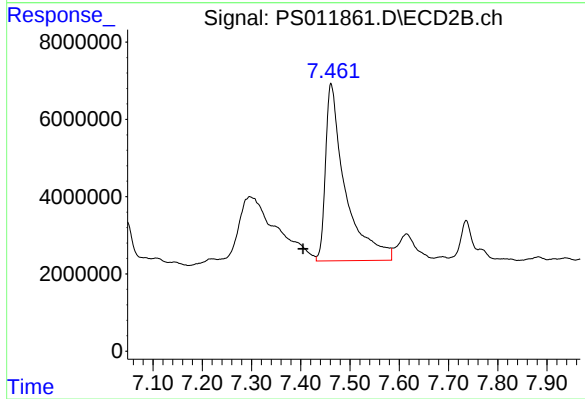

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.057 min
Response: 127686095
Conc: 46.60 ug/ml

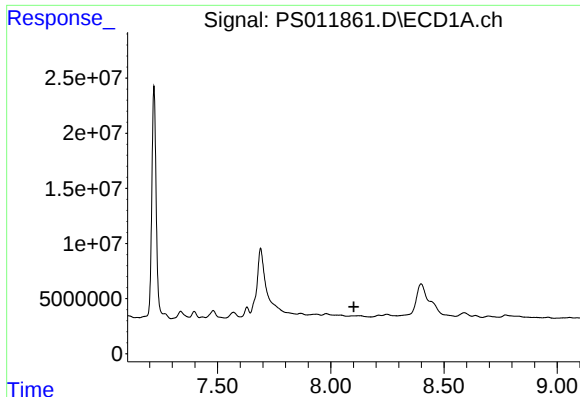

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

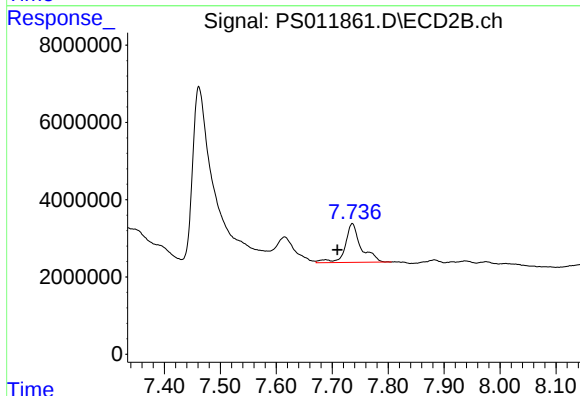


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 19767153
Conc: 35.01 ng/ml

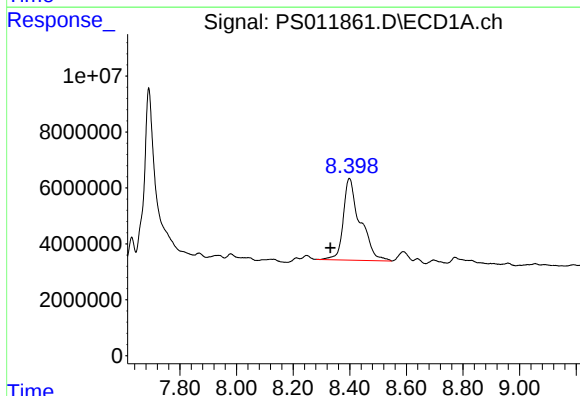


#9 2,4-D

R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 120927847
Conc: 107.10 ng/ml

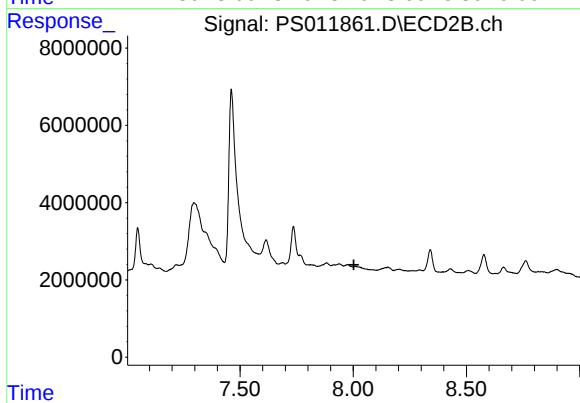

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

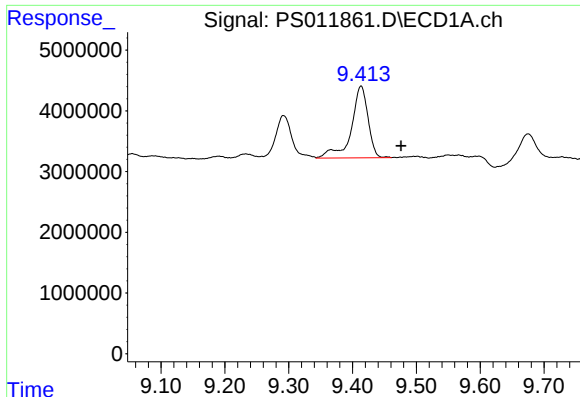

#12 2,4,5-T


R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 21573732
Conc: 3.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

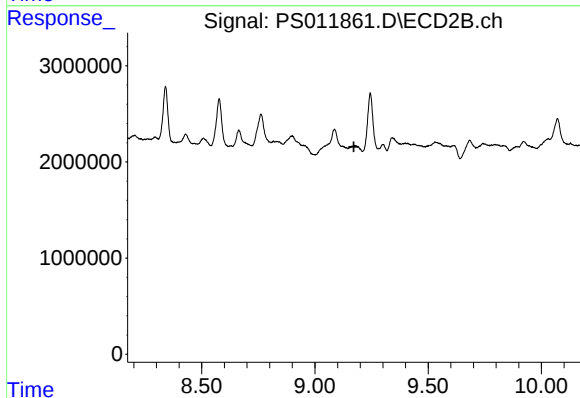


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

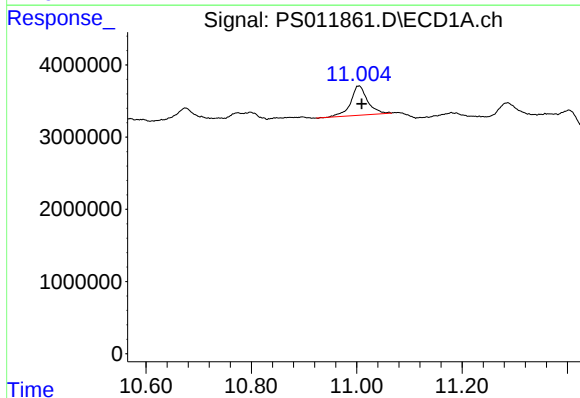

#15 Picloram

R.T.: 11.004 min
Delta R.T.: -0.005 min
Response: 8997745
Conc: 1.15 ng/ml

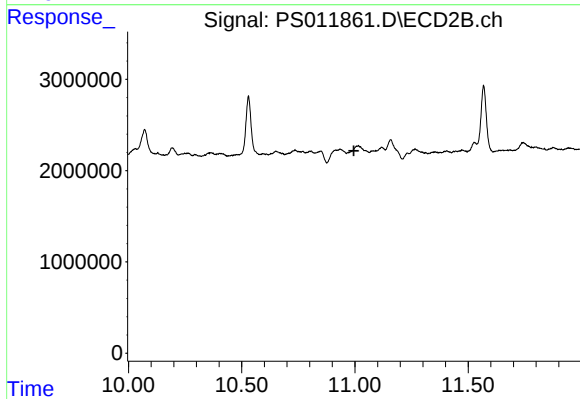

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.