

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
 Data File : PS011865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2020 20:16
 Operator : DD\AJ
 Sample : L3504-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:38:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	282.6E6	177.1E6	259.049	331.228 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	10152065	N.D.	12.341
5) T	DICAMBA	7.479	0.000	9824936	0	2.399	N.D. #
7) T	MCPA	7.688	7.461	218.3E6	184.9E6	47.998	67.482 #
8) T	DICHLORPROP	0.000	7.736	0	14941303	N.D.	26.462
9) T	2,4-D	8.397	0.000	124.2E6	0	110.006	N.D. #
11) T	2,4,5-TP ...	0.000	8.786	0	24802804	N.D.	8.484
12) T	2,4,5-T	9.412	0.000	15935527	0	2.689	N.D. #
15) T	Picloram	11.002	0.000	10391036	0	1.330	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082020\
Data File : PS011865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2020 20:16
Operator : DD\AJ
Sample : L3504-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:38:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

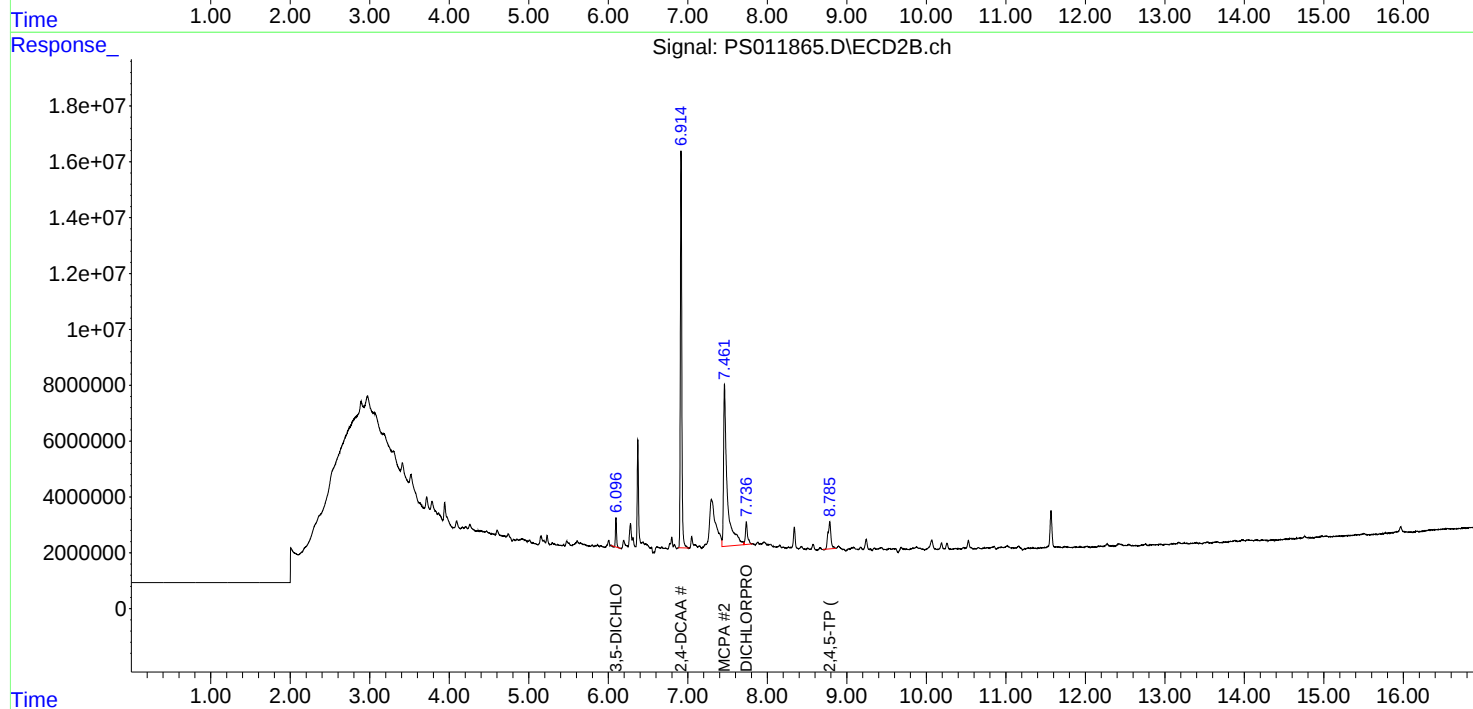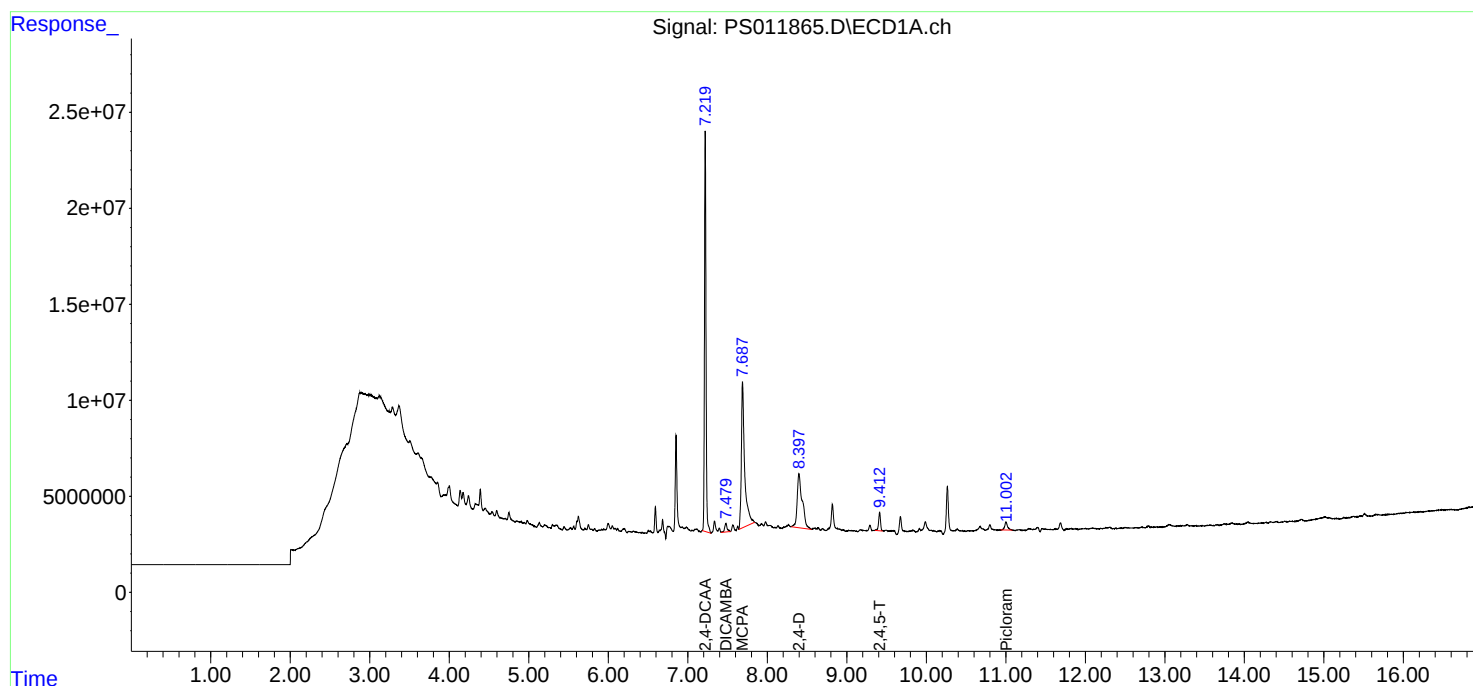


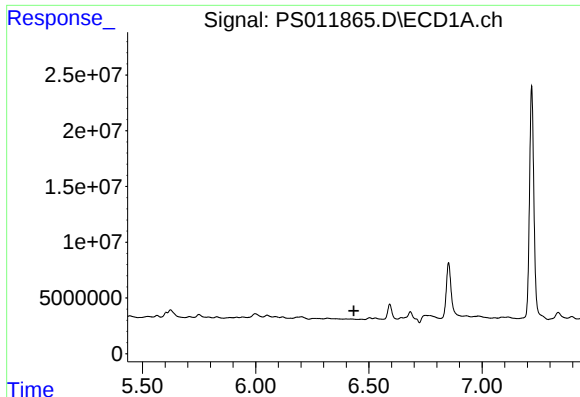

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

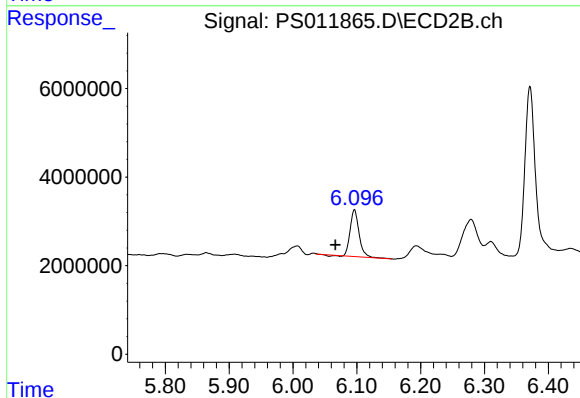


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 10152065
Conc: 12.34 ng/ml

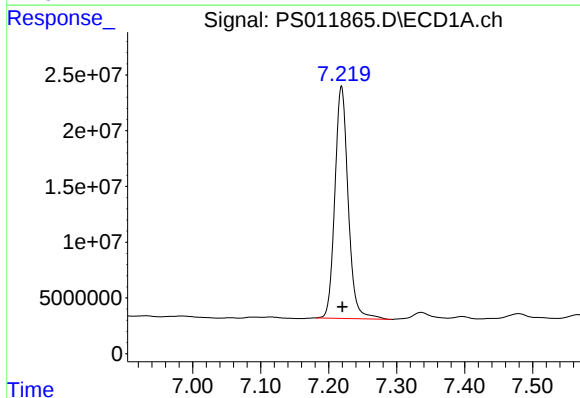


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 282562230
Conc: 259.05 ng/ml

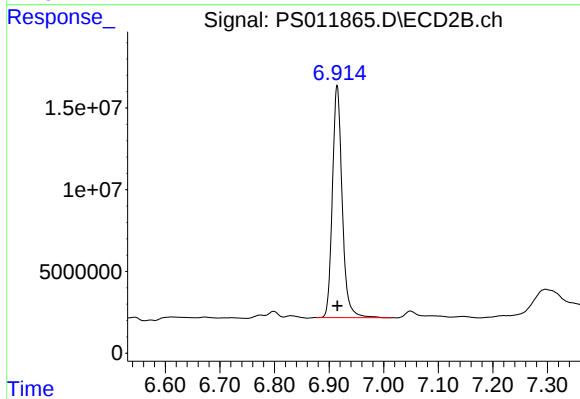

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 177136525
Conc: 331.23 ng/ml

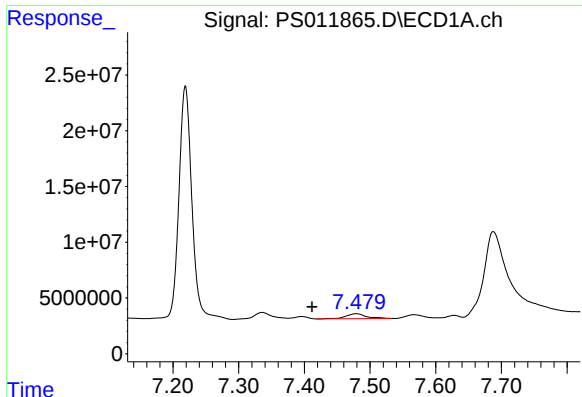

#5 DICAMBA


R.T.: 7.479 min
Delta R.T.: 0.068 min
Response: 9824936
Conc: 2.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

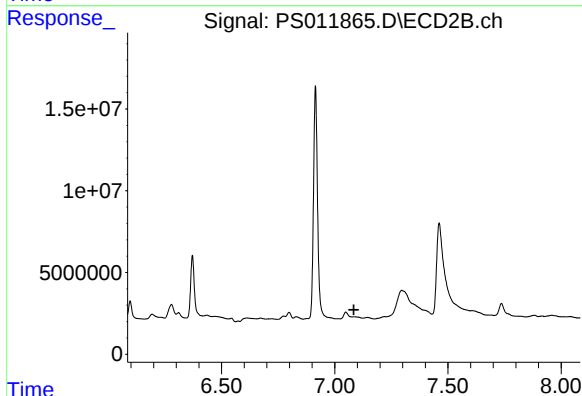


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

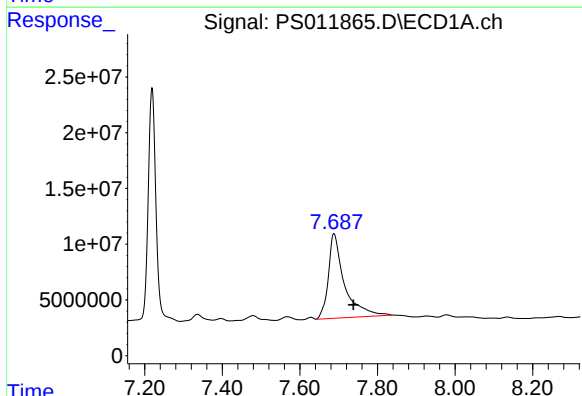


#7 MCPA

R.T.: 7.688 min
Delta R.T.: -0.050 min
Response: 218319851
Conc: 48.00 ug/ml

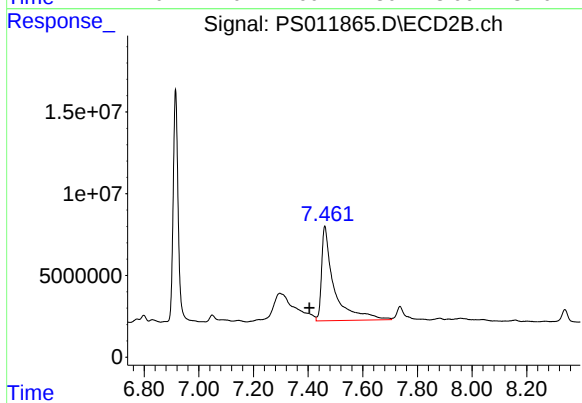

#7 MCPA


R.T.: 7.461 min
Delta R.T.: 0.056 min
Response: 184909737
Conc: 67.48 ug/ml

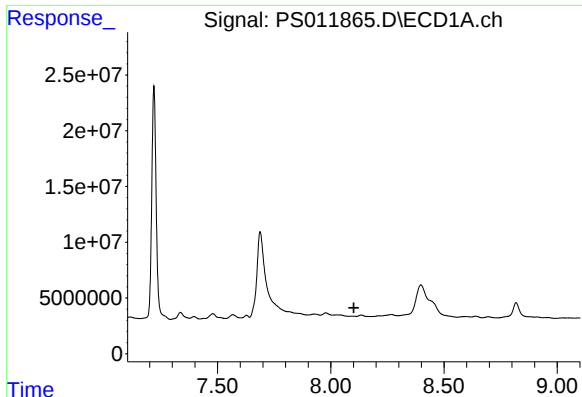

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

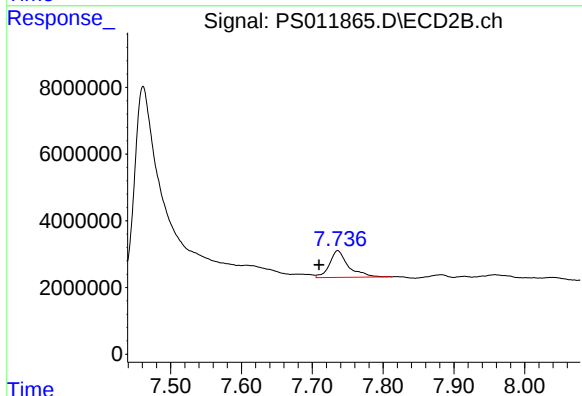


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.027 min
Response: 14941303
Conc: 26.46 ng/ml

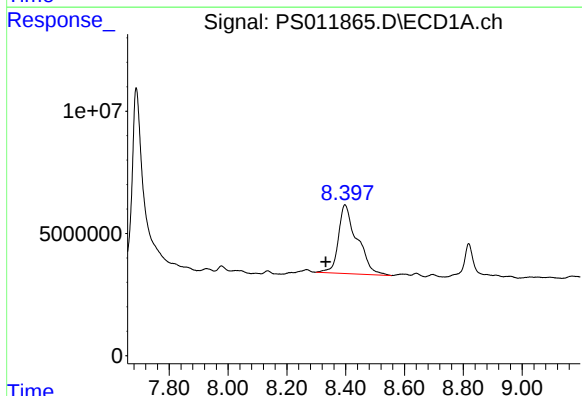


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 124207110
Conc: 110.01 ng/ml

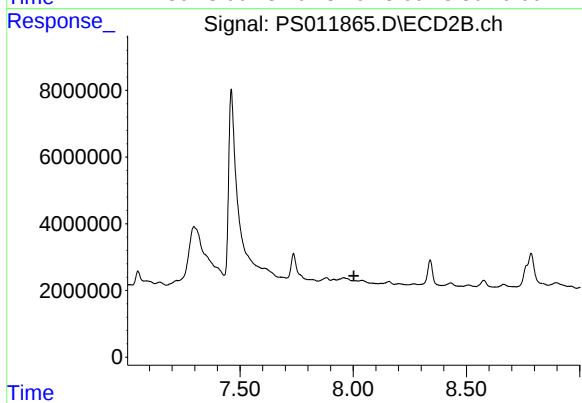

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

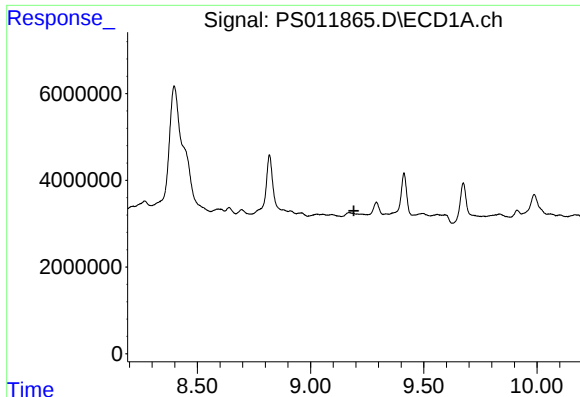

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

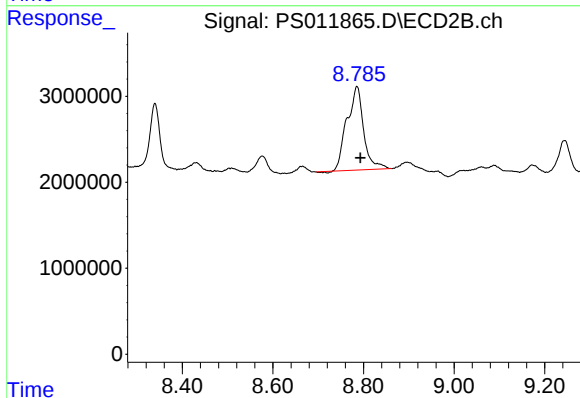


#11 2,4,5-TP (SILVEX)

R.T.: 8.786 min
Delta R.T.: -0.008 min
Response: 24802804
Conc: 8.48 ng/ml

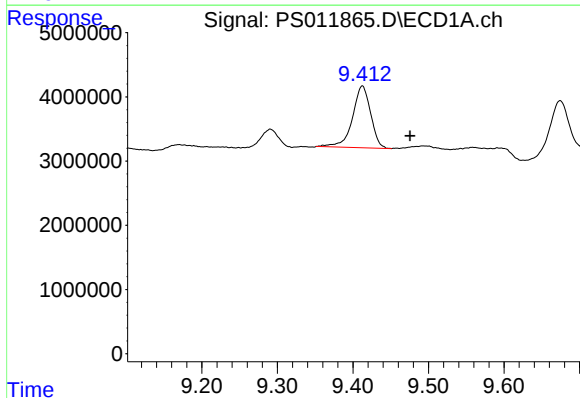


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.063 min
Response: 15935527
Conc: 2.69 ng/ml

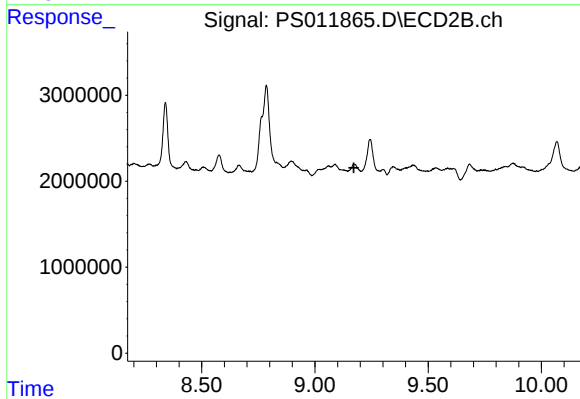

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

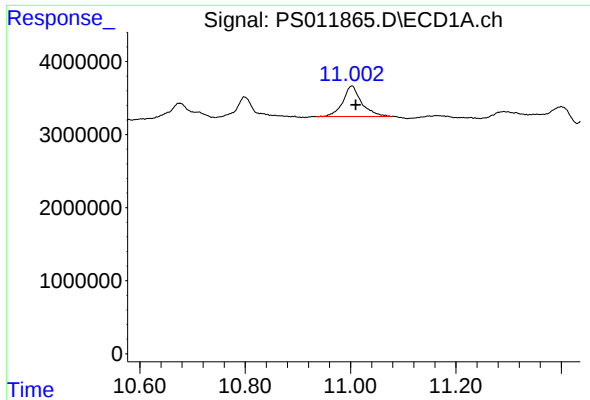

#15 Picloram

R.T.: 11.002 min
Delta R.T.: -0.007 min
Response: 10391036
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

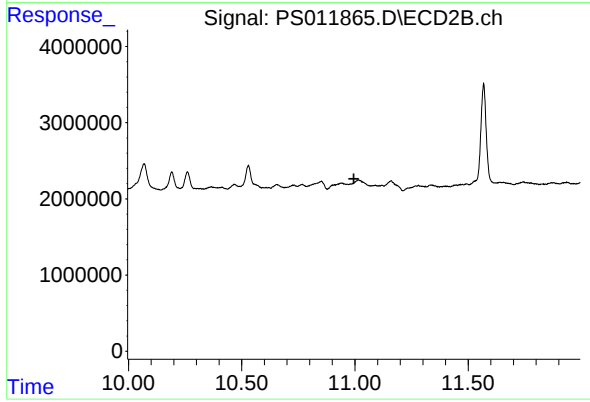

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.