

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082021\
 Data File : PS016518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 10:00
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 15:54:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) T	2,4-D	8.366f	0.000	71164250	0	47.060	N.D. #
12) T	2,4,5-T	0.000	9.067f	0	1537622	N.D.	<MDL
15) T	Picloram	10.995	10.829	22163434	11251130	2.221	2.794 #
16) T	DCPA	0.000	10.829f	0	11251130	N.D.	2.503



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082021\
Data File : PS016518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 10:00
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 15:54:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

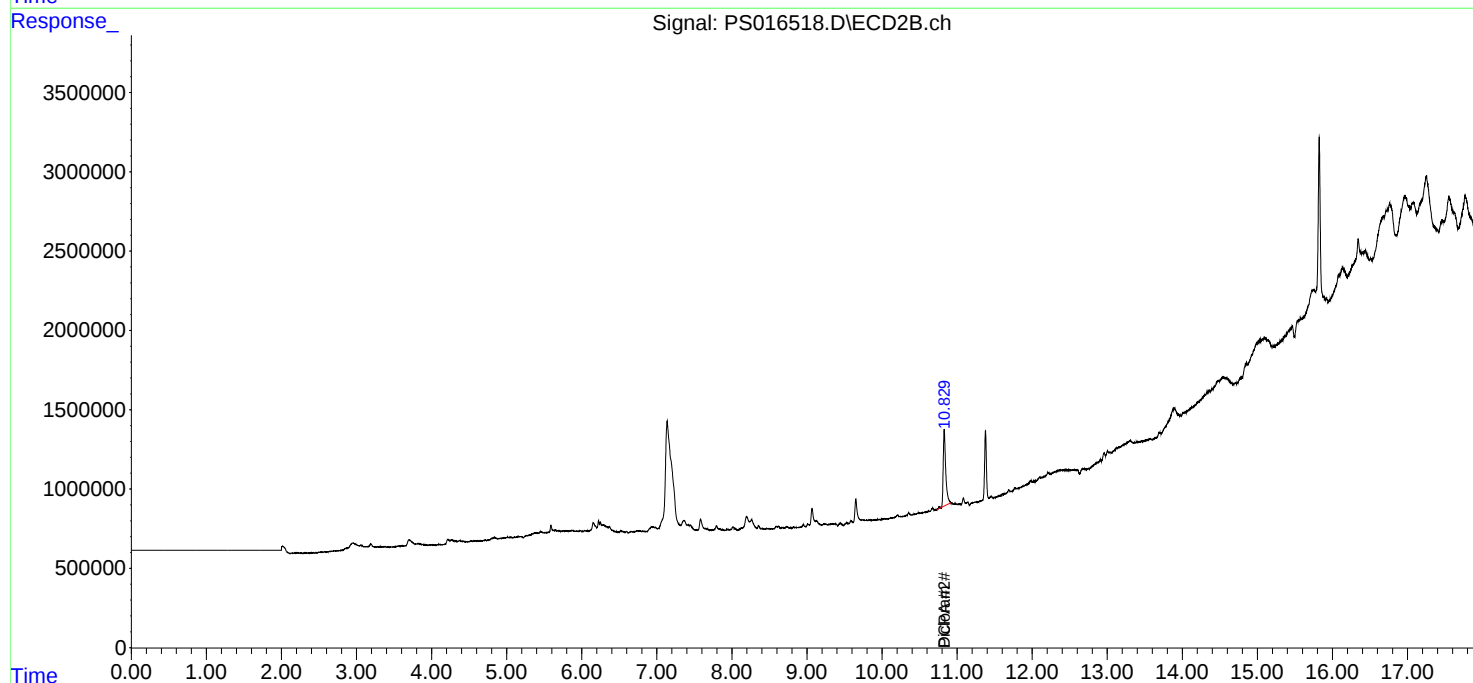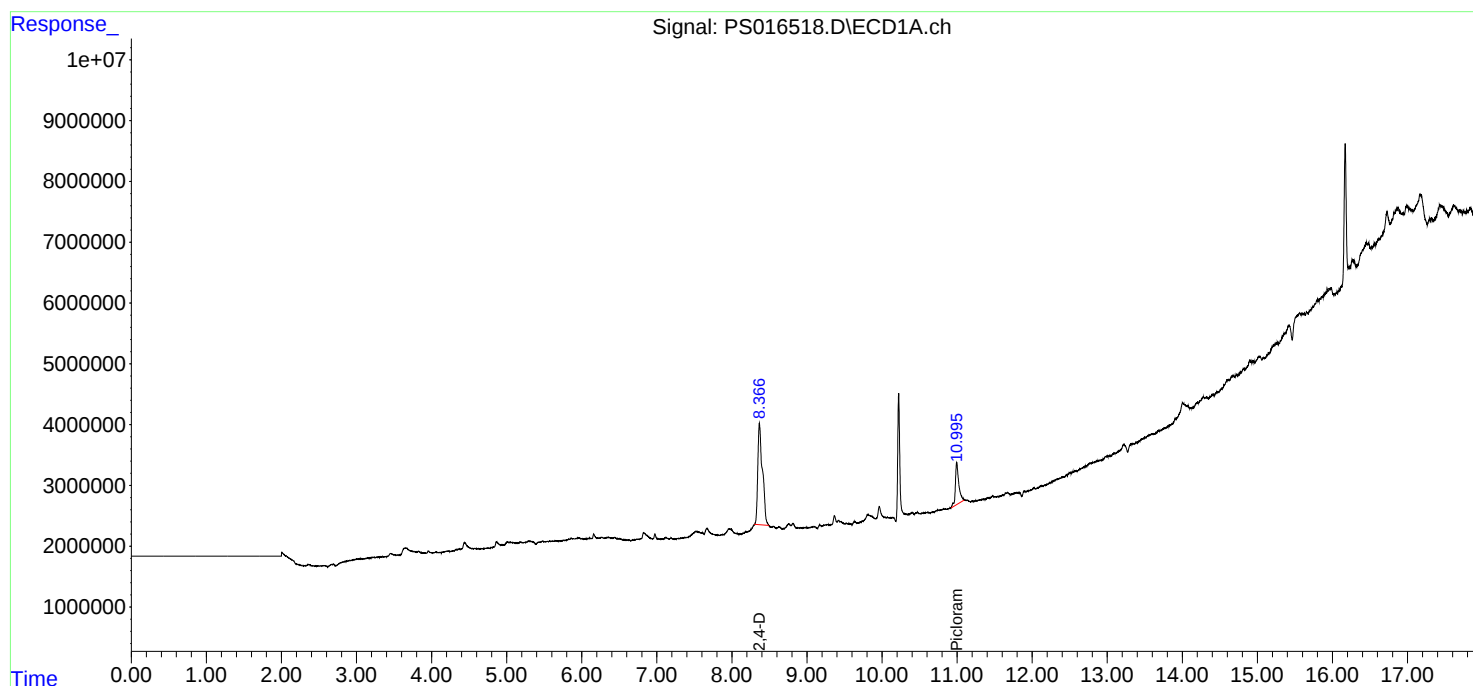


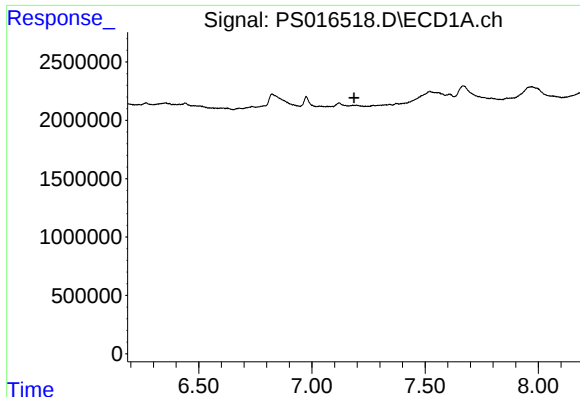

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

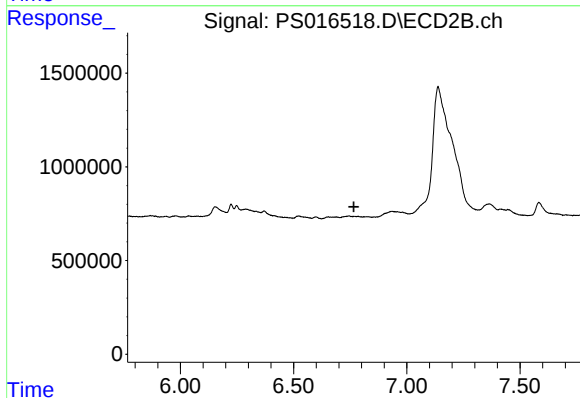


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.766 min
Response: 0
Conc: N.D.

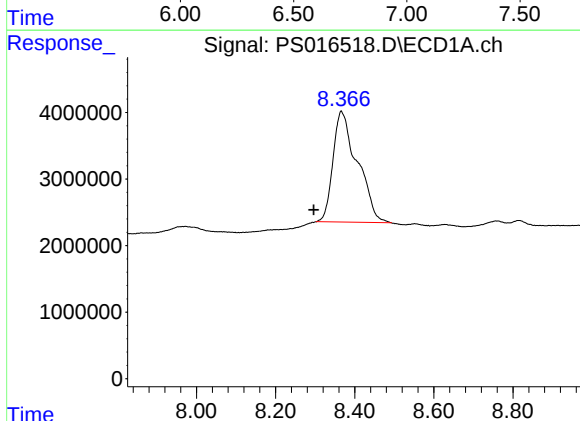


#9 2,4-D

R.T.: 8.366 min
Delta R.T.: 0.069 min
Response: 71164250
Conc: 47.06 ng/ml

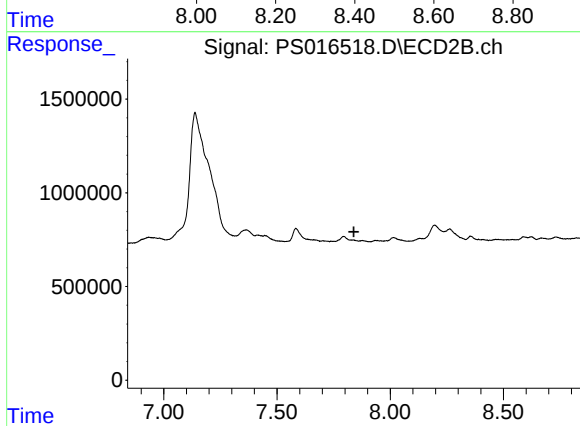

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.839 min
Response: 0
Conc: N.D.

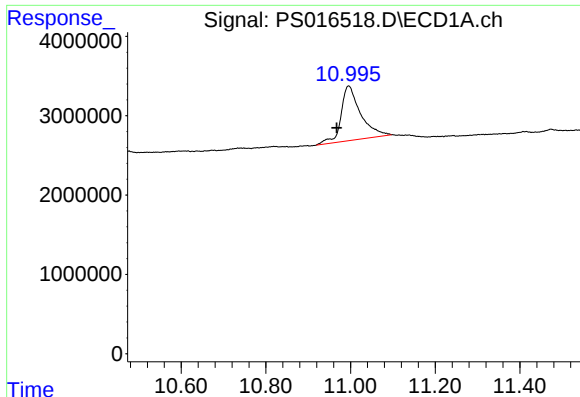

#15 Picloram


R.T.: 10.995 min
Delta R.T.: 0.028 min
Response: 22163434
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

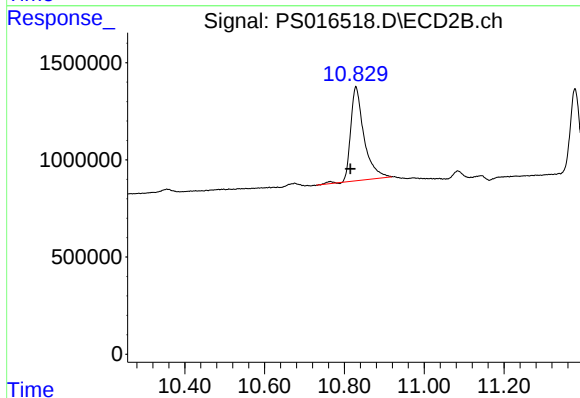


#15 Picloram

R.T.: 10.829 min
Delta R.T.: 0.013 min
Response: 11251130
Conc: 2.79 ng/ml

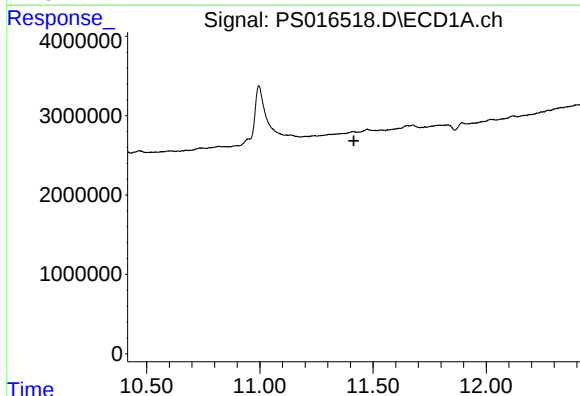

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.415 min
Response: 0
Conc: N.D.

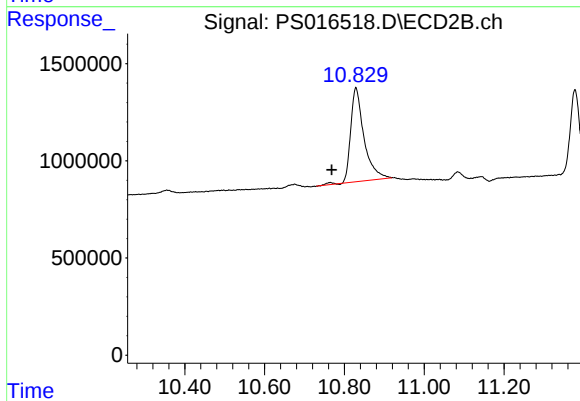

#16 DCPA

R.T.: 10.829 min
Delta R.T.: 0.061 min
Response: 11251130
Conc: 2.50 ng/ml