

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082021\  
 Data File : PS016543.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Aug 2021 20:04  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 20 23:18:04 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080221.M  
 Quant Title : 8080.M  
 QLast Update : Mon Aug 02 14:10:19 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound    | RT#1  | RT#2    | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-------------|-------|---------|---------|---------|---------|---------|
| -----                       |             |       |         |         |         |         |         |
| System Monitoring Compounds |             |       |         |         |         |         |         |
| 4) S                        | 2,4-DCAA    | 7.183 | 6.764   | 693.2E6 | 289.4E6 | 471.192 | 554.869 |
| Target Compounds            |             |       |         |         |         |         |         |
| 8) T                        | DICHLORPROP | 0.000 | 7.576   | 0       | 3217610 | N.D.    | 5.939   |
| 15) T                       | Picloram    | 0.000 | 10.825  | 0       | 6037738 | N.D.    | 1.499   |
| 16) T                       | DCPA        | 0.000 | 10.825f | 0       | 6037738 | N.D.    | 1.343   |
| -----                       |             |       |         |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082021\  
Data File : PS016543.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Aug 2021 20:04  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 20 23:18:04 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080221.M  
Quant Title : 8080.M  
QLast Update : Mon Aug 02 14:10:19 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

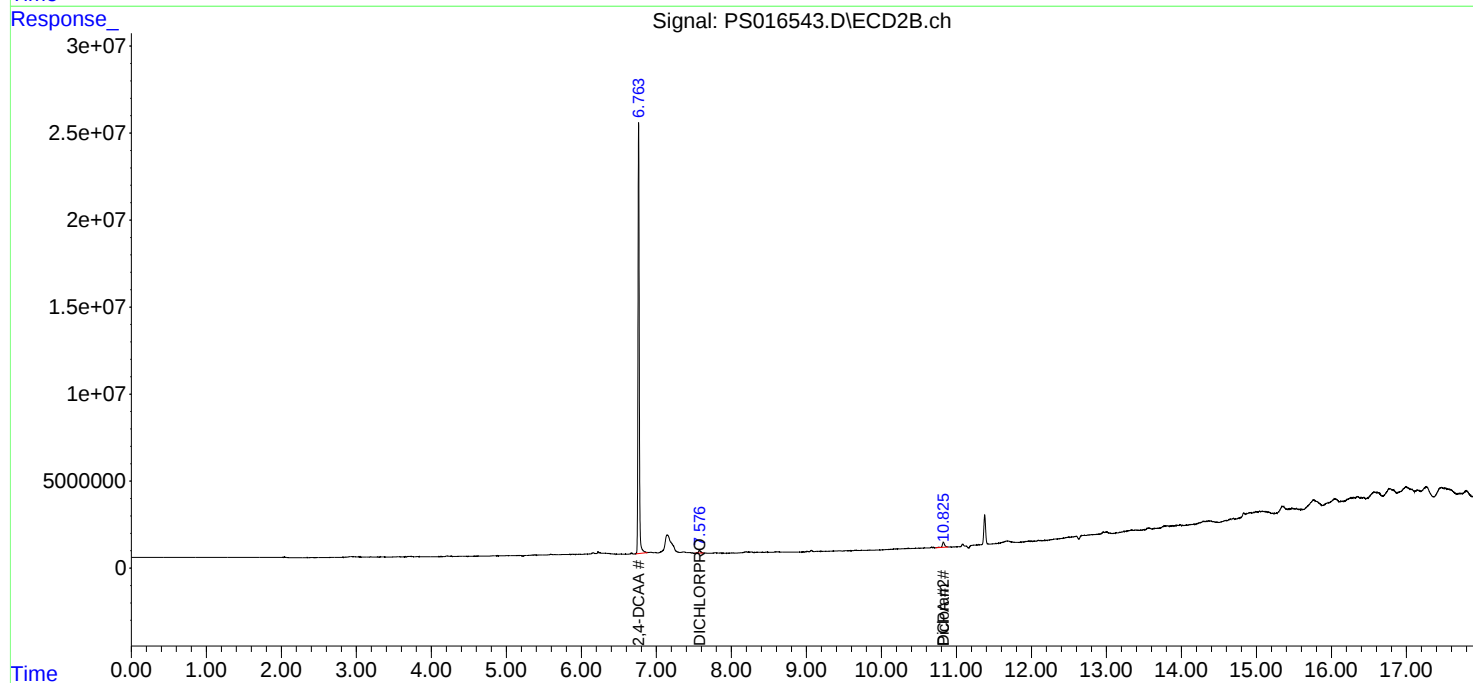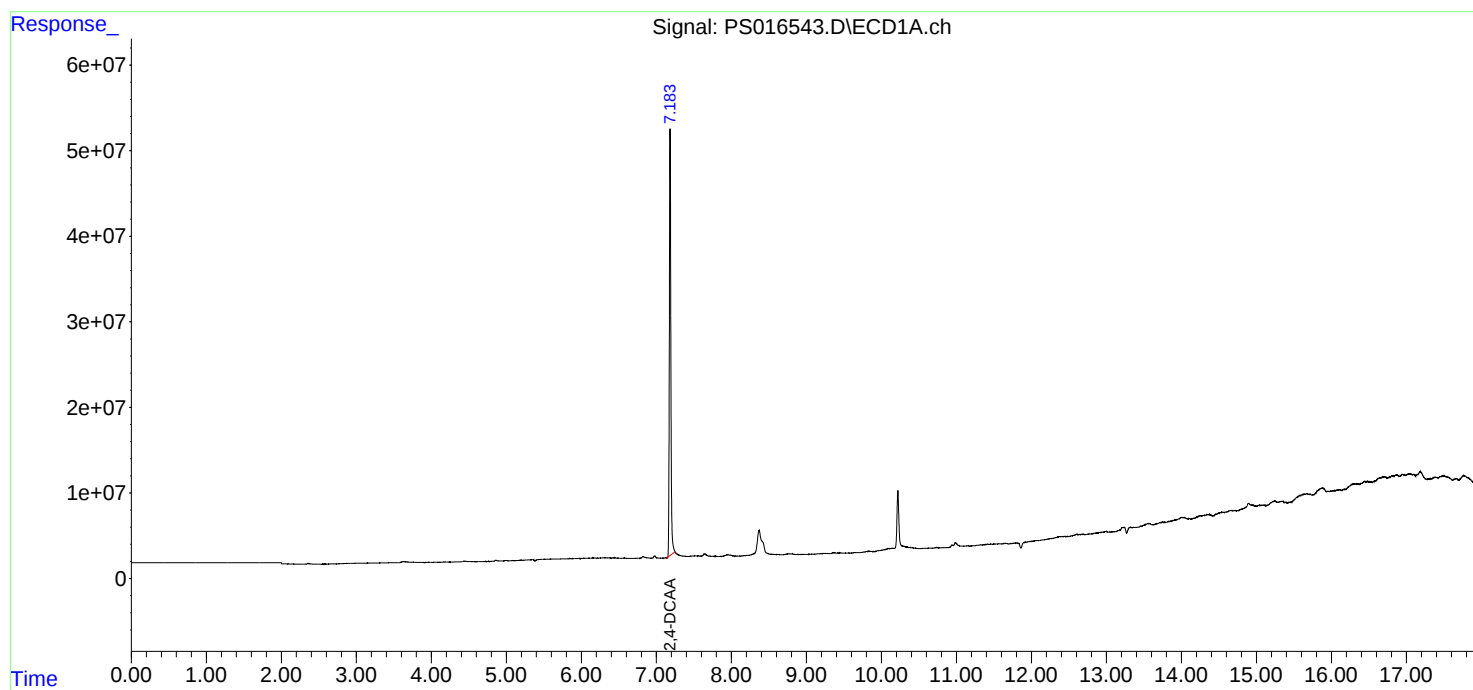


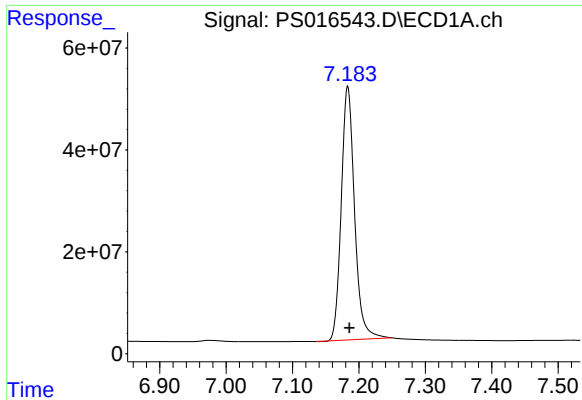

#4 2,4-DCAA


R.T.: 7.183 min  
Delta R.T.: -0.003 min  
Response: 693173379  
Conc: 471.19 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

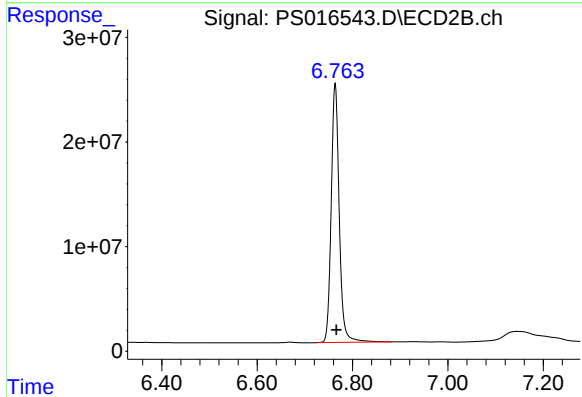


#4 2,4-DCAA

R.T.: 6.764 min  
Delta R.T.: -0.002 min  
Response: 289433071  
Conc: 554.87 ng/ml

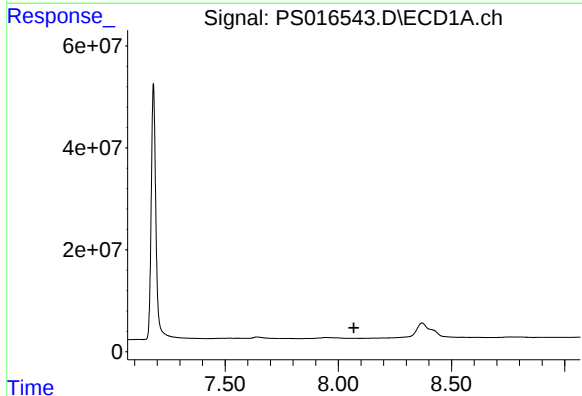


#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T. : 8.069 min  
Response: 0  
Conc: N.D.

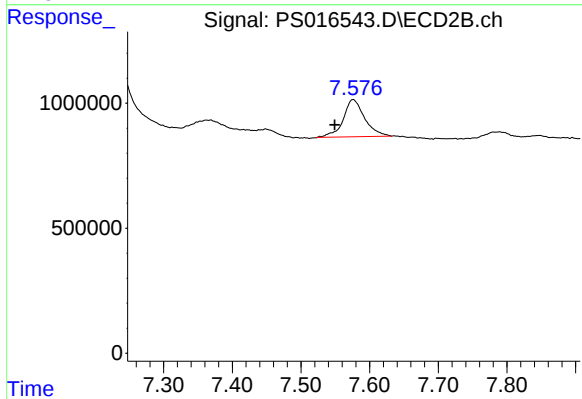

#8 DICHLORPROP


R.T.: 7.576 min  
Delta R.T.: 0.026 min  
Response: 3217610  
Conc: 5.94 ng/ml

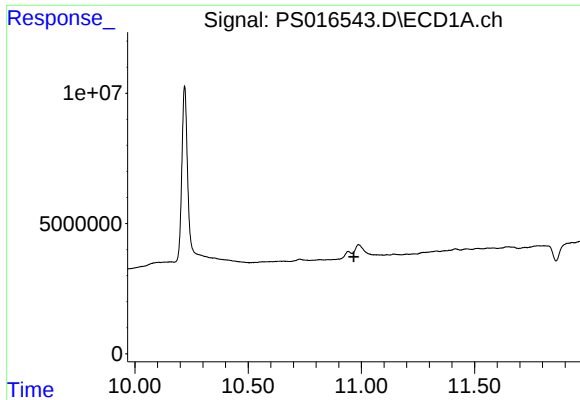

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 10.967 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

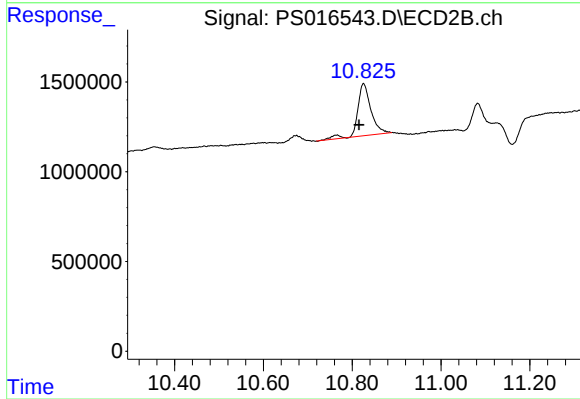


#15 Picloram

R.T.: 10.825 min  
Delta R.T.: 0.010 min  
Response: 6037738  
Conc: 1.50 ng/ml

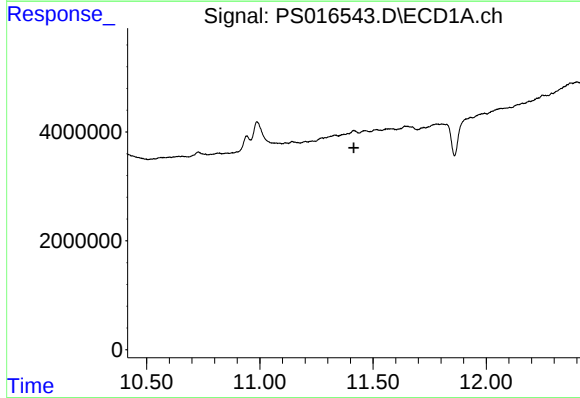

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 11.415 min  
Response: 0  
Conc: N.D.

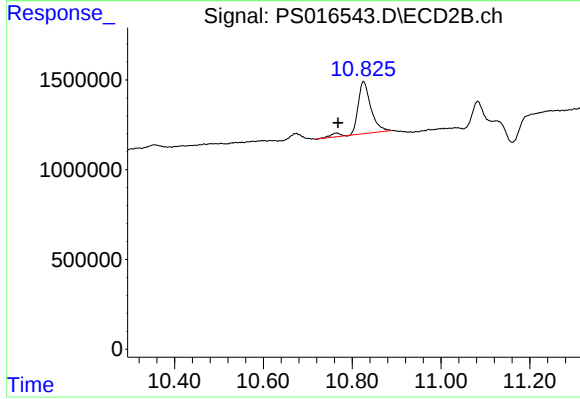

#16 DCPA

R.T.: 10.825 min  
Delta R.T.: 0.057 min  
Response: 6037738  
Conc: 1.34 ng/ml