

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082024\
 Data File : PS027488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2024 09:10
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:24:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	7.755	0	2348166	N.D.	1.189
Target Compounds							
1) T	Dalapon	0.000	2.699	0	3766353	N.D.	1.031
3) T	4-Nitroph...	6.954	0.000	3204517	0	2.058	N.D. #
5) T	DICAMBA	0.000	7.937	0	6106488	N.D.	<MDL
6) T	MCP	0.000	8.027	0	107590	N.D.	<MDL
10) T	Pentachlo...	8.552	9.466f	1183671	4868780	<MDL	<MDL #
11) T	2,4,5-TP ...	9.123	9.880	1698031	1728604	<MDL	<MDL #
12) T	2,4,5-T	9.428	10.302	6327418	3598614	<MDL	<MDL #
13) T	2,4-DB	0.000	10.894f	0	434980	N.D.	<MDL
14) T	DINOSEB	11.161	11.238	4819161	527520	<MDL	<MDL #
15) T	Picloram	11.012f	12.337	59941251	38597759	2.983	1.972 #
16) T	DCPA	0.000	12.243f	0	2812391	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082024\
Data File : PS027488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2024 09:10
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:24:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

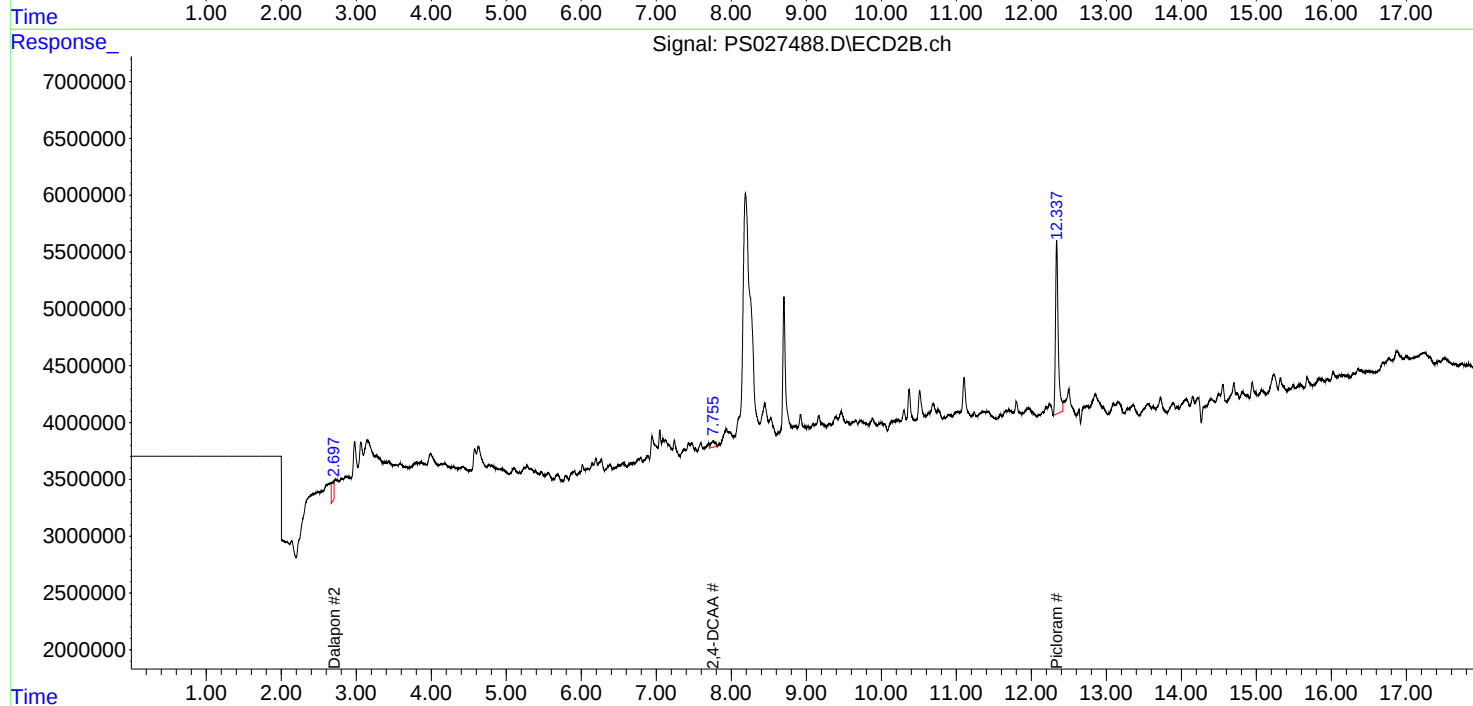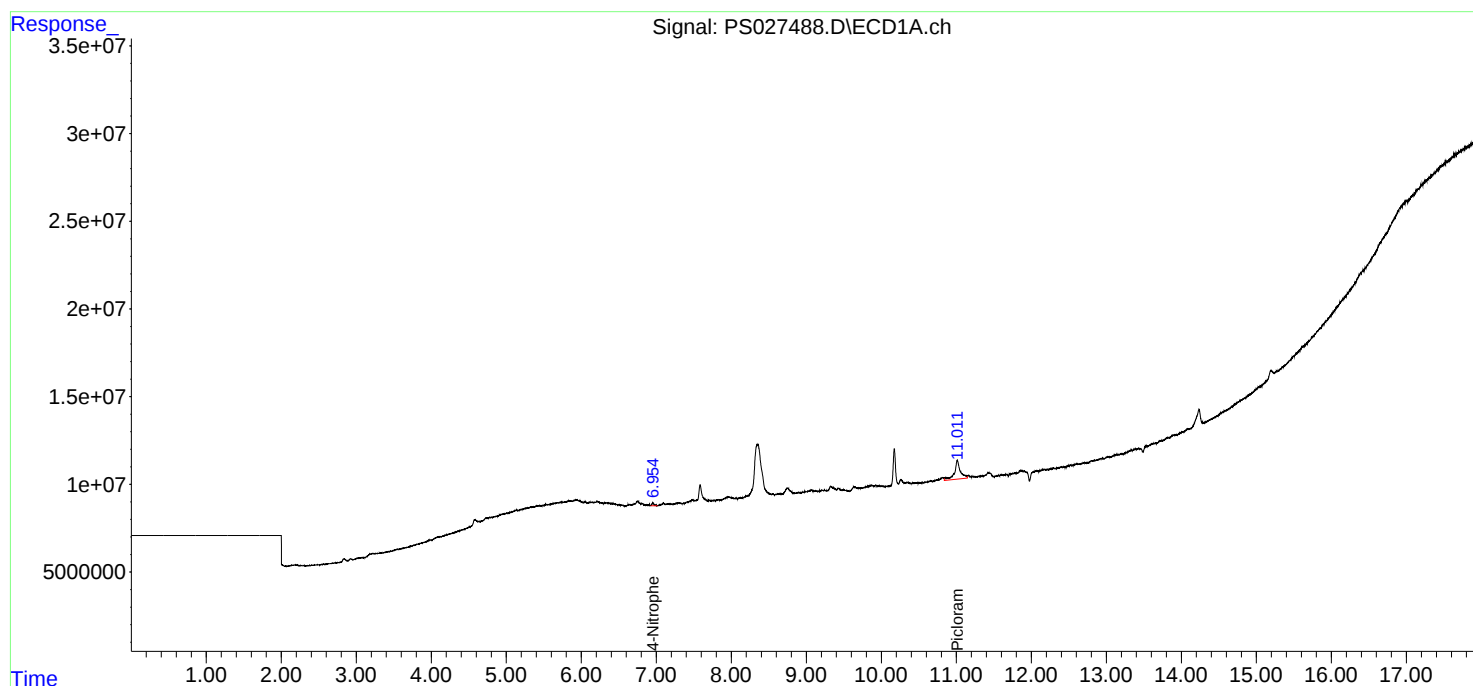


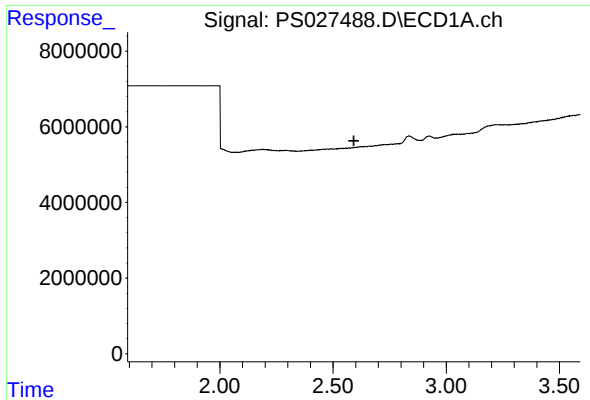

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

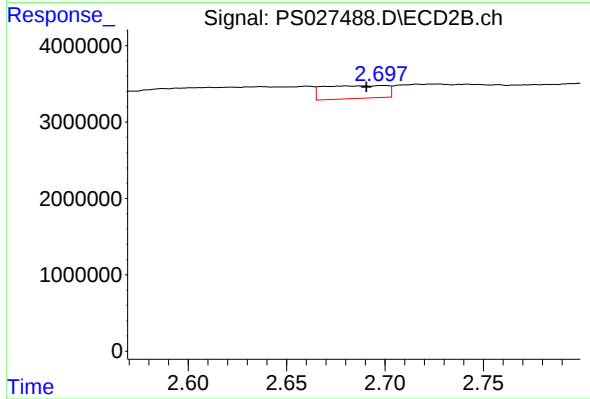


#1 Dalapon

R.T.: 2.699 min
Delta R.T.: 0.008 min
Response: 3766353
Conc: 1.03 ng/ml

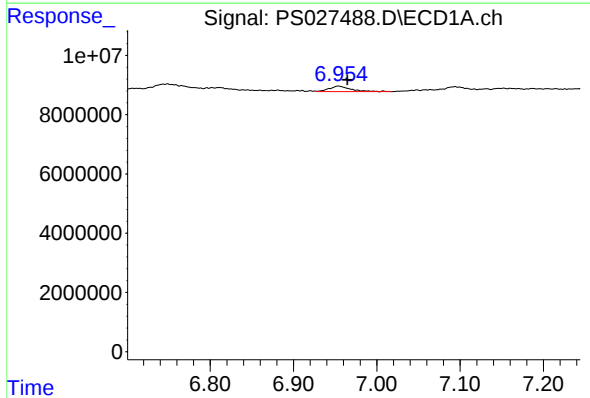


#3 4-Nitrophenol

R.T.: 6.954 min
Delta R.T.: -0.010 min
Response: 3204517
Conc: 2.06 ng/ml

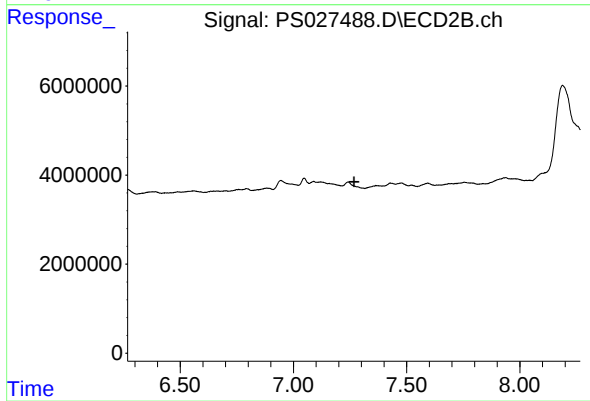

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

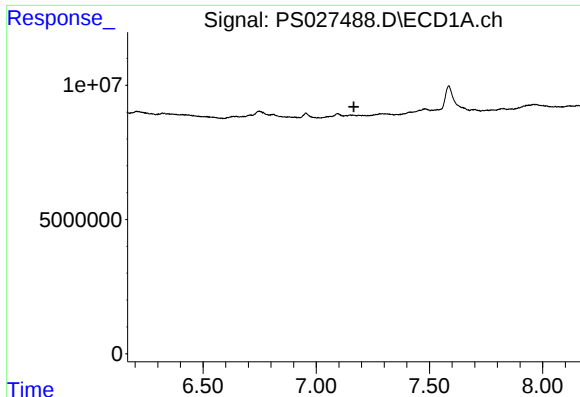

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

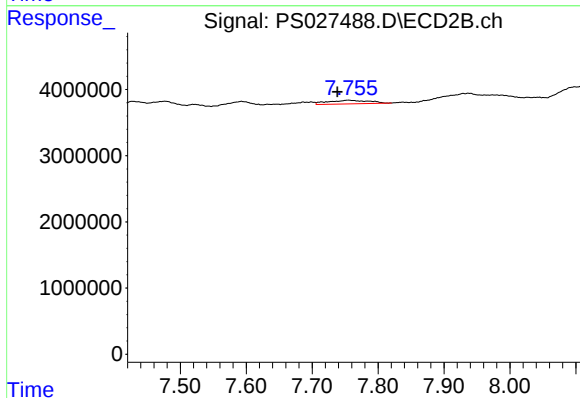


#4 2,4-DCAA

R.T.: 7.755 min
Delta R.T.: 0.016 min
Response: 2348166
Conc: 1.19 ng/ml

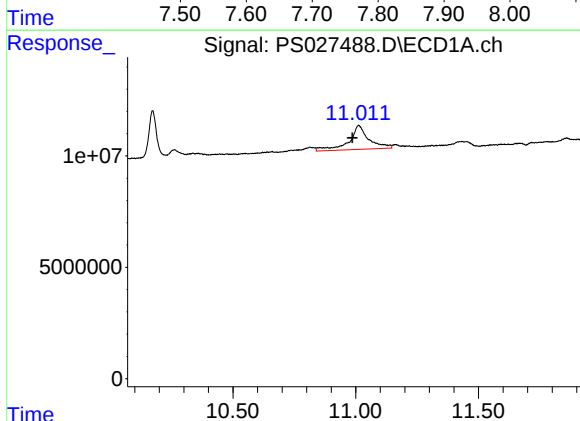

#15 Picloram

R.T.: 11.012 min
Delta R.T.: 0.025 min
Response: 59941251
Conc: 2.98 ng/ml

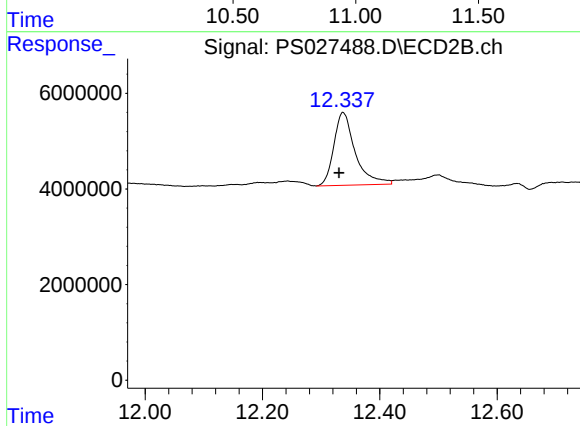

#15 Picloram

R.T.: 12.337 min
Delta R.T.: 0.007 min
Response: 38597759
Conc: 1.97 ng/ml