

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082024\
 Data File : PS027499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2024 18:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:27:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	7.736	1211.5E6	958.8E6	468.440	485.662
Target Compounds							
1) T	Dalapon	0.000	2.715	0	20921517	N.D.	5.727
3) T	4-Nitroph...	6.955	0.000	9648258	0	6.196	N.D. #
5) T	DICAMBA	0.000	7.933	0	5284790	N.D.	<MDL
6) T	MCP	0.000	8.037	0	3054038	N.D.	<MDL
8) T	DICHLORPROP	8.065f	8.698f	556446	10297726	<MDL	4.631 #
9) T	2,4-D	8.274	0.000	39495916	0	13.551	N.D. #
10) T	Pentachlo...	8.566	9.496	1769916	2779365	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.879	0	2826791	N.D.	<MDL
12) T	2,4,5-T	9.458f	10.283	3352744	1134531	<MDL	<MDL #
13) T	2,4-DB	10.005	0.000	2479056	0	1.159	N.D. #
14) T	DINOSEB	11.157	11.257	5440004	1678777	<MDL	<MDL #
15) T	Picloram	10.959f	12.331	65542545	35522179	3.262	1.814 #
16) T	DCPA	11.436f	0.000	3529329	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082024\
Data File : PS027499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2024 18:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:27:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

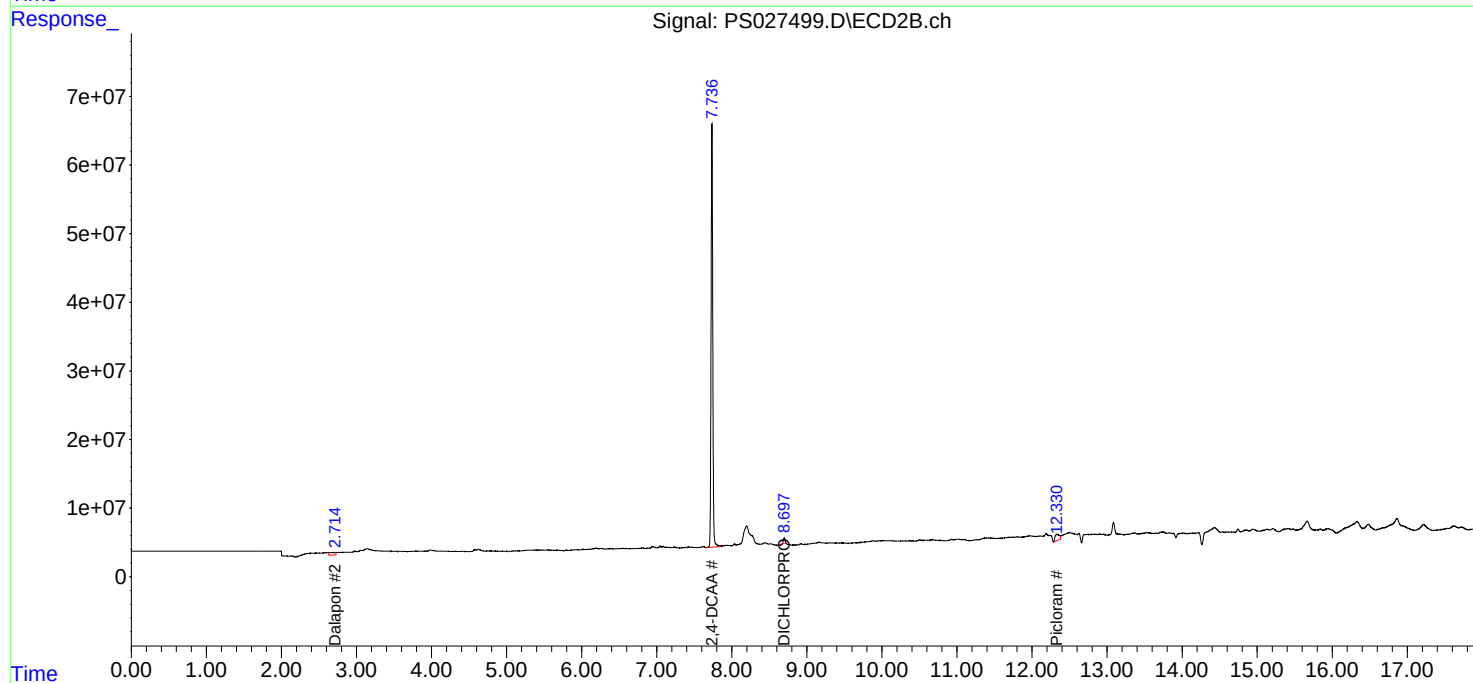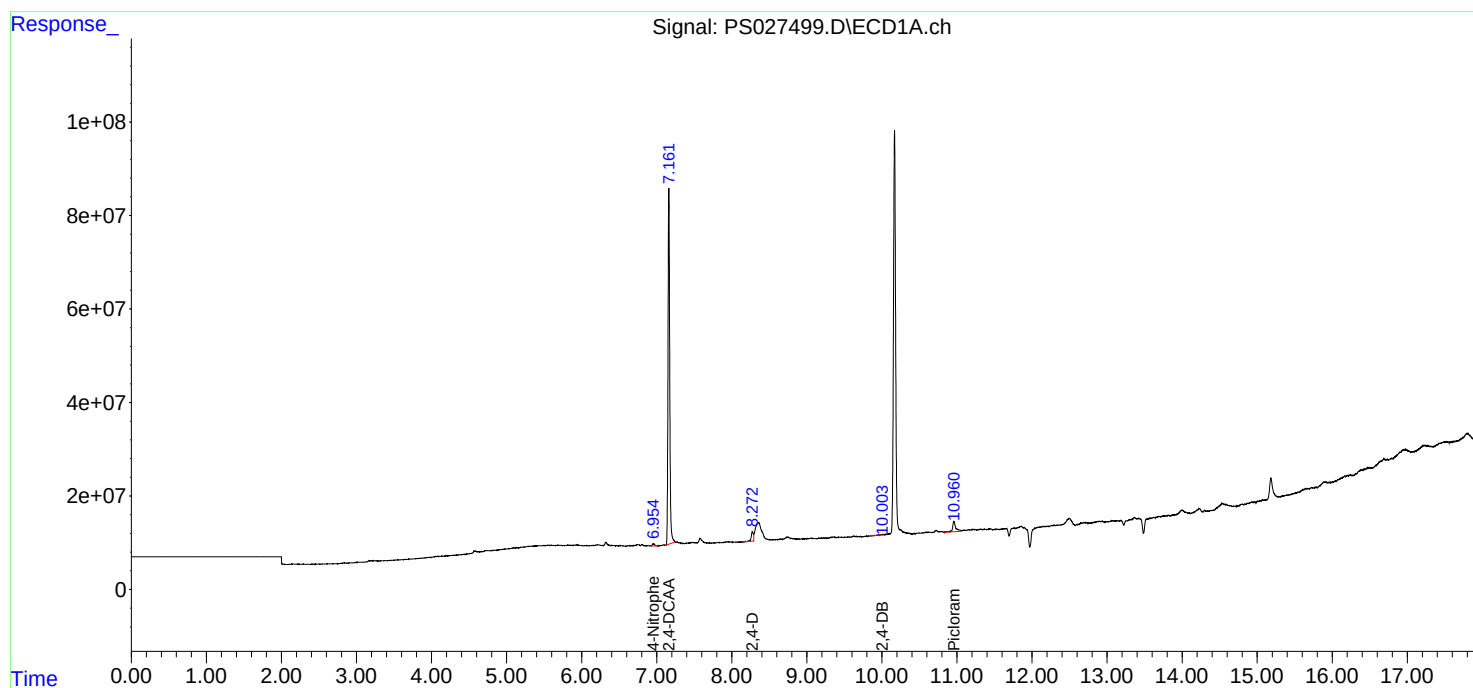


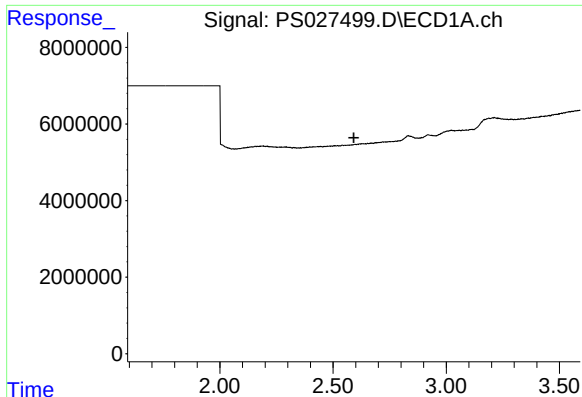

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

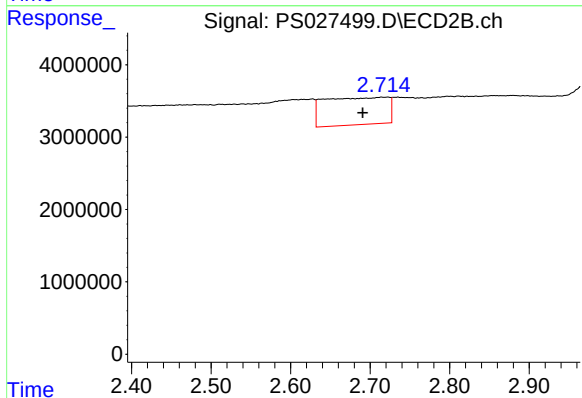


#1 Dalapon

R.T.: 2.715 min
Delta R.T.: 0.024 min
Response: 20921517
Conc: 5.73 ng/ml

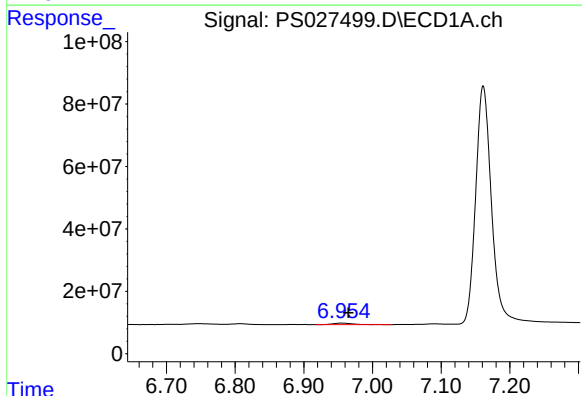


#3 4-Nitrophenol

R.T.: 6.955 min
Delta R.T.: -0.009 min
Response: 9648258
Conc: 6.20 ng/ml

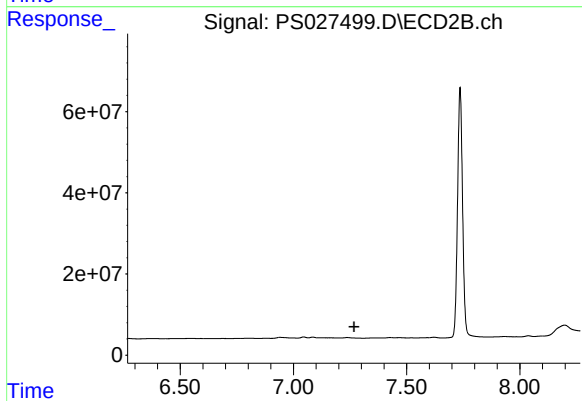

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

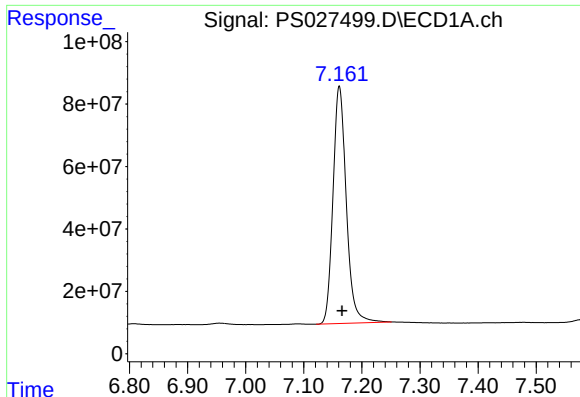

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: -0.005 min
Response: 1211508485
Conc: 468.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

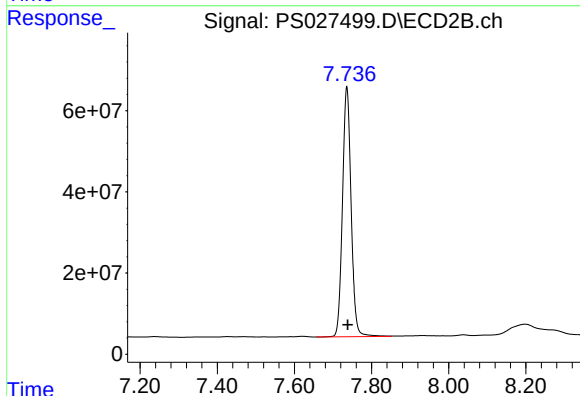


#4 2,4-DCAA

R.T.: 7.736 min
Delta R.T.: -0.003 min
Response: 958810263
Conc: 485.66 ng/ml

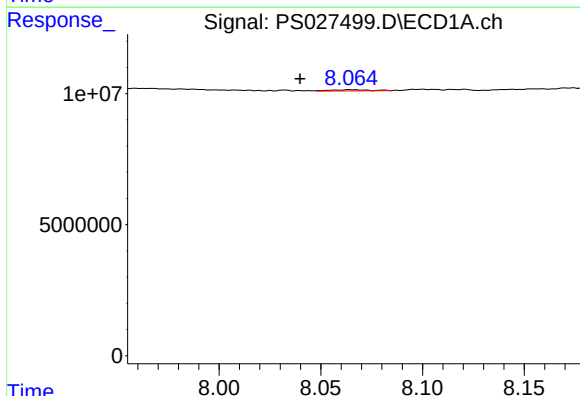


#8 DICHLORPROP

R.T.: 8.065 min
Delta R.T.: 0.026 min
Response: 556446
Conc: N.D.

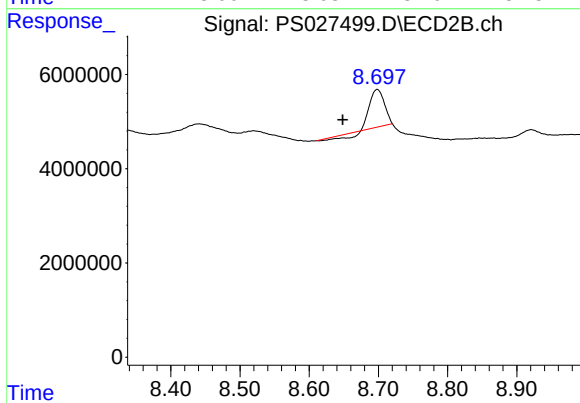

#8 DICHLORPROP


R.T.: 8.698 min
Delta R.T.: 0.050 min
Response: 10297726
Conc: 4.63 ng/ml

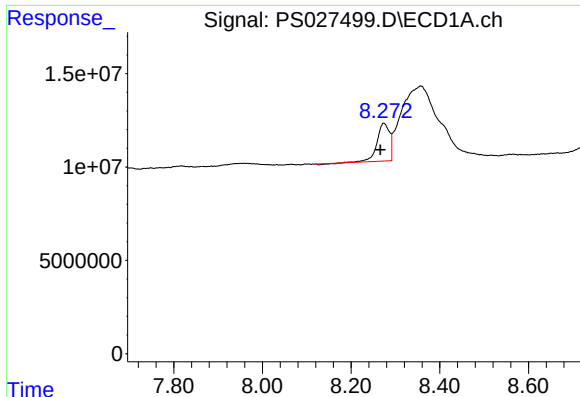

#9 2,4-D


R.T.: 8.274 min
Delta R.T.: 0.008 min
Response: 39495916
Conc: 13.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

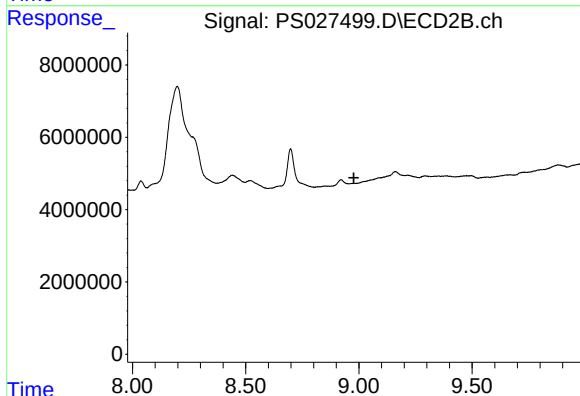


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

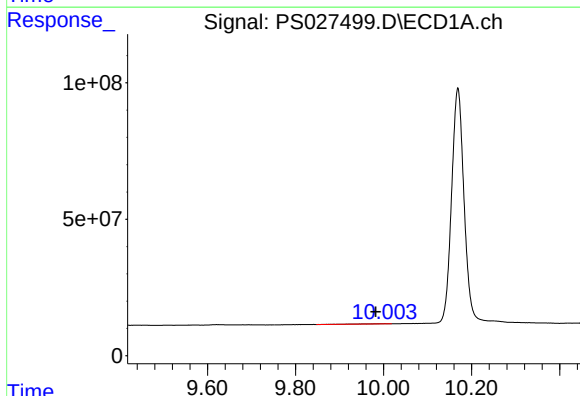


#13 2,4-DB

R.T.: 10.005 min
Delta R.T.: 0.023 min
Response: 2479056
Conc: 1.16 ng/ml

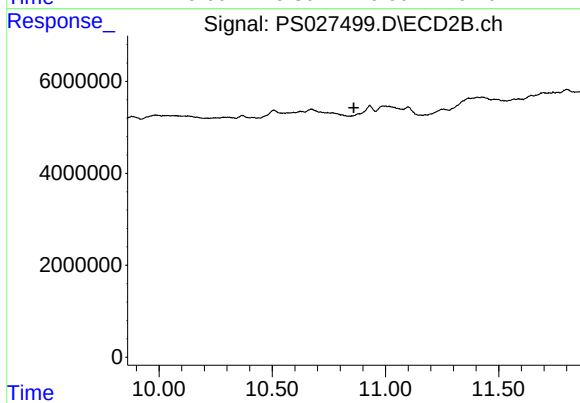

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.861 min
Response: 0
Conc: N.D.

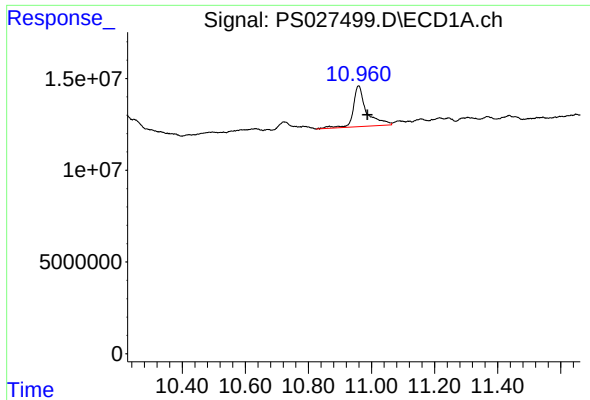

#15 Picloram

R.T.: 10.959 min
Delta R.T.: -0.028 min
Response: 65542545
Conc: 3.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

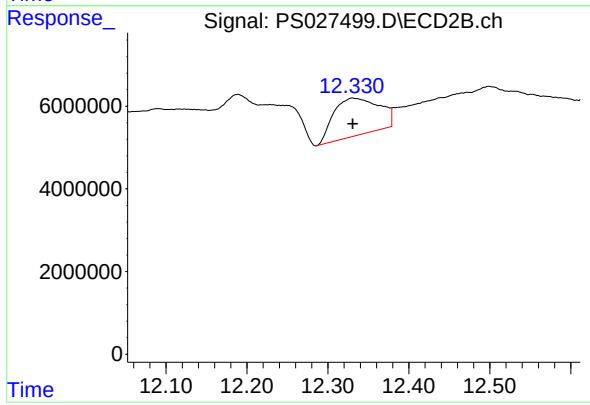

#15 Picloram

R.T.: 12.331 min
Delta R.T.: 0.000 min
Response: 35522179
Conc: 1.81 ng/ml