

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
 Data File : PS031515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 08:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 10:55:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.289	7.744	1601.4E6	458.9E6	504.543	542.827
Target Compounds							
2) T	3,5-DICHL...	6.465	0.000	1517188	0	<MDL	N.D. #
7) T	MCPA	0.000	8.246f	0	32550843	N.D.	11.602
8) T	DICHLORPROP	8.190	0.000	1752562	0	<MDL	N.D. #
10) T	Pentachlo...	8.714	9.513	8035191	6404538	<MDL	<MDL #
11) T	2,4,5-TP ...	9.296	0.000	3923981	0	<MDL	N.D. #
12) T	2,4,5-T	9.625f	0.000	3705771	0	<MDL	N.D. #
13) T	2,4-DB	10.214f	0.000	1813203	0	<MDL	N.D. #
14) T	DINOSEB	11.361	0.000	2992566	0	<MDL	N.D. #
15) T	Picloram	11.180	0.000	1822625	0	<MDL	N.D. #
16) T	DCPA	11.662	12.317	6770911	1231201	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
Data File : PS031515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 08:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 10:55:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

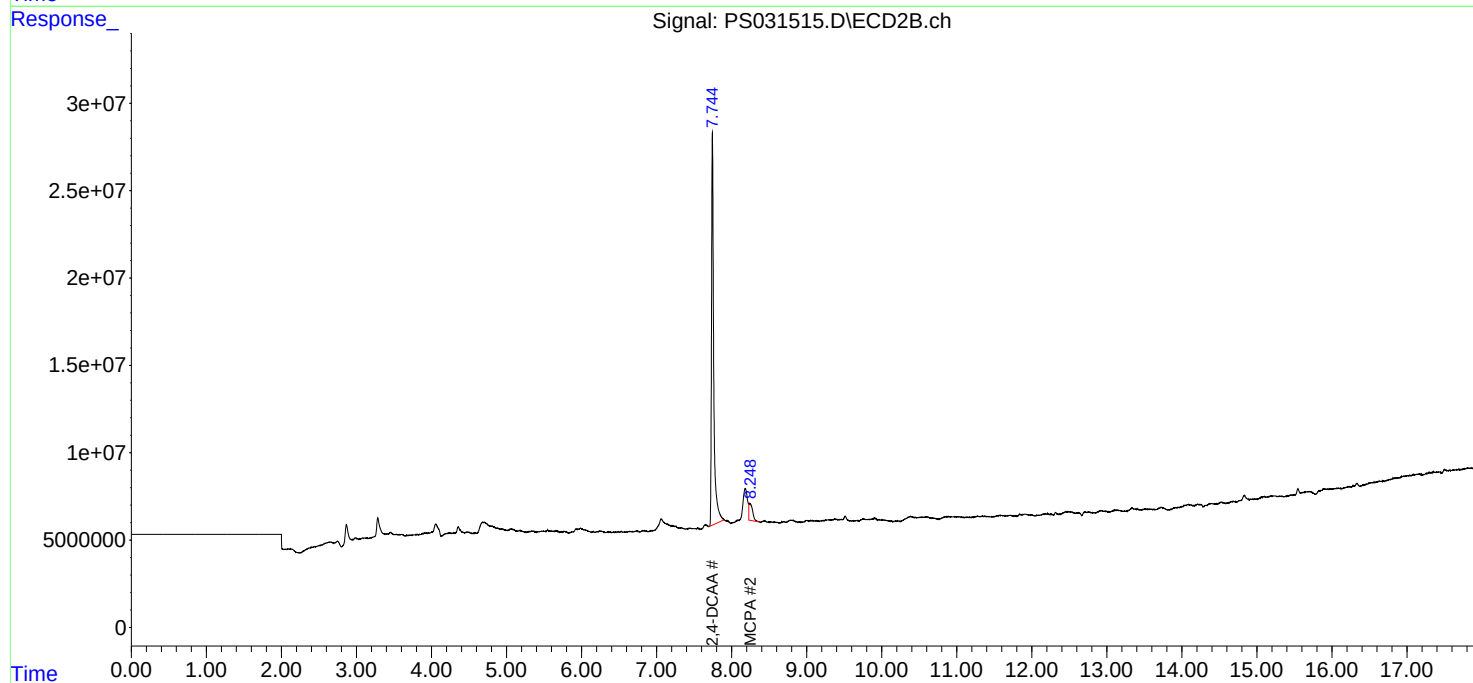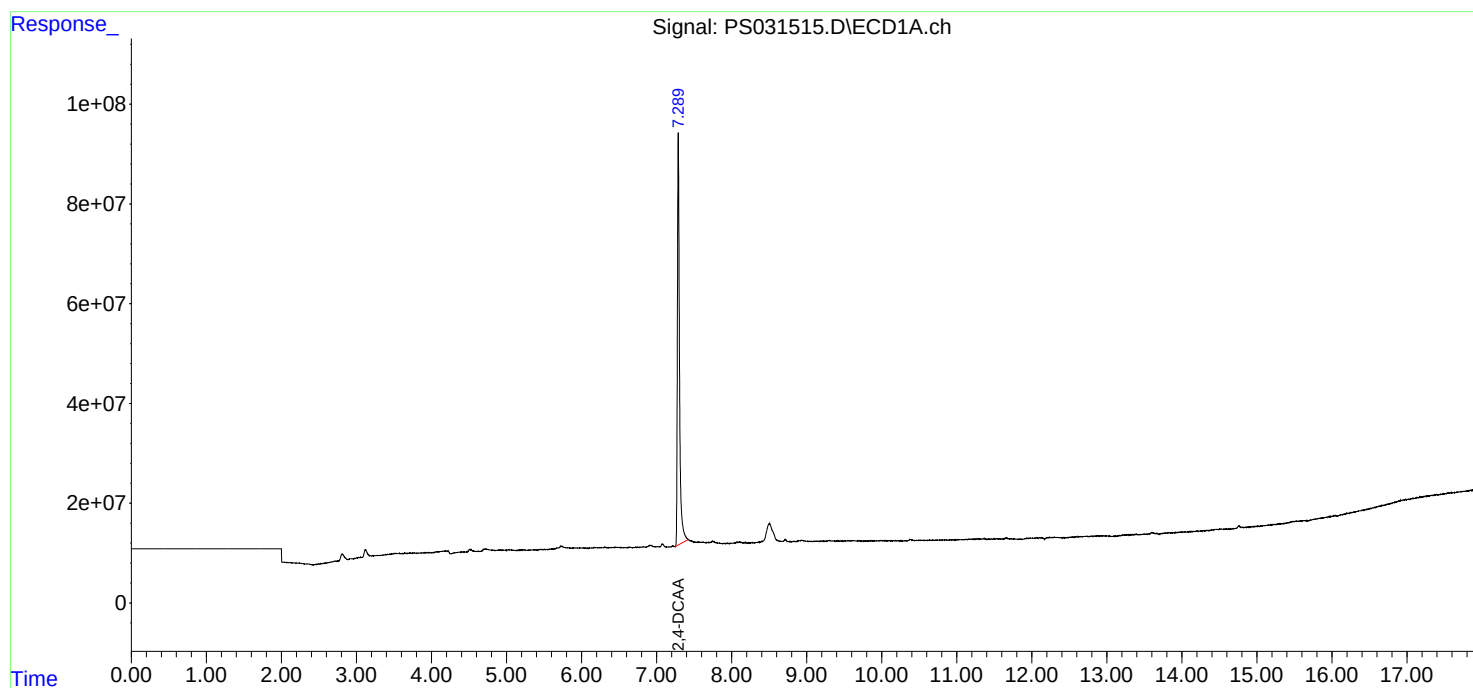


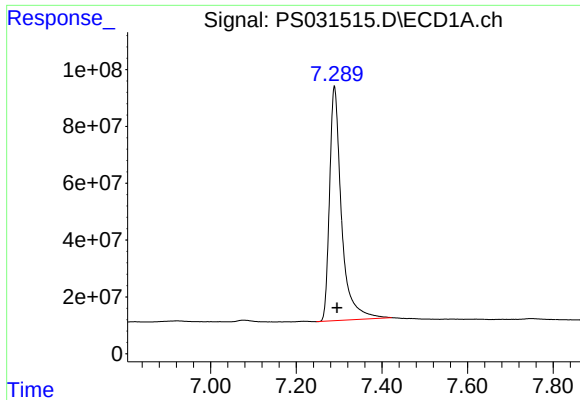

#4 2,4-DCAA


R.T.: 7.289 min
Delta R.T.: -0.005 min
Response: 1601412349
Conc: 504.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

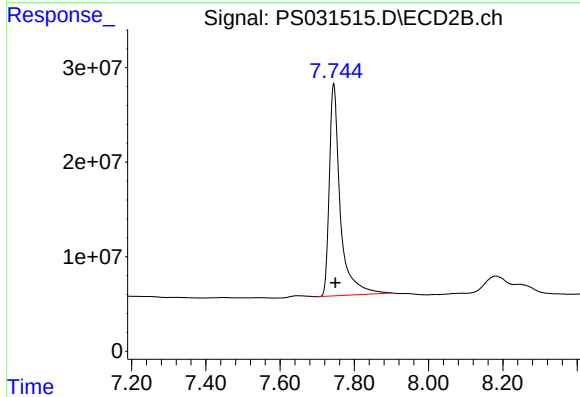


#4 2,4-DCAA

R.T.: 7.744 min
Delta R.T.: -0.005 min
Response: 458873368
Conc: 542.83 ng/ml

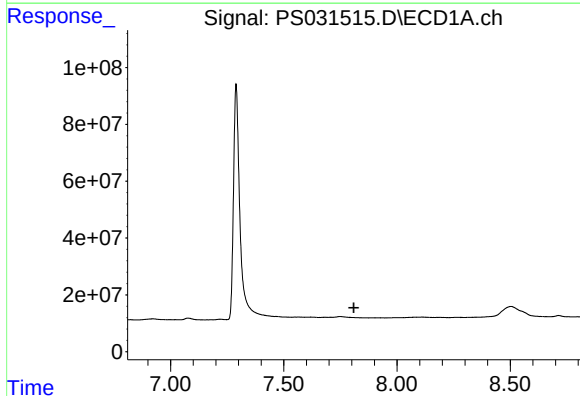

#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.809 min
Response: 0
Conc: N.D.

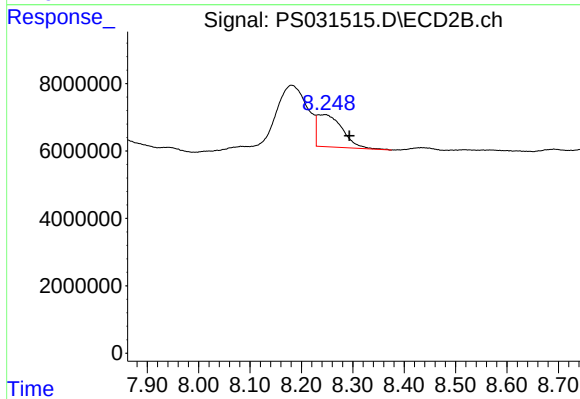

#7 MCPA

R.T.: 8.246 min
Delta R.T.: -0.048 min
Response: 32550843
Conc: 11.60 ug/ml